

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100125\
 Data File : PS031912.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2025 13:29
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 16:54:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.283	7.739	1686.6E6	491.1E6	468.304	540.329
Target Compounds							
1) T	Dalapon	2.718f	2.729f	11245630	17284496	1.945	6.134 #
2) T	3,5-DICHL...	6.447	0.000	3409345	0	<MDL	N.D. #
3) T	4-Nitroph...	7.077	0.000	4116900	0	3.732	N.D. #
6) T	MCP	0.000	8.043	0	2062514	N.D.	1.095
8) T	DICHLORPROP	8.193	8.684f	-1078156	2648460	N.D.	1.820
10) T	Pentachlo...	8.706	9.503	8013168	8875164	<MDL	<MDL #
11) T	2,4,5-TP ...	9.290	9.898	7494563	4774941	<MDL	<MDL #
12) T	2,4,5-T	9.613f	10.360f	2646157	10943715	<MDL	<MDL #
13) T	2,4-DB	10.151	0.000	5020103	0	2.152	N.D. #
14) T	DINOSEB	11.346	0.000	4687121	0	<MDL	N.D. #
15) T	Picloram	11.175	0.000	3749418	0	<MDL	N.D. #
16) T	DCPA	11.651	0.000	6286703	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100125\
Data File : PS031912.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2025 13:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 16:54:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

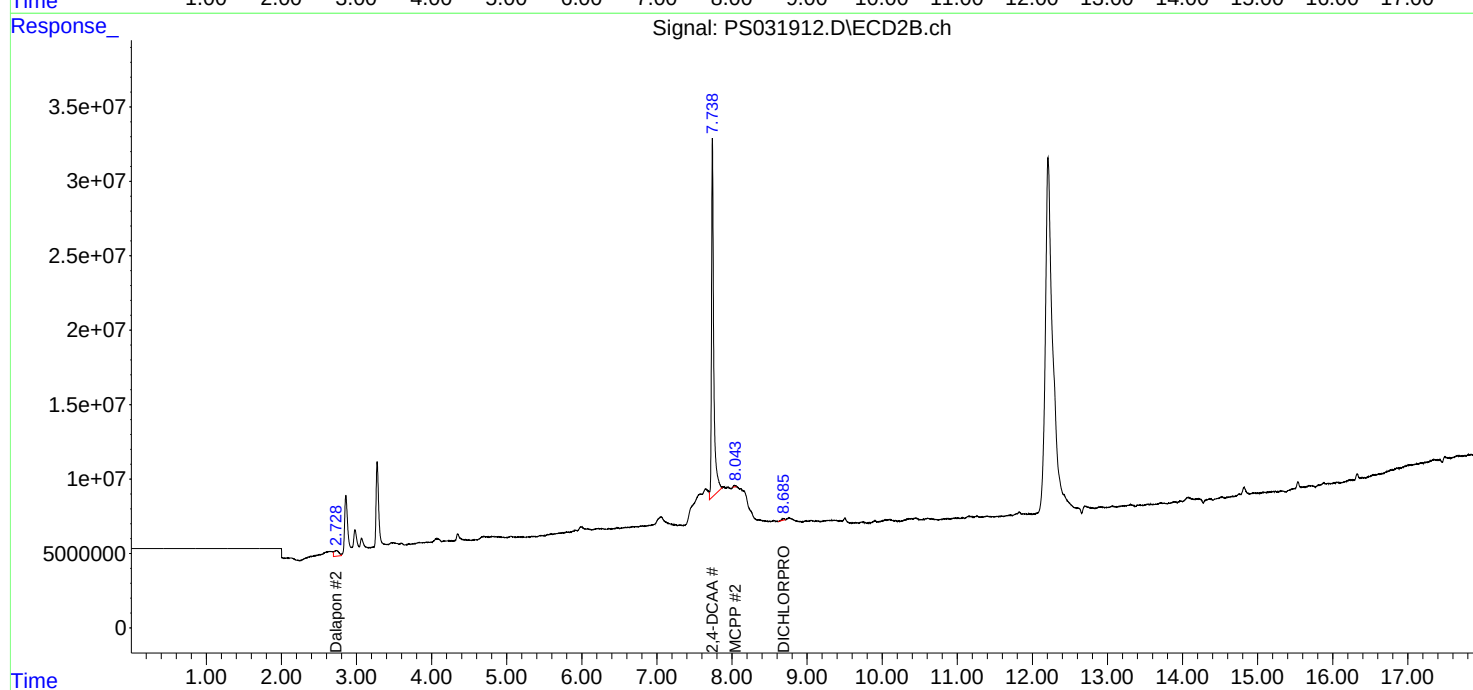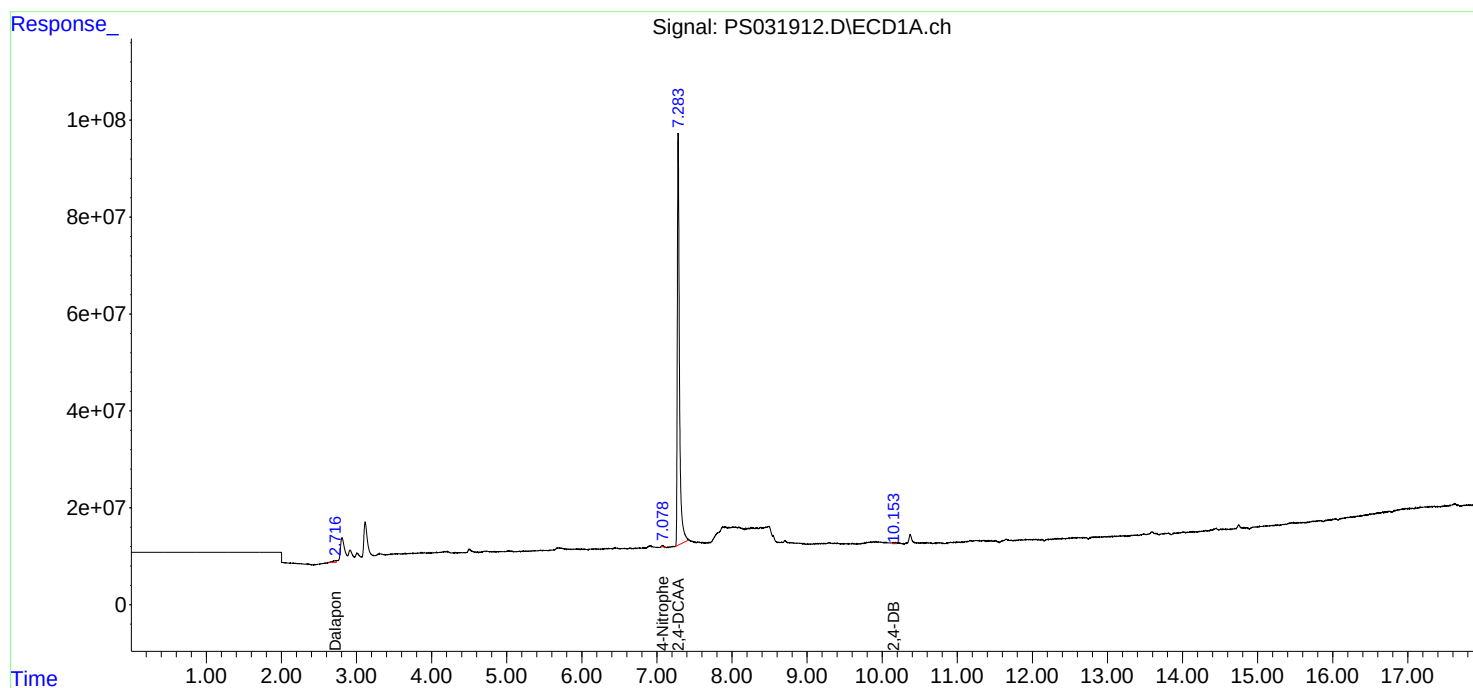


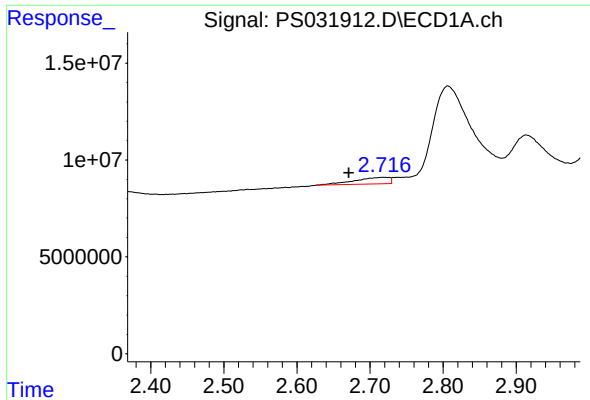

#1 Dalapon


R.T.: 2.718 min
Delta R.T.: 0.047 min
Response: 11245630
Conc: 1.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

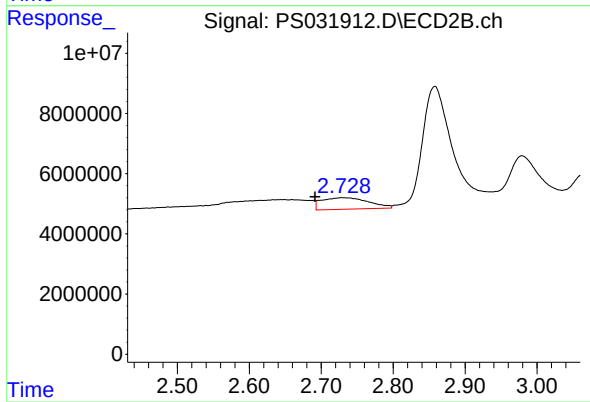


#1 Dalapon

R.T.: 2.729 min
Delta R.T.: 0.037 min
Response: 17284496
Conc: 6.13 ng/ml

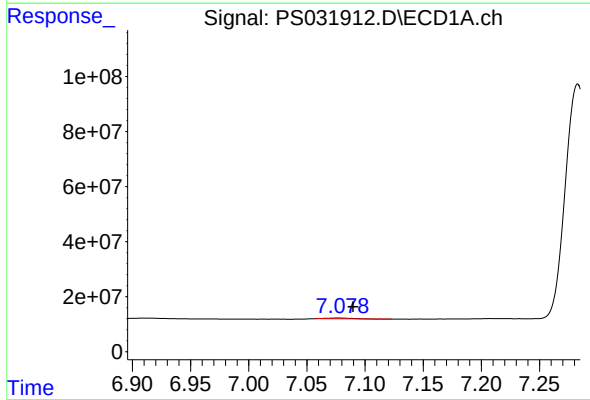


#3 4-Nitrophenol

R.T.: 7.077 min
Delta R.T.: -0.012 min
Response: 4116900
Conc: 3.73 ng/ml

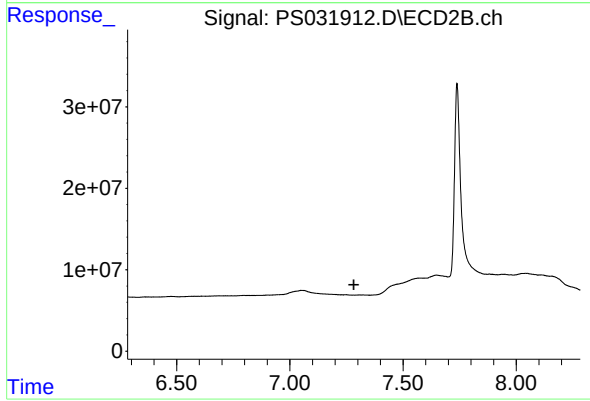

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.283 min
Response: 0
Conc: N.D.

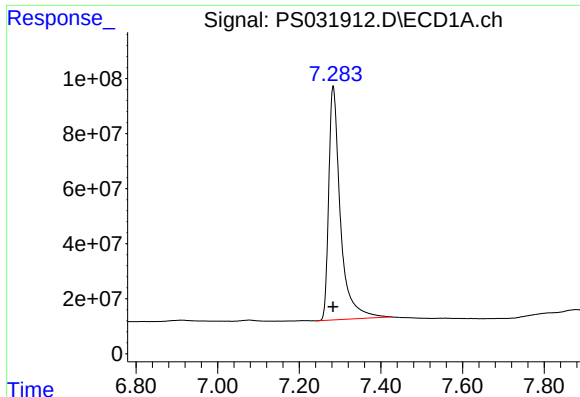

#4 2,4-DCAA


R.T.: 7.283 min
Delta R.T.: 0.000 min
Response: 1686608142
Conc: 468.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

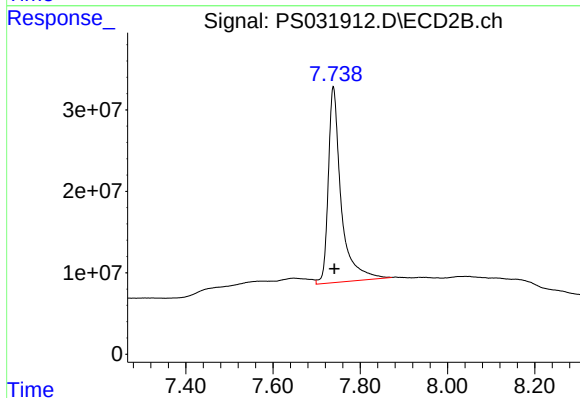


#4 2,4-DCAA

R.T.: 7.739 min
Delta R.T.: -0.002 min
Response: 491104574
Conc: 540.33 ng/ml

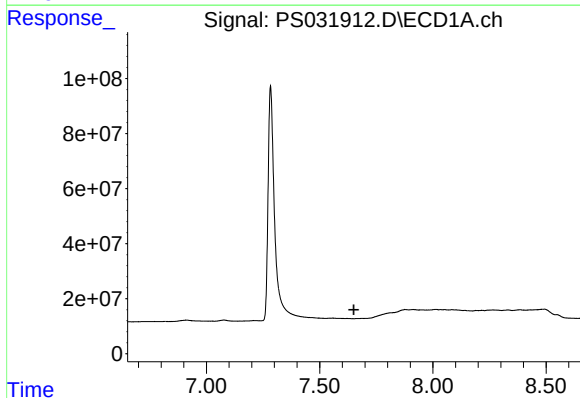


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.651 min
Response: 0
Conc: N.D.

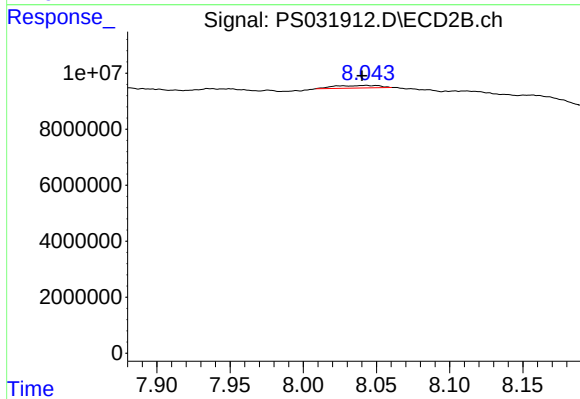

#6 MCP


R.T.: 8.043 min
Delta R.T.: 0.002 min
Response: 2062514
Conc: 1.10 ug/ml

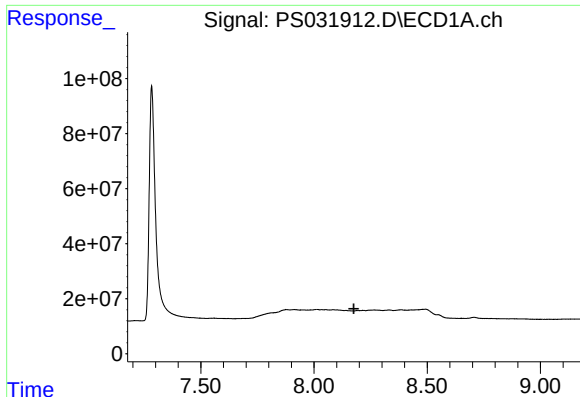

#8 DICHLORPROP


R.T.: 8.193 min
Delta R.T.: 0.016 min
Response: -1078156
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

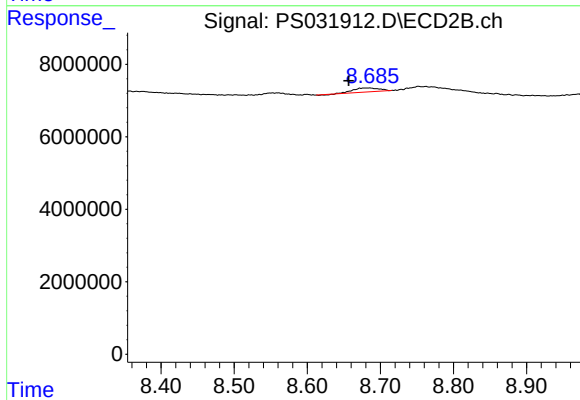


#8 DICHLORPROP

R.T.: 8.684 min
Delta R.T.: 0.027 min
Response: 2648460
Conc: 1.82 ng/ml

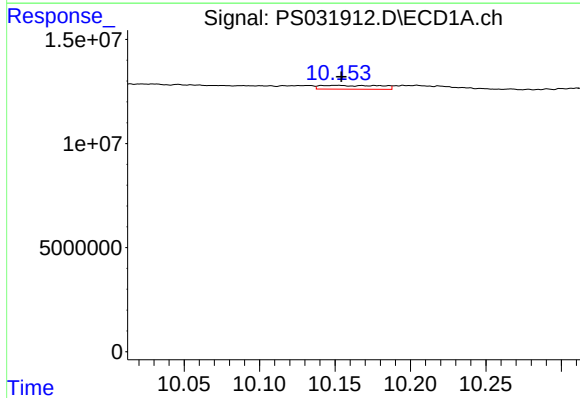

#13 2,4-DB

R.T.: 10.151 min
Delta R.T.: -0.003 min
Response: 5020103
Conc: 2.15 ng/ml

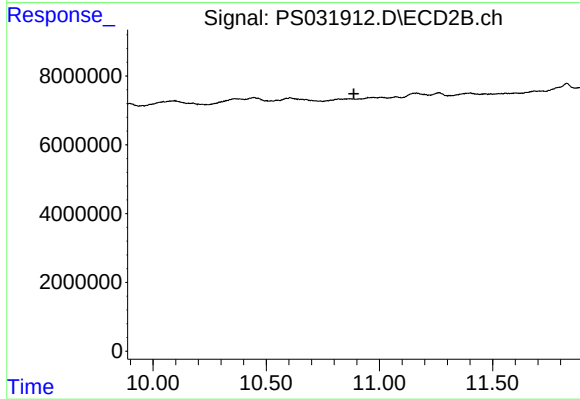

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.887 min
Response: 0
Conc: N.D.