

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100218\
 Data File : PL040553.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2018 10:42
 Operator : AJ\SJ
 Sample : J5170-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 02:39:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.805	174.2E6	63907163	23.804	20.238
28)	SA Decachlor...	7.809	8.729	159.6E6	45424179	16.792	14.344
Target Compounds							
2)	A alpha-BHC	3.638	0.000	22410627	0	1.915	N.D. #
7)	B delta-BHC	0.000	4.846	0	5564137	N.D.	1.205 #
9)	A Endosulfan I	5.134	5.967	15470379	46141724	1.535	12.402 #
11)	B alpha-Chl...	5.134	5.967f	15470379	46141724	1.477	11.758 #
15)	B Endosulfa...	0.000	6.669	0	33466494	N.D.	9.574 #
16)	A 4,4'-DDD	5.783	0.000	13131388	0	1.422	N.D. #
26)	Chlordane-4	5.134	5.967	15470379	46141724	13.056	69.916 #
27)	Chlordane-5	0.000	6.669	0	33466494	N.D.	274.838 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100218\
Data File : PL040553.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2018 10:42
Operator : AJ\SJ
Sample : J5170-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 02:39:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

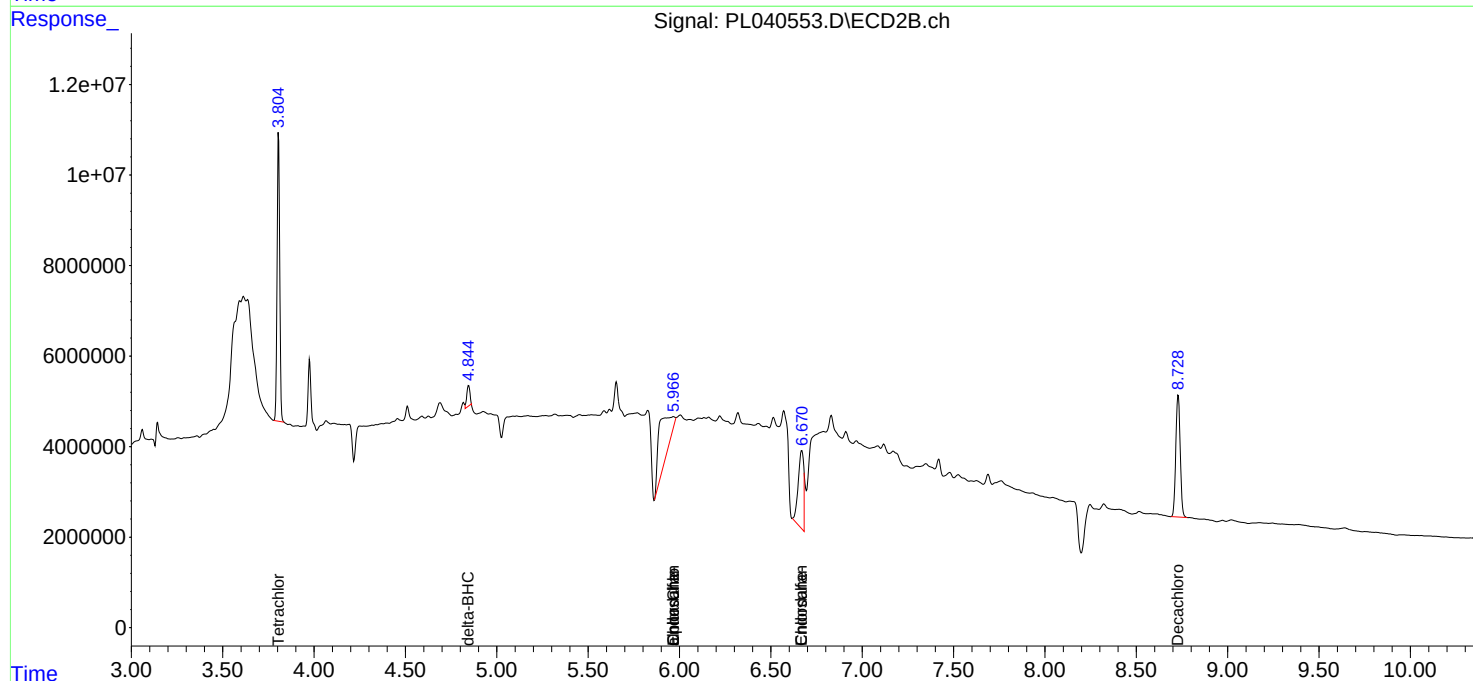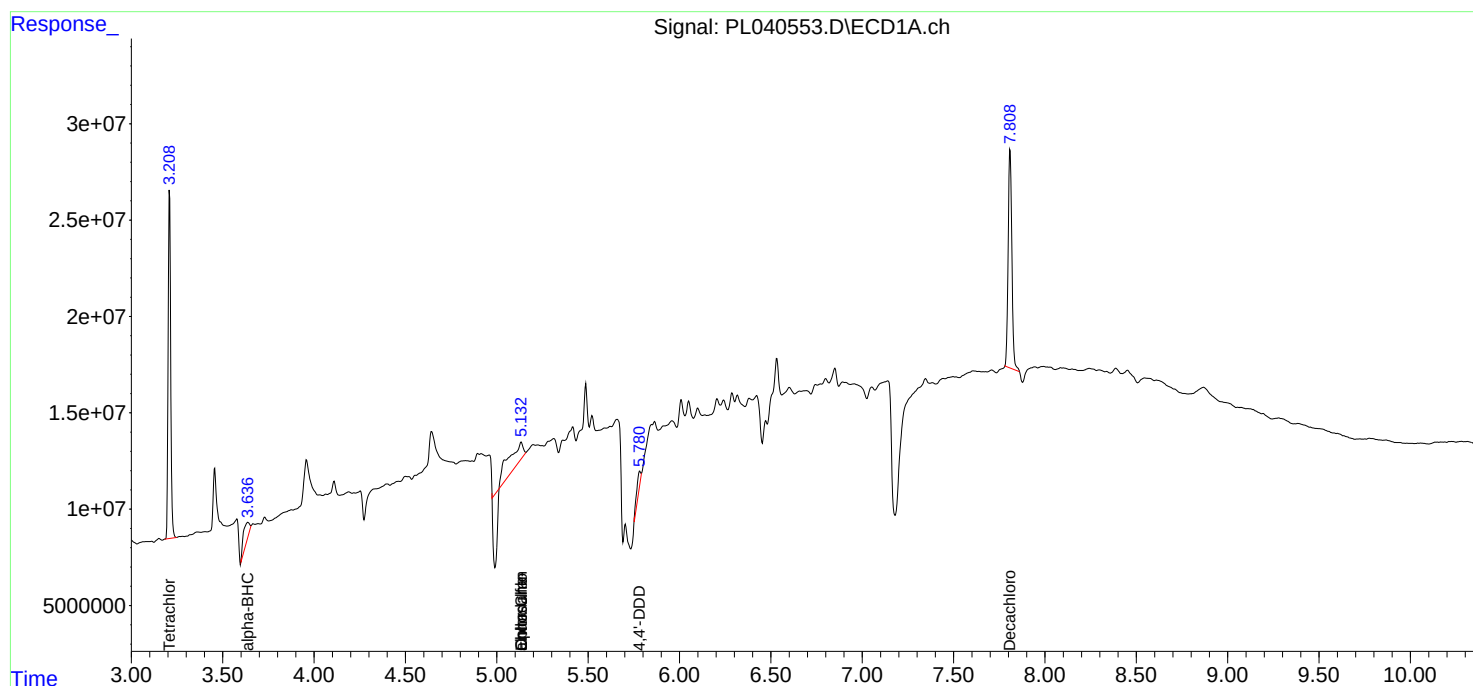


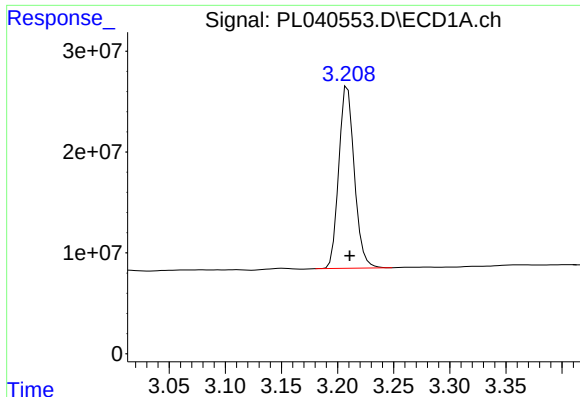

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.002 min
Response: 174245468
Conc: 23.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

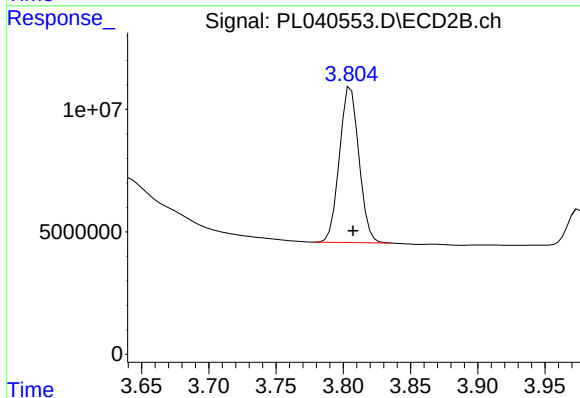


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: -0.002 min
Response: 63907163
Conc: 20.24 ng/ml

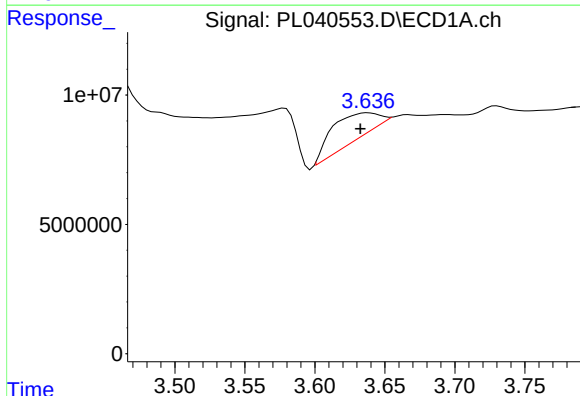


#2 alpha-BHC

R.T.: 3.638 min
Delta R.T.: 0.005 min
Response: 22410627
Conc: 1.92 ng/ml

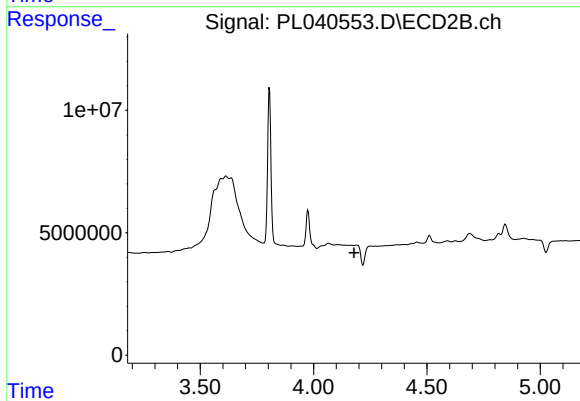

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.179 min
Response: 0
Conc: N.D.

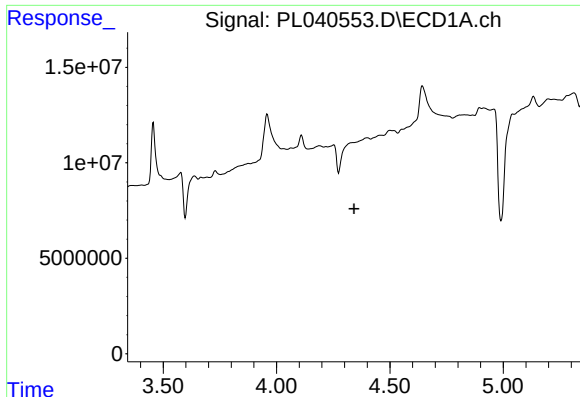

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

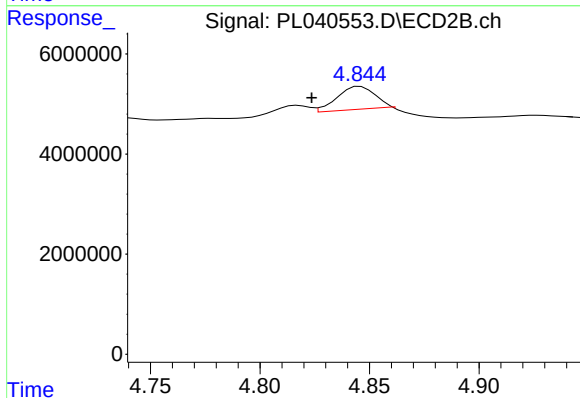


#7 delta-BHC

R.T.: 4.846 min
Delta R.T.: 0.022 min
Response: 5564137
Conc: 1.21 ng/ml

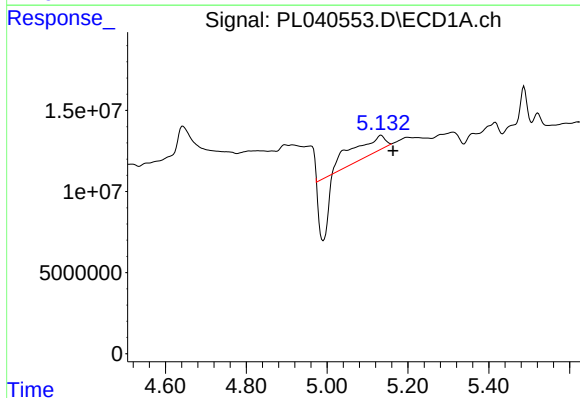


#9 Endosulfan I

R.T.: 5.134 min
Delta R.T.: -0.030 min
Response: 15470379
Conc: 1.53 ng/ml

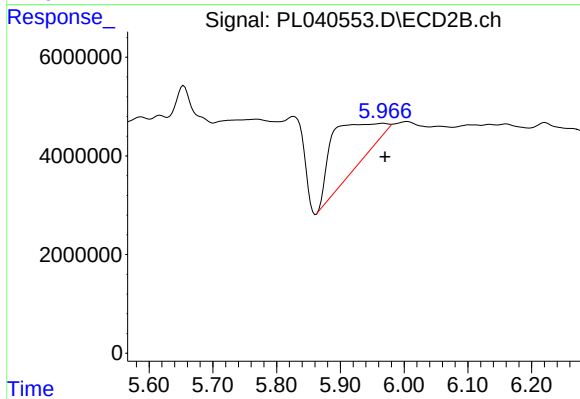

#9 Endosulfan I


R.T.: 5.967 min
Delta R.T.: -0.003 min
Response: 46141724
Conc: 12.40 ng/ml

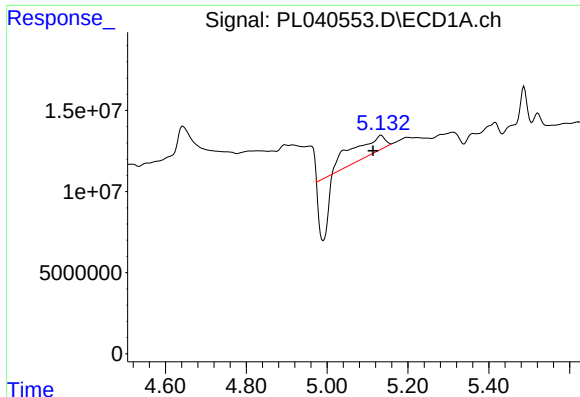

#11 alpha-Chlordane


R.T.: 5.134 min
Delta R.T.: 0.020 min
Response: 15470379
Conc: 1.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

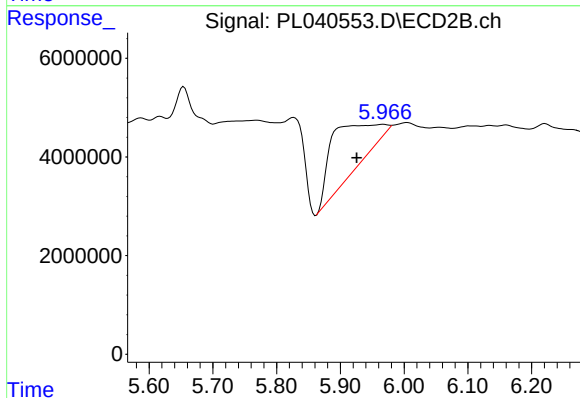


#11 alpha-Chlordane

R.T.: 5.967 min
Delta R.T.: 0.042 min
Response: 46141724
Conc: 11.76 ng/ml

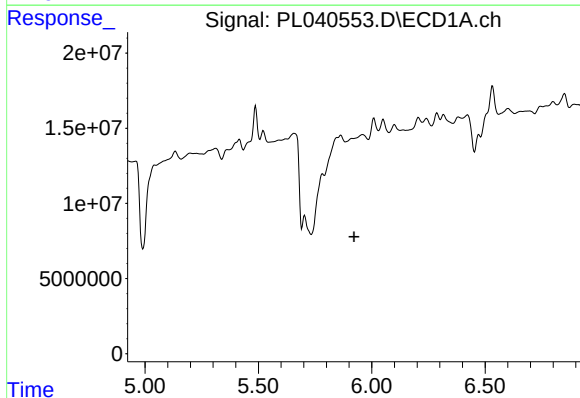


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.922 min
Response: 0
Conc: N.D.

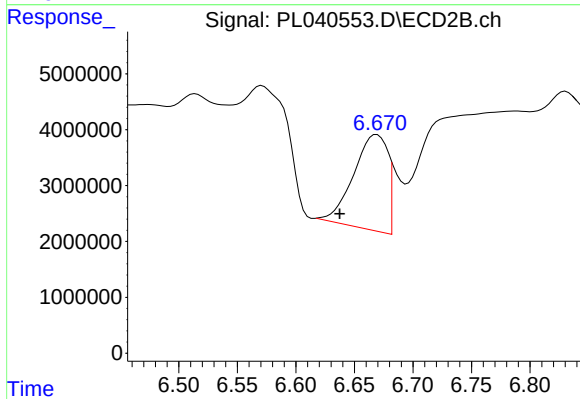

#15 Endosulfan II


R.T.: 6.669 min
Delta R.T.: 0.032 min
Response: 33466494
Conc: 9.57 ng/ml

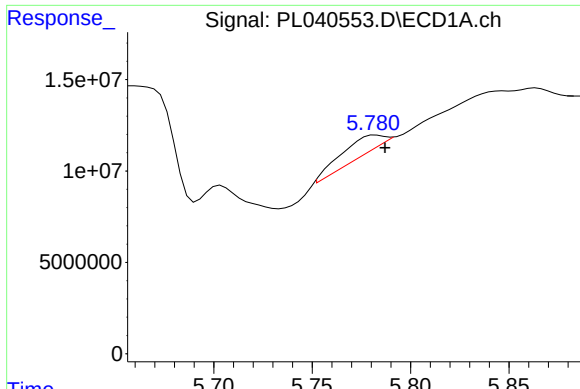

#16 4,4'-DDD


R.T.: 5.783 min
Delta R.T.: -0.004 min
Response: 13131388
Conc: 1.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

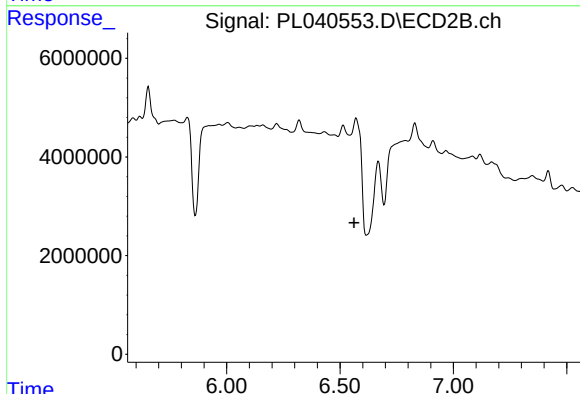


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.562 min
Response: 0
Conc: N.D.

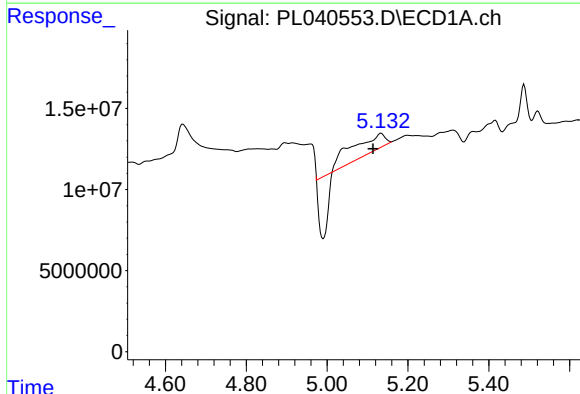


#26 Chlordane-4

R.T.: 5.134 min
Delta R.T.: 0.020 min
Response: 15470379
Conc: 13.06 ng/ml

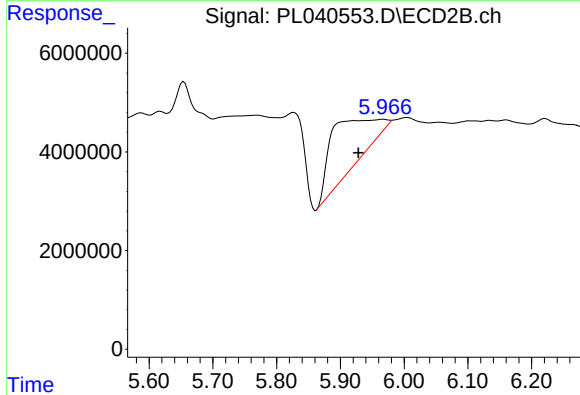

#26 Chlordane-4


R.T.: 5.967 min
Delta R.T.: 0.039 min
Response: 46141724
Conc: 69.92 ng/ml

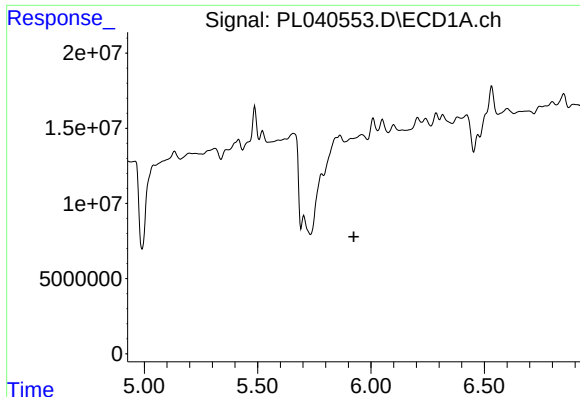

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.924 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

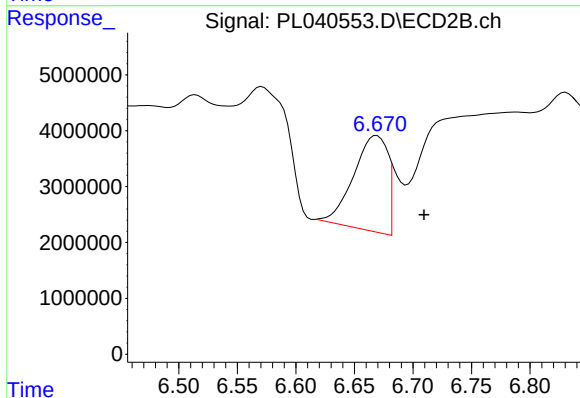


#27 Chlordane-5

R.T.: 6.669 min
Delta R.T.: -0.040 min
Response: 33466494
Conc: 274.84 ng/ml

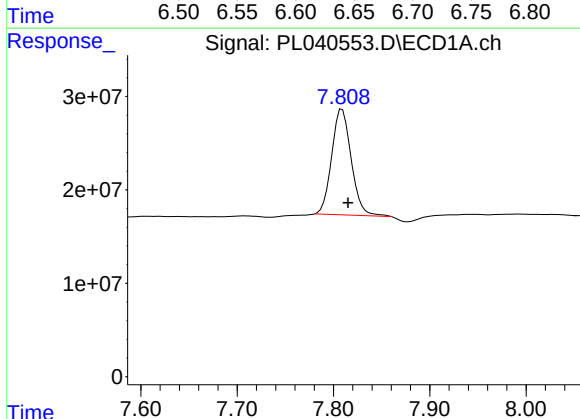

#28 Decachlorobiphenyl

R.T.: 7.809 min
Delta R.T.: -0.006 min
Response: 159625744
Conc: 16.79 ng/ml

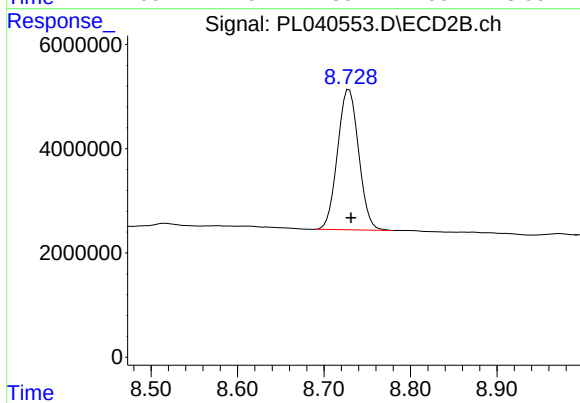

#28 Decachlorobiphenyl

R.T.: 8.729 min
Delta R.T.: -0.002 min
Response: 45424179
Conc: 14.34 ng/ml