

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100218\
 Data File : PL040579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2018 17:22
 Operator : AJ\SJ
 Sample : PB113442B
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 02:44:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.806	172.6E6	65032218	23.577	20.594
28)	SA Decachlor...	7.811	8.731	206.0E6	61845218	21.671	19.529
Target Compounds							
2)	A alpha-BHC	3.612	4.190	15885325	4787957	1.358	1.010 #
3)	MA gamma-BHC...	3.939f	0.000	4527677	0	0.416	N.D. #
4)	MA Heptachlor	4.114f	0.000	6230346	0	0.529	N.D. #
6)	B beta-BHC	4.114f	0.000	6230346	0	1.476	N.D. #
7)	B delta-BHC	0.000	4.815	0	3745502	N.D.	0.811 #
19)	B Endosulfa...	6.317	6.994	52501084	9624589	5.485	2.992 #
20)	A Methoxychlor	6.496f	7.256f	146.8E6	11333265	30.386	7.437 #
23)	Chlordane-1	0.000	4.815	0	3745502	N.D.	24.270 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100218\
Data File : PL040579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2018 17:22
Operator : AJ\SJ
Sample : PB113442B
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 02:44:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

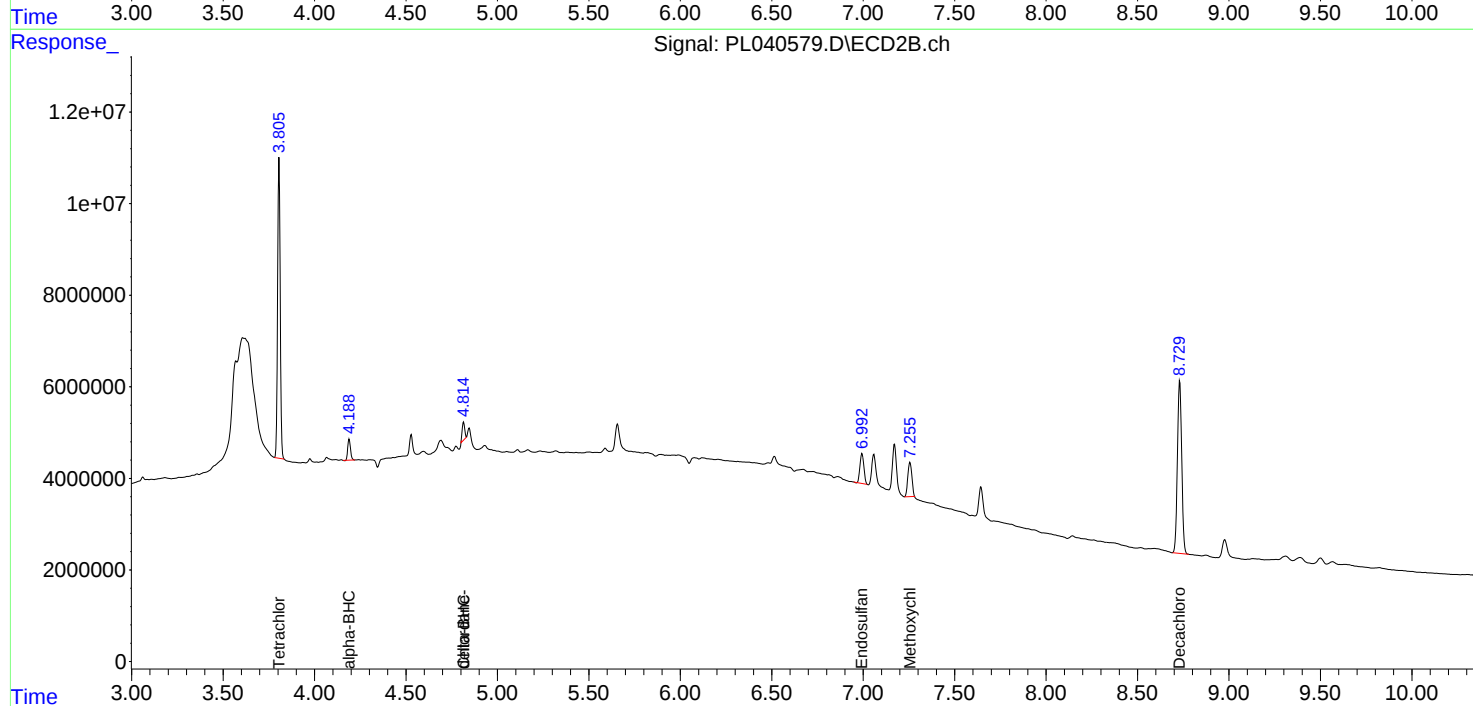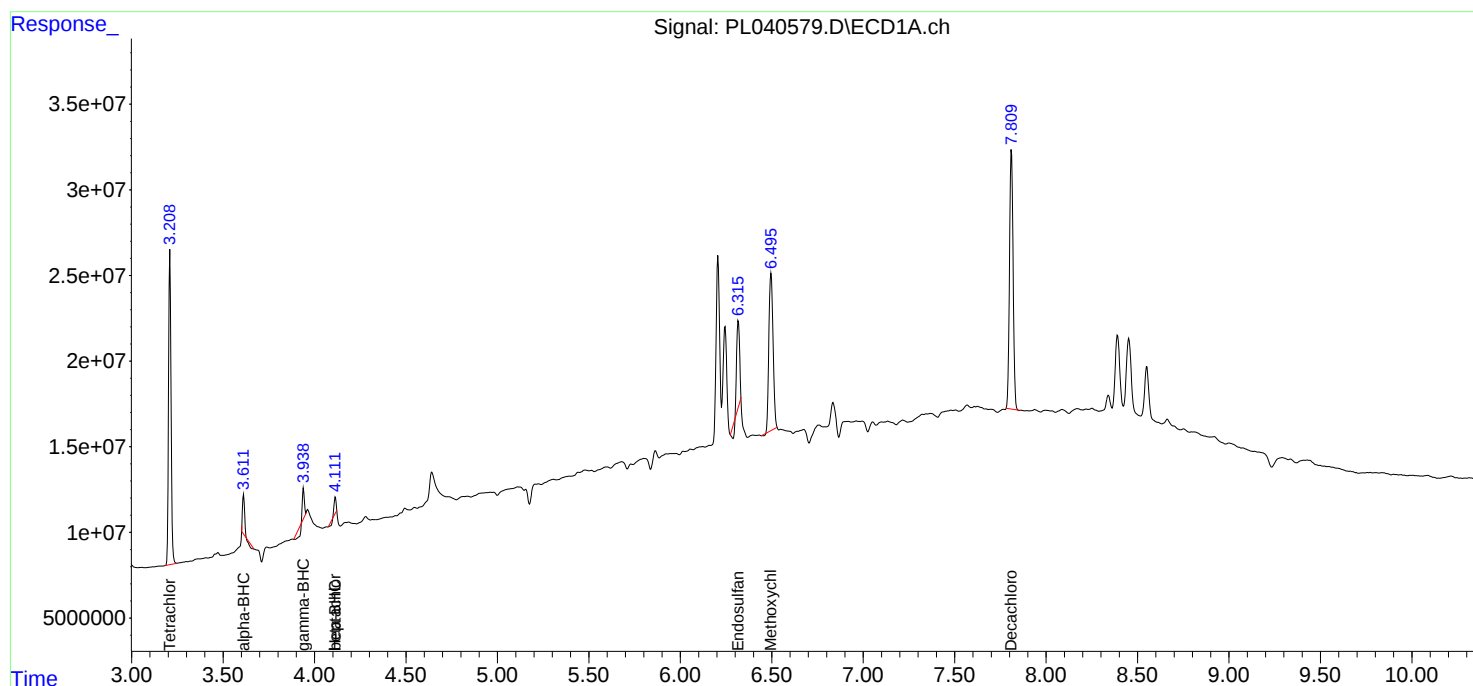


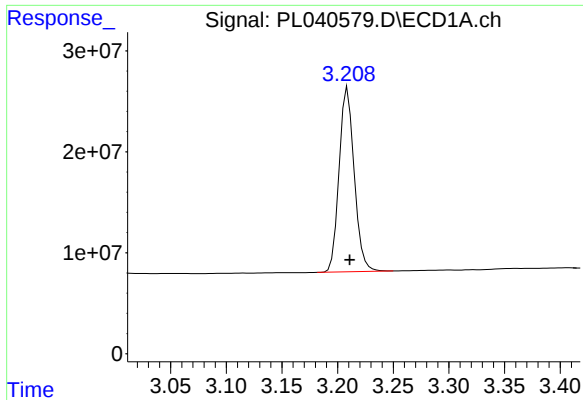

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.002 min
Response: 172582662
Conc: 23.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

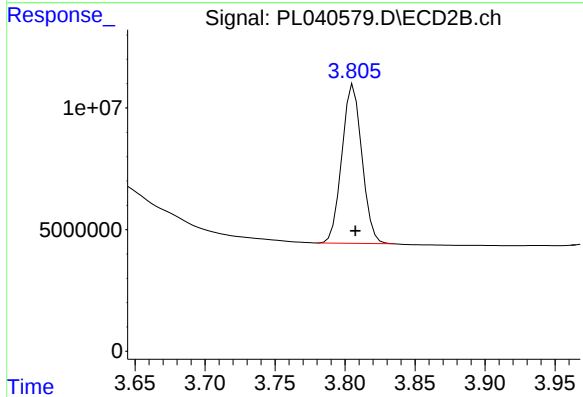


#1 Tetrachloro-m-xylene

R.T.: 3.806 min
Delta R.T.: -0.001 min
Response: 65032218
Conc: 20.59 ng/ml

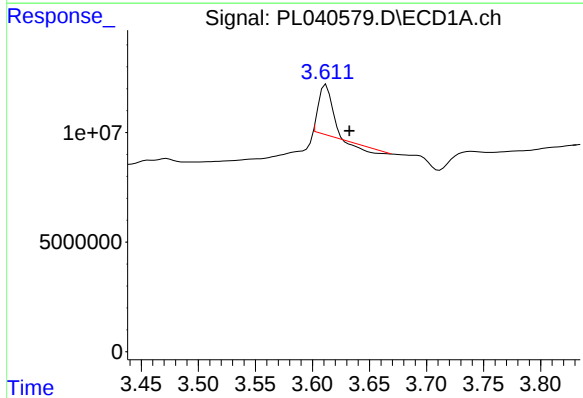


#2 alpha-BHC

R.T.: 3.612 min
Delta R.T.: -0.020 min
Response: 15885325
Conc: 1.36 ng/ml

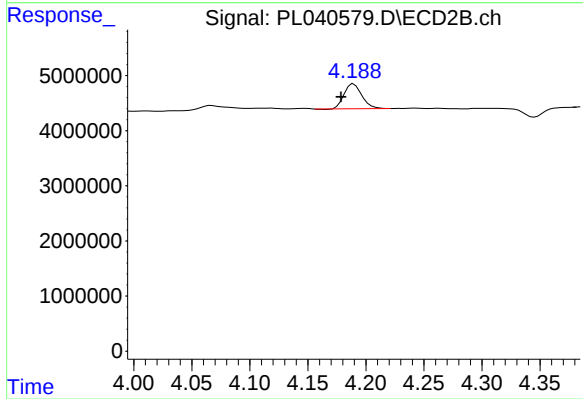

#2 alpha-BHC


R.T.: 4.190 min
Delta R.T.: 0.011 min
Response: 4787957
Conc: 1.01 ng/ml

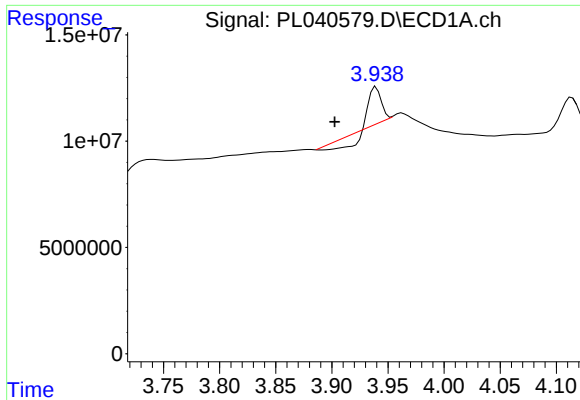

#3 gamma-BHC (Lindane)


R.T.: 3.939 min
Delta R.T.: 0.037 min
Response: 4527677
Conc: 0.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

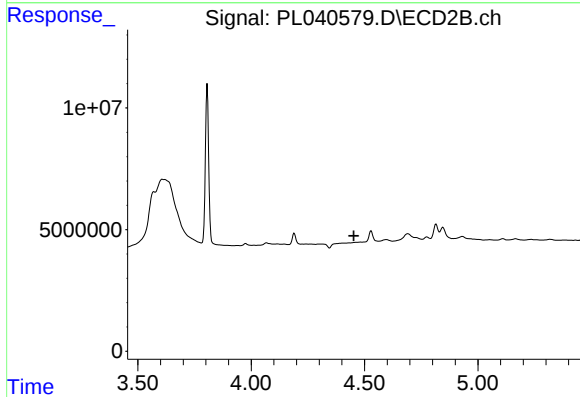


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.452 min
Response: 0
Conc: N.D.

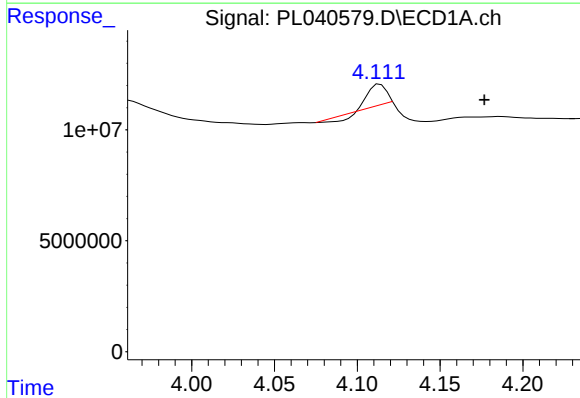


#4 Heptachlor

R.T.: 4.114 min
Delta R.T.: -0.063 min
Response: 6230346
Conc: 0.53 ng/ml

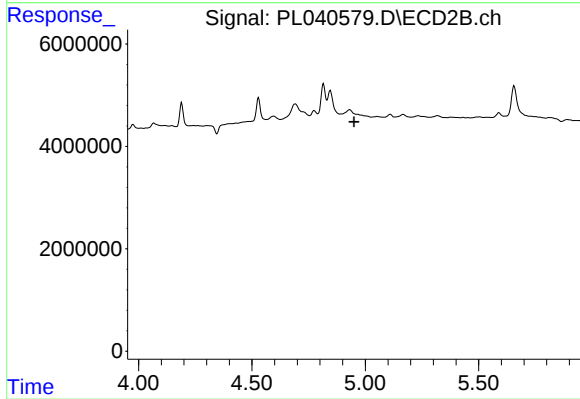

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.951 min
Response: 0
Conc: N.D.

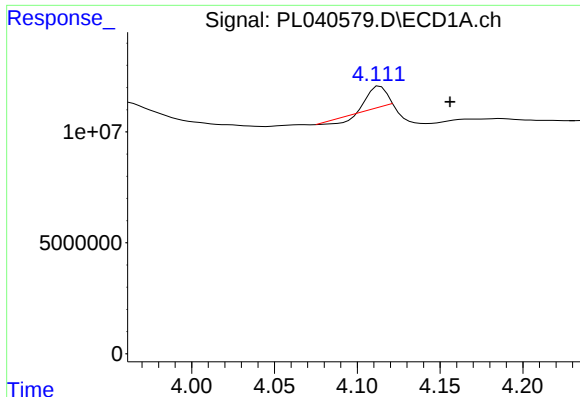

#6 beta-BHC


R.T.: 4.114 min
Delta R.T.: -0.042 min
Response: 6230346
Conc: 1.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

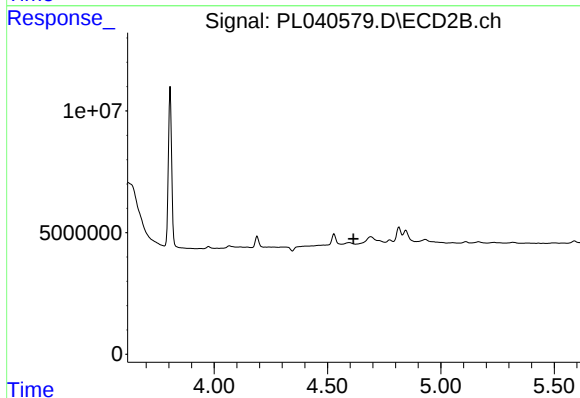


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.615 min
Response: 0
Conc: N.D.

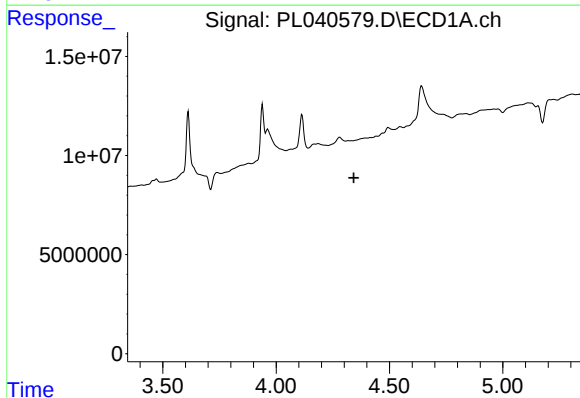


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

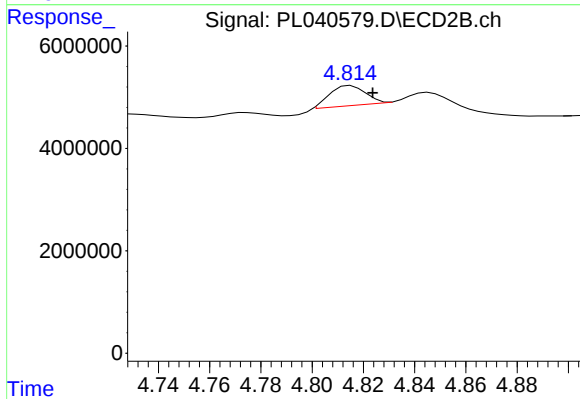

#7 delta-BHC


R.T.: 4.815 min
Delta R.T.: -0.009 min
Response: 3745502
Conc: 0.81 ng/ml

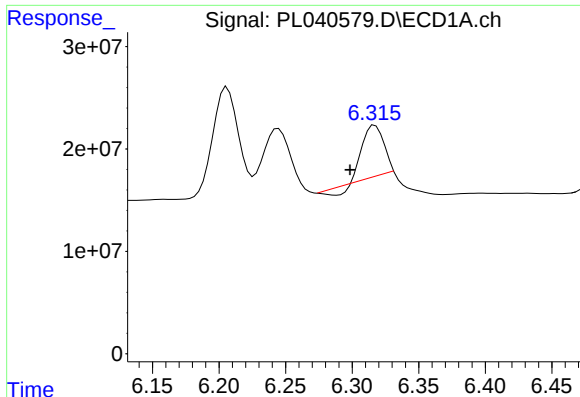

#19 Endosulfan Sulfate


R.T.: 6.317 min
Delta R.T.: 0.019 min
Response: 52501084
Conc: 5.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

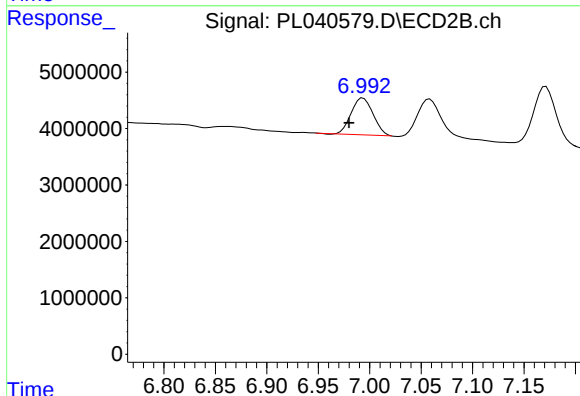


#19 Endosulfan Sulfate

R.T.: 6.994 min
Delta R.T.: 0.014 min
Response: 9624589
Conc: 2.99 ng/ml

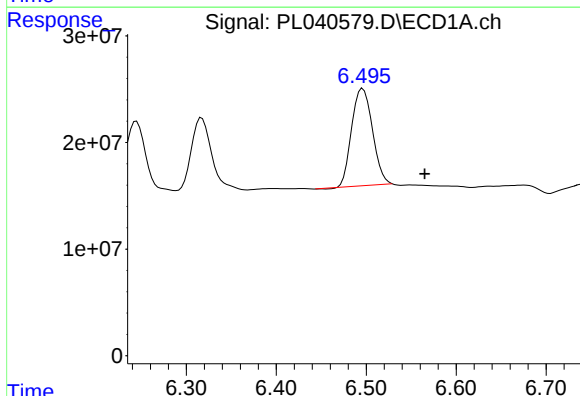


#20 Methoxychlor

R.T.: 6.496 min
Delta R.T.: -0.069 min
Response: 146774584
Conc: 30.39 ng/ml

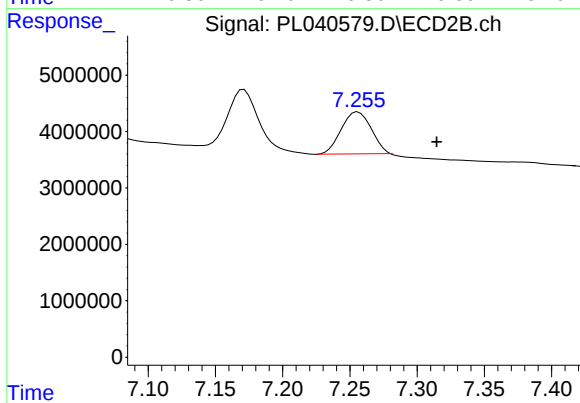

#20 Methoxychlor


R.T.: 7.256 min
Delta R.T.: -0.058 min
Response: 11333265
Conc: 7.44 ng/ml

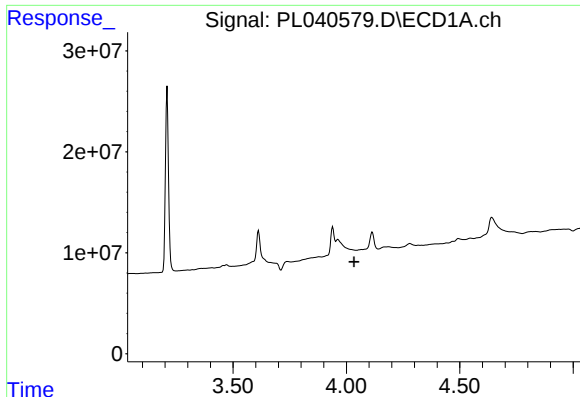

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

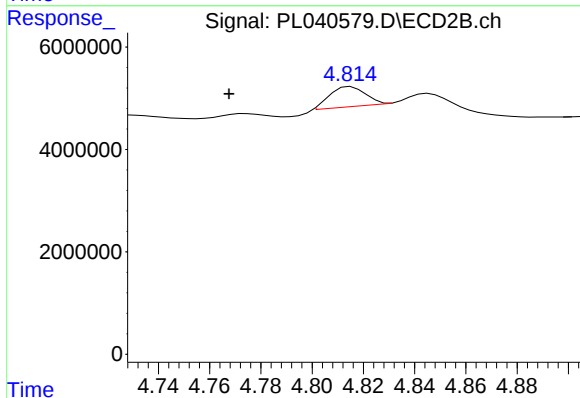


#23 Chlordane-1

R.T.: 4.815 min
Delta R.T.: 0.048 min
Response: 3745502
Conc: 24.27 ng/ml

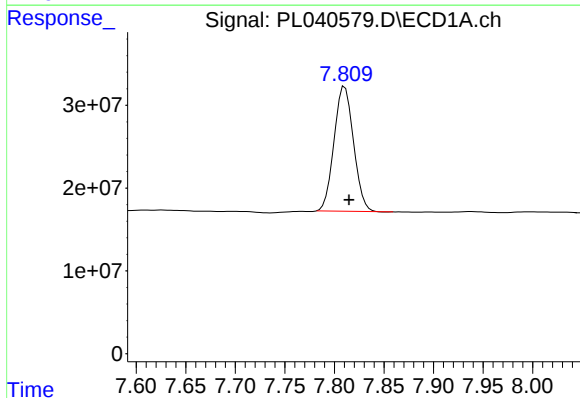

#28 Decachlorobiphenyl

R.T.: 7.811 min
Delta R.T.: -0.004 min
Response: 205996931
Conc: 21.67 ng/ml

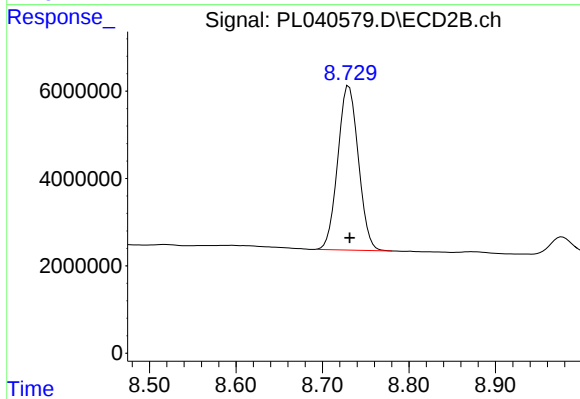

#28 Decachlorobiphenyl

R.T.: 8.731 min
Delta R.T.: 0.000 min
Response: 61845218
Conc: 19.53 ng/ml