

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100218\
 Data File : PL040581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2018 17:50
 Operator : AJ\SJ
 Sample : PB113442TB
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 02:45:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.806	159.8E6	60105548	21.831	19.034
28)	SA Decachlor...	7.810	8.730	198.7E6	58851579	20.904	18.584
Target Compounds							
20)	A Methoxychlor	6.497f	0.000	55057661	0	11.398	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100218\
Data File : PL040581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2018 17:50
Operator : AJ\SJ
Sample : PB113442TB
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 02:45:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

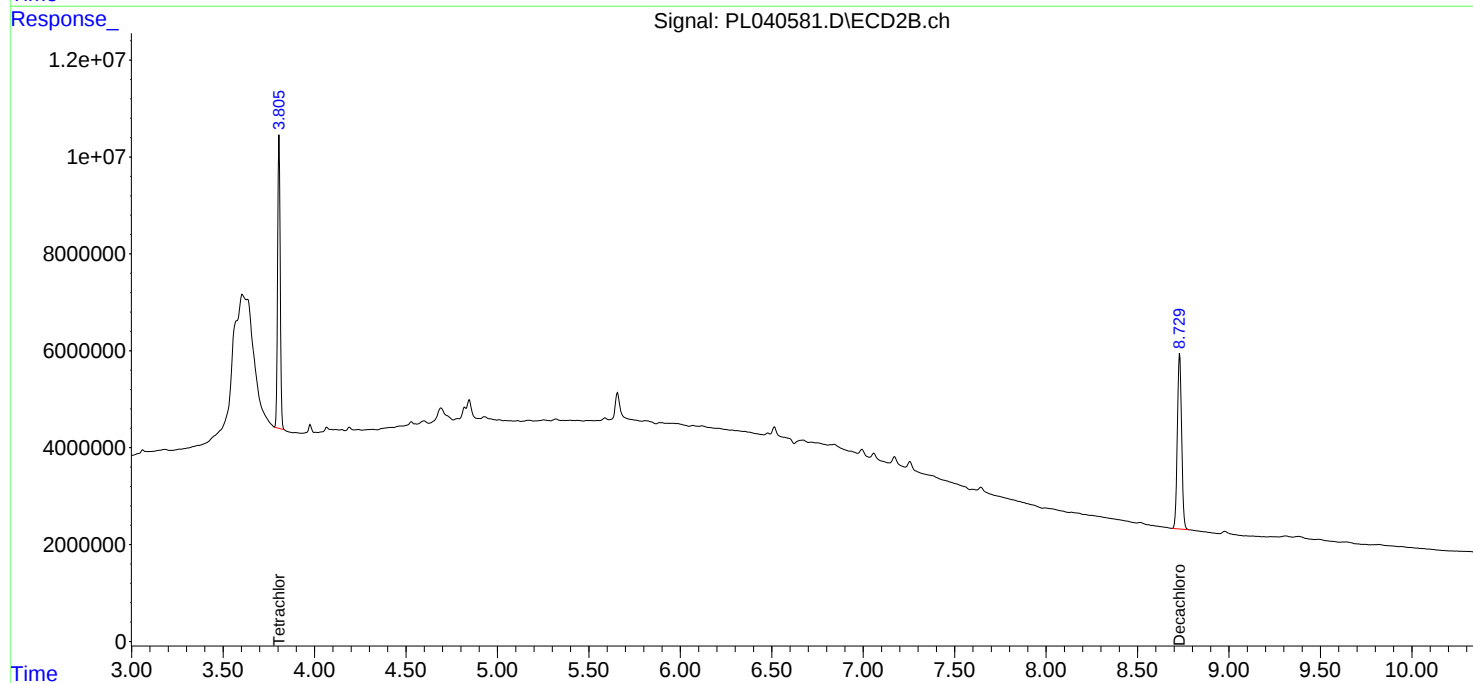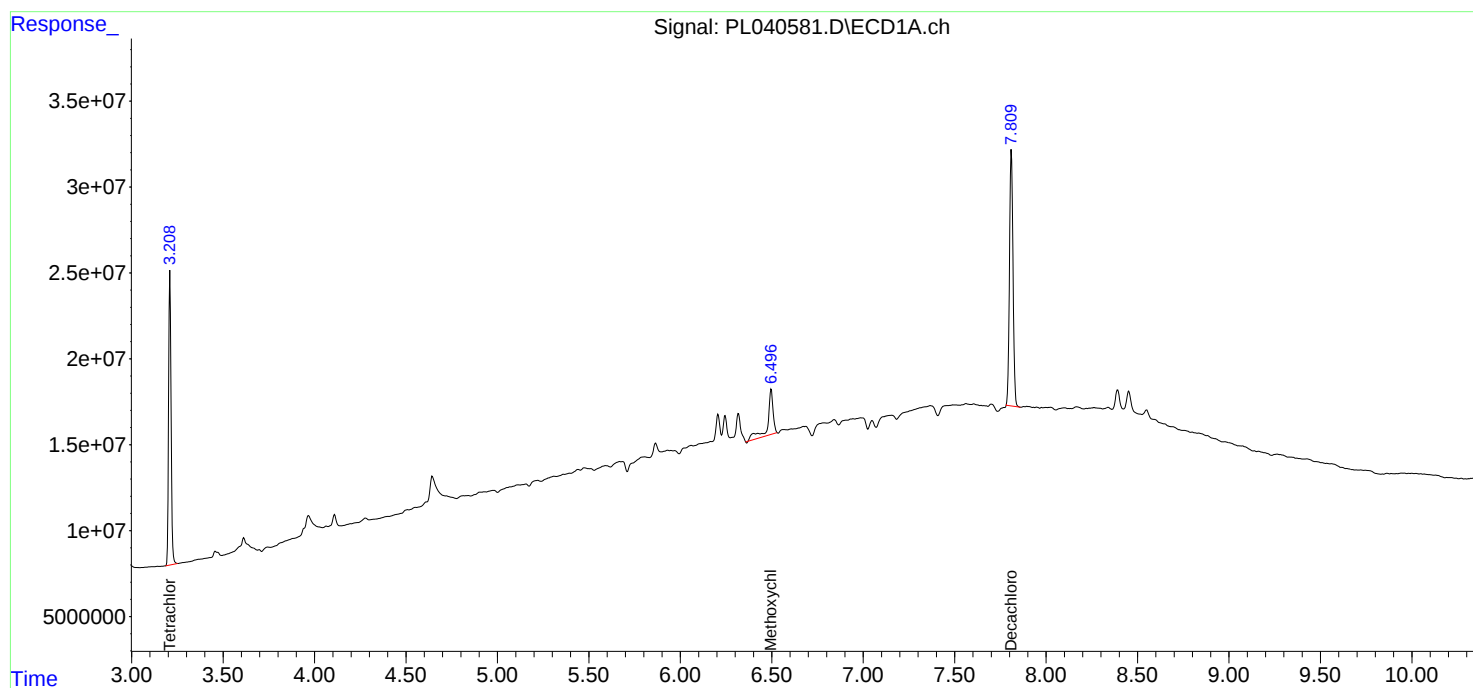


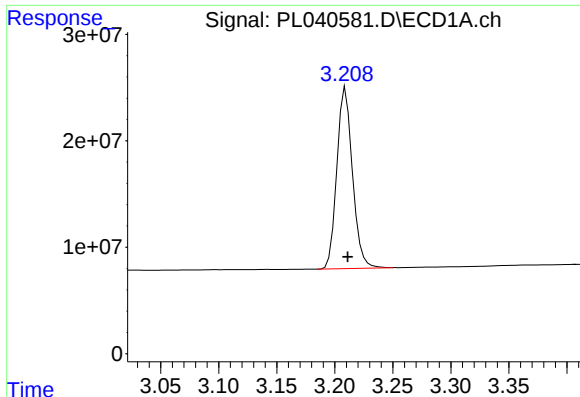

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.002 min
Response: 159803584
Conc: 21.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

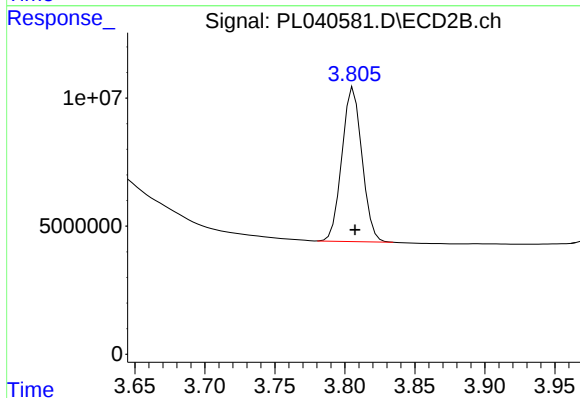


#1 Tetrachloro-m-xylene

R.T.: 3.806 min
Delta R.T.: -0.001 min
Response: 60105548
Conc: 19.03 ng/ml

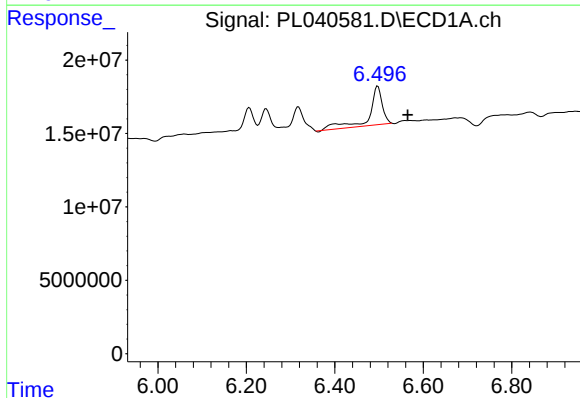


#20 Methoxychlor

R.T.: 6.497 min
Delta R.T.: -0.068 min
Response: 55057661
Conc: 11.40 ng/ml

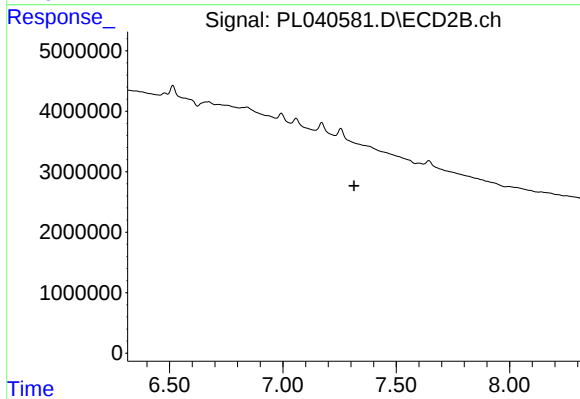

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.314 min
Response: 0
Conc: N.D.

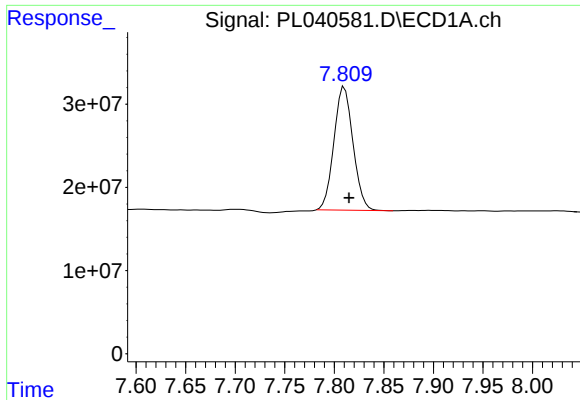

#28 Decachlorobiphenyl

R.T.: 7.810 min
Delta R.T.: -0.005 min
Response: 198710492
Conc: 20.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

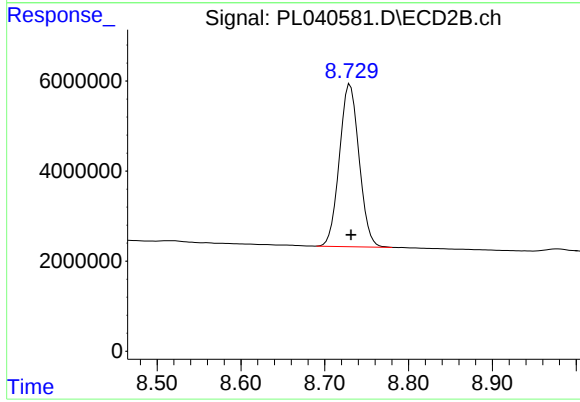

#28 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: -0.001 min
Response: 58851579
Conc: 18.58 ng/ml