

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100218\
 Data File : PL040583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2018 18:18
 Operator : AJ\SJ
 Sample : J5191-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 02:45:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.807	147.7E6	59485407	20.173	18.838
28)	SA Decachlor...	7.811	8.732	204.5E6	59368907	21.513	18.747
Target Compounds							
4)	MA Heptachlor	4.109f	0.000	12596891	0	1.071	N.D. #
6)	B beta-BHC	4.109f	0.000	12596891	0	2.984	N.D. #
7)	B delta-BHC	0.000	4.820	0	5976676	N.D.	1.295 #
20)	A Methoxychlor	6.497f	0.000	79119139	0	16.380	N.D. #
23)	Chlordane-1	0.000	4.820	0	5976676	N.D.	38.727 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100218\
Data File : PL040583.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2018 18:18
Operator : AJ\SJ
Sample : J5191-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 02:45:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

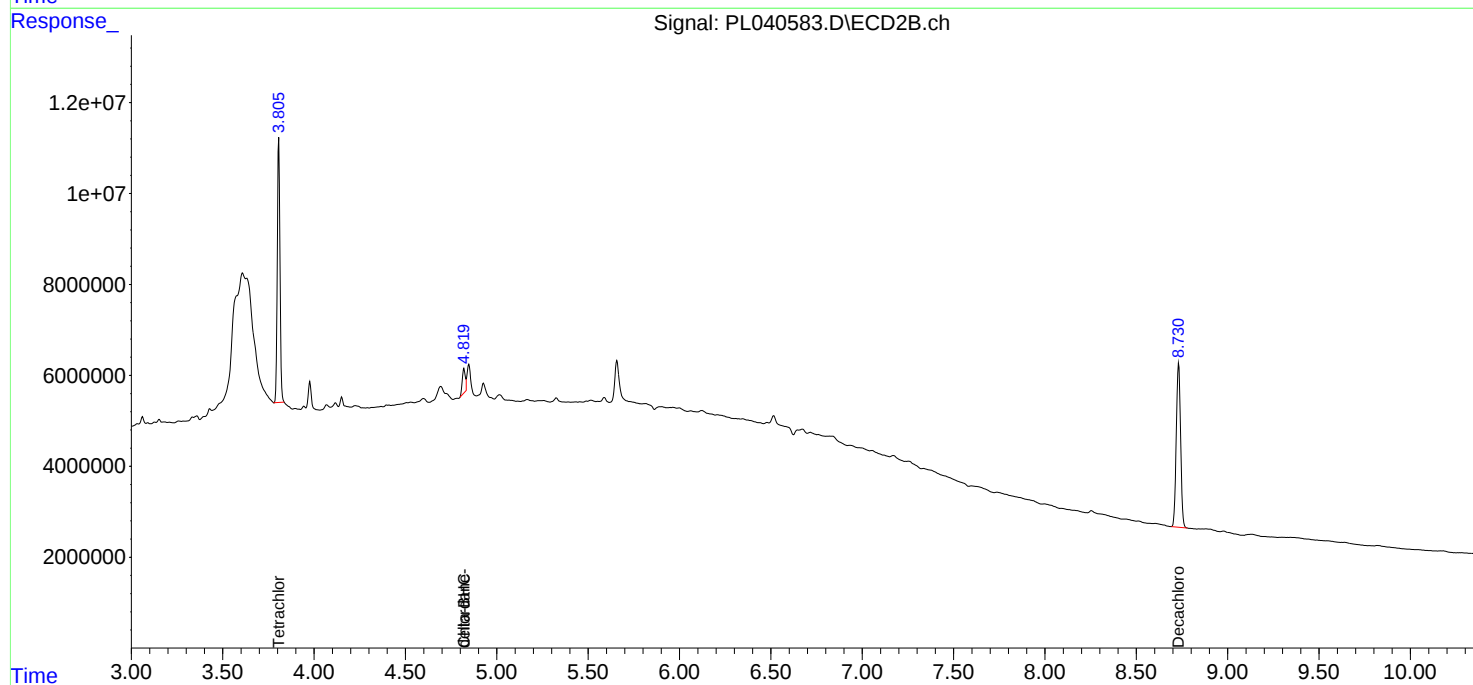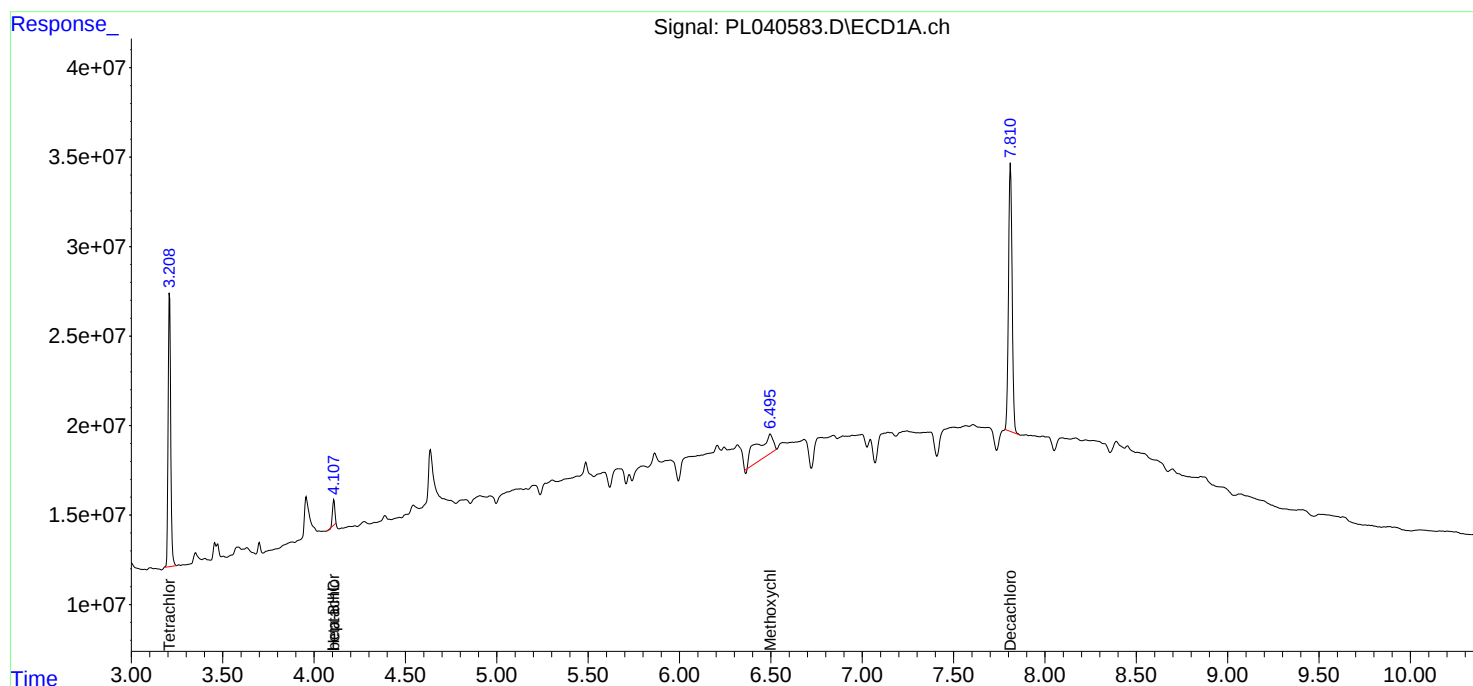


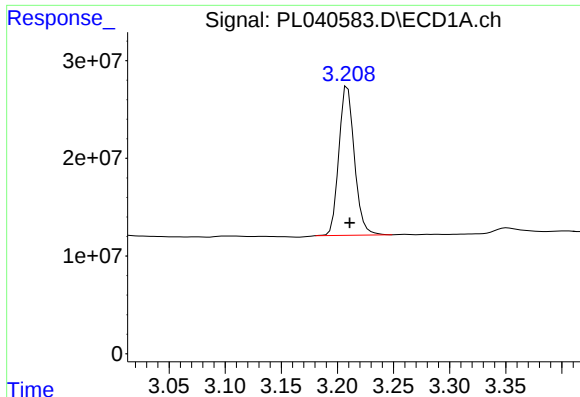

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.002 min
Response: 147668605
Conc: 20.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

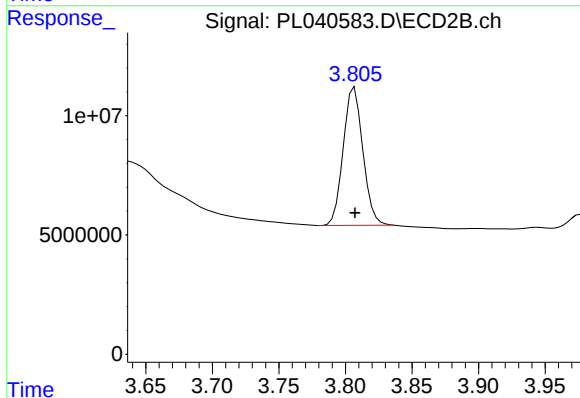


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 59485407
Conc: 18.84 ng/ml

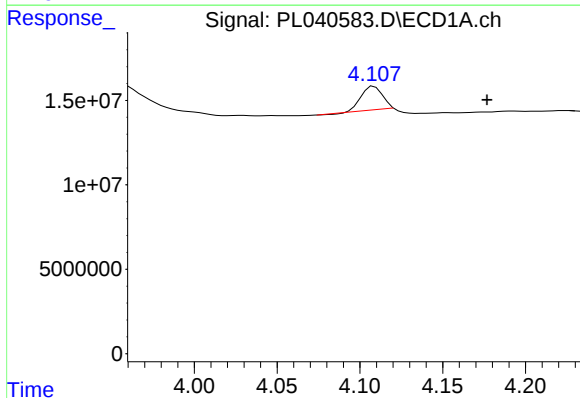


#4 Heptachlor

R.T.: 4.109 min
Delta R.T.: -0.068 min
Response: 12596891
Conc: 1.07 ng/ml

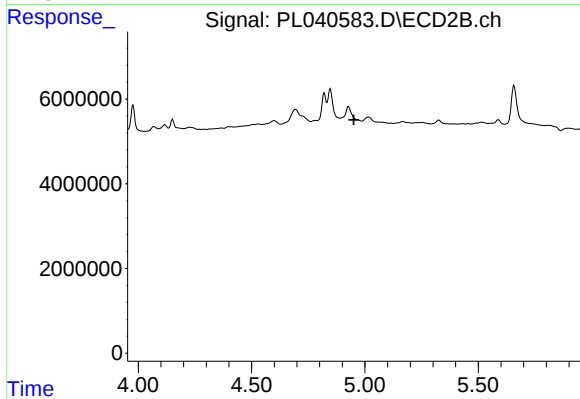

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.951 min
Response: 0
Conc: N.D.

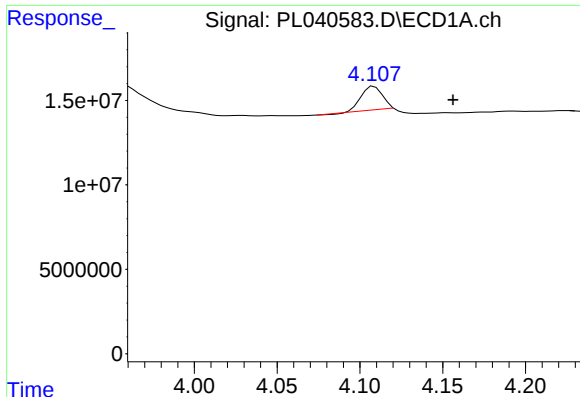

#6 beta-BHC


R.T.: 4.109 min
Delta R.T.: -0.048 min
Response: 12596891
Conc: 2.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

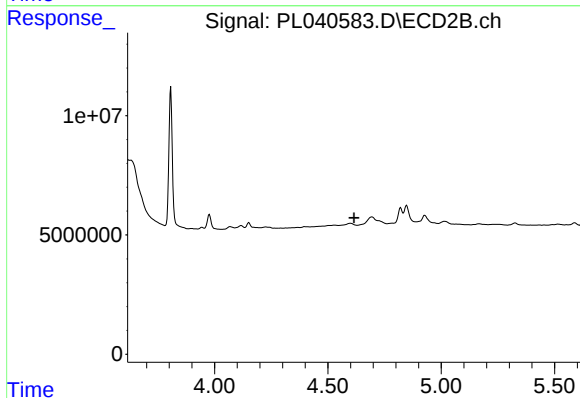


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.615 min
Response: 0
Conc: N.D.

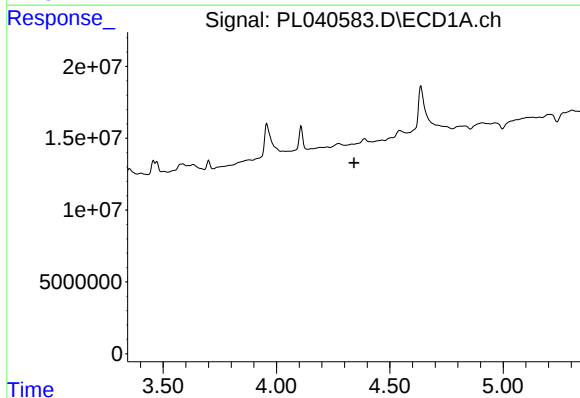


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

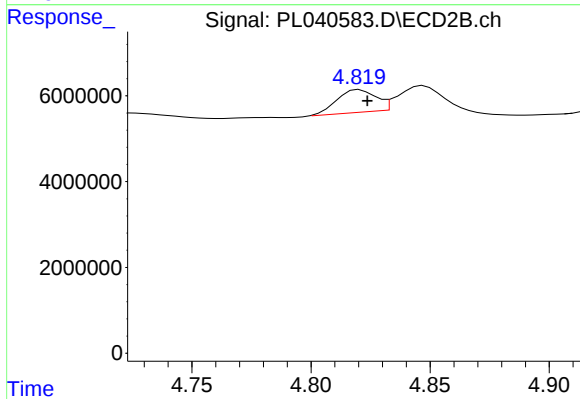

#7 delta-BHC


R.T.: 4.820 min
Delta R.T.: -0.003 min
Response: 5976676
Conc: 1.29 ng/ml

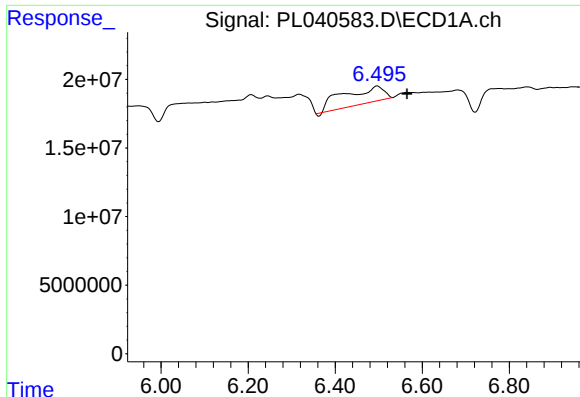

#20 Methoxychlor


R.T.: 6.497 min
Delta R.T.: -0.068 min
Response: 79119139
Conc: 16.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

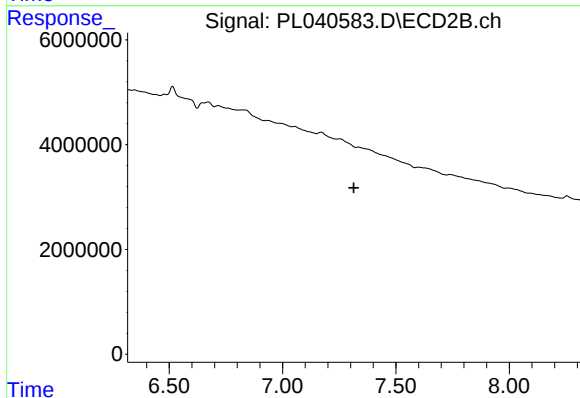


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.314 min
Response: 0
Conc: N.D.

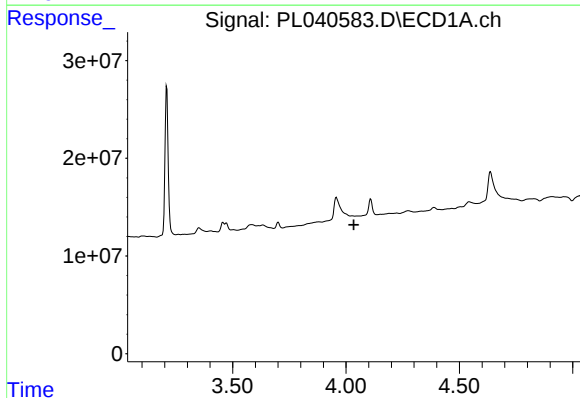


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.034 min
Response: 0
Conc: N.D.

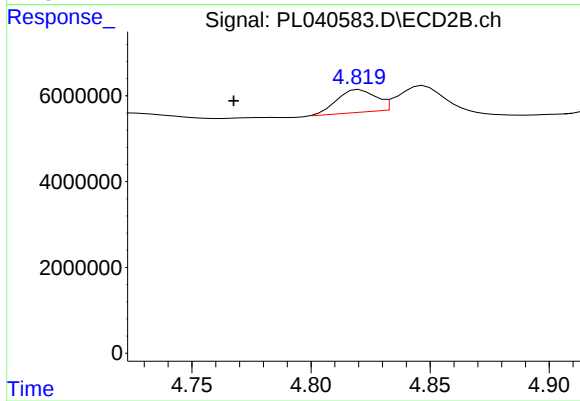

#23 Chlordane-1


R.T.: 4.820 min
Delta R.T.: 0.053 min
Response: 5976676
Conc: 38.73 ng/ml

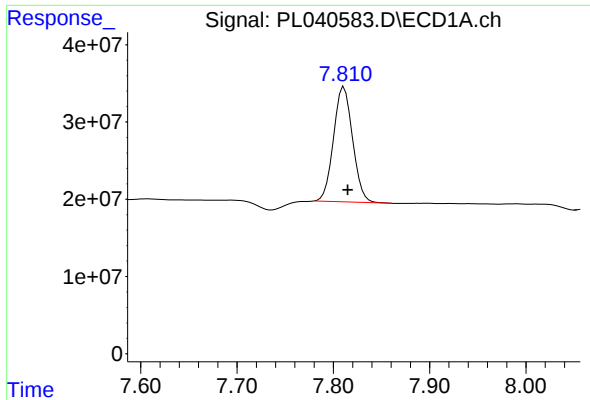

#28 Decachlorobiphenyl

R.T.: 7.811 min
Delta R.T.: -0.004 min
Response: 204498321
Conc: 21.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

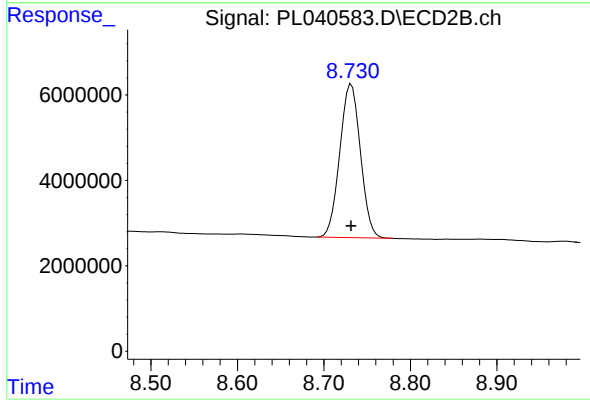

#28 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: 0.000 min
Response: 59368907
Conc: 18.75 ng/ml