

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100218\
 Data File : PL040586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2018 19:01
 Operator : AJ\SJ
 Sample : J5191-08
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 02:46:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.806	158.5E6	61521884	21.647	19.482
28)	SA Decachlor...	7.811	8.731	207.2E6	60077024	21.798	18.971
Target Compounds							
4)	MA Heptachlor	4.109f	0.000	18959176	0	1.611	N.D. #
6)	B beta-BHC	4.109f	0.000	18959176	0	4.492	N.D. #
7)	B delta-BHC	0.000	4.820	0	7113483	N.D.	1.541 #
23)	Chlordane-1	0.000	4.820	0	7113483	N.D.	46.093 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100218\
Data File : PL040586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2018 19:01
Operator : AJ\SJ
Sample : J5191-08
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 02:46:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

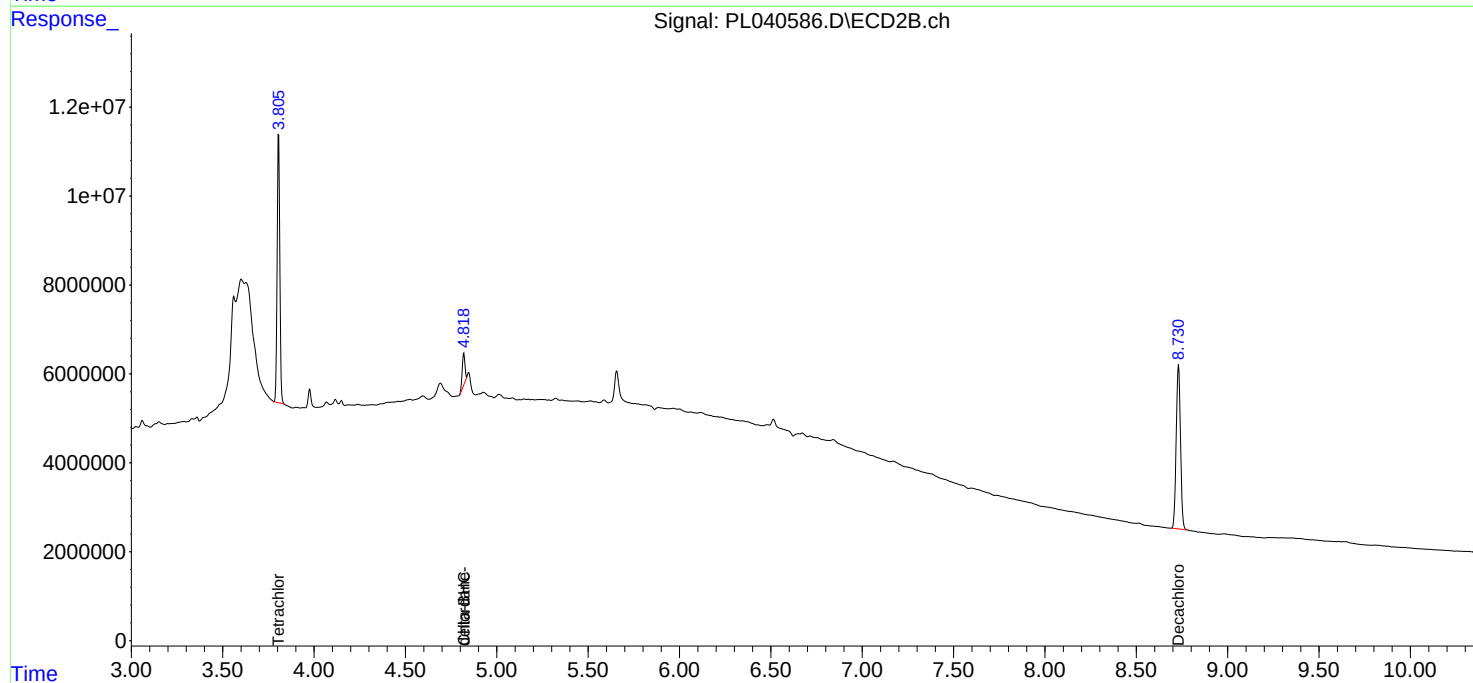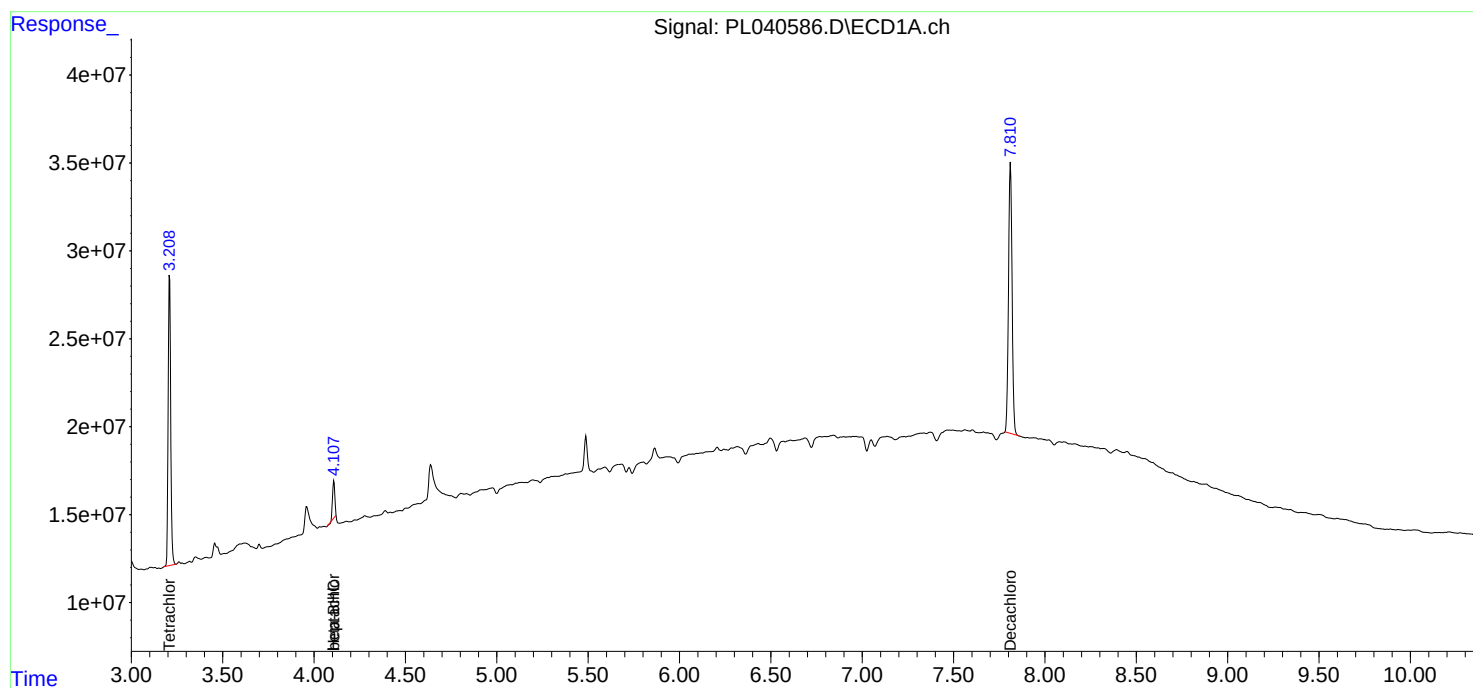


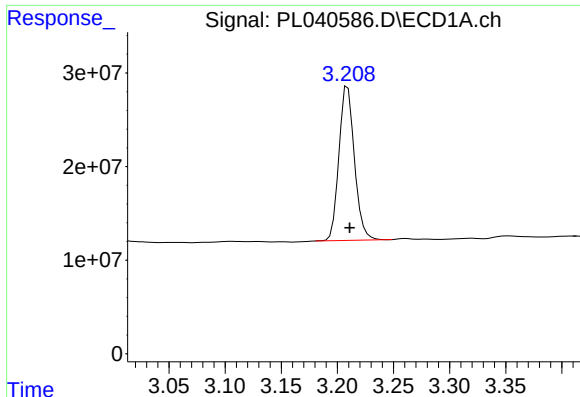

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.002 min
Response: 158456052
Conc: 21.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

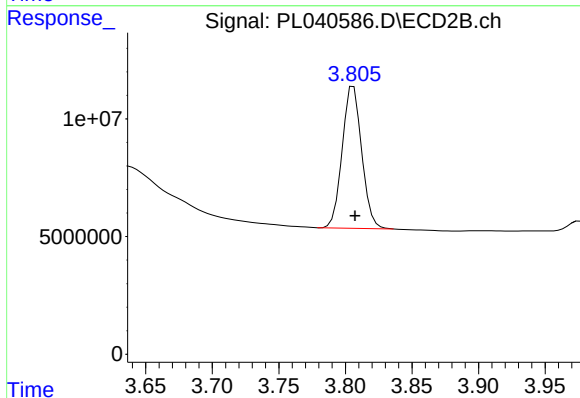


#1 Tetrachloro-m-xylene

R.T.: 3.806 min
Delta R.T.: -0.001 min
Response: 61521884
Conc: 19.48 ng/ml

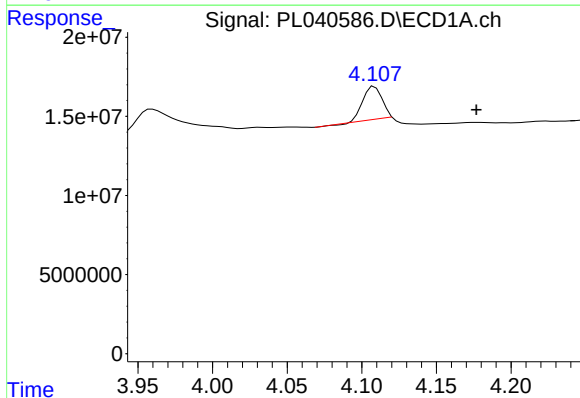


#4 Heptachlor

R.T.: 4.109 min
Delta R.T.: -0.068 min
Response: 18959176
Conc: 1.61 ng/ml

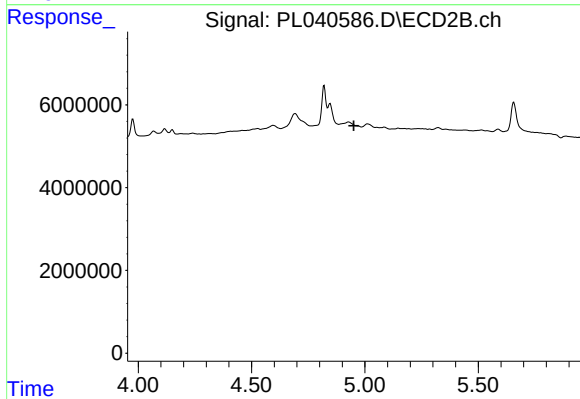

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.951 min
Response: 0
Conc: N.D.

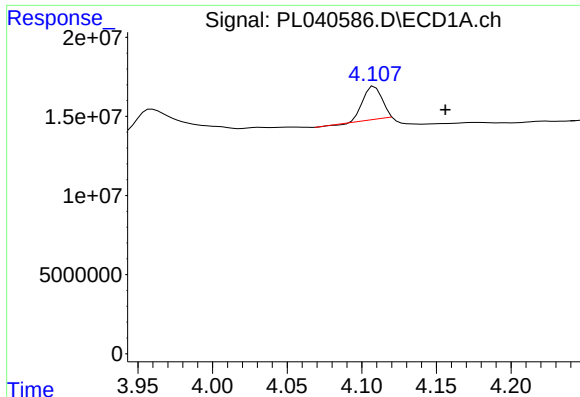

#6 beta-BHC


R.T.: 4.109 min
Delta R.T.: -0.048 min
Response: 18959176
Conc: 4.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

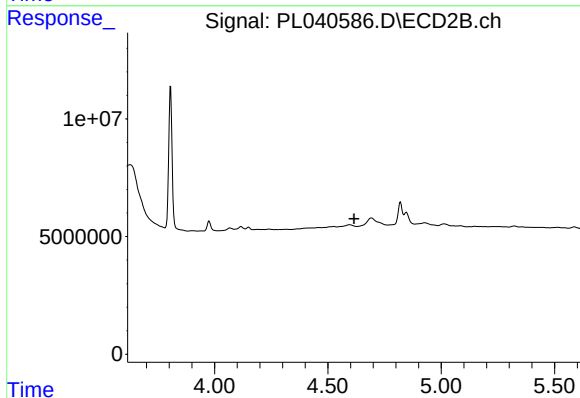


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.615 min
Response: 0
Conc: N.D.

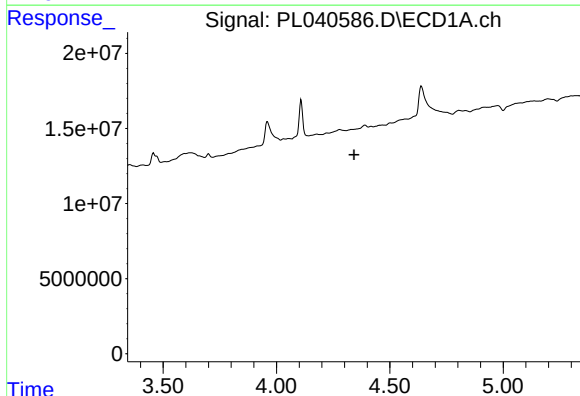


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

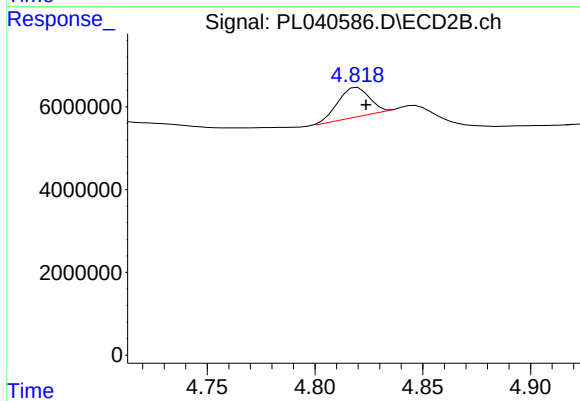

#7 delta-BHC


R.T.: 4.820 min
Delta R.T.: -0.004 min
Response: 7113483
Conc: 1.54 ng/ml

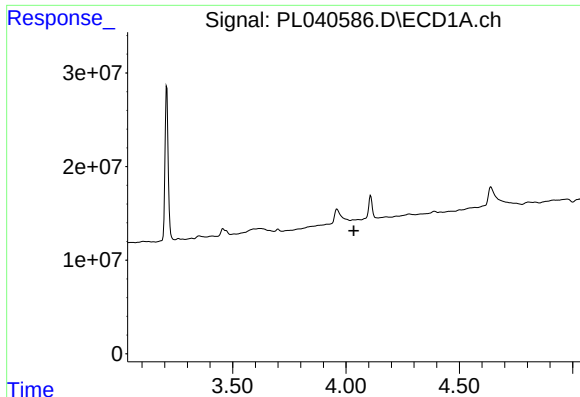

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

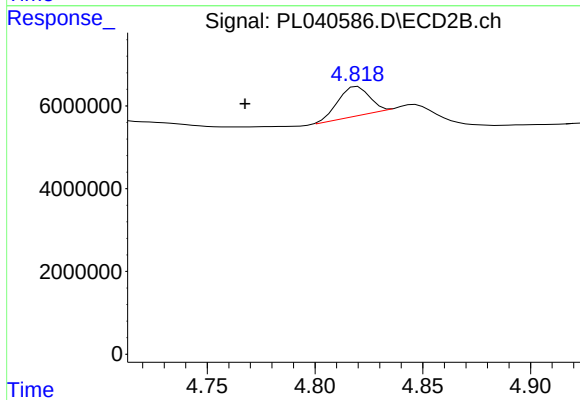


#23 Chlordane-1

R.T.: 4.820 min
Delta R.T.: 0.052 min
Response: 7113483
Conc: 46.09 ng/ml

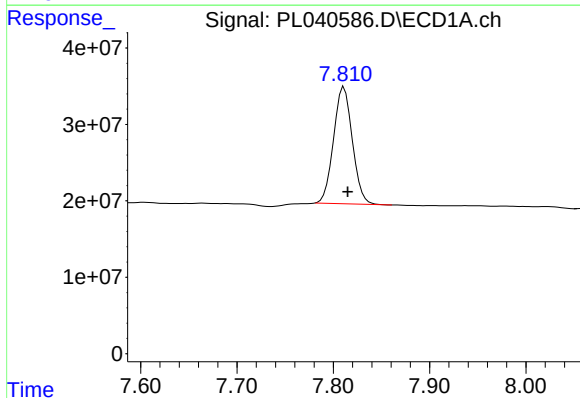

#28 Decachlorobiphenyl

R.T.: 7.811 min
Delta R.T.: -0.004 min
Response: 207203800
Conc: 21.80 ng/ml

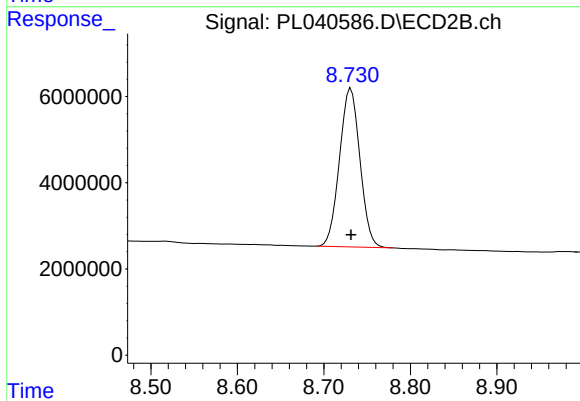

#28 Decachlorobiphenyl

R.T.: 8.731 min
Delta R.T.: 0.000 min
Response: 60077024
Conc: 18.97 ng/ml