

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100218\
 Data File : PS001869.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2018 13:08
 Operator : EI\SJ
 Sample : PB113398BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 13:41:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.501	10.999	119.2E6	121.4E6	531.241	477.925
Target Compounds							
1) T	Dalapon	2.932	2.414	40521299	44391210	124.617	150.266
2) T	3,5-DICHL...	0.000	9.089	0	1991585	N.D.	6.310 #
5) T	DICAMBA	0.000	11.241	0	24416546	N.D.	27.376 #
6) T	MCP	12.093	0.000	2094276	0	3.287	N.D. #
7) T	MCPA	0.000	11.859	0	21159071	N.D.	24.410 #
9) T	2,4-D	0.000	12.833	0	6214406	N.D.	19.975 #
10) T	Pentachlo...	0.000	13.355	0	4186846	N.D.	1.222 #
13) T	2,4-DB	15.750	0.000	6731371	0	41.334	N.D. #
15) T	Picloram	17.008	0.000	4301594	0	2.470	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100218\
Data File : PS001869.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2018 13:08
Operator : EI\SJ
Sample : PB113398BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 13:41:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

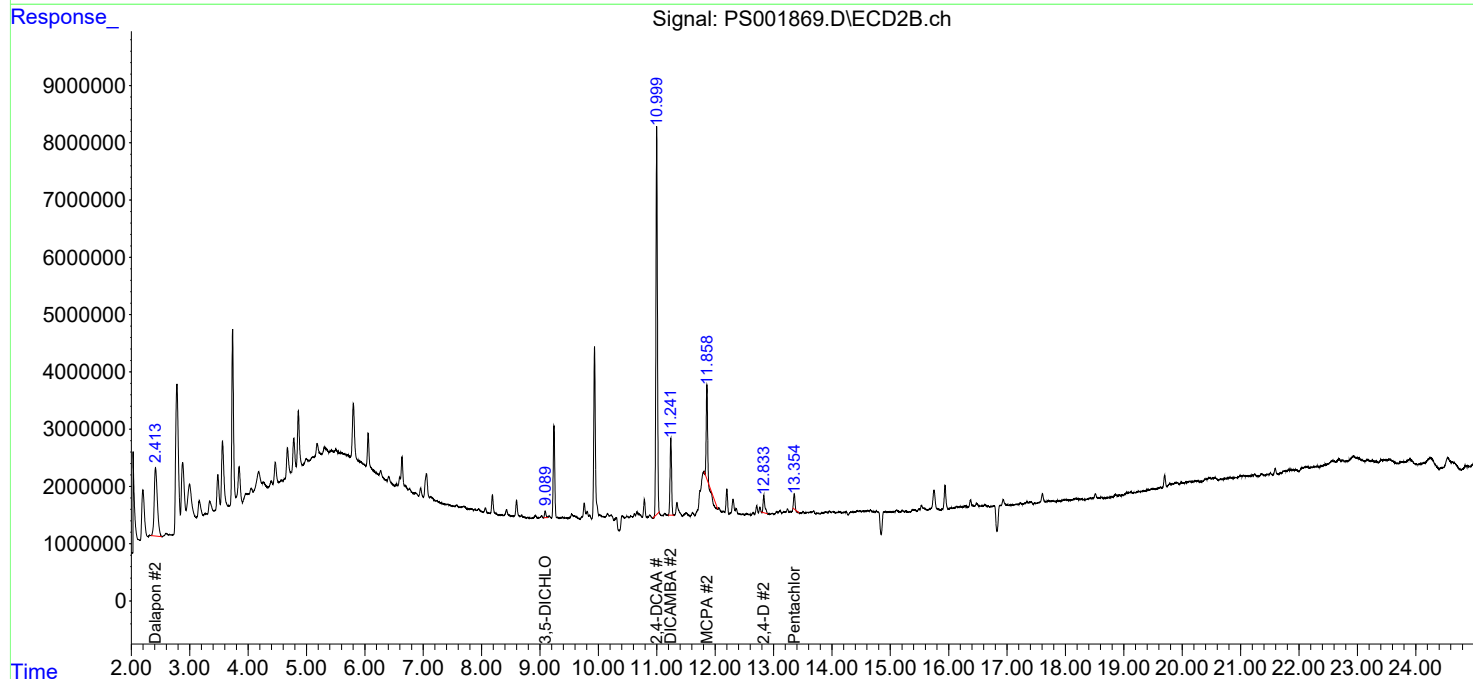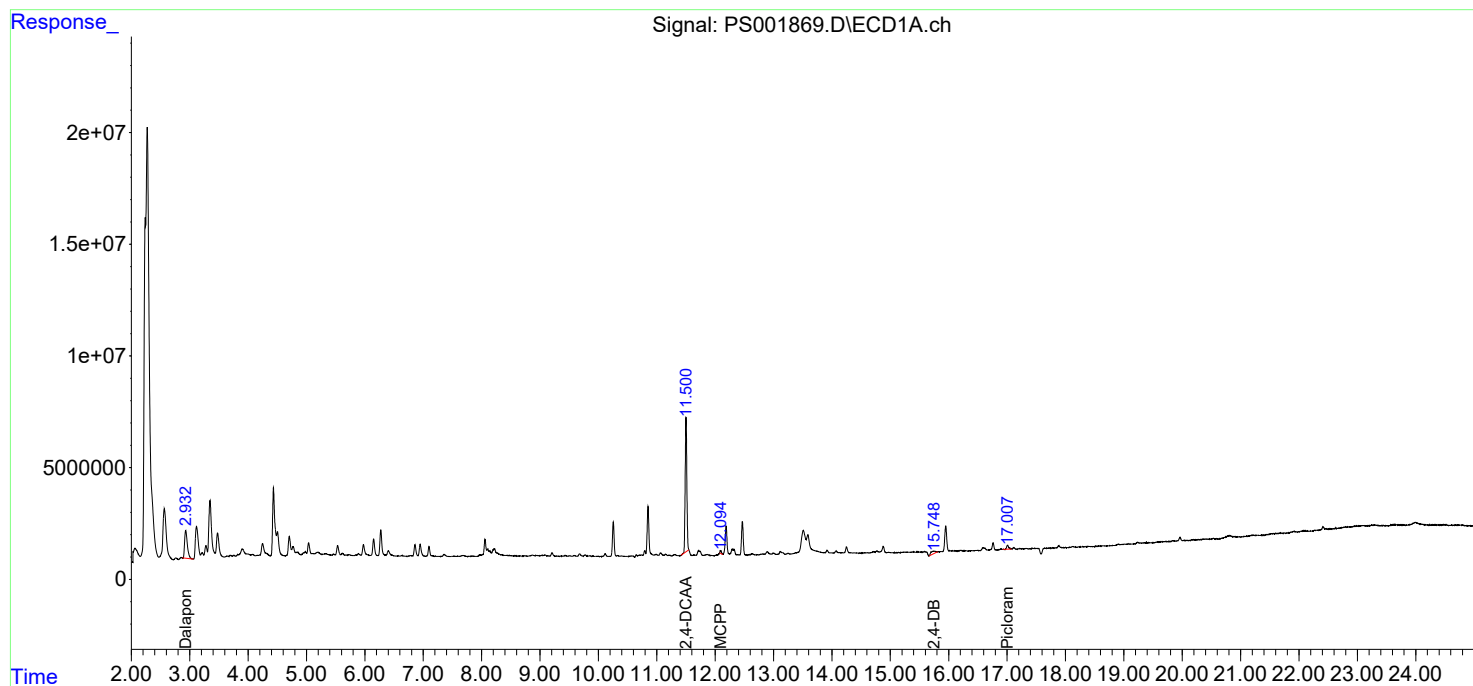


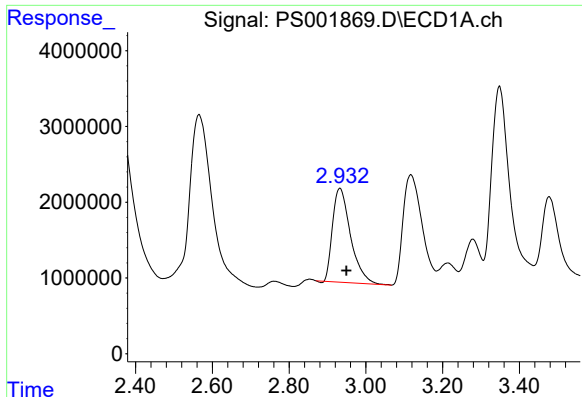

#1 Dalapon


R.T.: 2.932 min
Delta R.T.: -0.017 min
Response: 40521299
Conc: 124.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

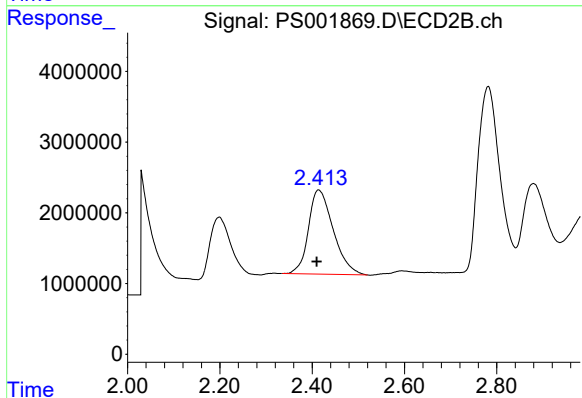


#1 Dalapon

R.T.: 2.414 min
Delta R.T.: 0.004 min
Response: 44391210
Conc: 150.27 ng/ml

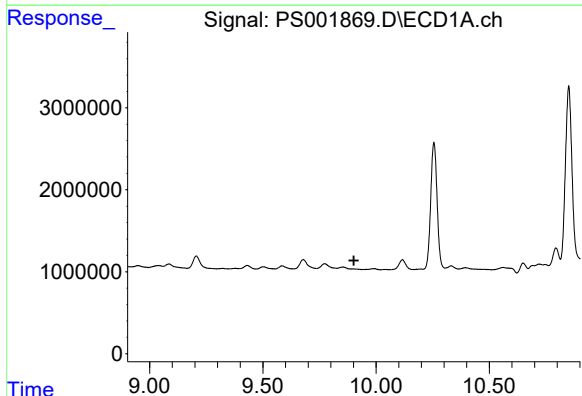


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.902 min
Response: 0
Conc: N.D.

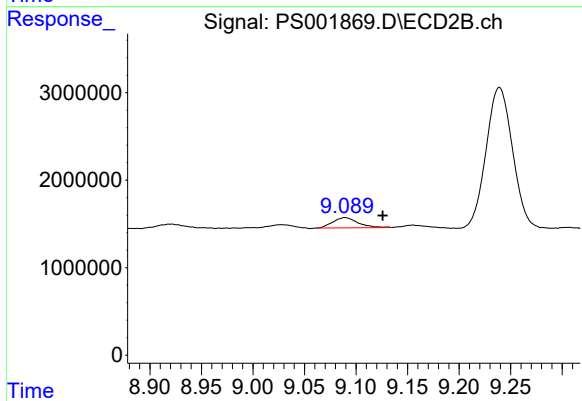

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.089 min
Delta R.T.: -0.037 min
Response: 1991585
Conc: 6.31 ng/ml

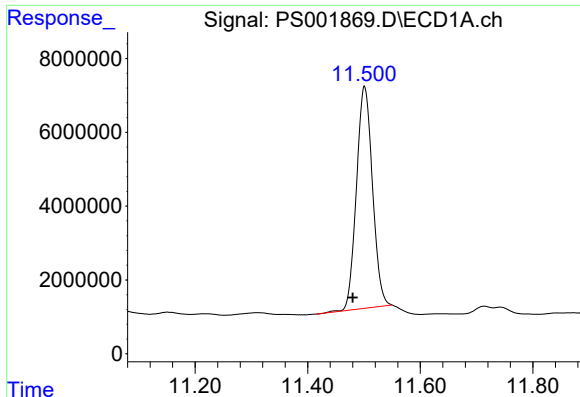

#4 2,4-DCAA


R.T.: 11.501 min
Delta R.T.: 0.021 min
Response: 119165676
Conc: 531.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

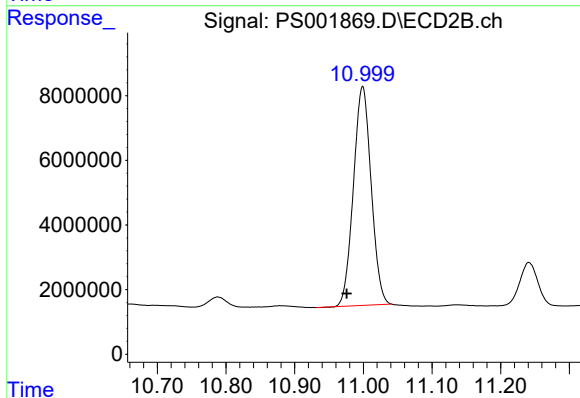


#4 2,4-DCAA

R.T.: 10.999 min
Delta R.T.: 0.023 min
Response: 121401033
Conc: 477.93 ng/ml

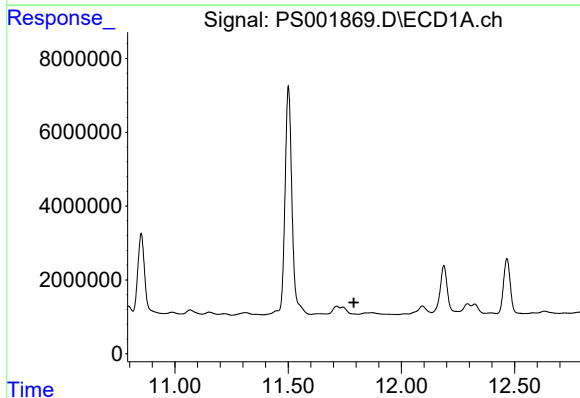


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.790 min
Response: 0
Conc: N.D.

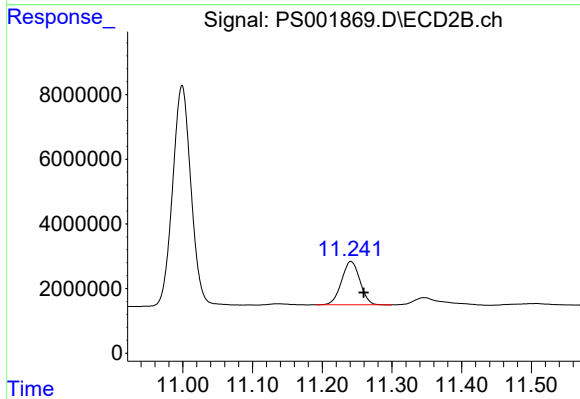

#5 DICAMBA


R.T.: 11.241 min
Delta R.T.: -0.019 min
Response: 24416546
Conc: 27.38 ng/ml

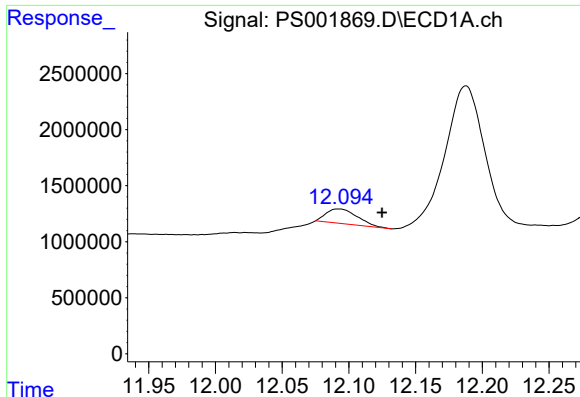

#6 MCPP


R.T.: 12.093 min
Delta R.T.: -0.032 min
Response: 2094276
Conc: 3.29 ug/ml

Instrument :
ECD_S
ClientSampleId :

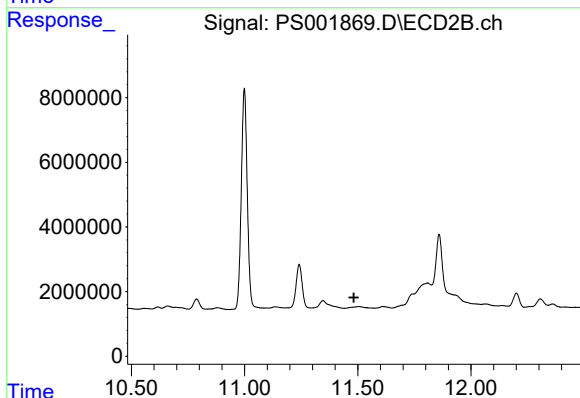


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.483 min
Response: 0
Conc: N.D.

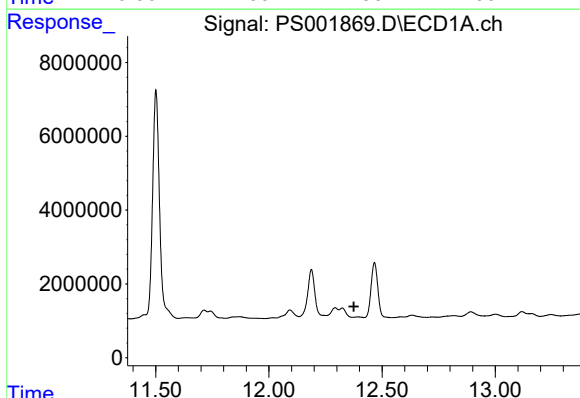


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.375 min
Response: 0
Conc: N.D.

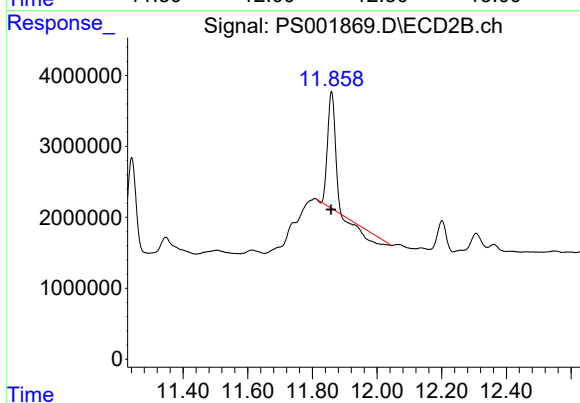

#7 MCPA


R.T.: 11.859 min
Delta R.T.: 0.001 min
Response: 21159071
Conc: 24.41 ug/ml

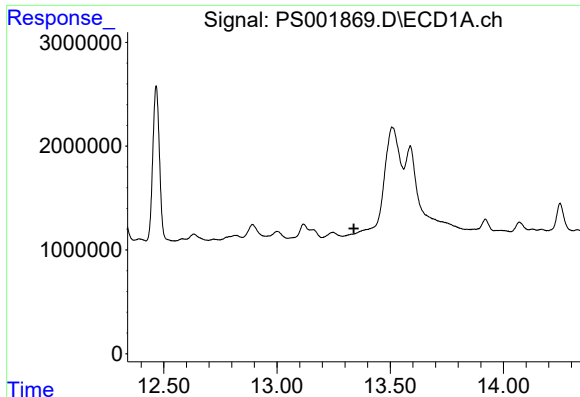

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 13.340 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

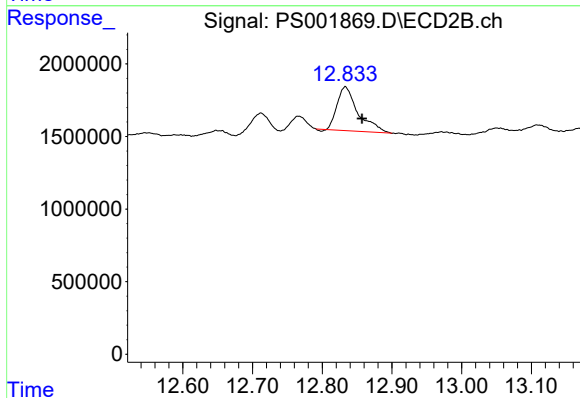


#9 2,4-D

R.T.: 12.833 min
Delta R.T.: -0.024 min
Response: 6214406
Conc: 19.98 ng/ml

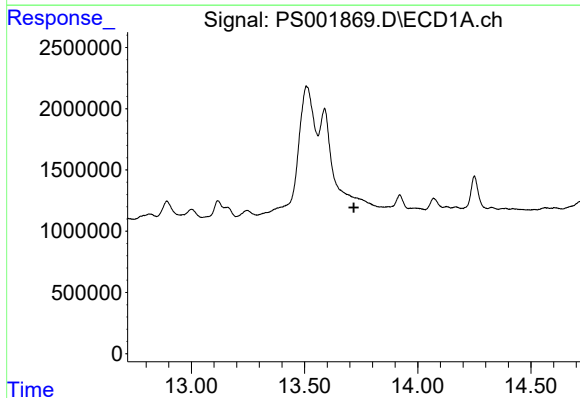


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.718 min
Response: 0
Conc: N.D.

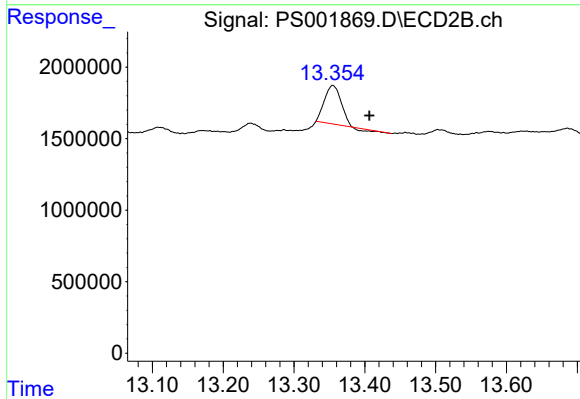

#10 Pentachlorophenol


R.T.: 13.355 min
Delta R.T.: -0.052 min
Response: 4186846
Conc: 1.22 ng/ml

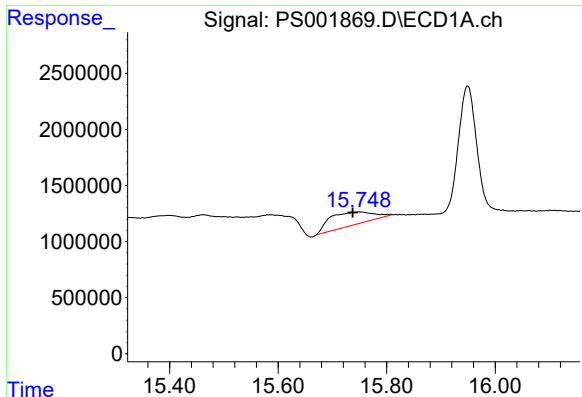

#13 2,4-DB


R.T.: 15.750 min
Delta R.T.: 0.012 min
Response: 6731371
Conc: 41.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

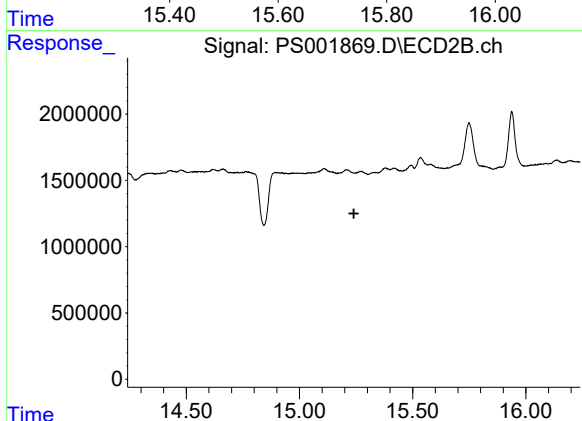


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.240 min
Response: 0
Conc: N.D.

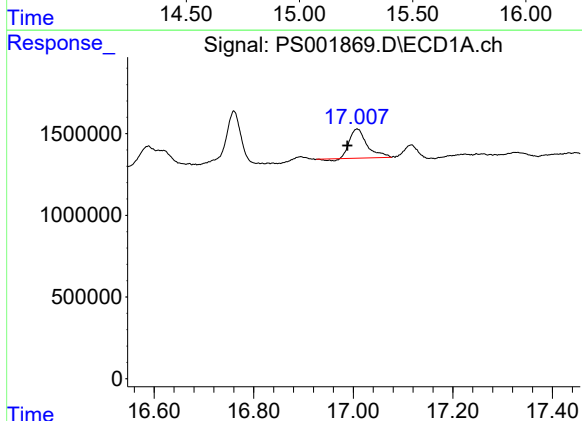

#15 Picloram

R.T.: 17.008 min
Delta R.T.: 0.019 min
Response: 4301594
Conc: 2.47 ng/ml

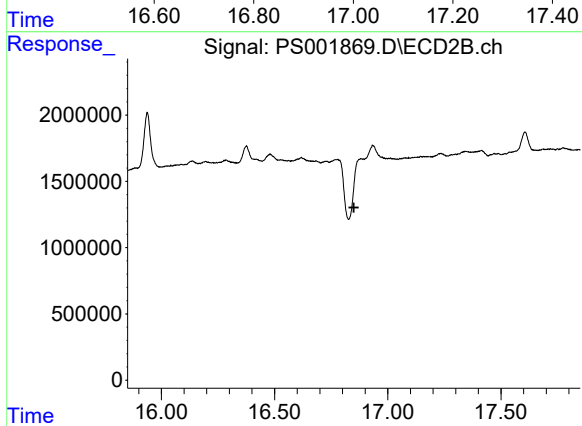

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.850 min
Response: 0
Conc: N.D.