

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100218\
 Data File : PS001873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2018 18:08
 Operator : EI\SJ
 Sample : PB113443BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 02:04:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.475	10.962	116.6E6	114.0E6	519.615	448.955
Target Compounds							
1) T	Dalapon	2.903	2.377	21369602	16807217	65.719	56.893
5) T	DICAMBA	0.000	11.205	0	10493689	N.D.	11.766 #
6) T	MCPD	12.162	0.000	22964800	0	36.038	N.D. #
7) T	MCPA	12.440	0.000	10693034	0	10.189	N.D. #
15) T	Picloram	16.998	16.903	6658938	14845589	3.824	8.729 #
16) T	DCPA	0.000	16.903	0	14845589	N.D.	8.049 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100218\
Data File : PS001873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2018 18:08
Operator : EI\SJ
Sample : PB113443BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 02:04:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

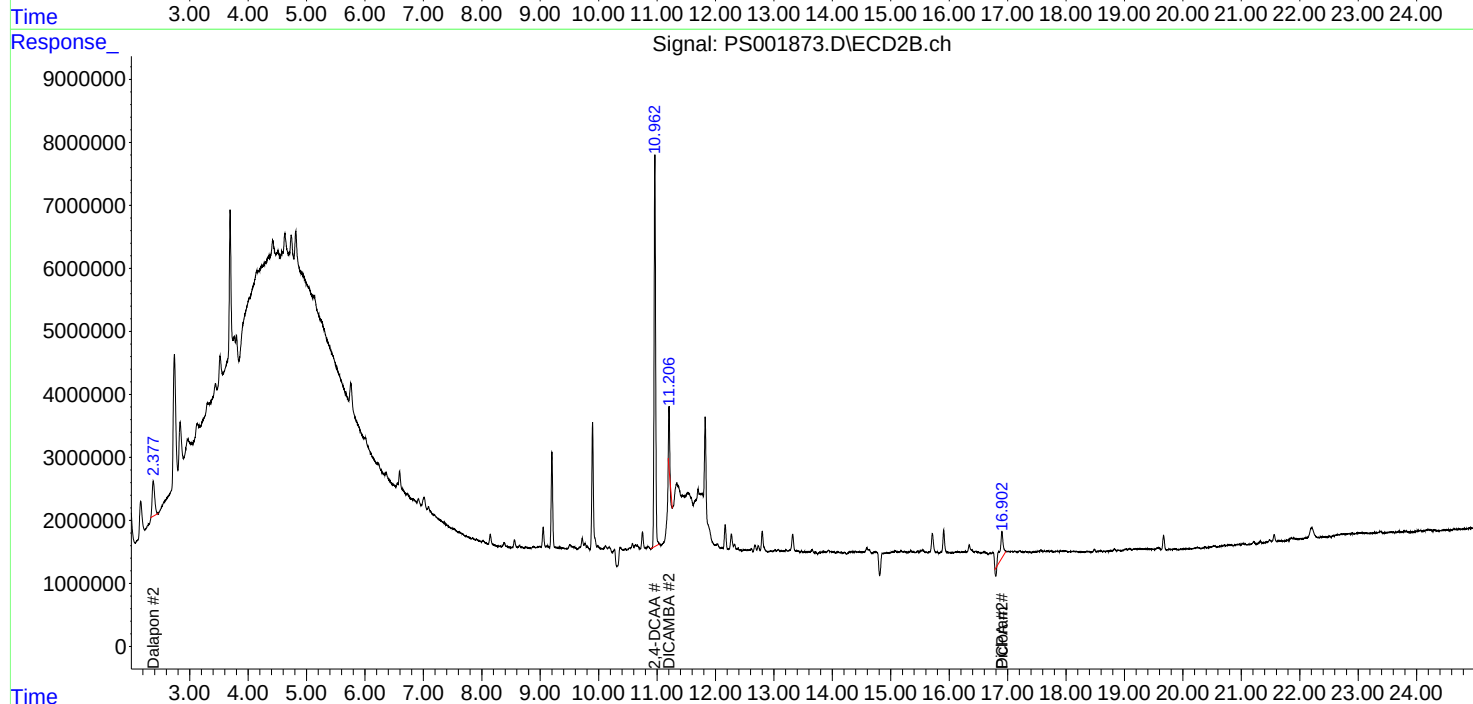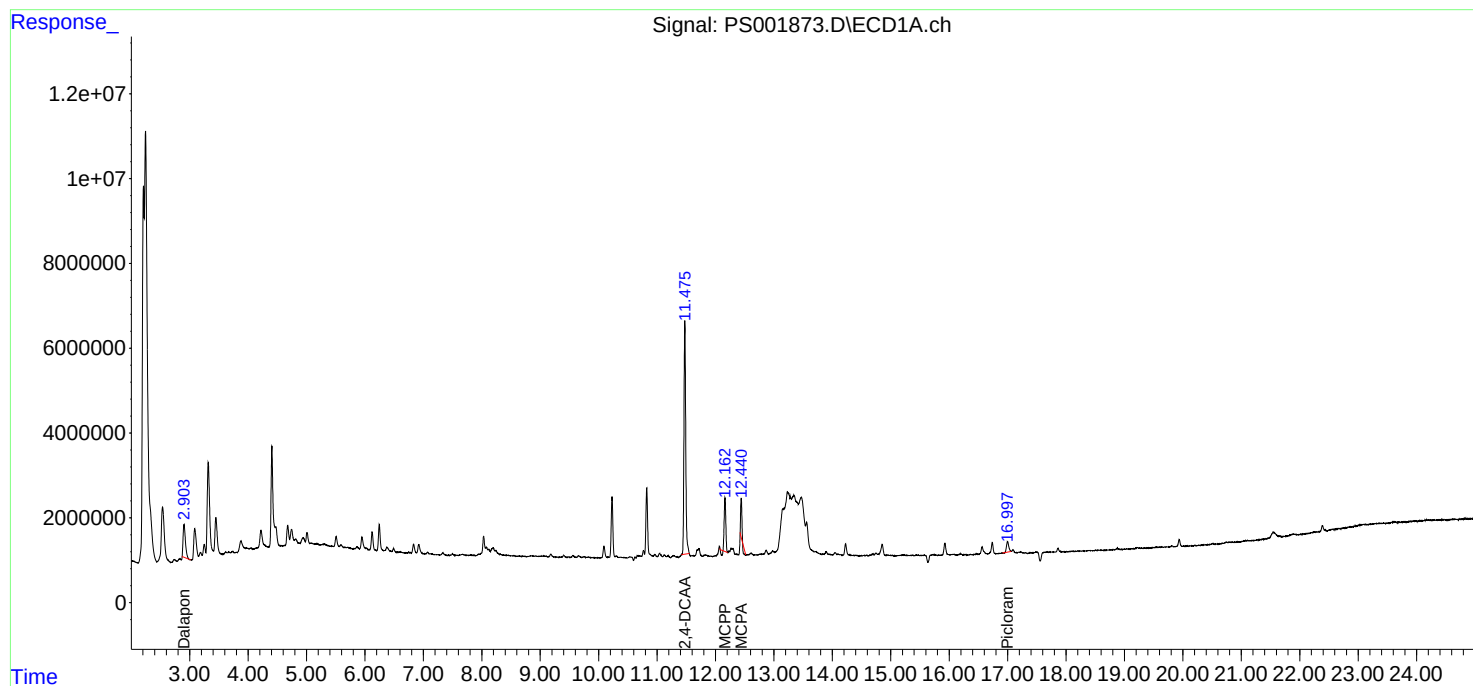


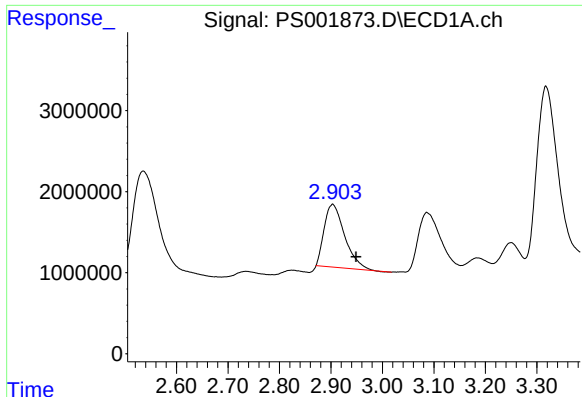

#1 Dalapon


R.T.: 2.903 min
Delta R.T.: -0.046 min
Response: 21369602
Conc: 65.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

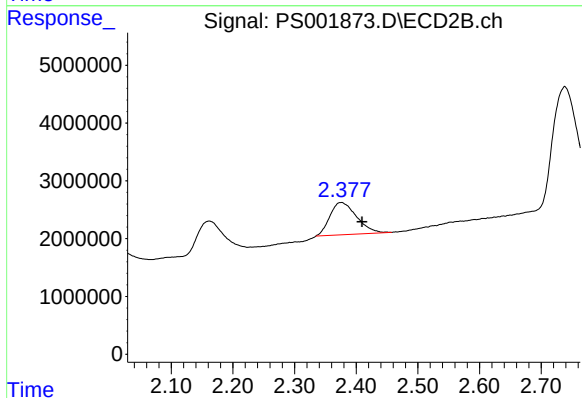


#1 Dalapon

R.T.: 2.377 min
Delta R.T.: -0.033 min
Response: 16807217
Conc: 56.89 ng/ml

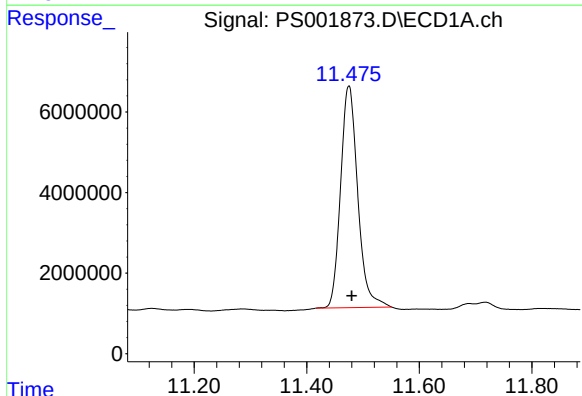


#4 2,4-DCAA

R.T.: 11.475 min
Delta R.T.: -0.005 min
Response: 116557672
Conc: 519.61 ng/ml

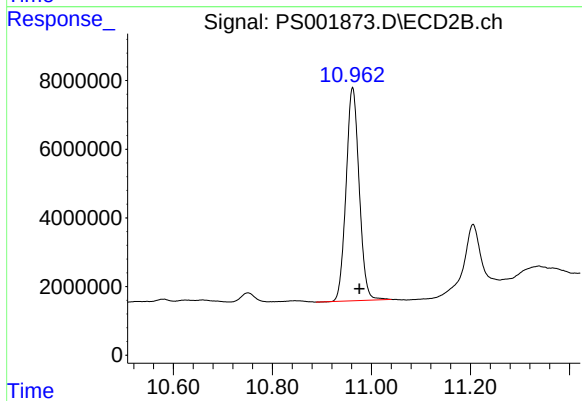

#4 2,4-DCAA


R.T.: 10.962 min
Delta R.T.: -0.014 min
Response: 114041946
Conc: 448.95 ng/ml

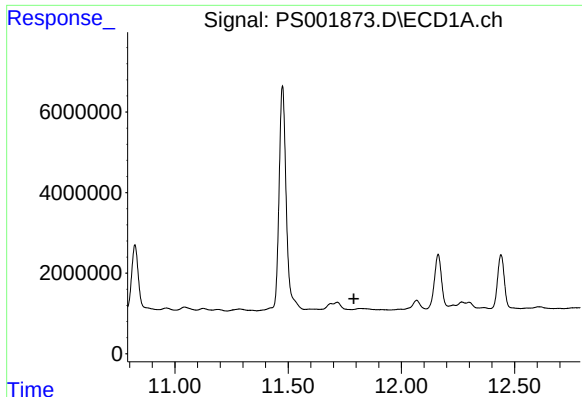

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

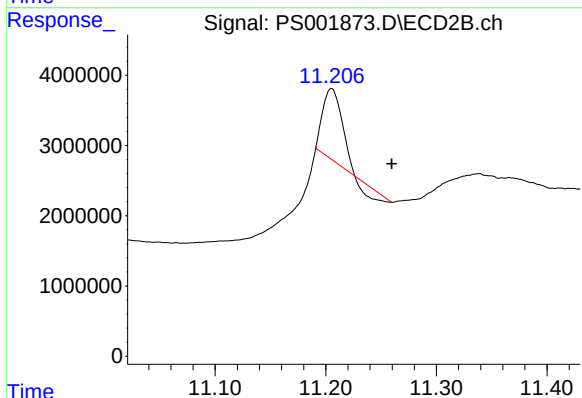


#5 DICAMBA

R.T.: 11.205 min
Delta R.T.: -0.054 min
Response: 10493689
Conc: 11.77 ng/ml

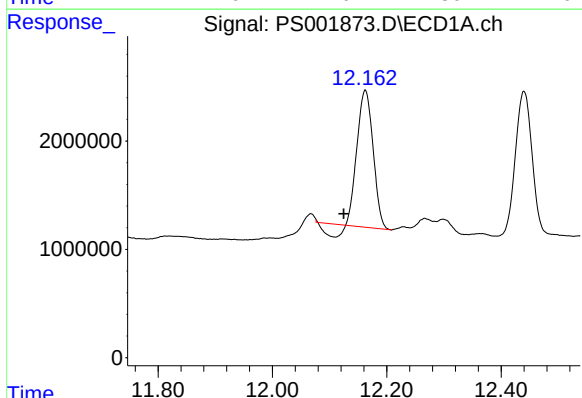


#6 MCP

R.T.: 12.162 min
Delta R.T.: 0.037 min
Response: 22964800
Conc: 36.04 ug/ml

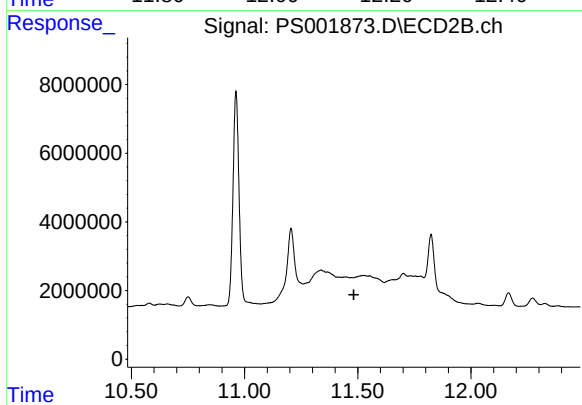

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.483 min
Response: 0
Conc: N.D.

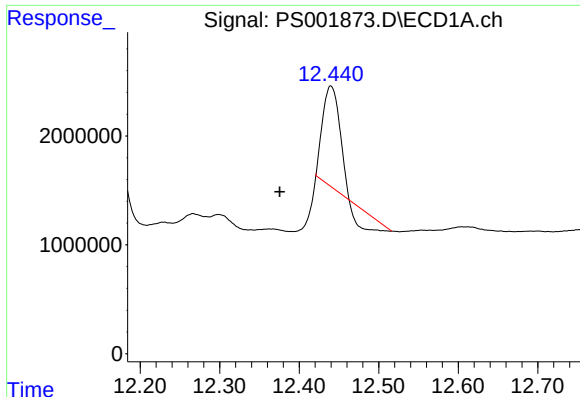

#7 MCPA


R.T.: 12.440 min
Delta R.T.: 0.065 min
Response: 10693034
Conc: 10.19 ug/ml

Instrument :
ECD_S
ClientSampleId :

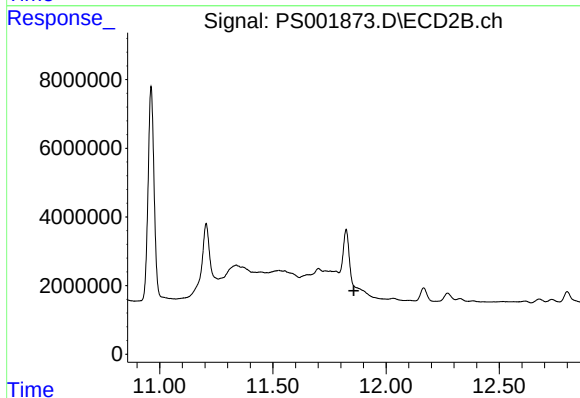


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 11.858 min
Response: 0
Conc: N.D.

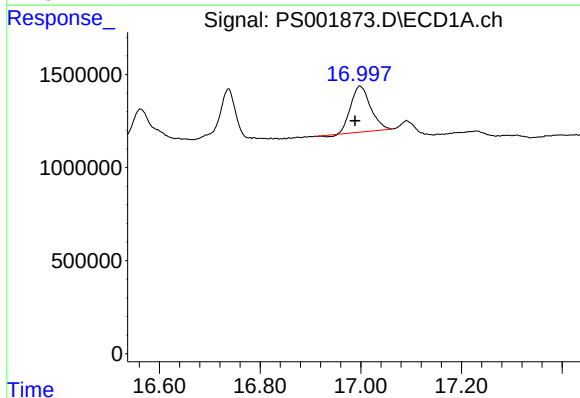


#15 Picloram

R.T.: 16.998 min
Delta R.T.: 0.010 min
Response: 6658938
Conc: 3.82 ng/ml

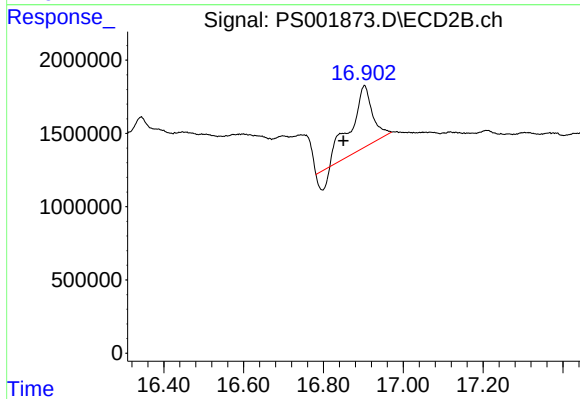

#15 Picloram


R.T.: 16.903 min
Delta R.T.: 0.053 min
Response: 14845589
Conc: 8.73 ng/ml

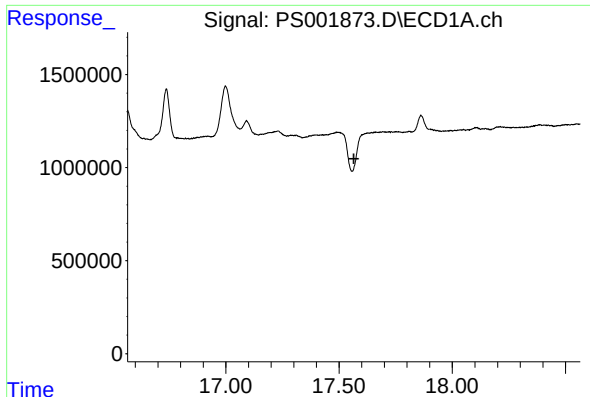

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

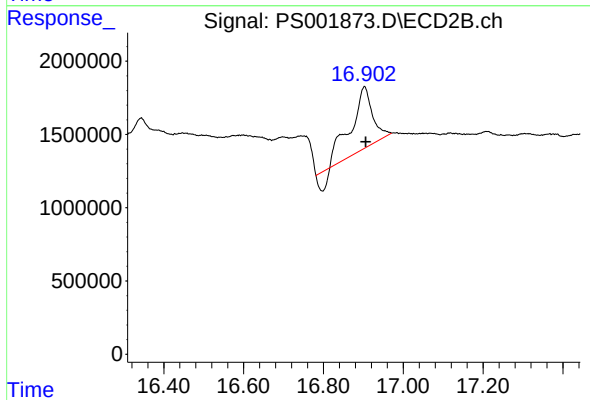

#16 DCPA

R.T.: 16.903 min
Delta R.T.: -0.003 min
Response: 14845589
Conc: 8.05 ng/ml