

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100218\
 Data File : PS001875.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2018 19:10
 Operator : EI\SJ
 Sample : PB113443TB
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 02:05:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.455	10.952	97161492	96352594	433.146	379.316
Target Compounds							
1) T	Dalapon	2.886	2.366	-372564	8692534	N.D.	29.425
2) T	3,5-DICHL...	0.000	9.193	0	25029949	N.D.	79.301 #
6) T	MCP	12.142	0.000	35774301	0	56.140	N.D. #
15) T	Picloram	16.966	16.882	4064012	12191160	2.334	7.168 #
16) T	DCPA	0.000	16.882	0	12191160	N.D.	6.610 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100218\
Data File : PS001875.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2018 19:10
Operator : EI\SJ
Sample : PB113443TB
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 02:05:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

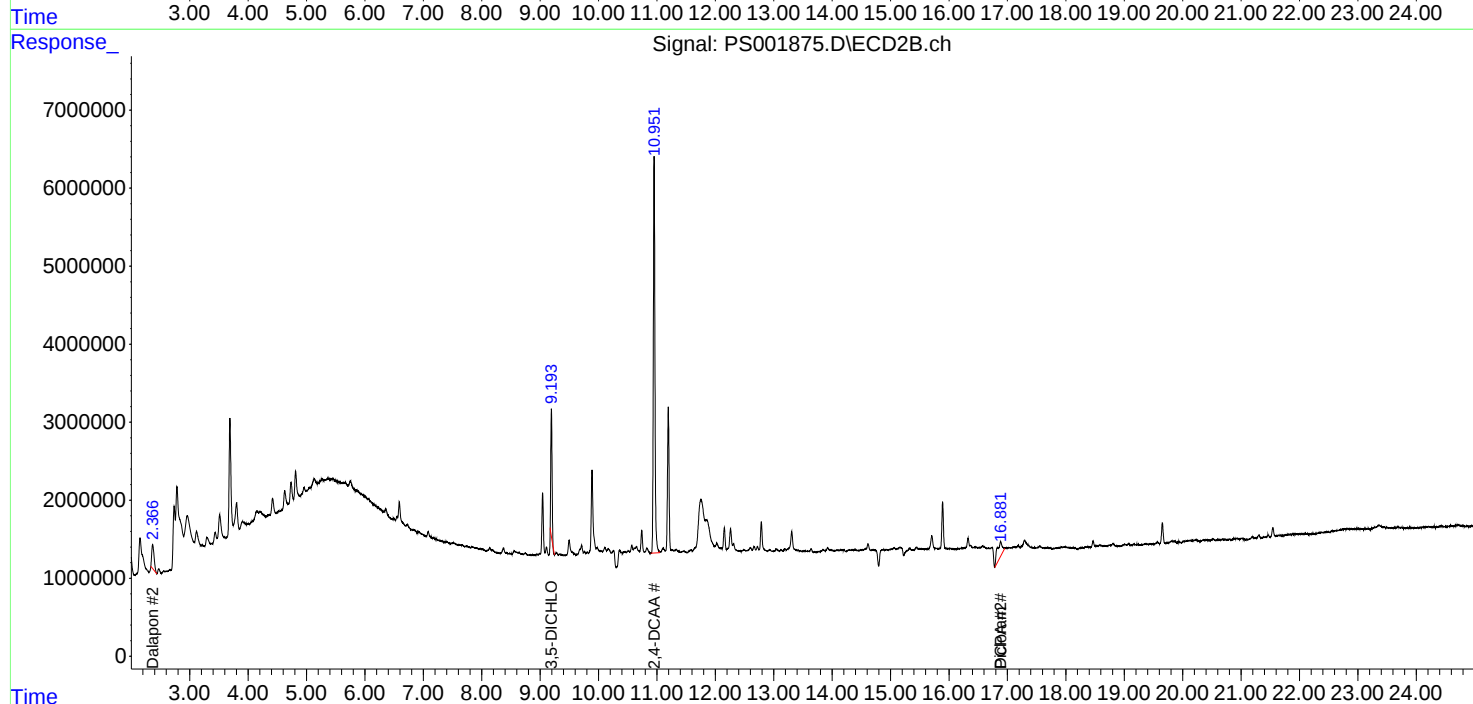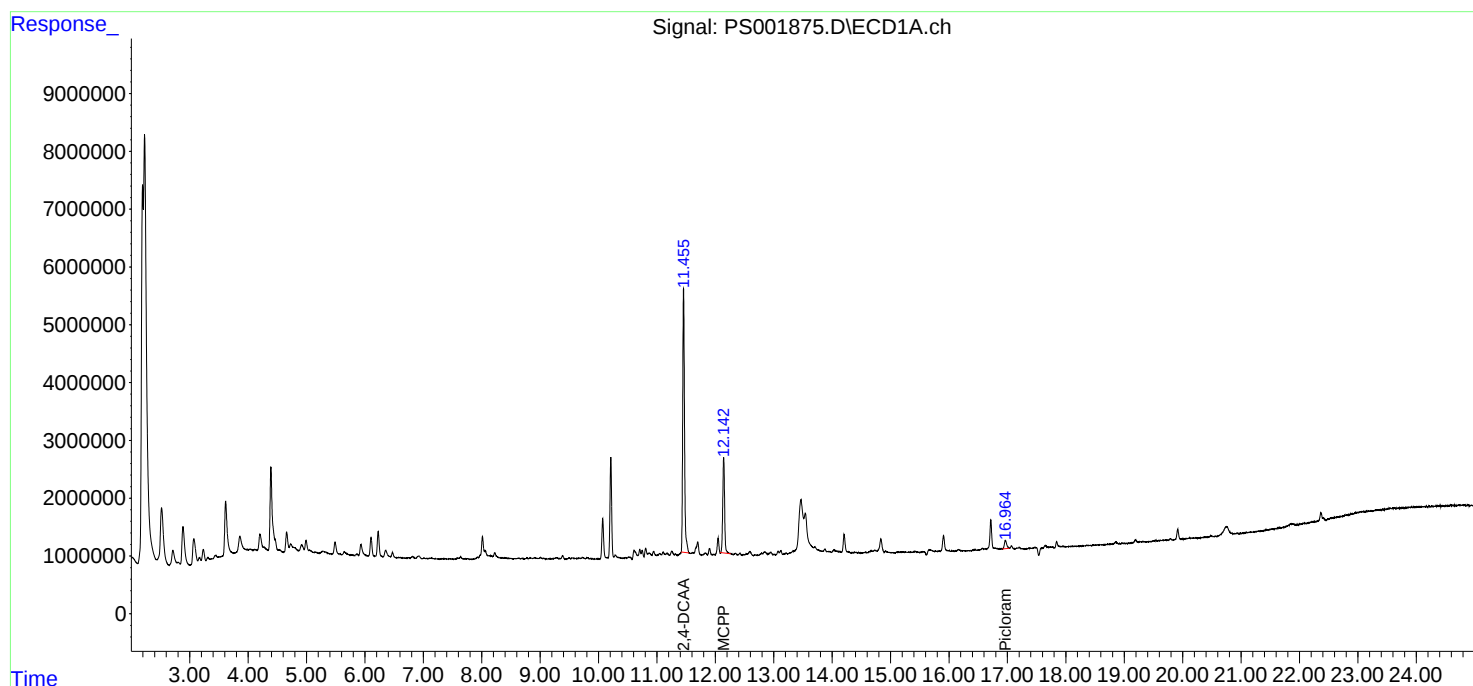


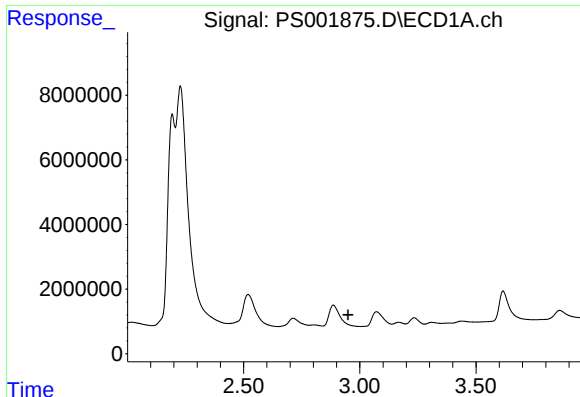

#1 Dalapon


R.T.: 2.886 min
Delta R.T.: -0.063 min
Response: -372564
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

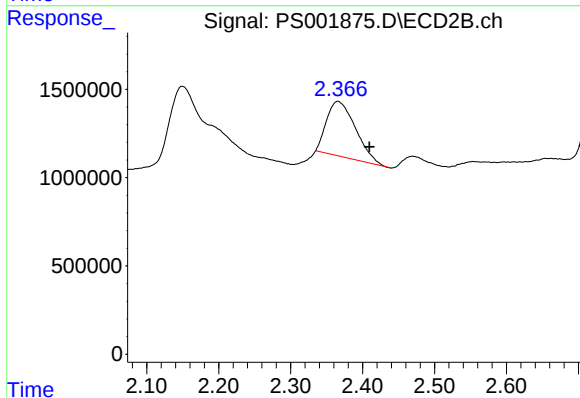


#1 Dalapon

R.T.: 2.366 min
Delta R.T.: -0.044 min
Response: 8692534
Conc: 29.42 ng/ml

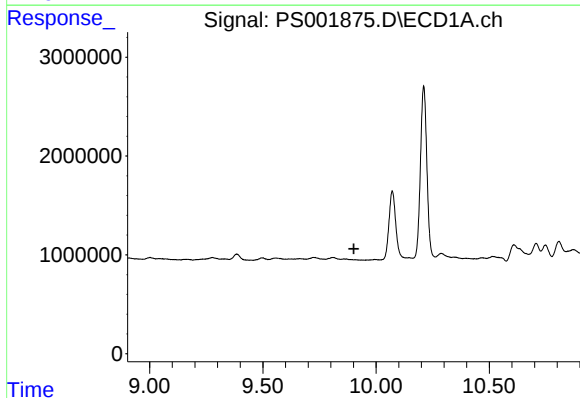


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.902 min
Response: 0
Conc: N.D.

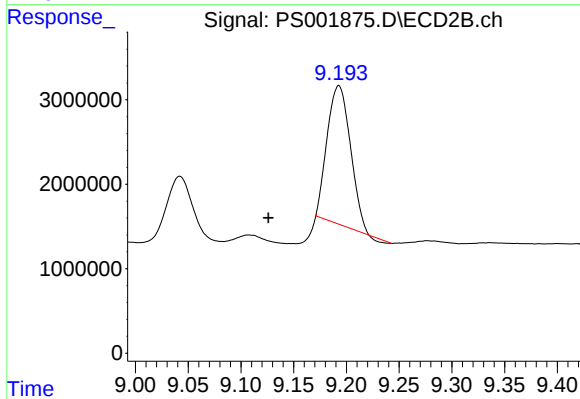

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.193 min
Delta R.T.: 0.067 min
Response: 25029949
Conc: 79.30 ng/ml

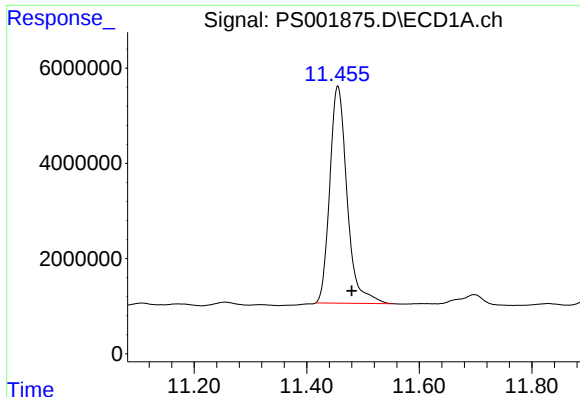

#4 2,4-DCAA


R.T.: 11.455 min
Delta R.T.: -0.025 min
Response: 97161492
Conc: 433.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

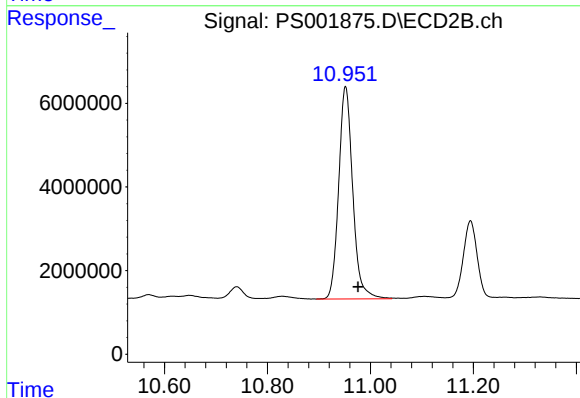


#4 2,4-DCAA

R.T.: 10.952 min
Delta R.T.: -0.024 min
Response: 96352594
Conc: 379.32 ng/ml

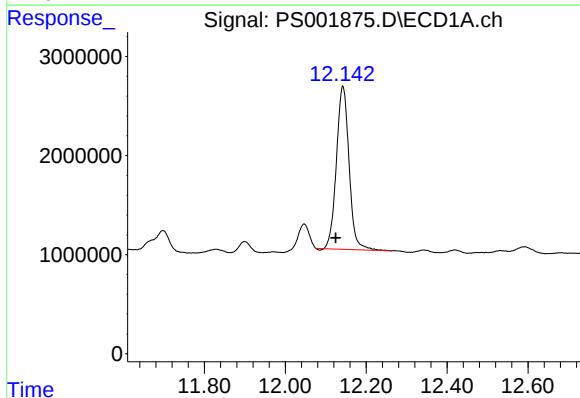


#6 MCPP

R.T.: 12.142 min
Delta R.T.: 0.017 min
Response: 35774301
Conc: 56.14 ug/ml

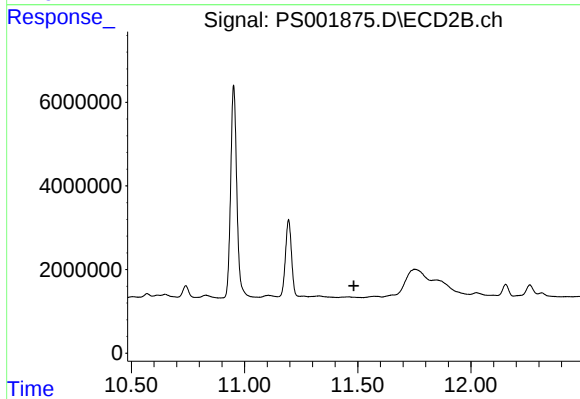

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 11.483 min
Response: 0
Conc: N.D.

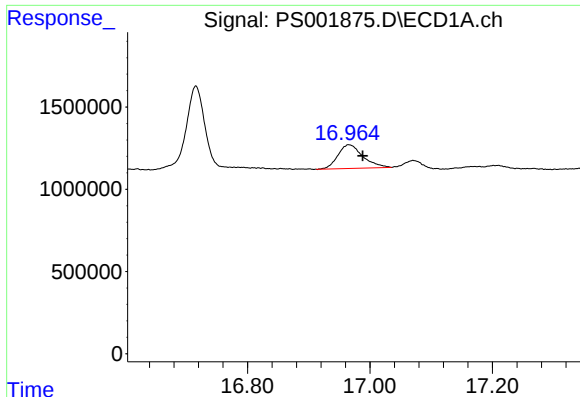

#15 Picloram


R.T.: 16.966 min
Delta R.T.: -0.023 min
Response: 4064012
Conc: 2.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

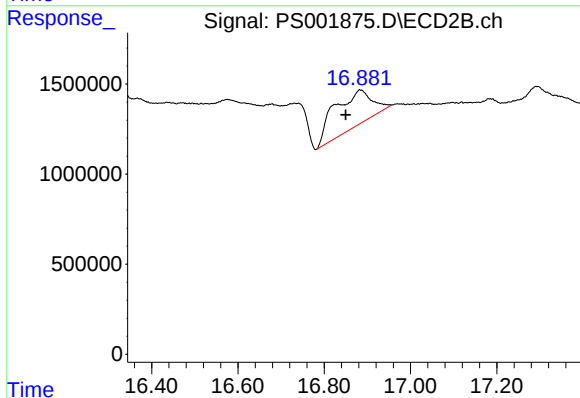


#15 Picloram

R.T.: 16.882 min
Delta R.T.: 0.032 min
Response: 12191160
Conc: 7.17 ng/ml

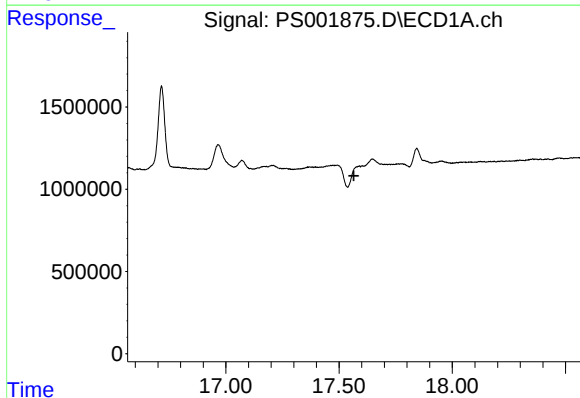

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.565 min
Response: 0
Conc: N.D.

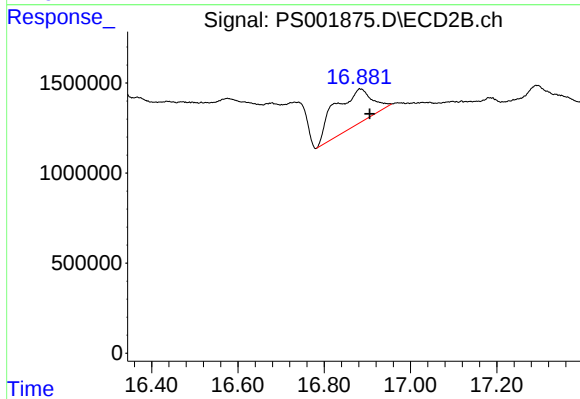

#16 DCPA

R.T.: 16.882 min
Delta R.T.: -0.024 min
Response: 12191160
Conc: 6.61 ng/ml