

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100218\
 Data File : PS001880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2018 21:46
 Operator : EI\SJ
 Sample : J5191-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 02:06:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.472	10.969	98415979	95435718	438.739	375.706
Target Compounds							
1) T	Dalapon	2.903	2.384	17432811	12839277	53.612	43.462
5) T	DICAMBA	0.000	11.211	0	21203687	N.D.	23.774 #
6) T	MCPD	12.159	0.000	28475581	0	44.686	N.D. #
15) T	Picloram	16.978	16.901	3821660	3854742	2.195	2.267
16) T	DCPA	0.000	16.901	0	3854742	N.D.	2.090 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100218\
Data File : PS001880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2018 21:46
Operator : EI\SJ
Sample : J5191-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 02:06:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

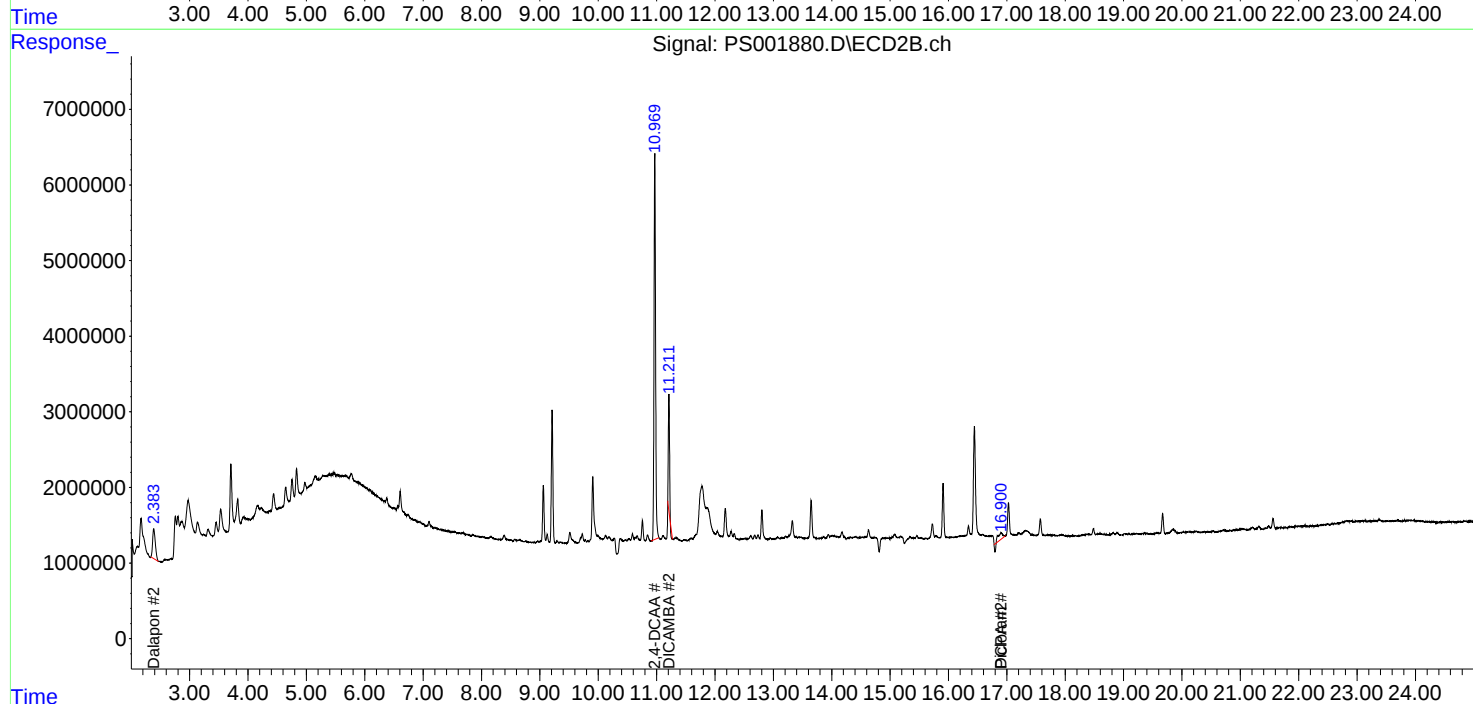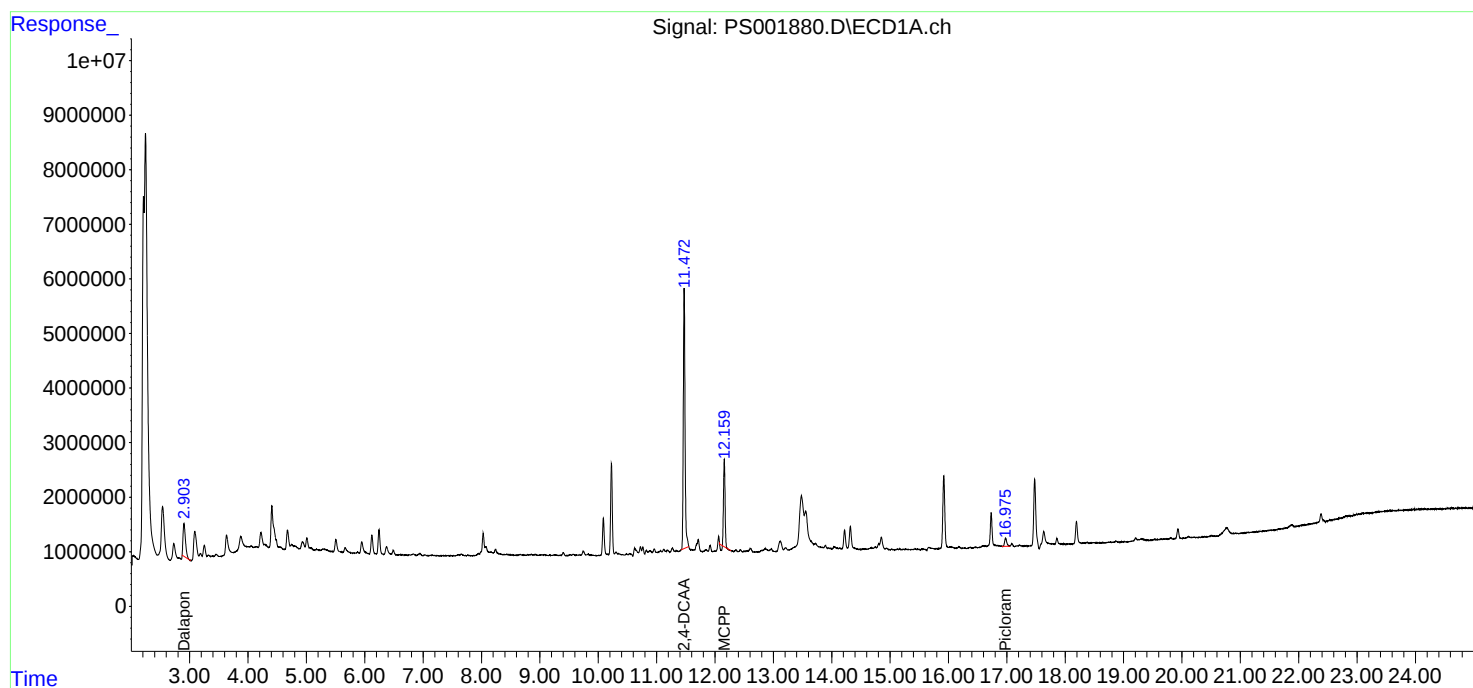


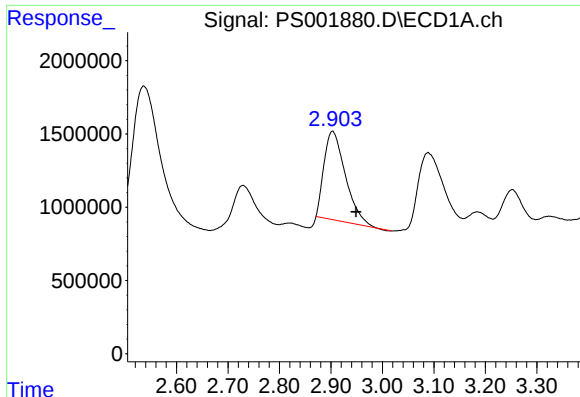

#1 Dalapon


R.T.: 2.903 min
Delta R.T.: -0.046 min
Response: 17432811
Conc: 53.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

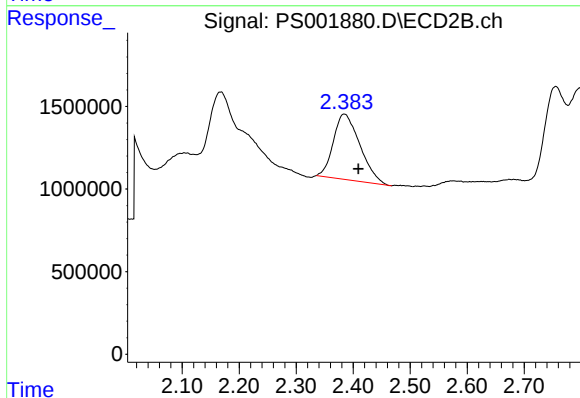


#1 Dalapon

R.T.: 2.384 min
Delta R.T.: -0.025 min
Response: 12839277
Conc: 43.46 ng/ml

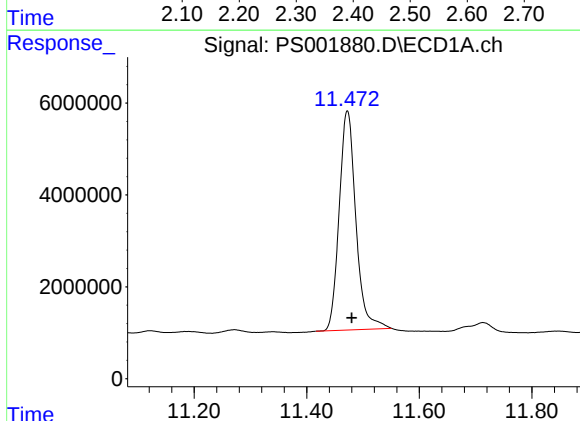


#4 2,4-DCAA

R.T.: 11.472 min
Delta R.T.: -0.008 min
Response: 98415979
Conc: 438.74 ng/ml

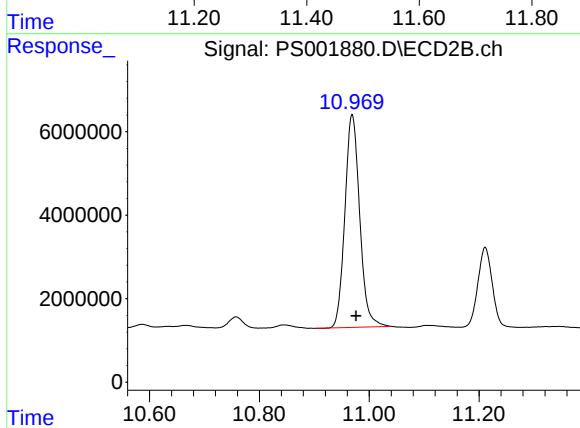

#4 2,4-DCAA


R.T.: 10.969 min
Delta R.T.: -0.007 min
Response: 95435718
Conc: 375.71 ng/ml

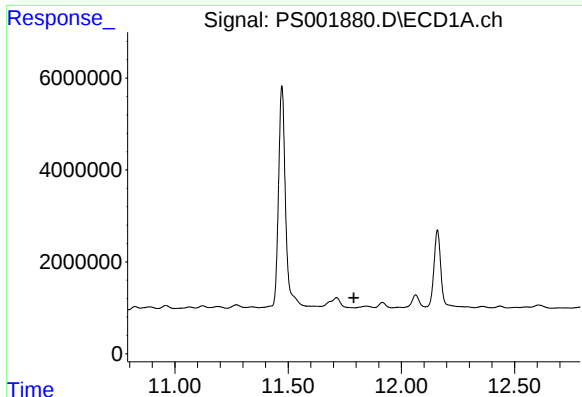

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

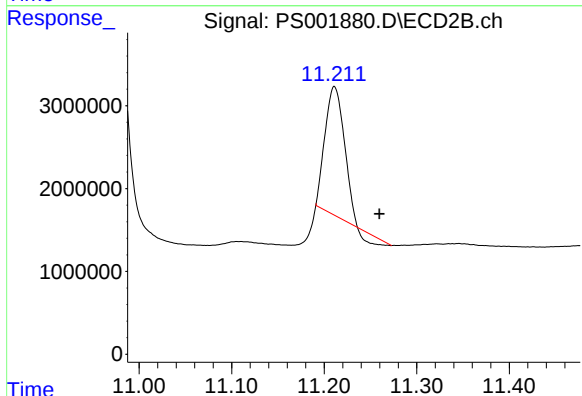


#5 DICAMBA

R.T.: 11.211 min
Delta R.T.: -0.049 min
Response: 21203687
Conc: 23.77 ng/ml

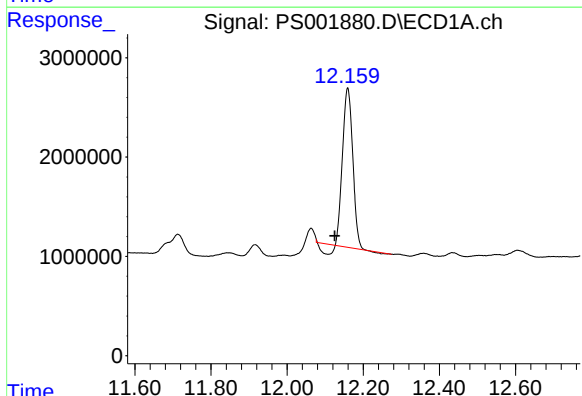


#6 MCP

R.T.: 12.159 min
Delta R.T.: 0.034 min
Response: 28475581
Conc: 44.69 ug/ml

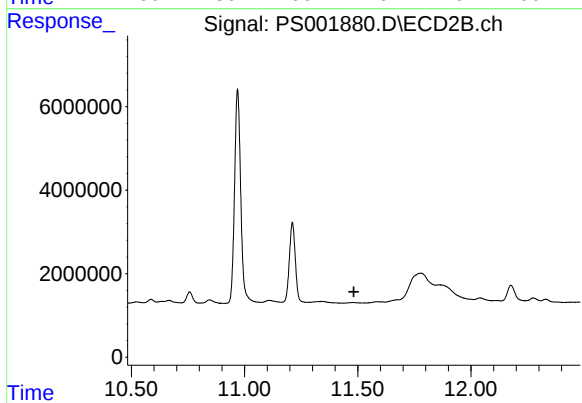

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.483 min
Response: 0
Conc: N.D.

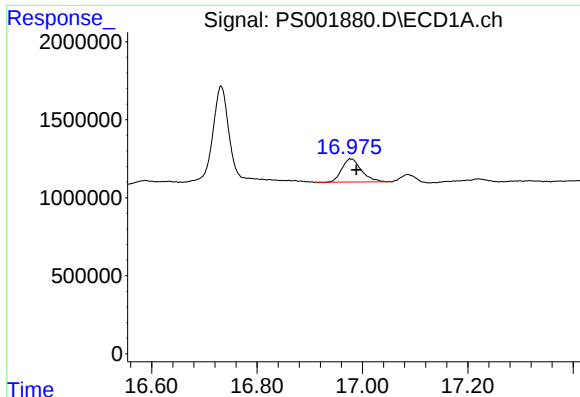

#15 Picloram


R.T.: 16.978 min
Delta R.T.: -0.011 min
Response: 3821660
Conc: 2.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

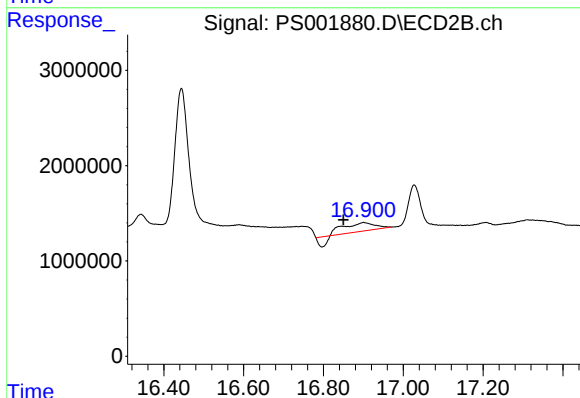


#15 Picloram

R.T.: 16.901 min
Delta R.T.: 0.051 min
Response: 3854742
Conc: 2.27 ng/ml

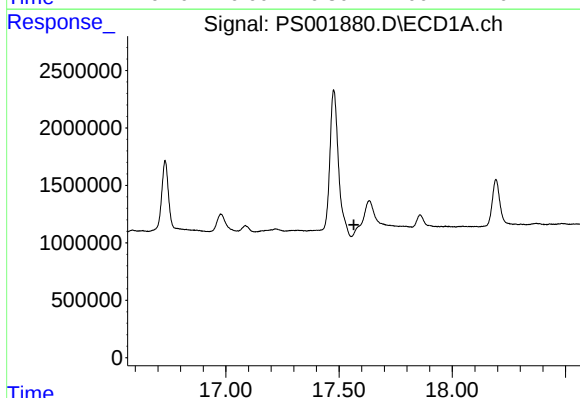

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.565 min
Response: 0
Conc: N.D.

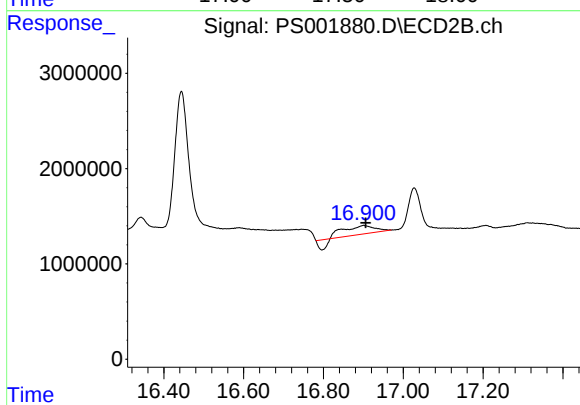

#16 DCPA

R.T.: 16.901 min
Delta R.T.: -0.005 min
Response: 3854742
Conc: 2.09 ng/ml