

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100219\
 Data File : PS006994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2019 00:36
 Operator : SM\AJ
 Sample : K4663-12
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:20:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.499	5.230	223.8E6	103.8E6	244.938	225.766
Target Compounds							
1) T	Dalapon	2.047	1.761	135.5E6	131.2E6	126.819	246.146 #
2) T	3,5-DICHL...	0.000	4.557	0	53757189	N.D.	93.513
3) T	4-Nitroph...	5.351	4.940	19237737	15381048	50.453	63.629 #
5) T	DICAMBA	5.679	0.000	57546815	0	17.811	N.D. #
6) T	MCP	5.771	0.000	18132293	0	8.523	N.D. #
9) T	2,4-D	6.567	6.150	120.8E6	7504224	147.384	14.712 #
10) T	Pentachlo...	6.833	0.000	15871011	0	1.332	N.D. #
11) T	2,4,5-TP ...	0.000	6.848	0	56944049	N.D.	23.773



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100219\
Data File : PS006994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2019 00:36
Operator : SM\AJ
Sample : K4663-12
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:20:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

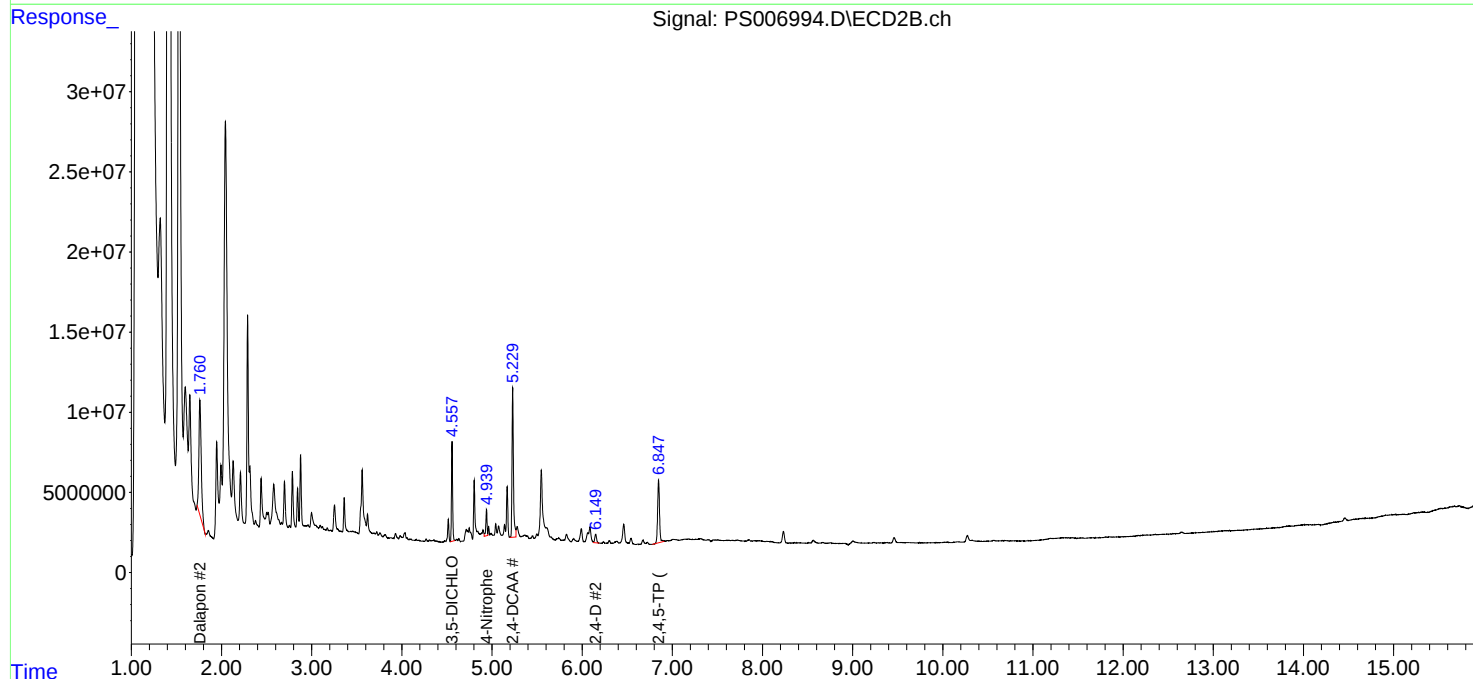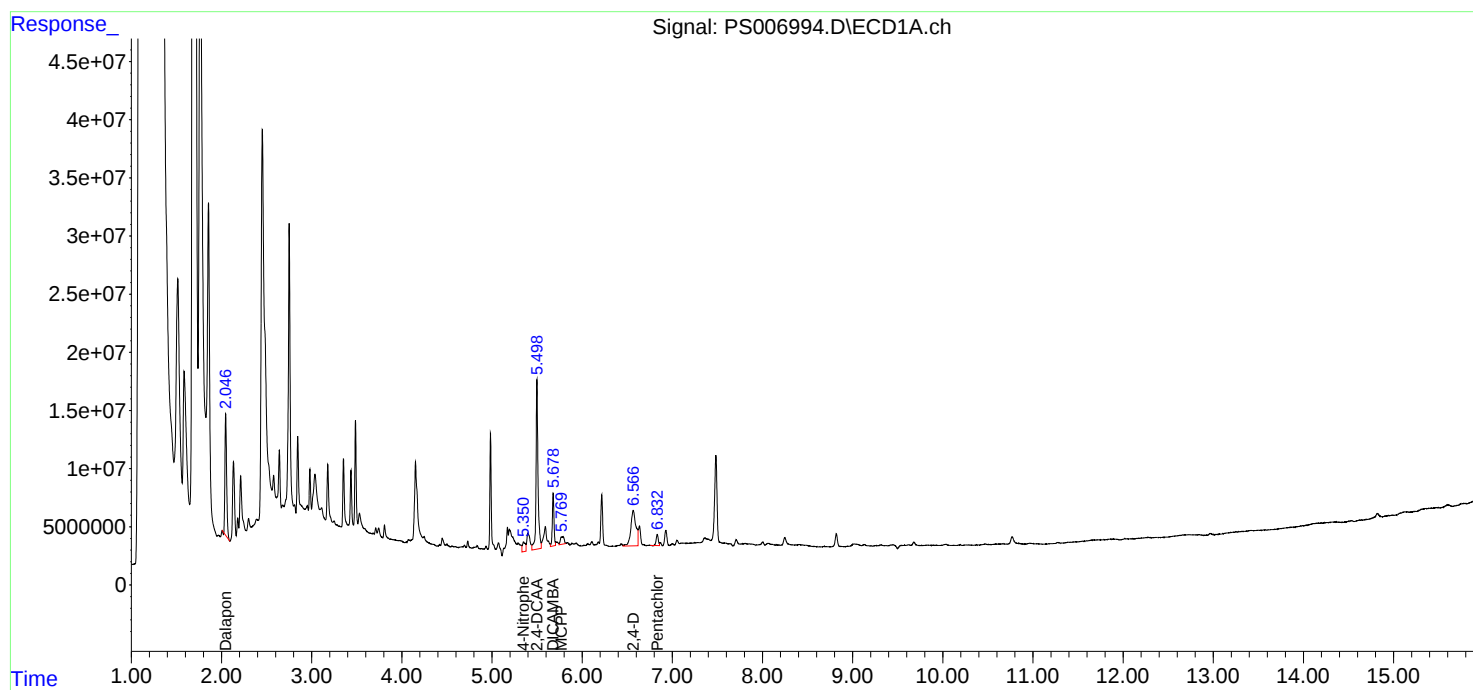


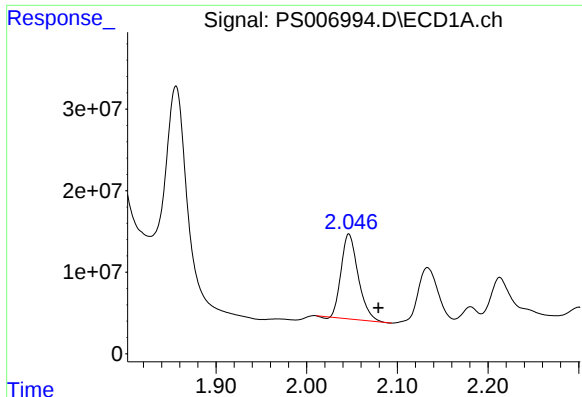

#1 Dalapon


R.T.: 2.047 min
Delta R.T.: -0.032 min
Response: 135493674
Conc: 126.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

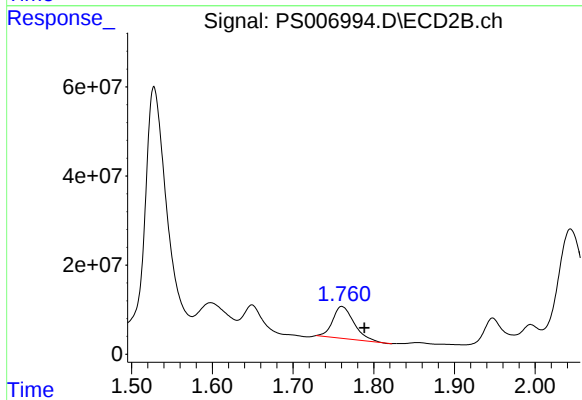


#1 Dalapon

R.T.: 1.761 min
Delta R.T.: -0.028 min
Response: 131213054
Conc: 246.15 ng/ml

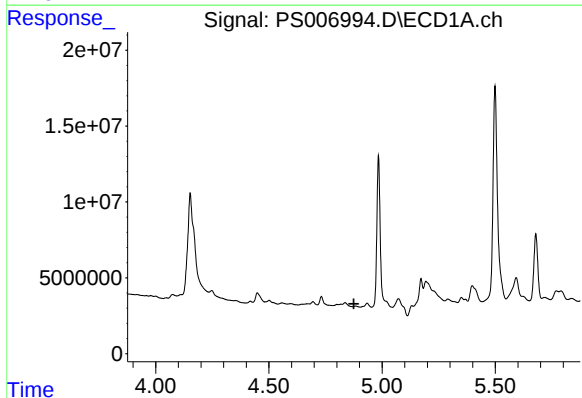


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.876 min
Response: 0
Conc: N.D.

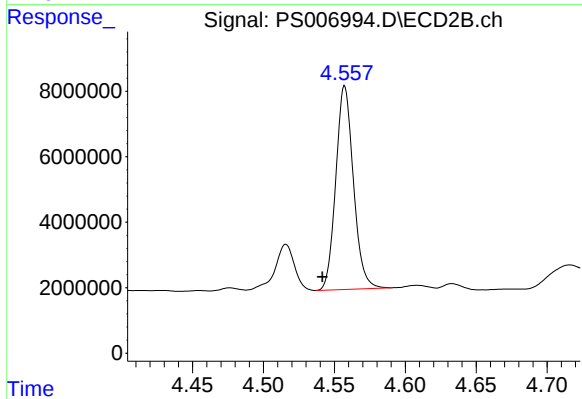

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.557 min
Delta R.T.: 0.016 min
Response: 53757189
Conc: 93.51 ng/ml

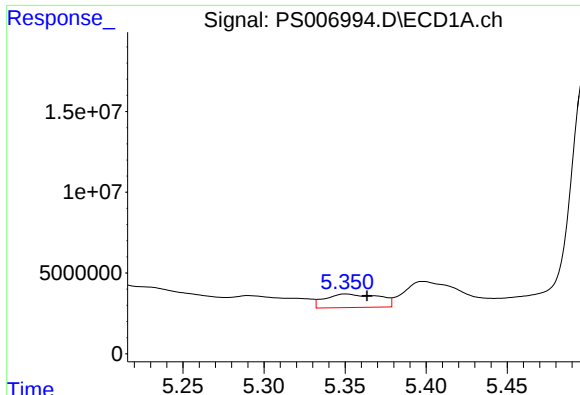

#3 4-Nitrophenol


R.T.: 5.351 min
Delta R.T.: -0.013 min
Response: 19237737
Conc: 50.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

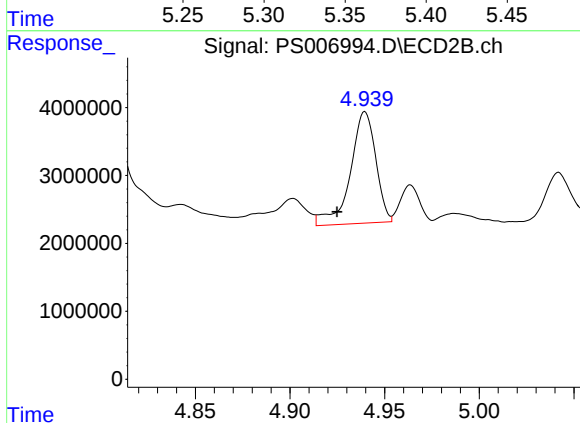


#3 4-Nitrophenol

R.T.: 4.940 min
Delta R.T.: 0.015 min
Response: 15381048
Conc: 63.63 ng/ml

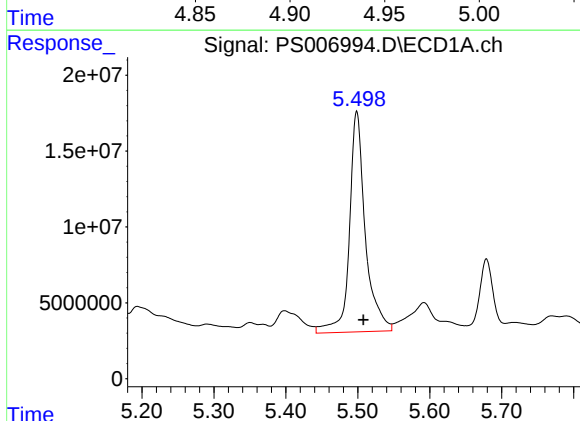


#4 2,4-DCAA

R.T.: 5.499 min
Delta R.T.: -0.009 min
Response: 223827715
Conc: 244.94 ng/ml

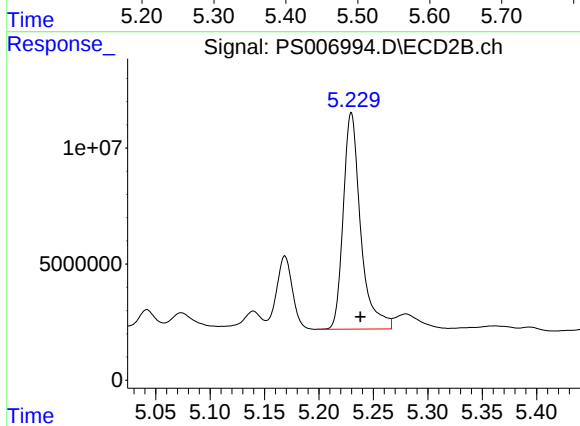

#4 2,4-DCAA


R.T.: 5.230 min
Delta R.T.: -0.008 min
Response: 103816731
Conc: 225.77 ng/ml

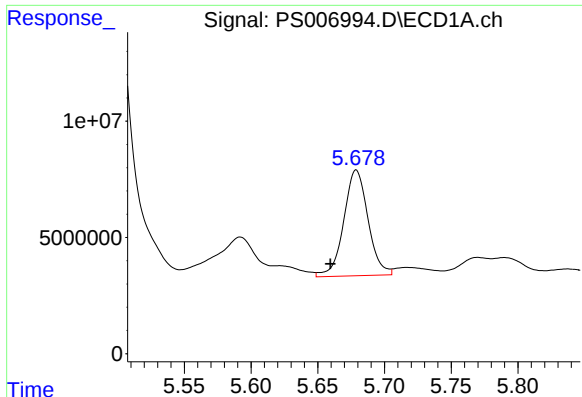

#5 DICAMBA


R.T.: 5.679 min
Delta R.T.: 0.019 min
Response: 57546815
Conc: 17.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

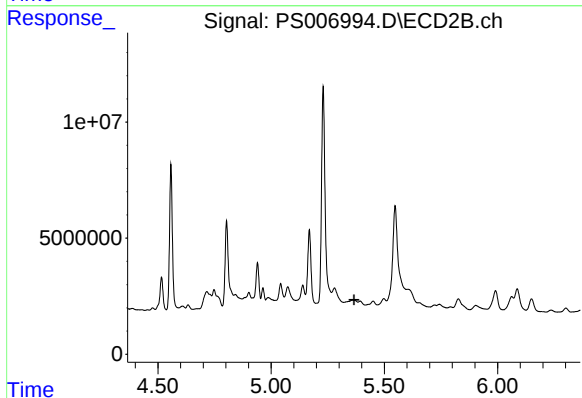


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.366 min
Response: 0
Conc: N.D.

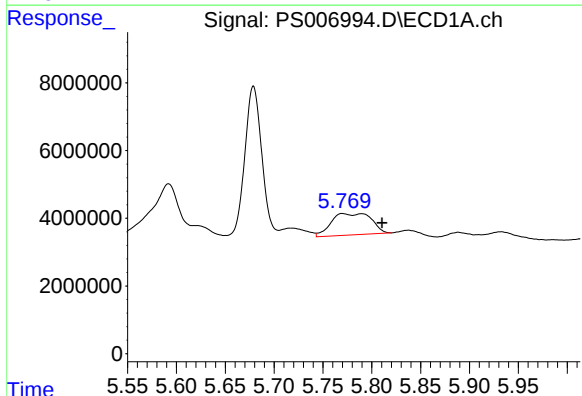


#6 MCPP

R.T.: 5.771 min
Delta R.T.: -0.040 min
Response: 18132293
Conc: 8.52 ug/ml

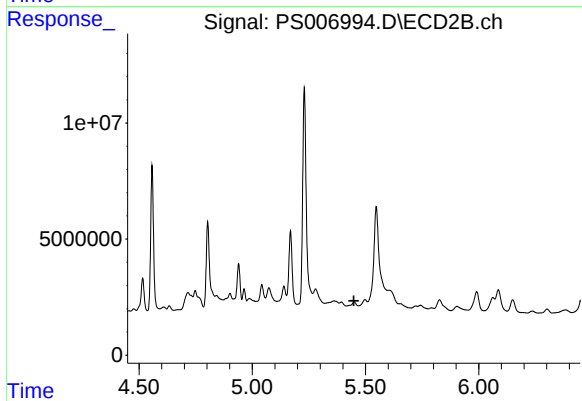

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 5.449 min
Response: 0
Conc: N.D.

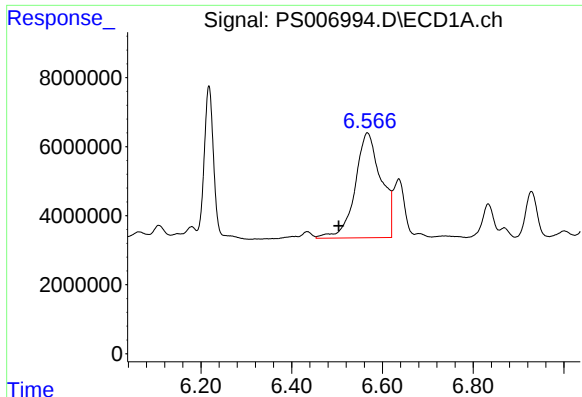

#9 2,4-D


R.T.: 6.567 min
Delta R.T.: 0.063 min
Response: 120783059
Conc: 147.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

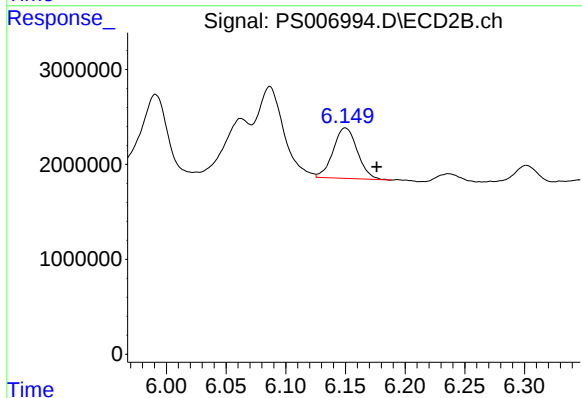


#9 2,4-D

R.T.: 6.150 min
Delta R.T.: -0.026 min
Response: 7504224
Conc: 14.71 ng/ml

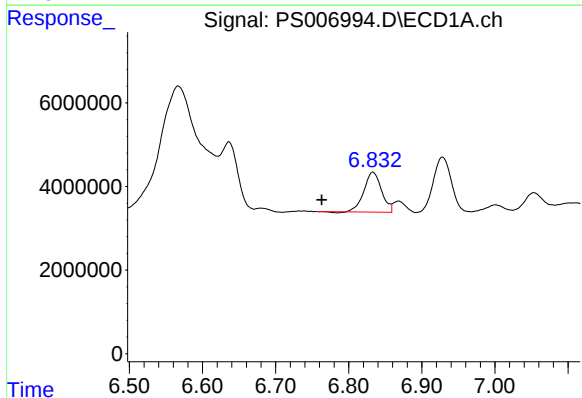


#10 Pentachlorophenol

R.T.: 6.833 min
Delta R.T.: 0.070 min
Response: 15871011
Conc: 1.33 ng/ml

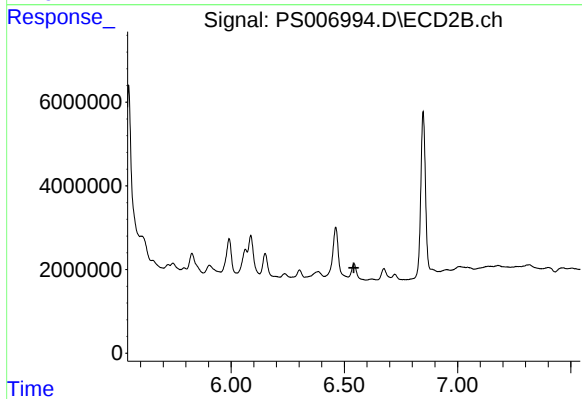

#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.542 min
Response: 0
Conc: N.D.

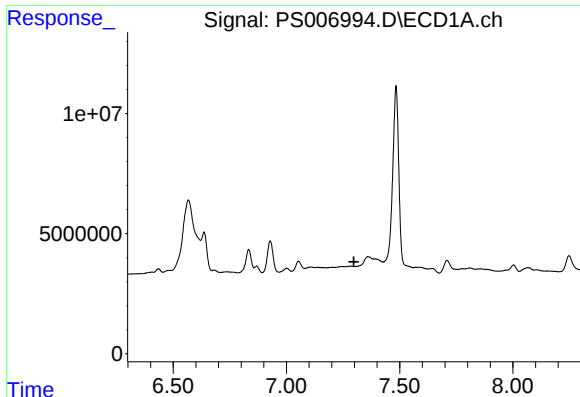

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min

Exp R.T.: 7.298 min

Response: 0

Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

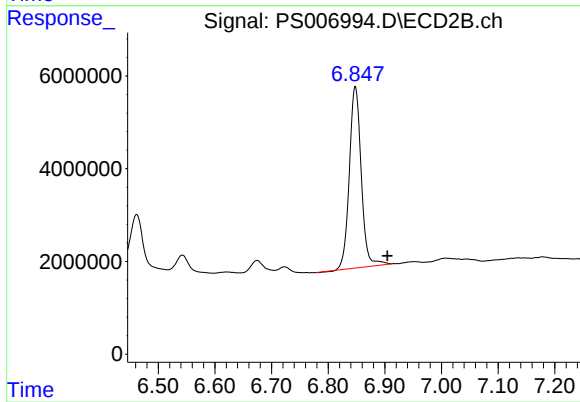

#11 2,4,5-TP (SILVEX)

R.T.: 6.848 min

Delta R.T.: -0.057 min

Response: 56944049

Conc: 23.77 ng/ml