

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100219\
 Data File : PS006999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2019 02:25
 Operator : SM\AJ
 Sample : K5095-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:22:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.476	5.256	305.3E6	15928999	334.083	34.640 #
Target Compounds							
1) T	Dalapon	2.113	0.000	178.8E6	0	167.389	N.D. #
2) T	3,5-DICHL...	4.860	4.536	6026472	63501788	5.540	110.464 #
3) T	4-Nitroph...	5.371	4.880	3764862	17353838	9.874	71.790 #
5) T	DICAMBA	0.000	5.351	0	15422439	N.D.	9.162
6) T	MCP	5.744	0.000	20404567	0	9.591	N.D. #
9) T	2,4-D	6.541	0.000	105.2E6	0	128.345	N.D. #
10) T	Pentachlo...	6.812	0.000	12000756	0	1.007	N.D. #
15) T	Picloram	9.043	0.000	21769971	0	3.246	N.D. #
16) T	DCPA	9.499	8.912	11311080	6792393	1.938	2.138



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100219\
Data File : PS006999.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2019 02:25
Operator : SM\AJ
Sample : K5095-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:22:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

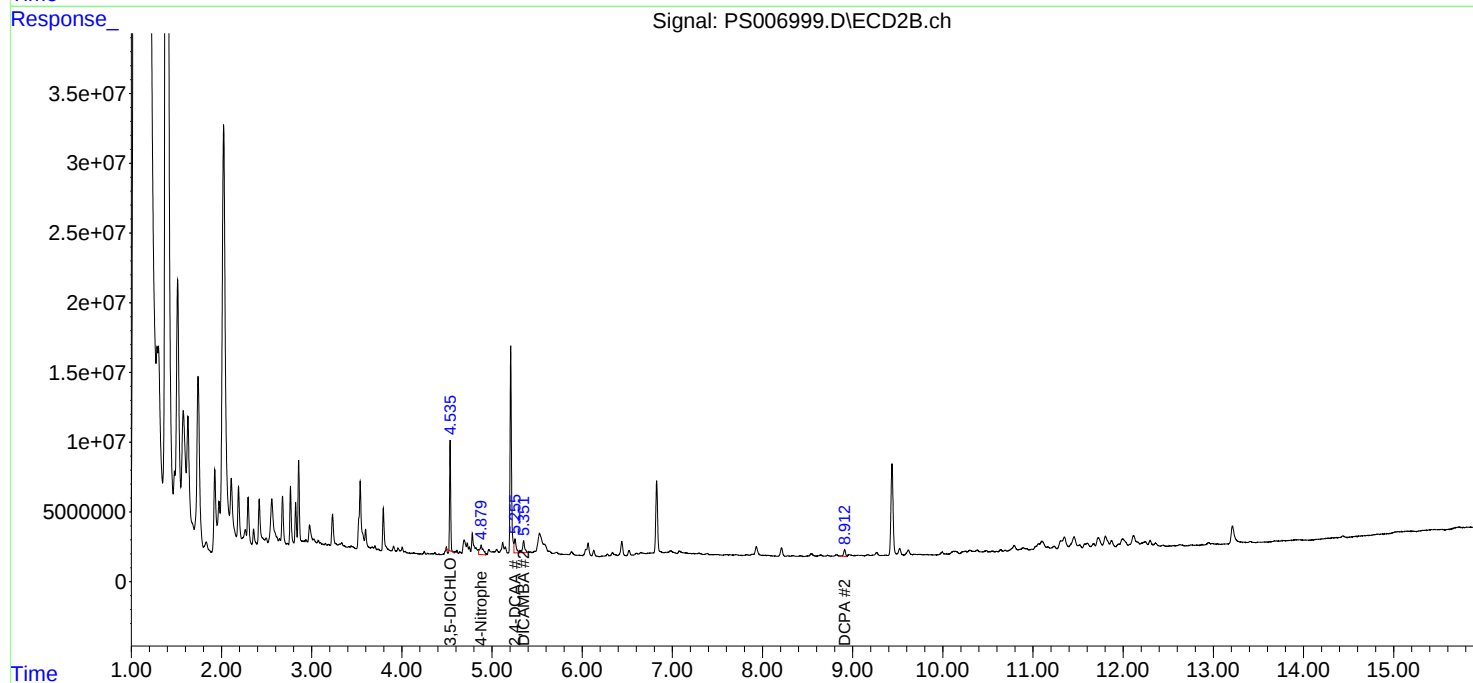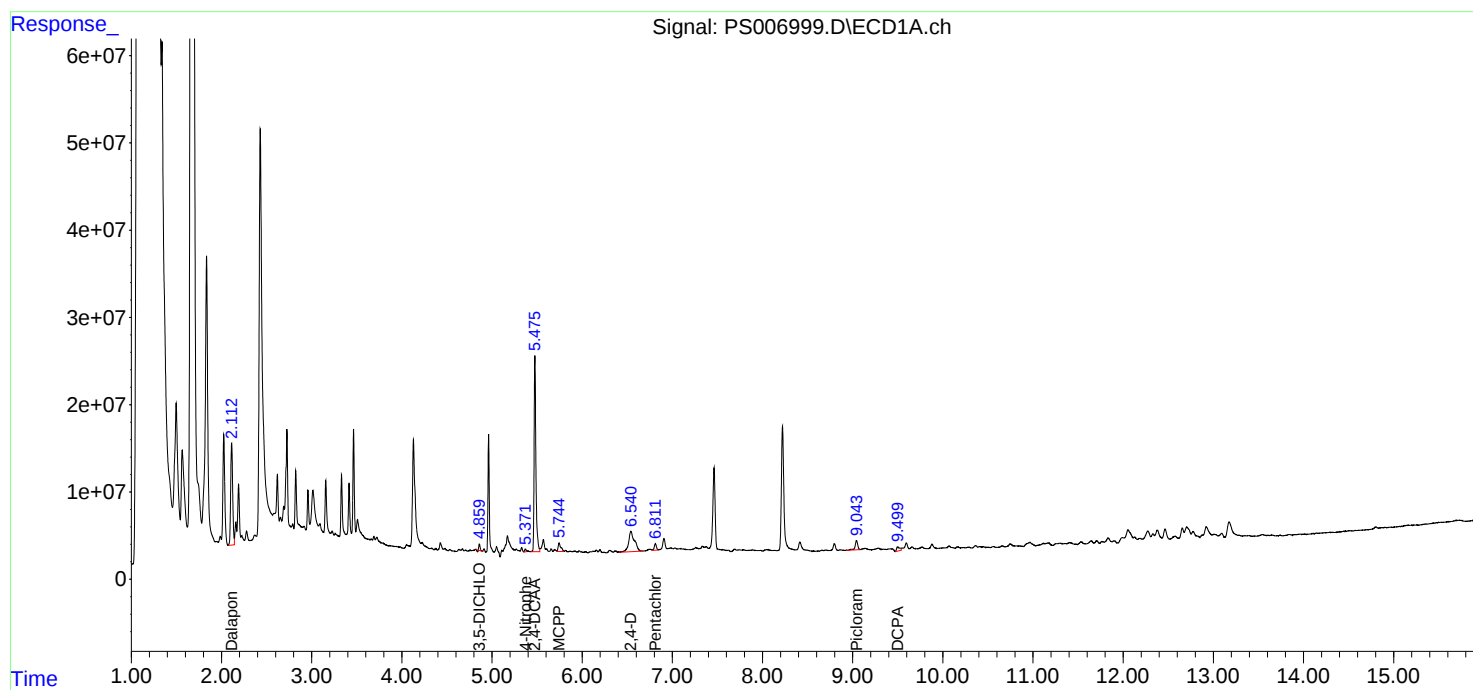


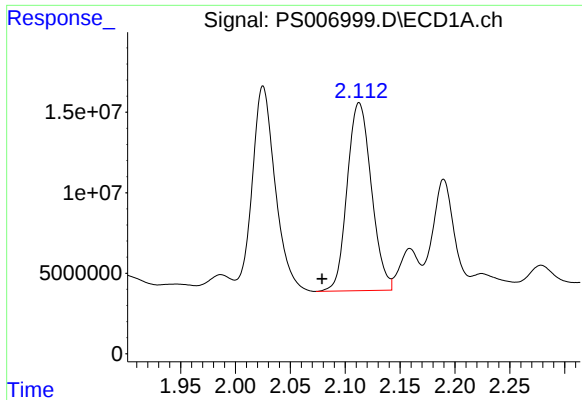

#1 Dalapon


R.T.: 2.113 min
Delta R.T.: 0.034 min
Response: 178839060
Conc: 167.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

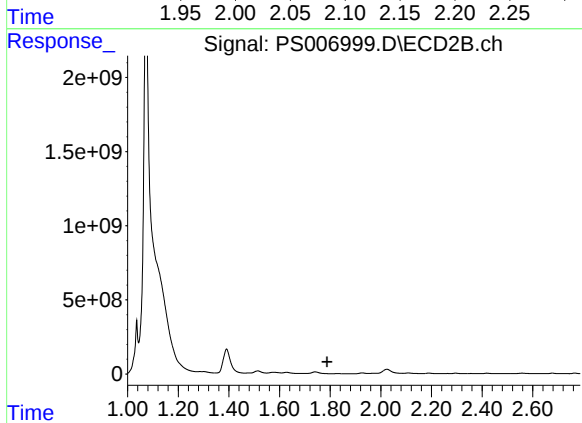


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

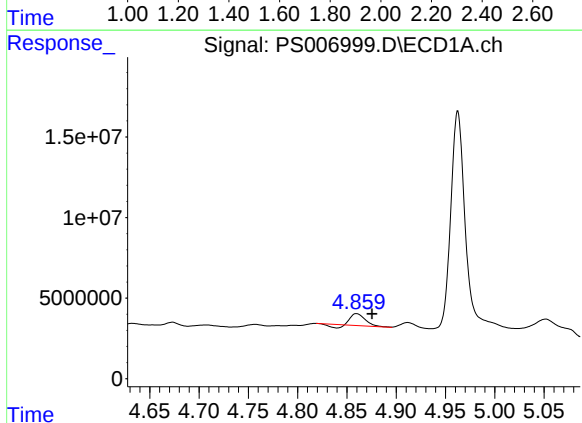


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.860 min
Delta R.T.: -0.015 min
Response: 6026472
Conc: 5.54 ng/ml

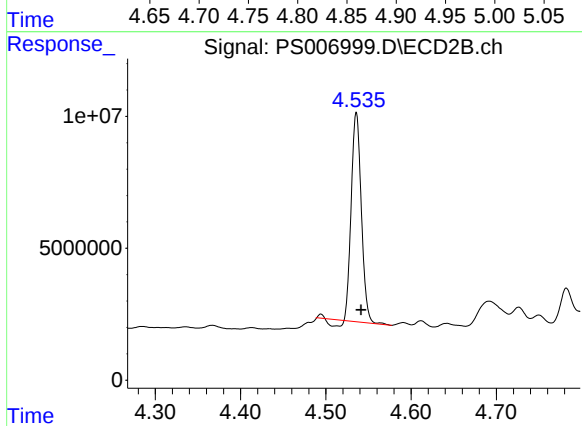

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.536 min
Delta R.T.: -0.006 min
Response: 63501788
Conc: 110.46 ng/ml

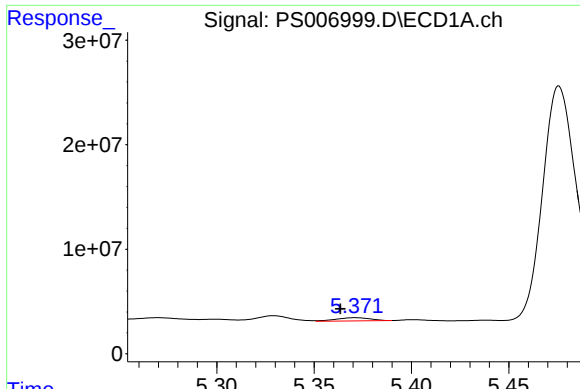

#3 4-Nitrophenol


R.T.: 5.371 min
Delta R.T.: 0.008 min
Response: 3764862
Conc: 9.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

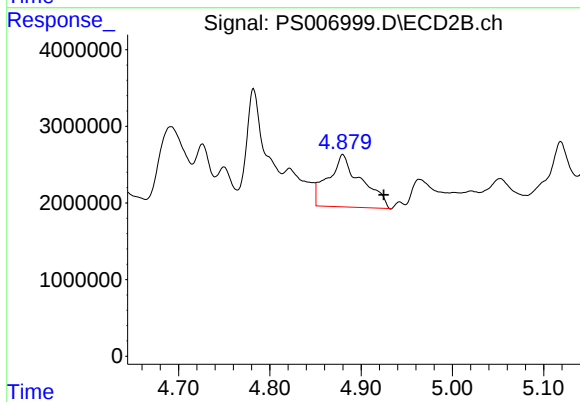


#3 4-Nitrophenol

R.T.: 4.880 min
Delta R.T.: -0.045 min
Response: 17353838
Conc: 71.79 ng/ml

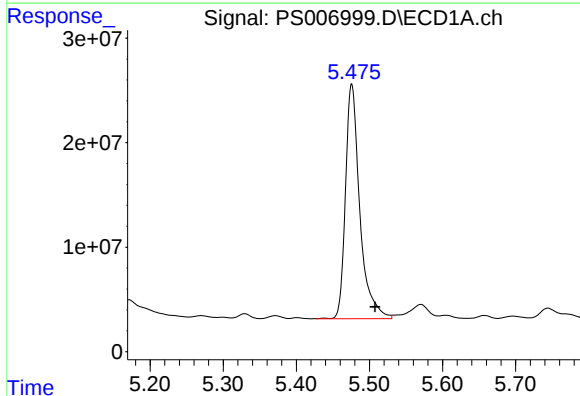


#4 2,4-DCAA

R.T.: 5.476 min
Delta R.T.: -0.032 min
Response: 305289474
Conc: 334.08 ng/ml

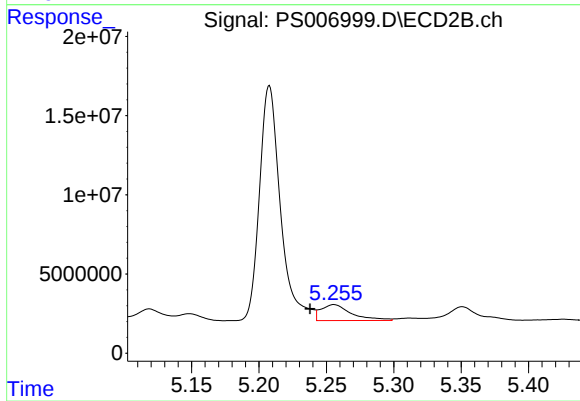

#4 2,4-DCAA


R.T.: 5.256 min
Delta R.T.: 0.018 min
Response: 15928999
Conc: 34.64 ng/ml

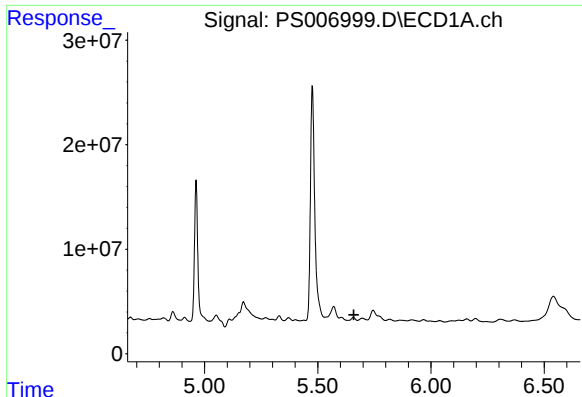

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

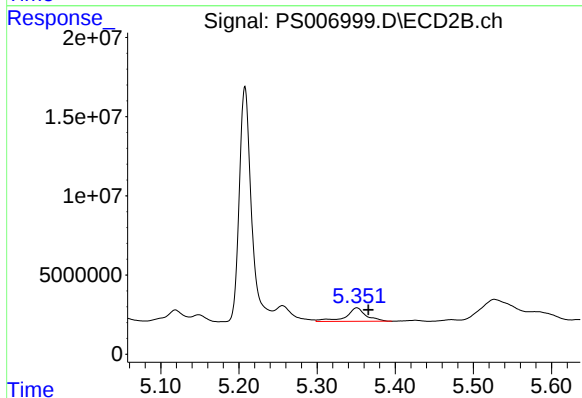


#5 DICAMBA

R.T.: 5.351 min
Delta R.T.: -0.015 min
Response: 15422439
Conc: 9.16 ng/ml

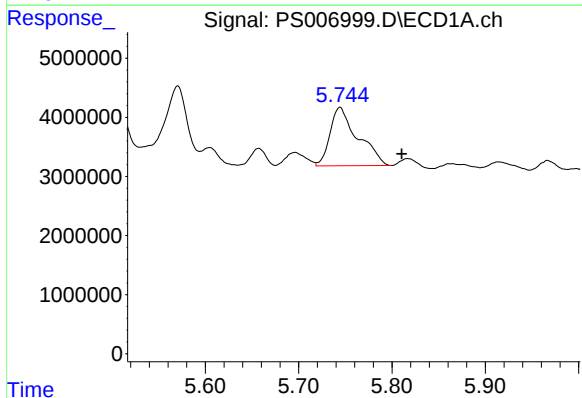


#6 MCP

R.T.: 5.744 min
Delta R.T.: -0.066 min
Response: 20404567
Conc: 9.59 ug/ml

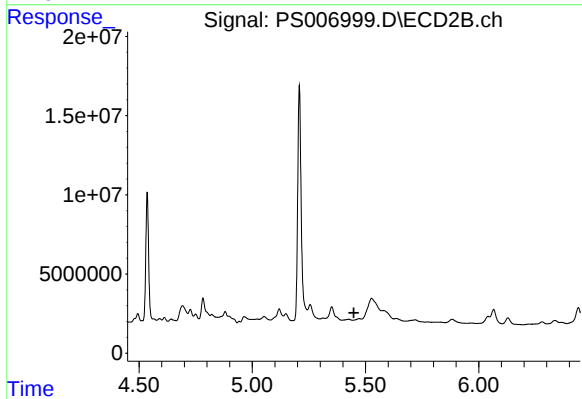

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.449 min
Response: 0
Conc: N.D.

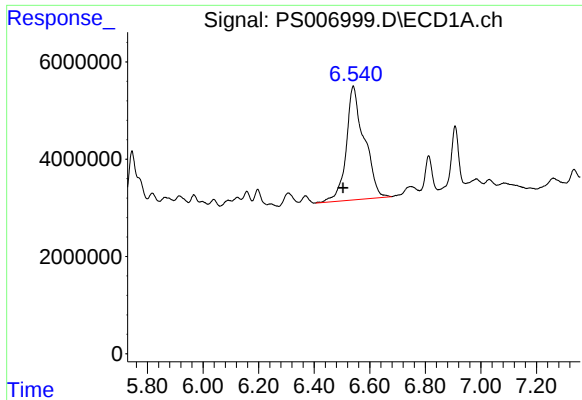

#9 2,4-D


R.T.: 6.541 min
Delta R.T.: 0.037 min
Response: 105180336
Conc: 128.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

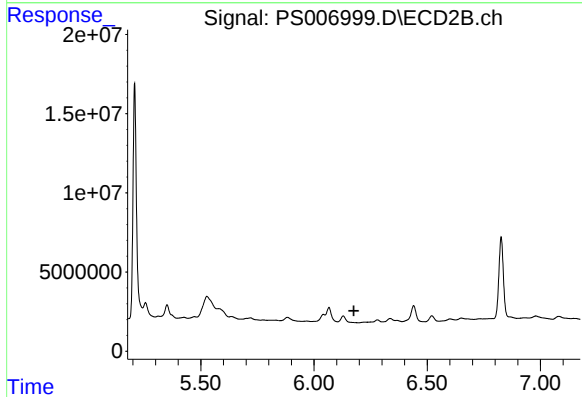


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

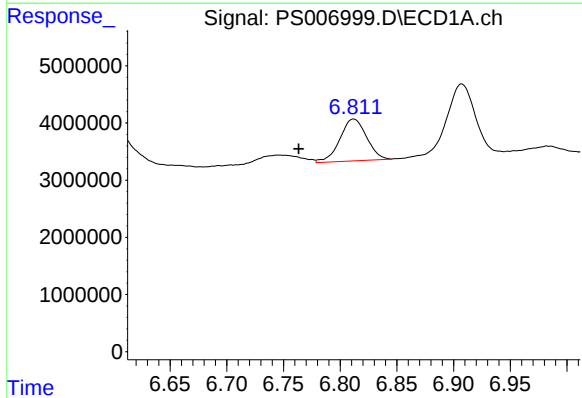


#10 Pentachlorophenol

R.T.: 6.812 min
Delta R.T.: 0.049 min
Response: 12000756
Conc: 1.01 ng/ml

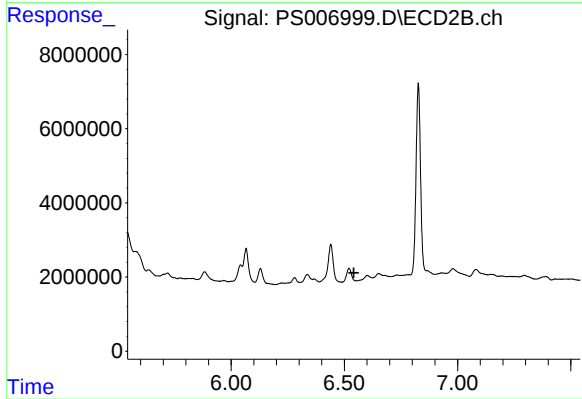

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.542 min
Response: 0
Conc: N.D.

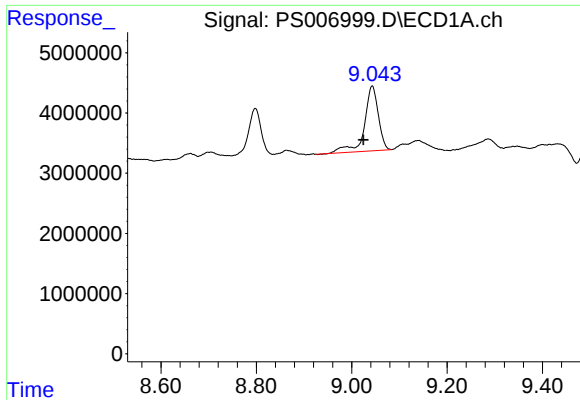

#15 Picloram


R.T.: 9.043 min
Delta R.T.: 0.018 min
Response: 21769971
Conc: 3.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

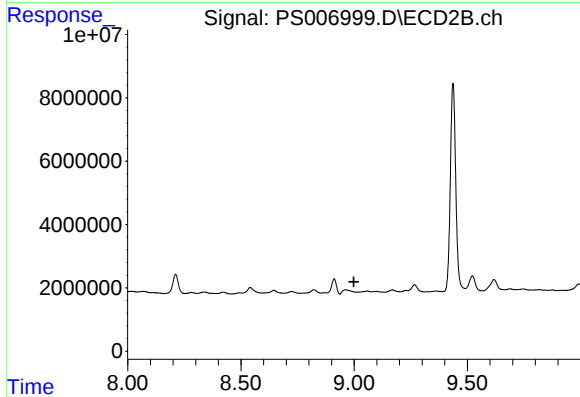


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.999 min
Response: 0
Conc: N.D.

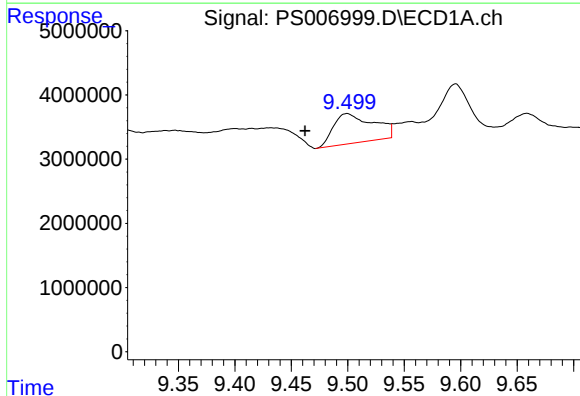

#16 DCPA

R.T.: 9.499 min
Delta R.T.: 0.037 min
Response: 11311080
Conc: 1.94 ng/ml

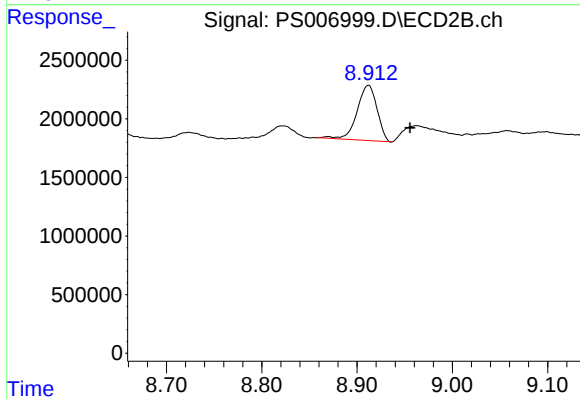

#16 DCPA

R.T.: 8.912 min
Delta R.T.: -0.044 min
Response: 6792393
Conc: 2.14 ng/ml