

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100219\
 Data File : PS006999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2019 02:25
 Operator : SM\AJ
 Sample : K5095-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMPOSITE-3

Manual Integrations
 APPROVED

Ankita
 10/3/2019 5:46:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:22:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.476	5.207	305.3E6	161.1E6	334.083	350.294m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100219\
Data File : PS006999.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2019 02:25
Operator : SM\AJ
Sample : K5095-03
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
COMPOSITE-3


Manual Integrations
APPROVED

Ankita
10/3/2019 5:46:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:22:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

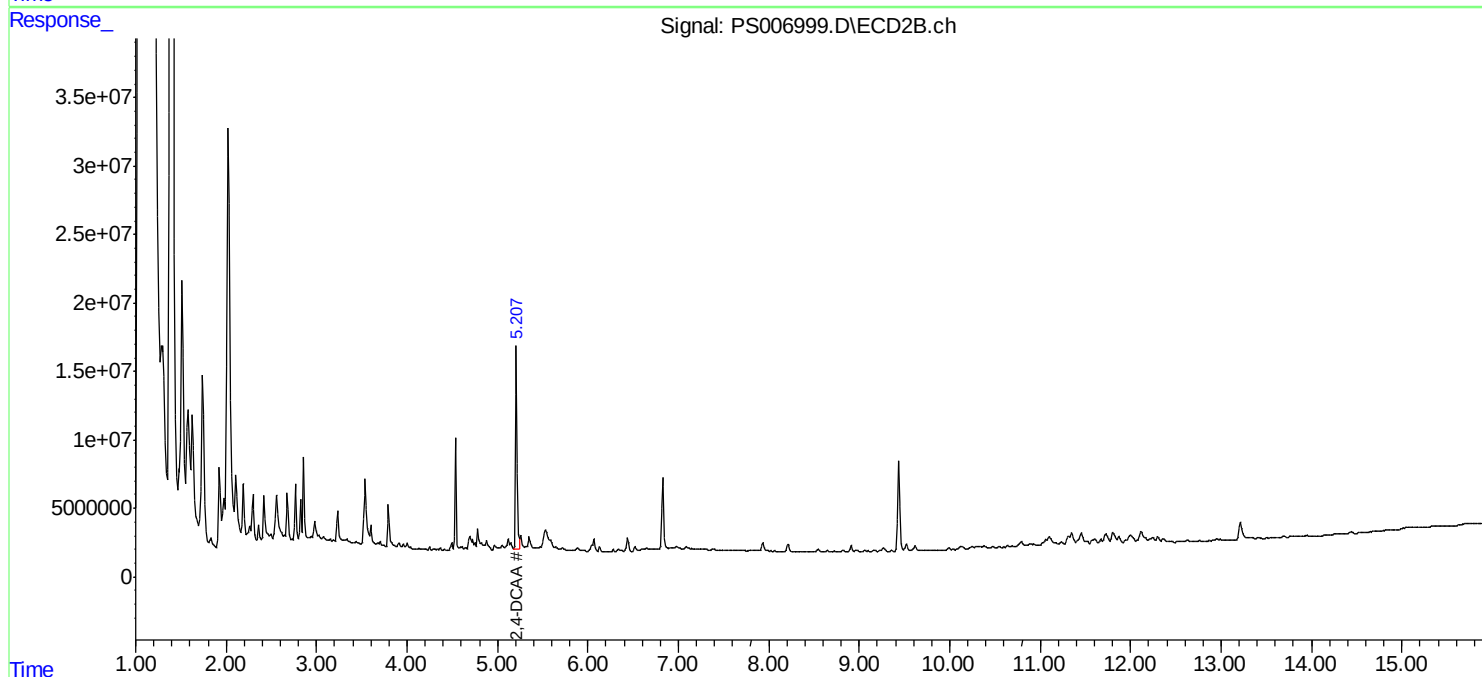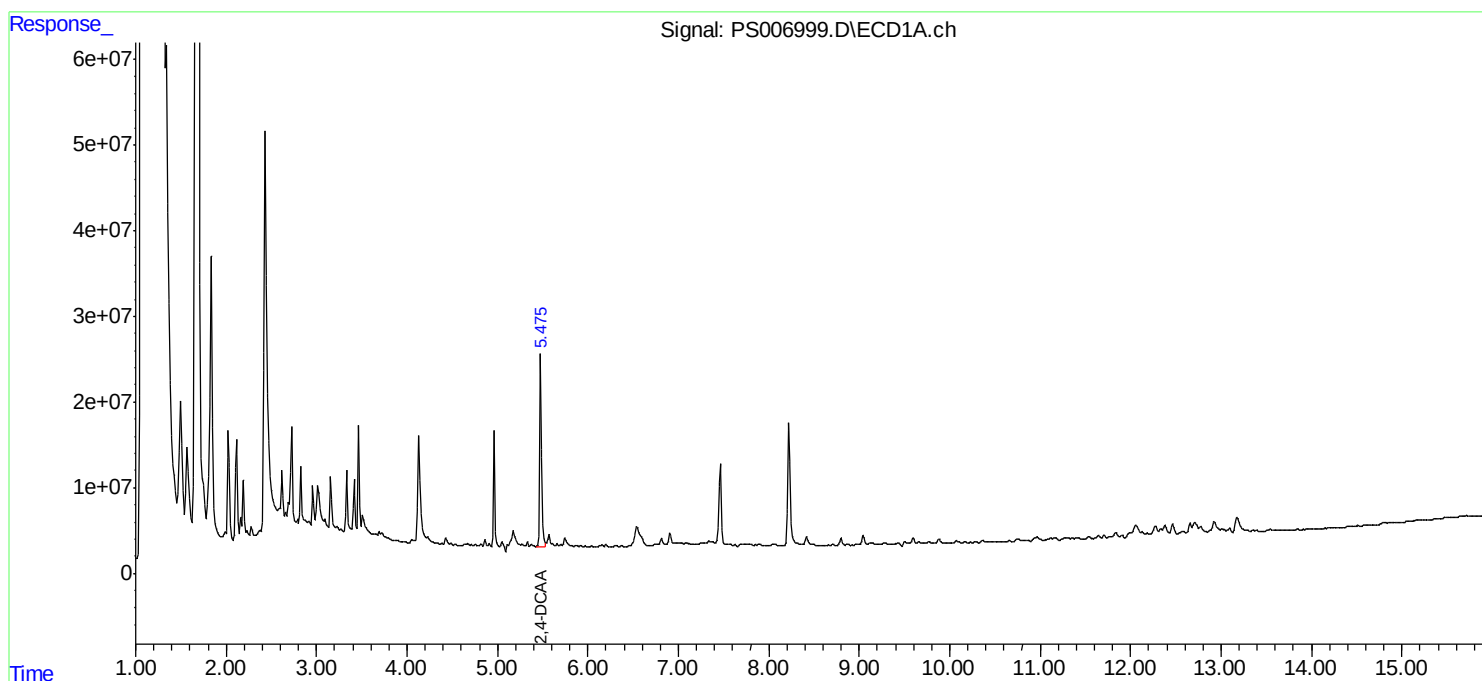

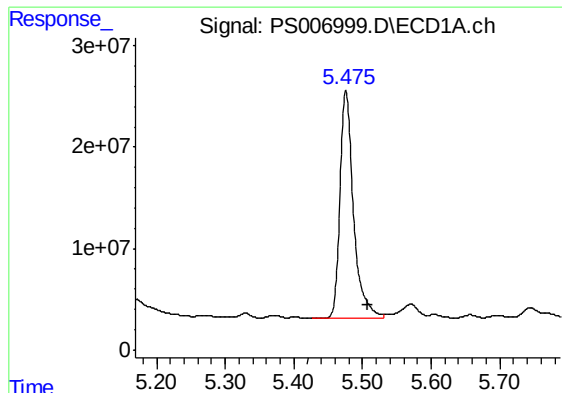


#4 2,4-DCAA

R.T.: 5.476 min
Delta R.T.: -0.032 min
Response: 305289474
Conc: 334.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMPOSITE-3

Manual Integrations
APPROVED

Ankita
10/3/2019 5:46:20 PM

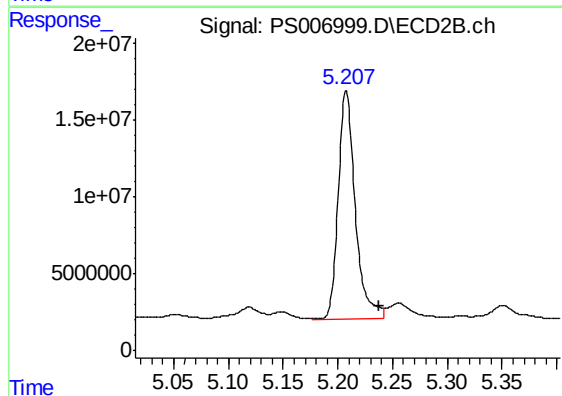

#4 2,4-DCAA

R.T.: 5.207 min
Delta R.T.: -0.031 min
Response: 161079909
Conc: 350.29 ng/ml m