

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100220\
 Data File : PS012587.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2020 16:57
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 05:34:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
7) T	MCPA	7.663	0.000	10196525	0	2.445	N.D. #
10) T	Pentachlo...	8.644	8.429	7305649	4318281	<MDL	<MDL #
12) T	2,4,5-T	9.411	0.000	14205796	0	2.527	N.D. #
15) T	Picloram	11.044	11.024	56106904	46596899	7.792	11.822 #
16) T	DCPA	0.000	10.934	0	5257978	N.D.	1.581



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100220\
Data File : PS012587.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2020 16:57
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 05:34:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

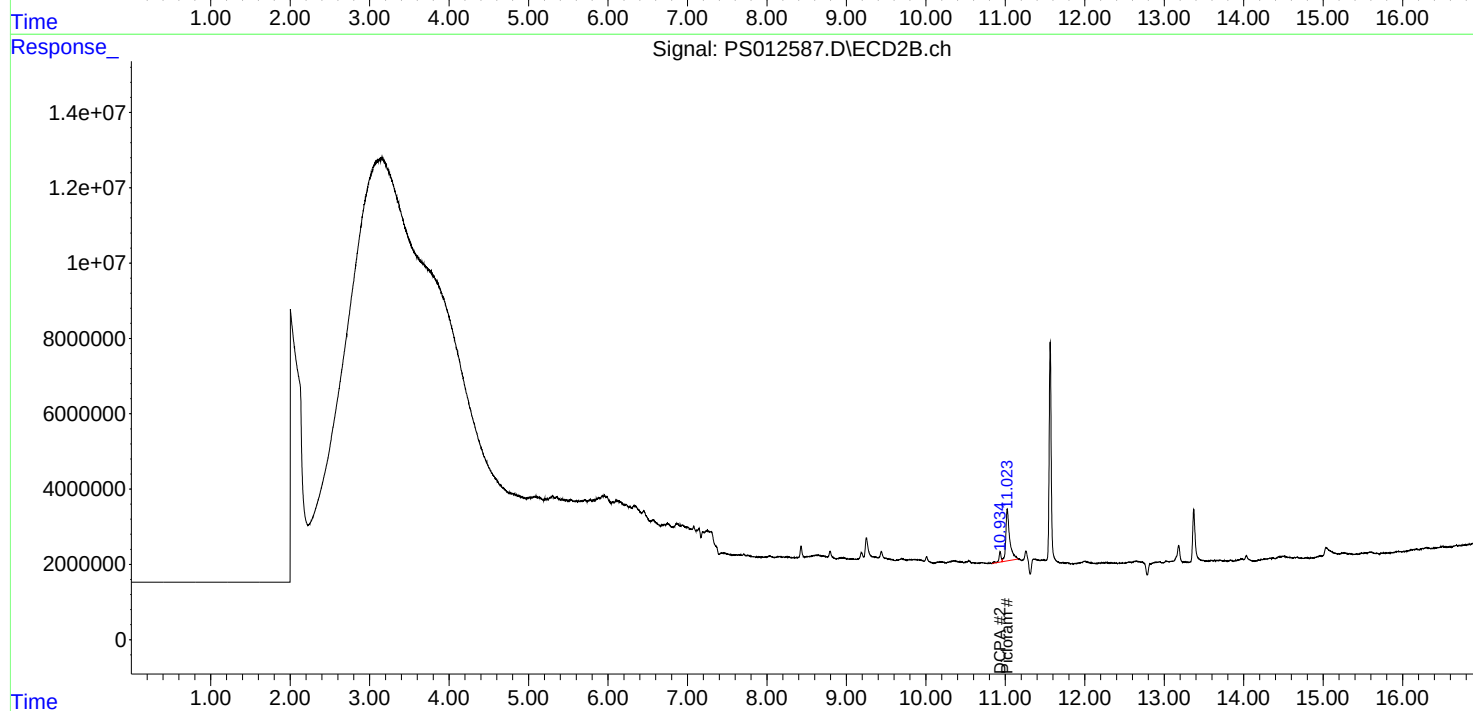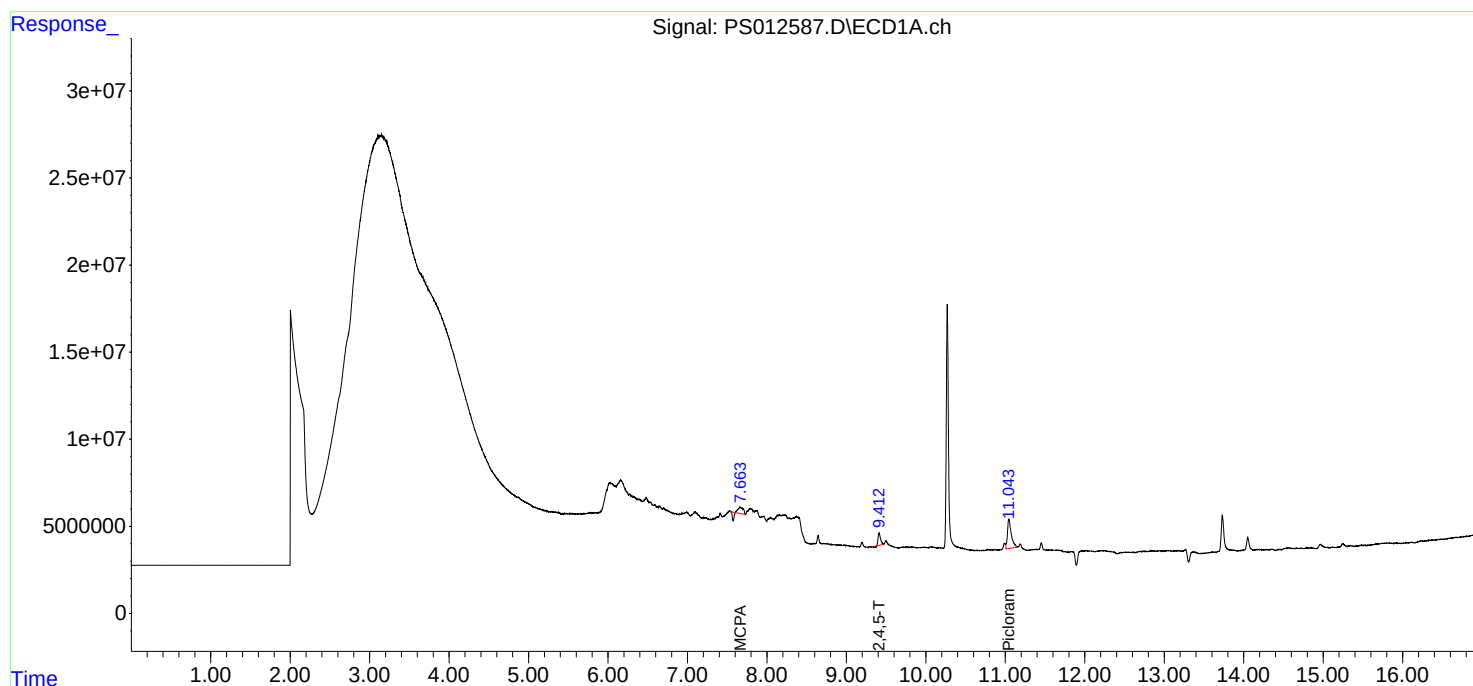


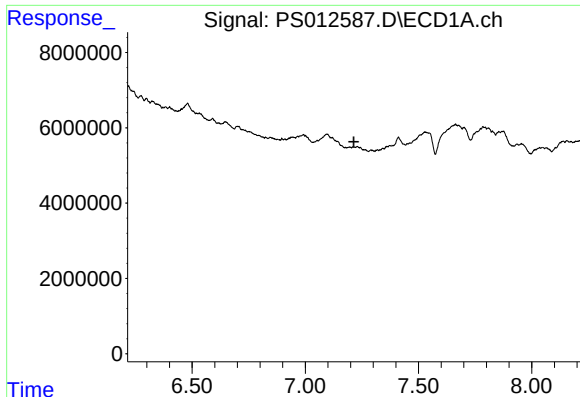

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.215 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

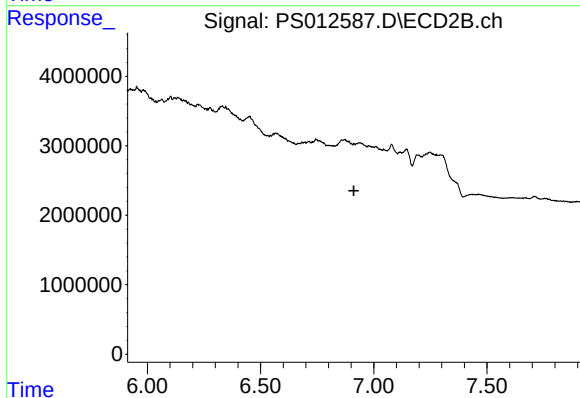


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

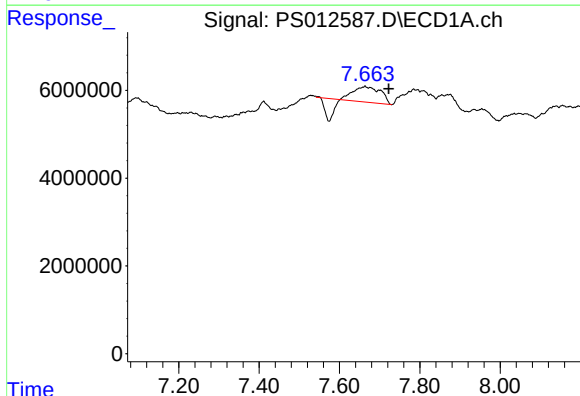


#7 MCPA

R.T.: 7.663 min
Delta R.T.: -0.059 min
Response: 10196525
Conc: 2.44 ug/ml

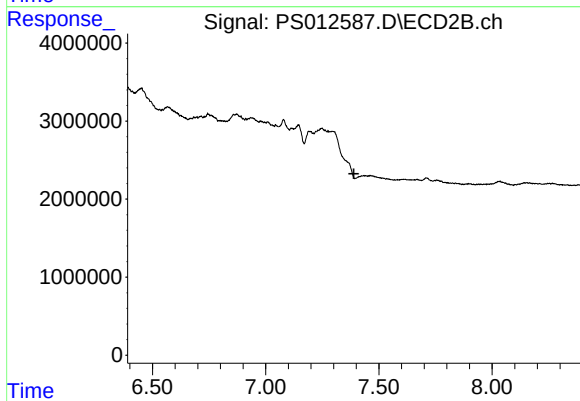

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.390 min
Response: 0
Conc: N.D.

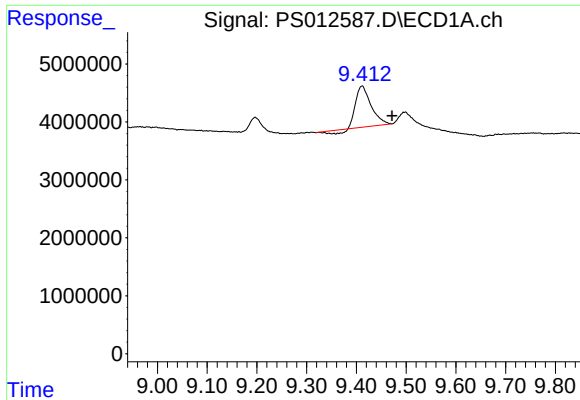

#12 2,4,5-T


R.T.: 9.411 min
Delta R.T.: -0.060 min
Response: 14205796
Conc: 2.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

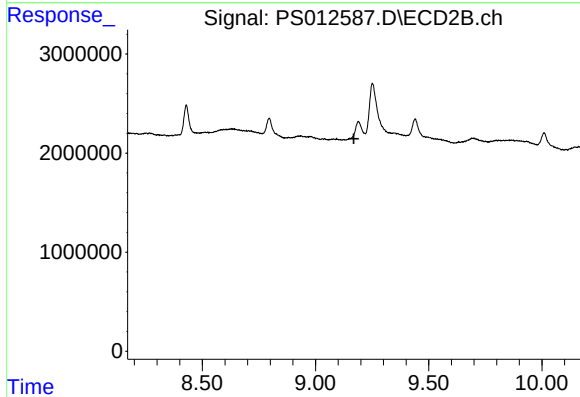


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.169 min
Response: 0
Conc: N.D.

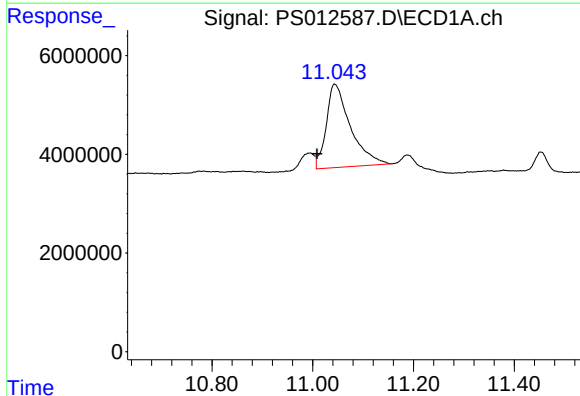


#15 Picloram

R.T.: 11.044 min
Delta R.T.: 0.035 min
Response: 56106904
Conc: 7.79 ng/ml

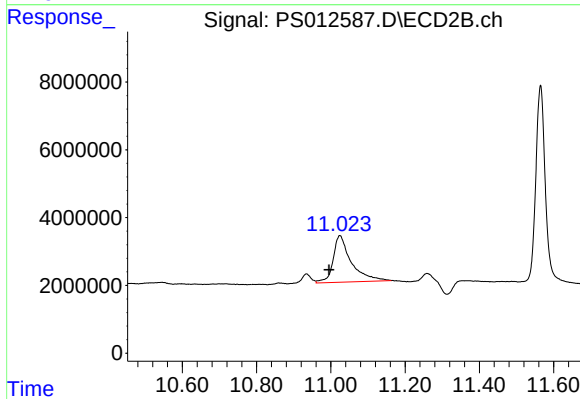

#15 Picloram


R.T.: 11.024 min
Delta R.T.: 0.029 min
Response: 46596899
Conc: 11.82 ng/ml

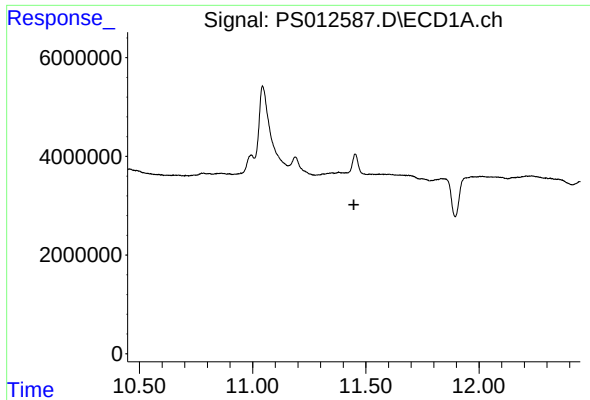

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

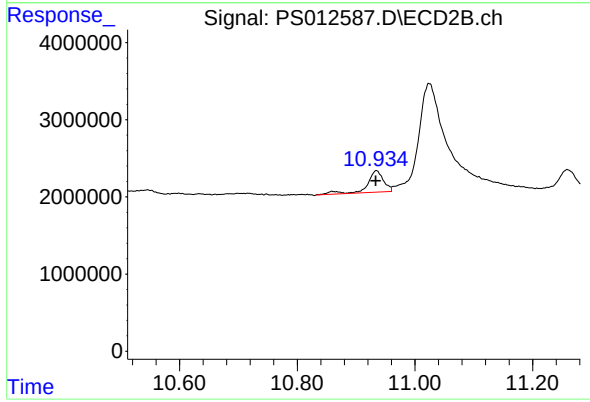

#16 DCPA

R.T.: 10.934 min
Delta R.T.: 0.001 min
Response: 5257978
Conc: 1.58 ng/ml