

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100220\
 Data File : PS012597.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Oct 2020 20:47
 Operator : DD\AJ
 Sample : L4194-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 05:39:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.913	377.0E6	208.7E6	384.938	453.633
Target Compounds							
1) T	Dalapon	2.996	2.591	66496935	108.9E6	58.517	181.979 #
2) T	3,5-DICHL...	6.499	6.094	6280804	82024748	4.658	115.048 #
3) T	4-Nitroph...	7.053	0.000	6617362	0	13.609	N.D. #
5) T	DICAMBA	7.393	7.046	9223758	10126775	2.391	5.311 #
6) T	MCPD	7.569	0.000	6396768	0	2.192	N.D. #
7) T	MCPA	7.711	7.349	144.6E6	7715948	34.668	3.219 #
9) T	2,4-D	8.396	0.000	77975783	0	68.676	N.D. #
10) T	Pentachlo...	8.690	0.000	9761973	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.798	0	9609598	N.D.	3.642
12) T	2,4,5-T	9.406	0.000	56352365	0	10.025	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100220\
Data File : PS012597.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Oct 2020 20:47
Operator : DD\AJ
Sample : L4194-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 05:39:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

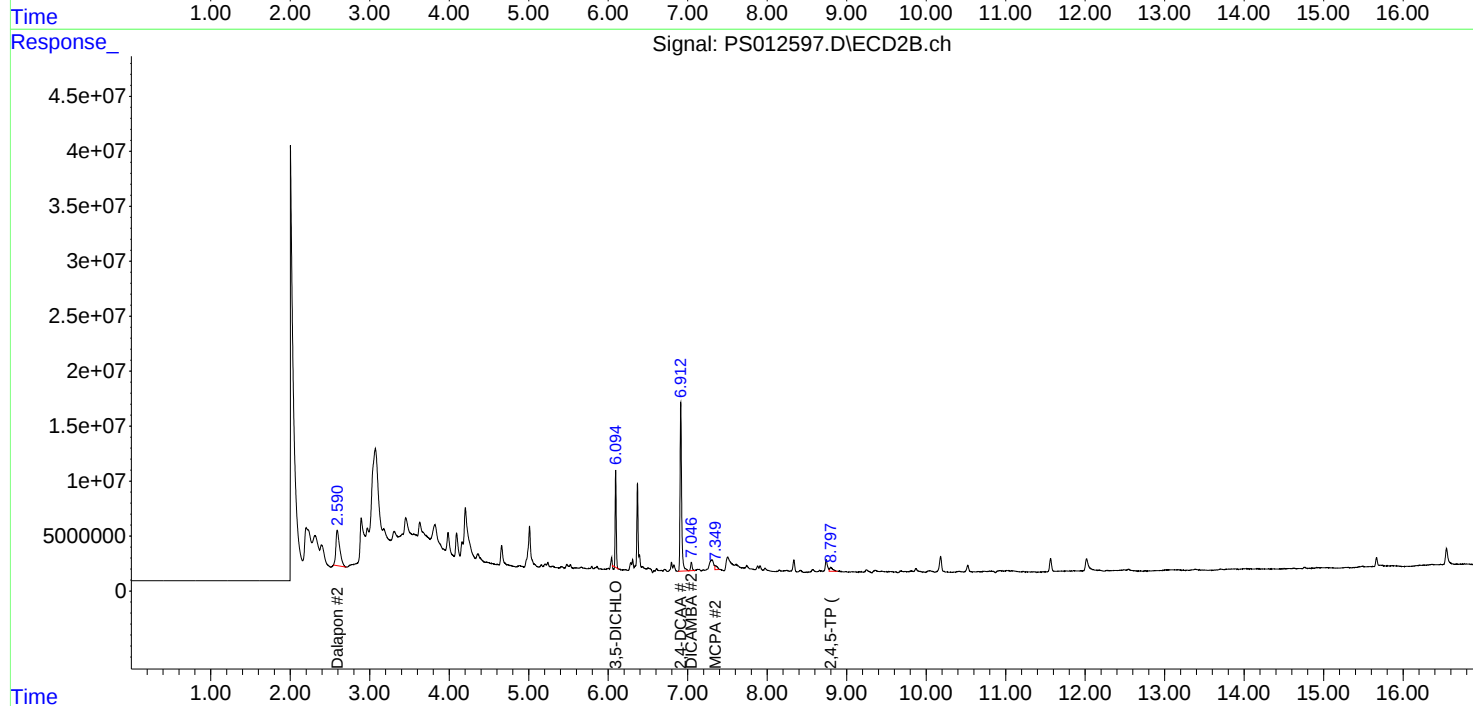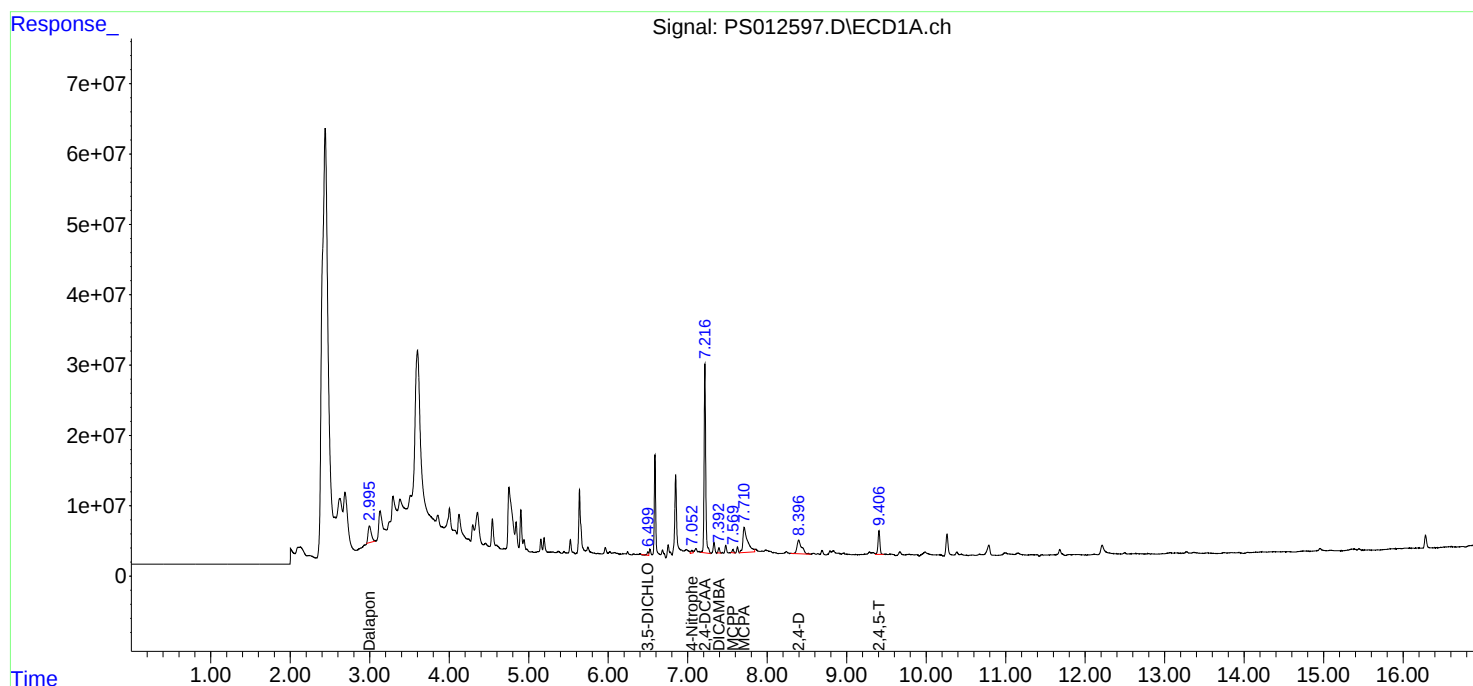


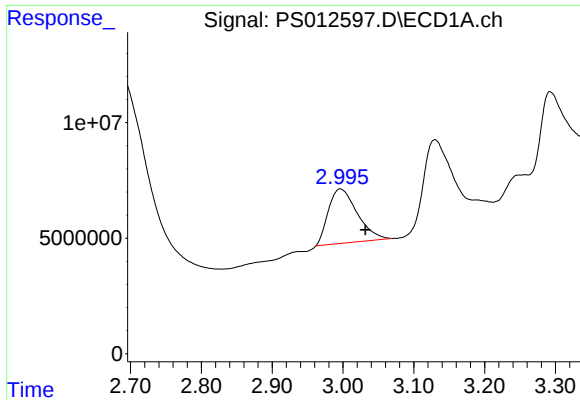

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.036 min
Response: 66496935
Conc: 58.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

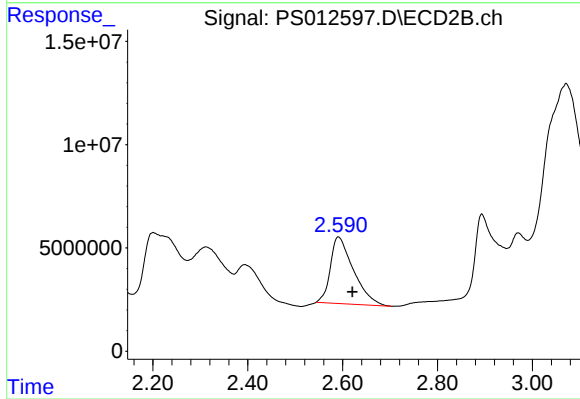


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.030 min
Response: 108858119
Conc: 181.98 ng/ml

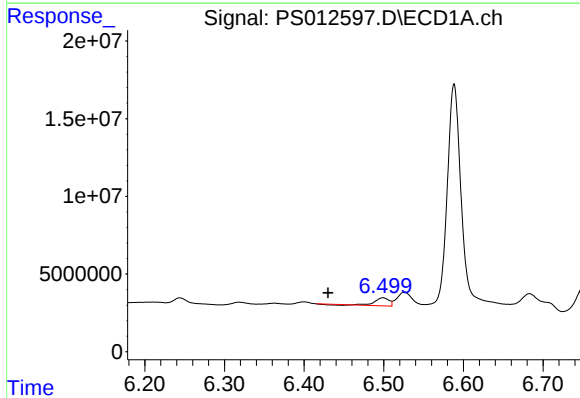


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.499 min
Delta R.T.: 0.069 min
Response: 6280804
Conc: 4.66 ng/ml

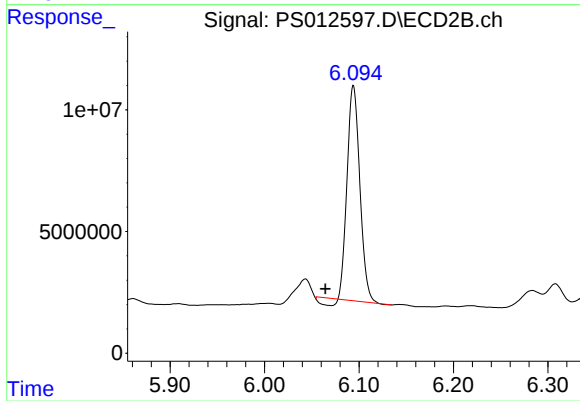

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.094 min
Delta R.T.: 0.030 min
Response: 82024748
Conc: 115.05 ng/ml

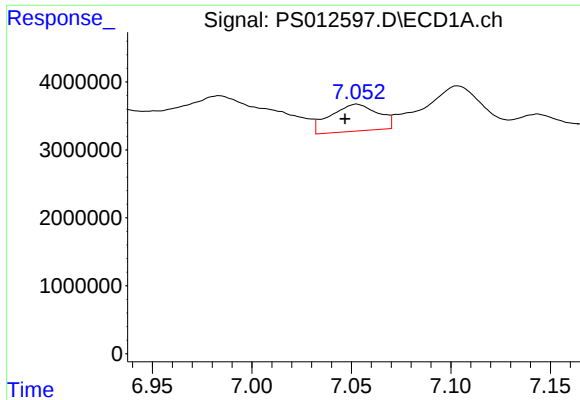

#3 4-Nitrophenol


R.T.: 7.053 min
Delta R.T.: 0.006 min
Response: 6617362
Conc: 13.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

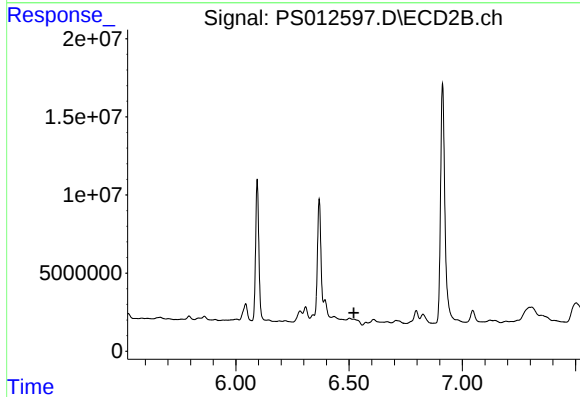


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.522 min
Response: 0
Conc: N.D.

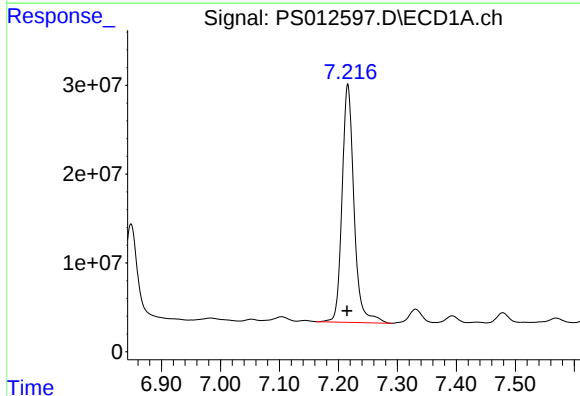


#4 2,4-DCAA

R.T.: 7.216 min
Delta R.T.: 0.002 min
Response: 377027413
Conc: 384.94 ng/ml

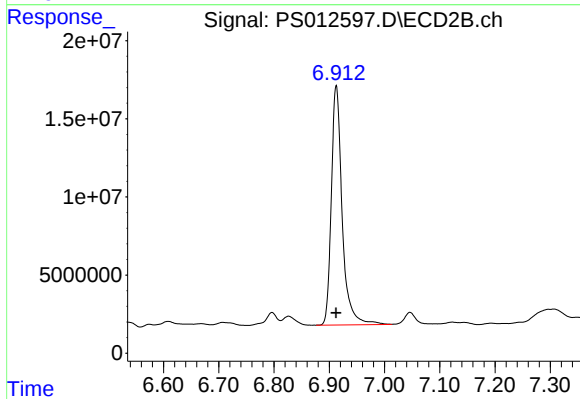

#4 2,4-DCAA


R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 208678557
Conc: 453.63 ng/ml

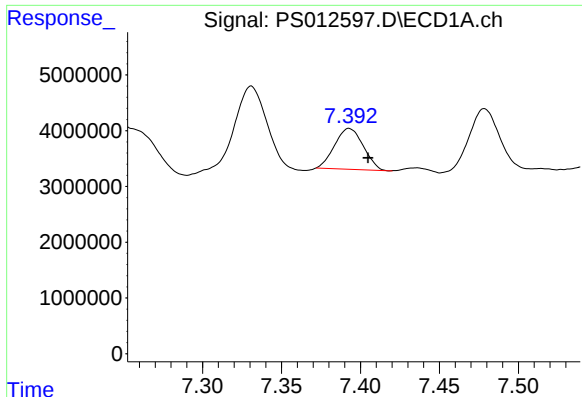

#5 DICAMBA


R.T.: 7.393 min
Delta R.T.: -0.012 min
Response: 9223758
Conc: 2.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

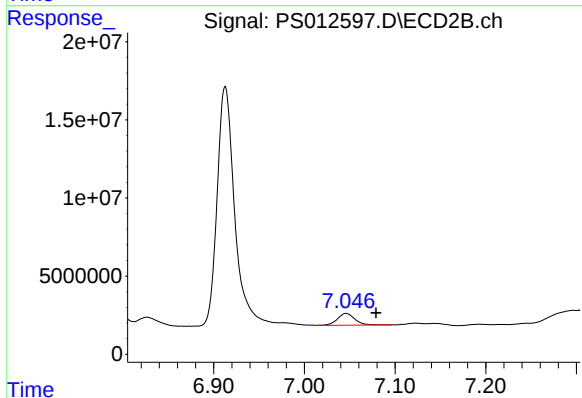


#5 DICAMBA

R.T.: 7.046 min
Delta R.T.: -0.033 min
Response: 10126775
Conc: 5.31 ng/ml

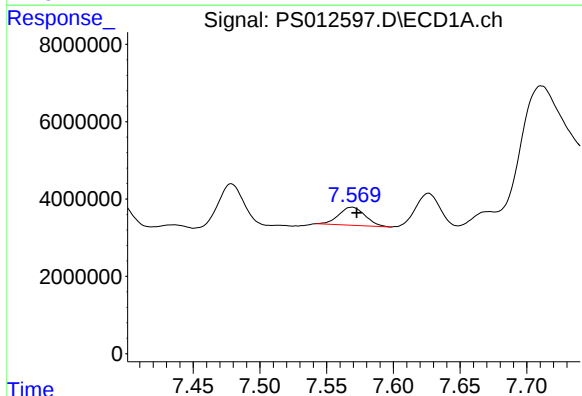


#6 MCP

R.T.: 7.569 min
Delta R.T.: -0.004 min
Response: 6396768
Conc: 2.19 ug/ml

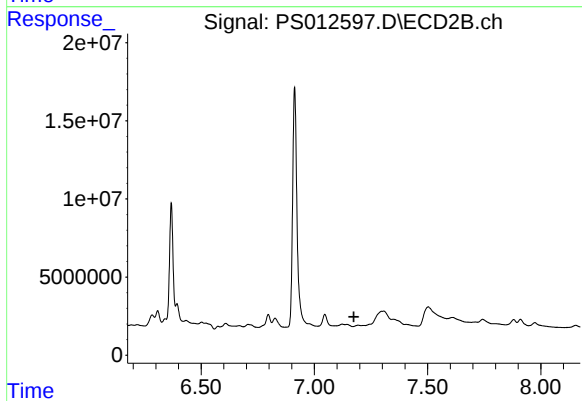

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.175 min
Response: 0
Conc: N.D.

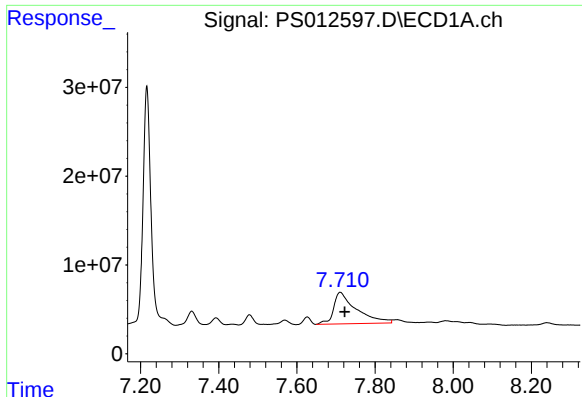

#7 MCPA


R.T.: 7.711 min
Delta R.T.: -0.011 min
Response: 144588063
Conc: 34.67 ug/ml

Instrument :
ECD_S
ClientSampleId :

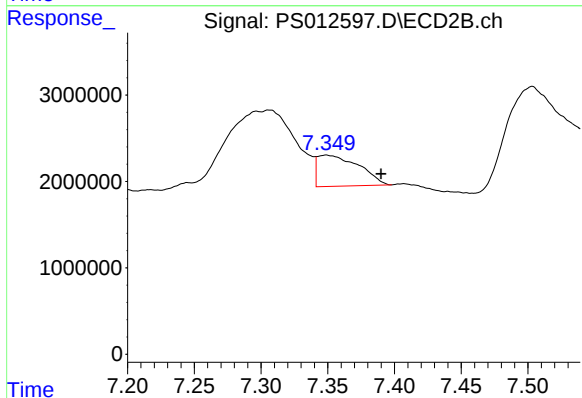


#7 MCPA

R.T.: 7.349 min
Delta R.T.: -0.041 min
Response: 7715948
Conc: 3.22 ug/ml

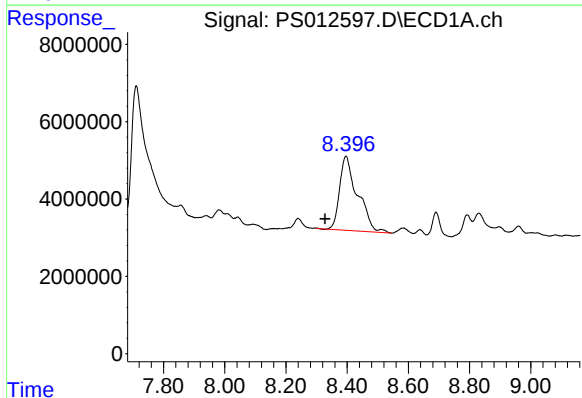


#9 2,4-D

R.T.: 8.396 min
Delta R.T.: 0.068 min
Response: 77975783
Conc: 68.68 ng/ml

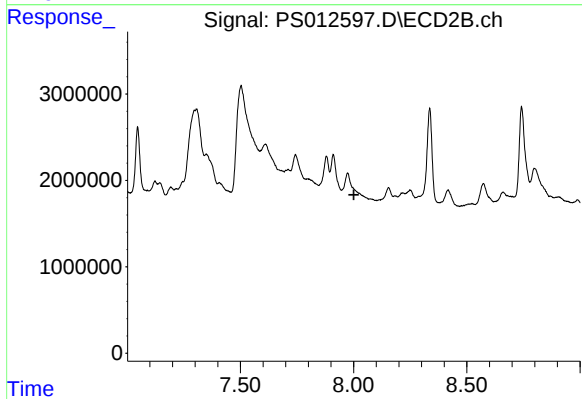

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.001 min
Response: 0
Conc: N.D.

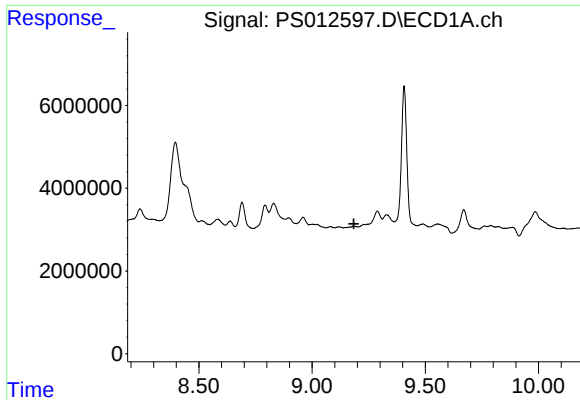

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.185 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

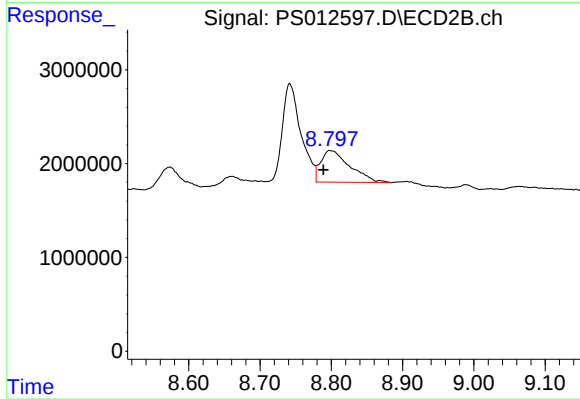


#11 2,4,5-TP (SILVEX)

R.T.: 8.798 min
Delta R.T.: 0.009 min
Response: 9609598
Conc: 3.64 ng/ml

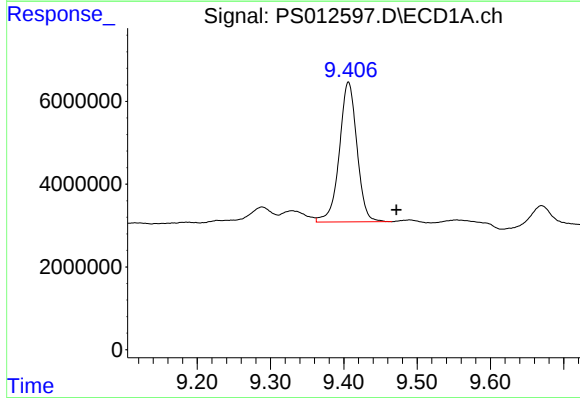

#12 2,4,5-T

R.T.: 9.406 min
Delta R.T.: -0.065 min
Response: 56352365
Conc: 10.02 ng/ml

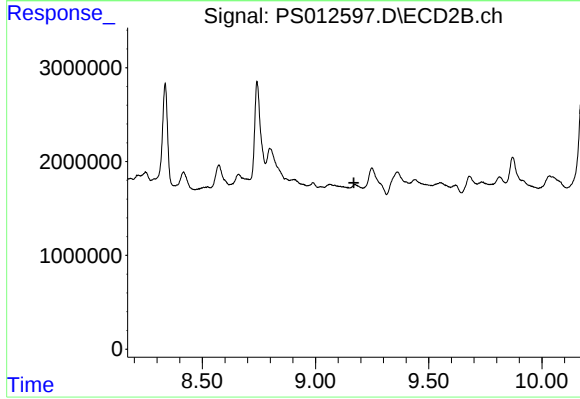

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.169 min
Response: 0
Conc: N.D.