

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100220\
 Data File : PS012608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2020 00:59
 Operator : DD\AJ
 Sample : L4198-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 05:43:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.913	261.1E6	142.6E6	266.556	310.087
Target Compounds							
1) T	Dalapon	2.995	2.591	68920001	178.9E6	60.649	299.126 #
2) T	3,5-DICHL...	0.000	6.094	0	85677586	N.D.	120.172
3) T	4-Nitroph...	7.051	0.000	4859344	0	9.993	N.D. #
5) T	DICAMBA	7.392	7.046	9293619	9544718	2.409	5.005 #
6) T	MCPD	7.626	0.000	8998001	0	3.084	N.D. #
7) T	MCPA	7.715	0.000	137.7E6	0	33.015	N.D. #
8) T	DICHLORPROP	0.000	7.741	0	9123668	N.D.	17.670
9) T	2,4-D	8.393	7.973	60051421	5911586	52.889	9.440 #
10) T	Pentachlo...	8.690	0.000	12671054	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.742	0	28598074	N.D.	10.839
12) T	2,4,5-T	9.405	0.000	46649646	0	8.299	N.D. #
14) T	DINOSEB	0.000	10.050	0	14572802	N.D.	7.608
15) T	Picloram	10.982	0.000	51012268	0	7.085	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100220\
Data File : PS012608.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2020 00:59
Operator : DD\AJ
Sample : L4198-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 05:43:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

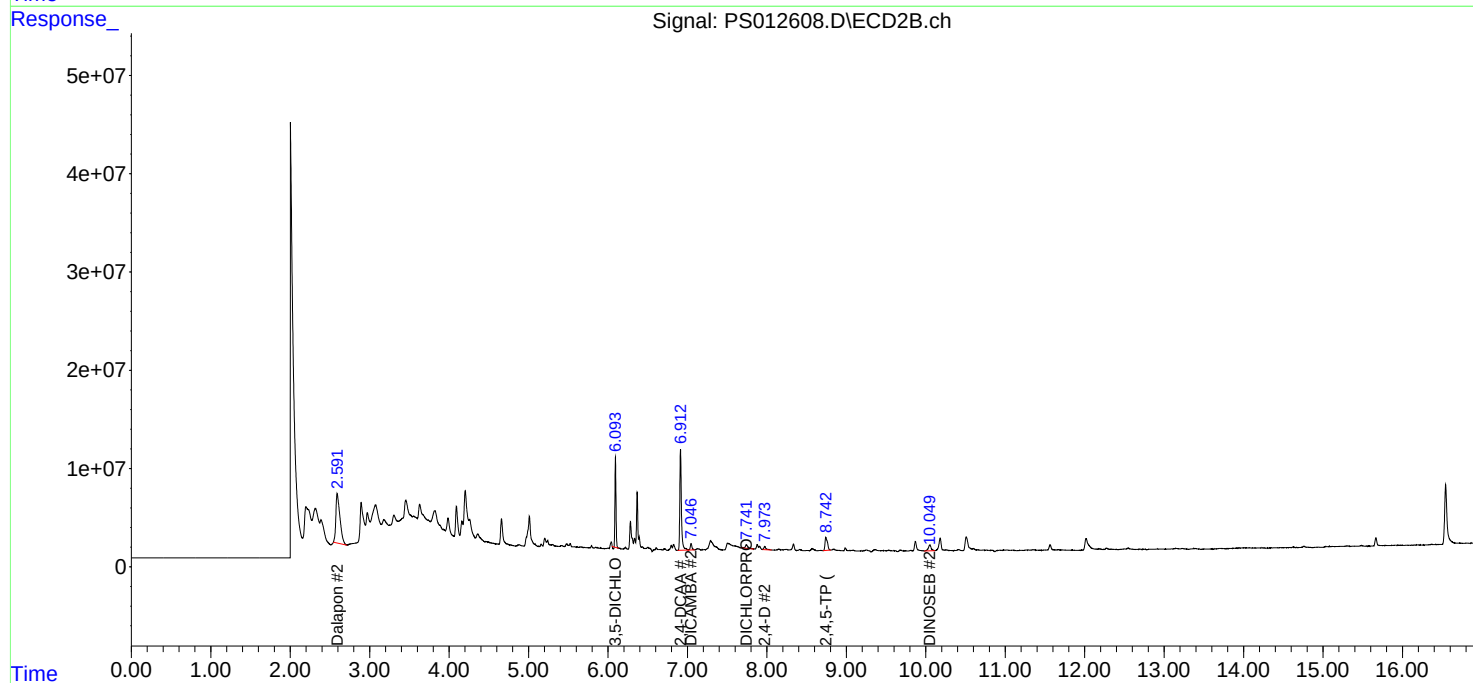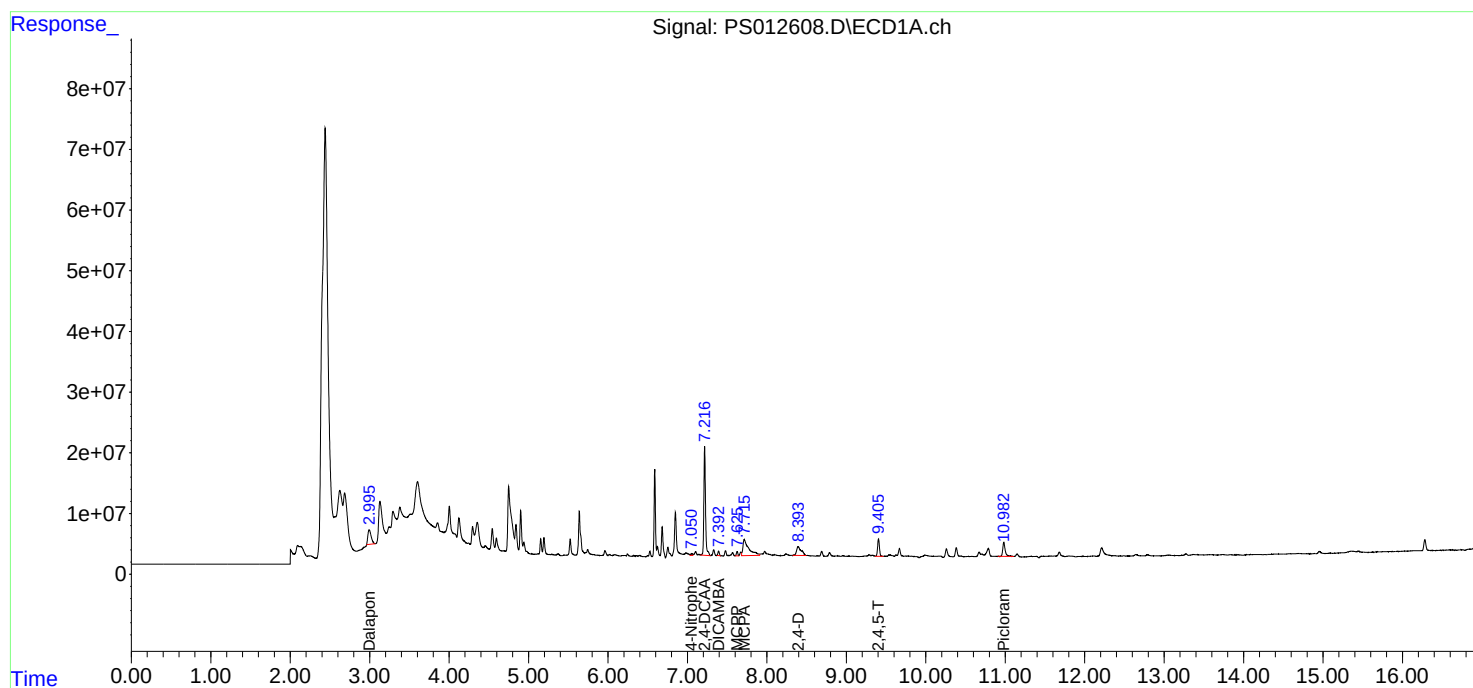


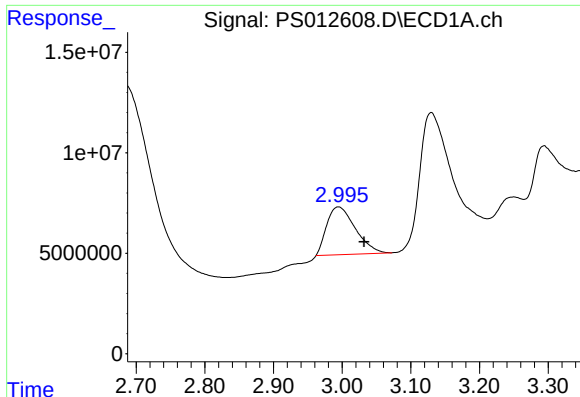

#1 Dalapon


R.T.: 2.995 min
Delta R.T.: -0.037 min
Response: 68920001
Conc: 60.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

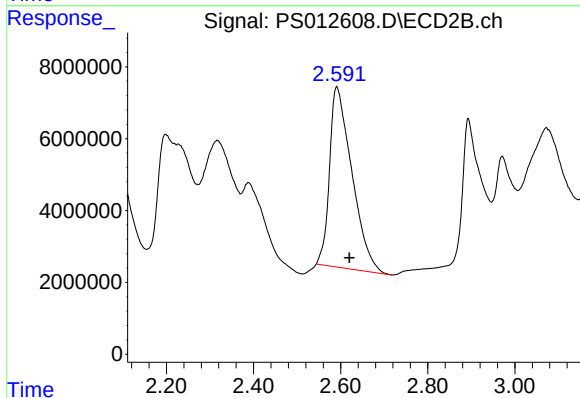


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.029 min
Response: 178934237
Conc: 299.13 ng/ml

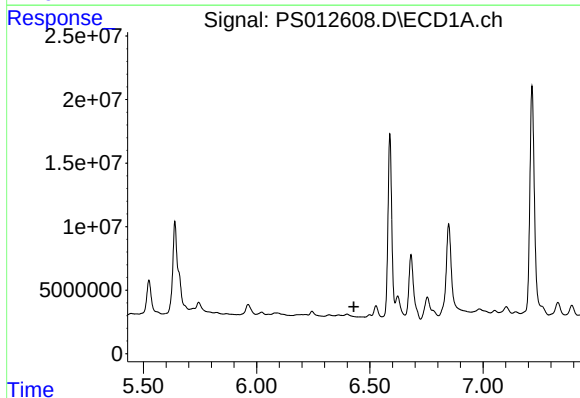


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.430 min
Response: 0
Conc: N.D.

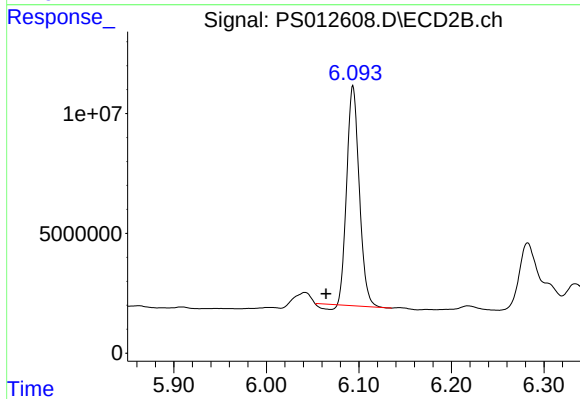

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 85677586
Conc: 120.17 ng/ml

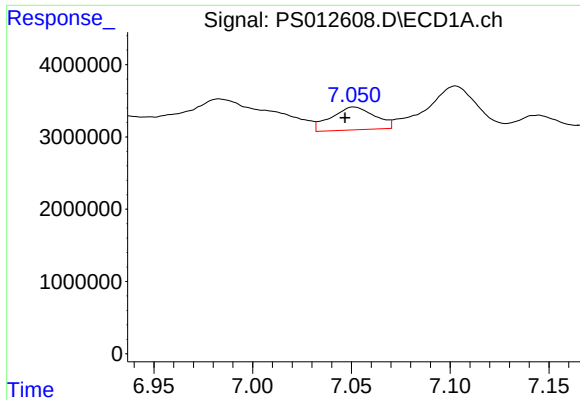

#3 4-Nitrophenol


R.T.: 7.051 min
Delta R.T.: 0.005 min
Response: 4859344
Conc: 9.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

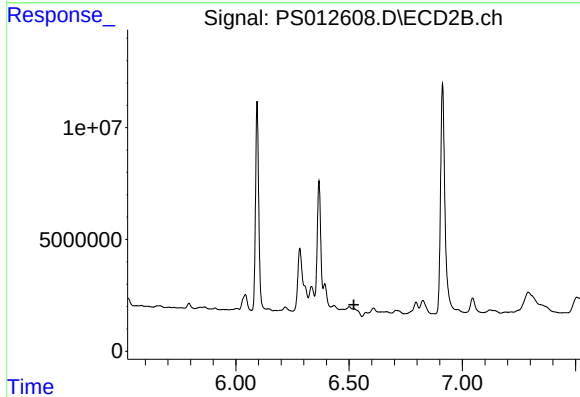


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.522 min
Response: 0
Conc: N.D.

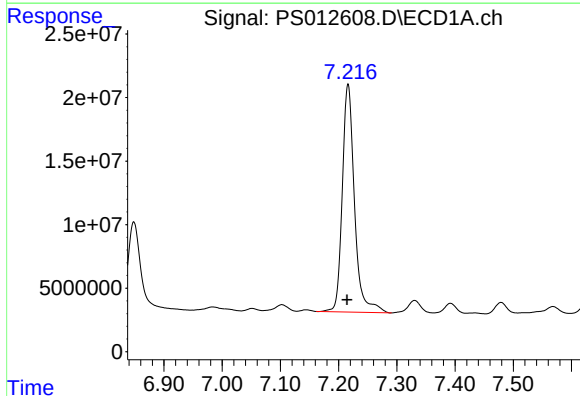


#4 2,4-DCAA

R.T.: 7.216 min
Delta R.T.: 0.002 min
Response: 261077641
Conc: 266.56 ng/ml

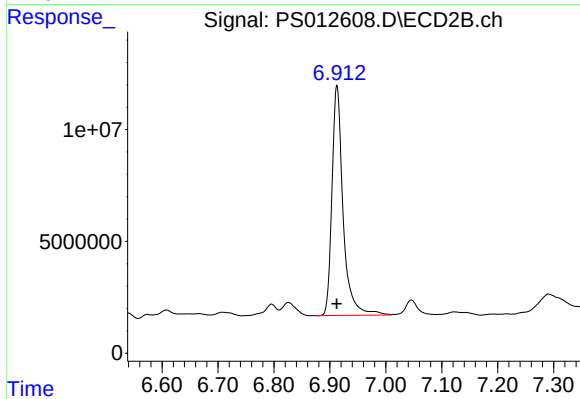

#4 2,4-DCAA


R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 142645288
Conc: 310.09 ng/ml

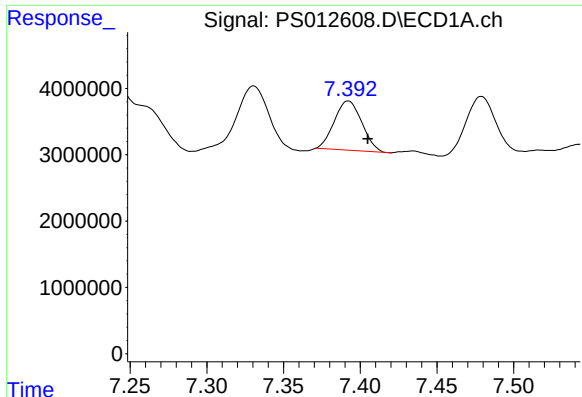

#5 DICAMBA


R.T.: 7.392 min
Delta R.T.: -0.013 min
Response: 9293619
Conc: 2.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

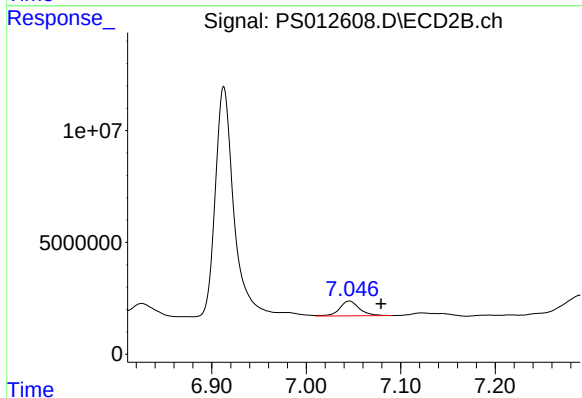


#5 DICAMBA

R.T.: 7.046 min
Delta R.T.: -0.033 min
Response: 9544718
Conc: 5.01 ng/ml

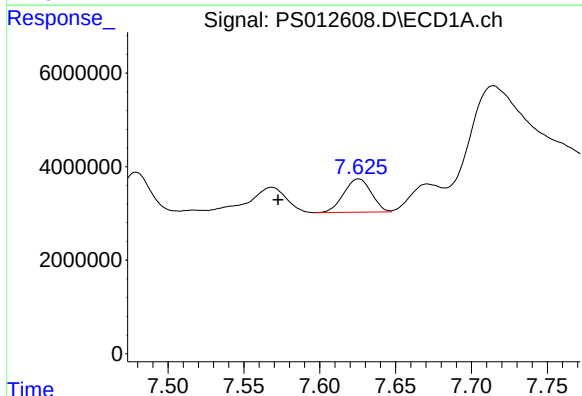


#6 MCP

R.T.: 7.626 min
Delta R.T.: 0.053 min
Response: 8998001
Conc: 3.08 ug/ml

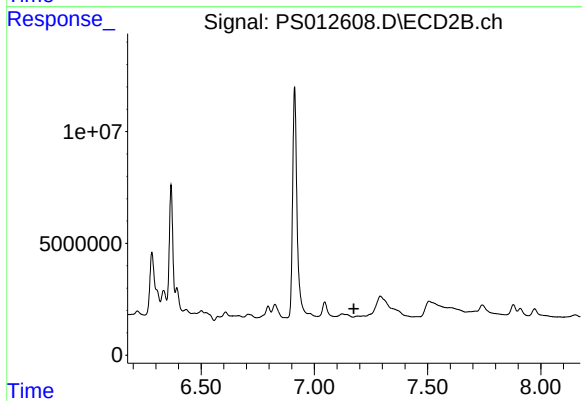

#6 MCP


R.T.: 0.000 min
Exp R.T. : 7.175 min
Response: 0
Conc: N.D.

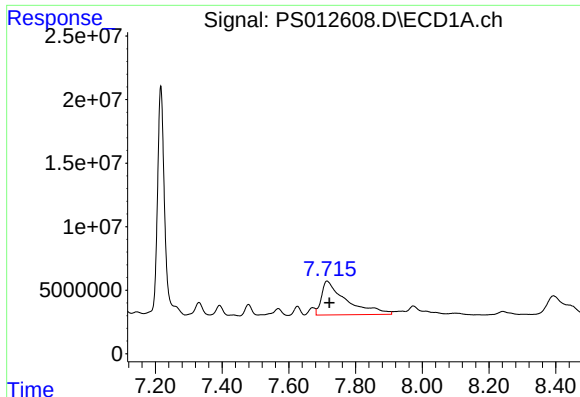

#7 MCPA


R.T.: 7.715 min
Delta R.T.: -0.007 min
Response: 137696777
Conc: 33.02 ug/ml

Instrument :
ECD_S
ClientSampleId :

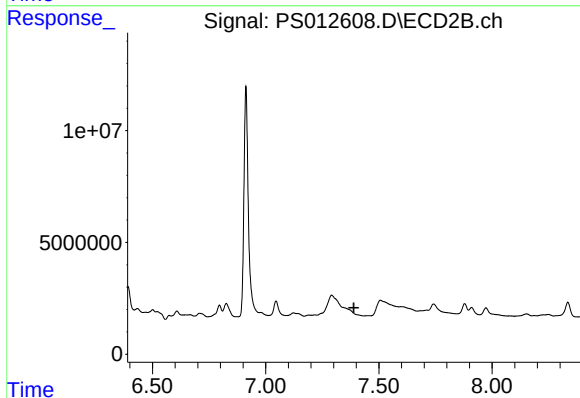


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.390 min
Response: 0
Conc: N.D.

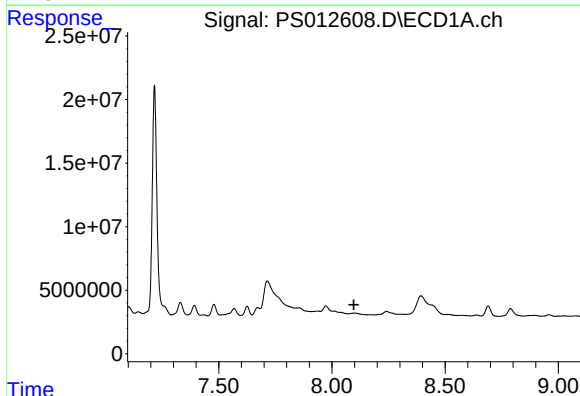


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.097 min
Response: 0
Conc: N.D.

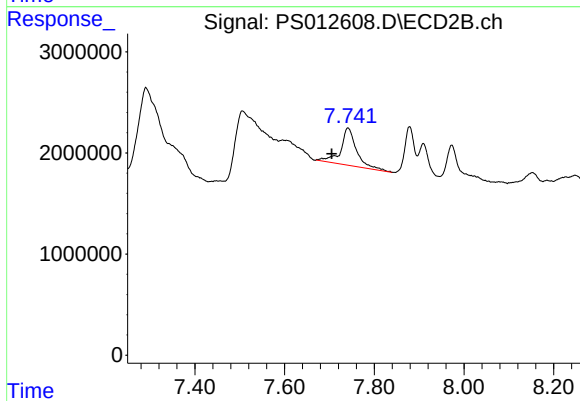

#8 DICHLORPROP


R.T.: 7.741 min
Delta R.T.: 0.036 min
Response: 9123668
Conc: 17.67 ng/ml

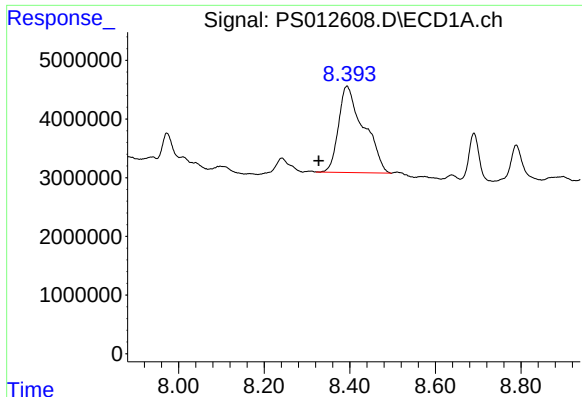

#9 2,4-D


R.T.: 8.393 min
Delta R.T.: 0.065 min
Response: 60051421
Conc: 52.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

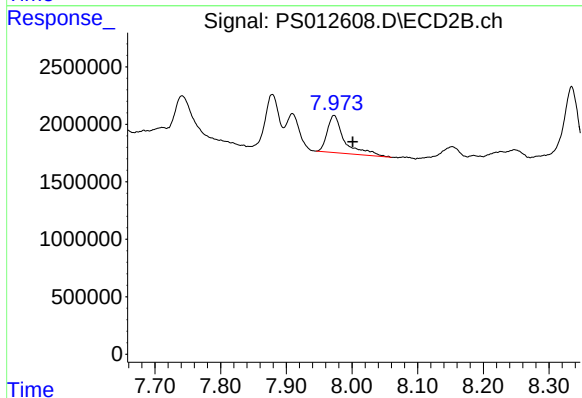


#9 2,4-D

R.T.: 7.973 min
Delta R.T.: -0.028 min
Response: 5911586
Conc: 9.44 ng/ml

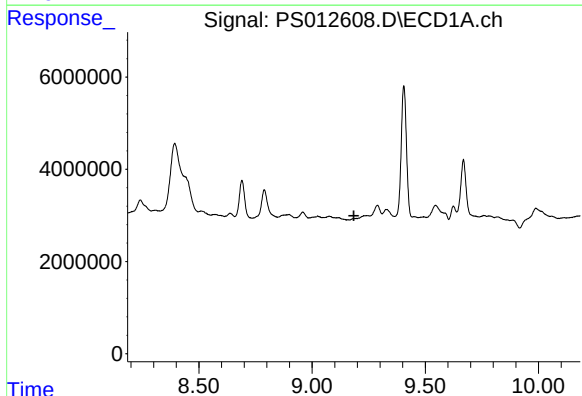


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.185 min
Response: 0
Conc: N.D.

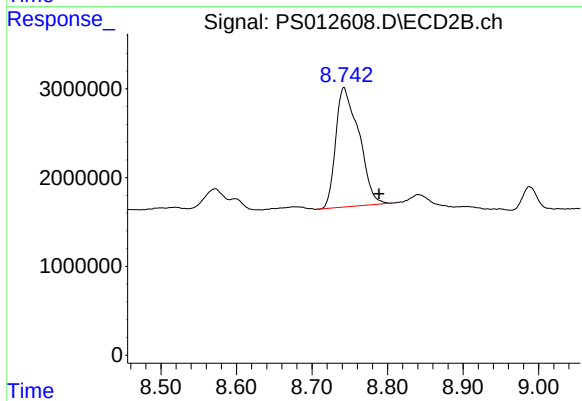

#11 2,4,5-TP (SILVEX)


R.T.: 8.742 min
Delta R.T.: -0.047 min
Response: 28598074
Conc: 10.84 ng/ml

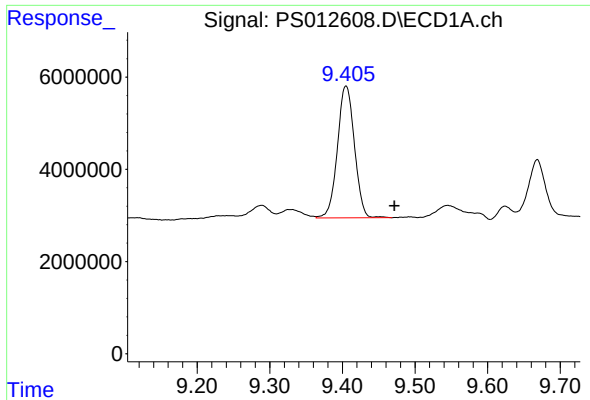

#12 2,4,5-T


R.T.: 9.405 min
Delta R.T.: -0.067 min
Response: 46649646
Conc: 8.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

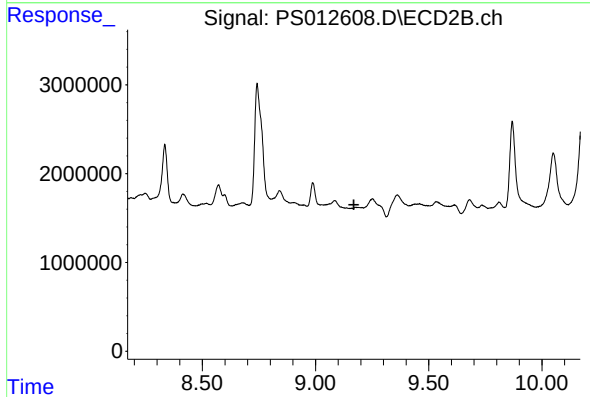


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.169 min
Response: 0
Conc: N.D.

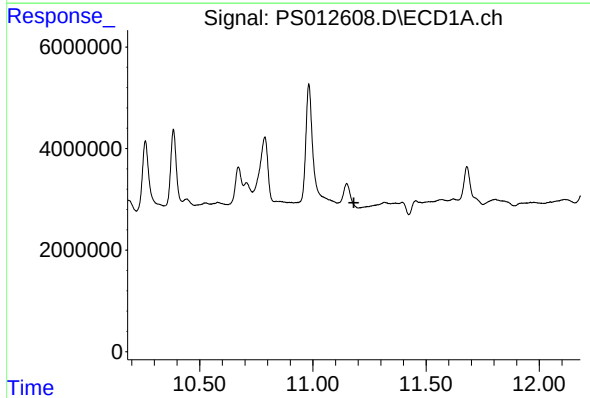


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.181 min
Response: 0
Conc: N.D.

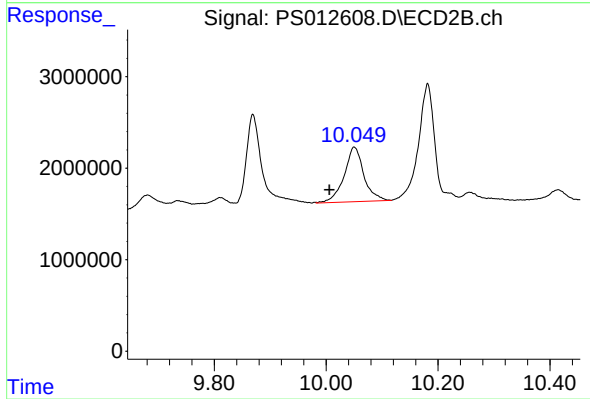

#14 DINOSEB


R.T.: 10.050 min
Delta R.T.: 0.044 min
Response: 14572802
Conc: 7.61 ng/ml

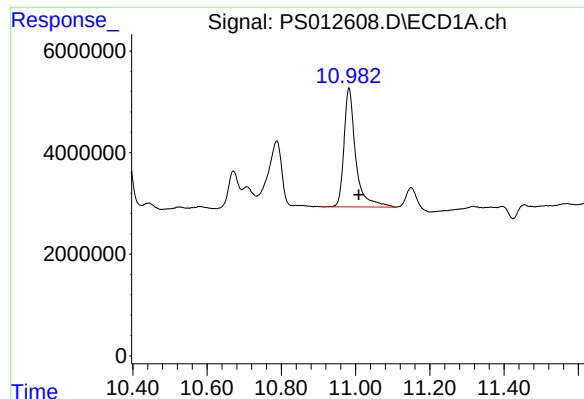

#15 Picloram

R.T.: 10.982 min
Delta R.T.: -0.026 min
Response: 51012268
Conc: 7.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

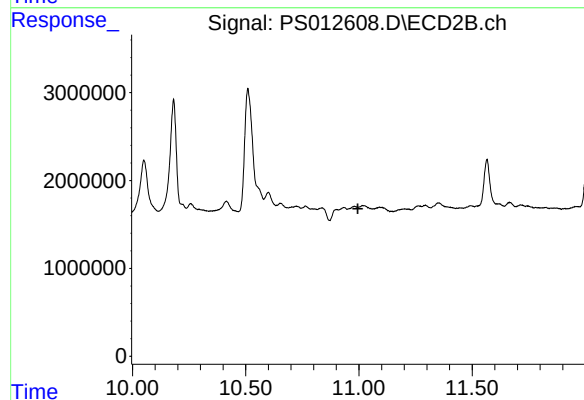

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.