

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100220\
 Data File : PS012612.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2020 02:31
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 05:44:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.217	6.914	434.2E6	241.3E6	443.360	524.505
Target Compounds							
7) T	MCPA	0.000	7.347	0	9639814	N.D.	4.021
9) T	2,4-D	8.395	0.000	70753083	0	62.314	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100220\
Data File : PS012612.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2020 02:31
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 05:44:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

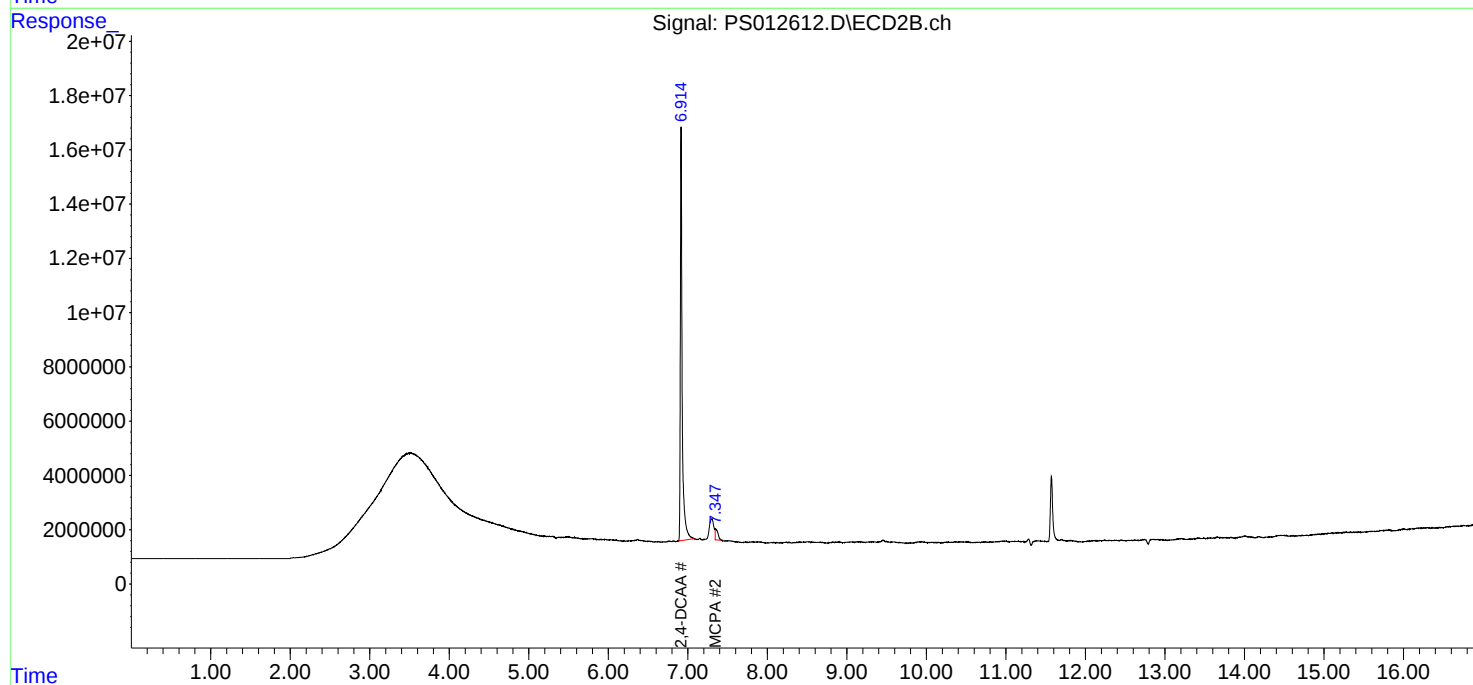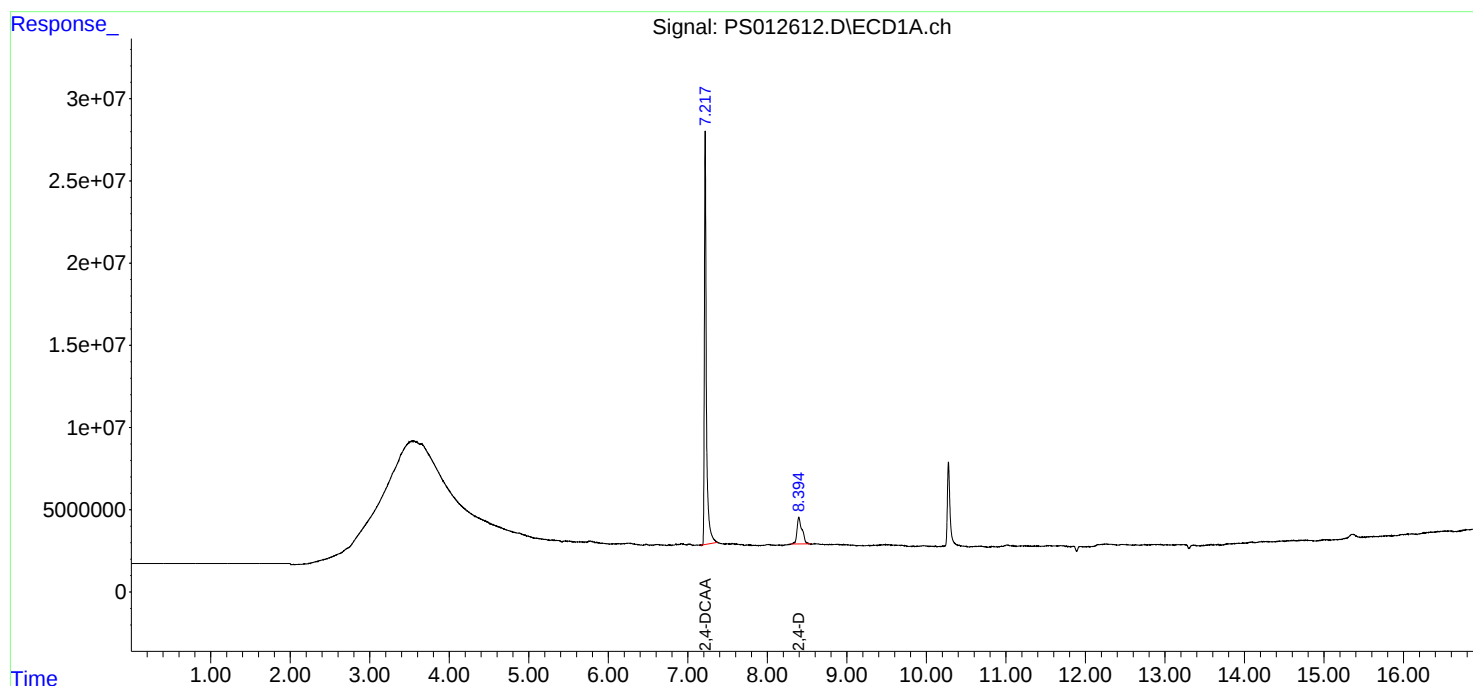


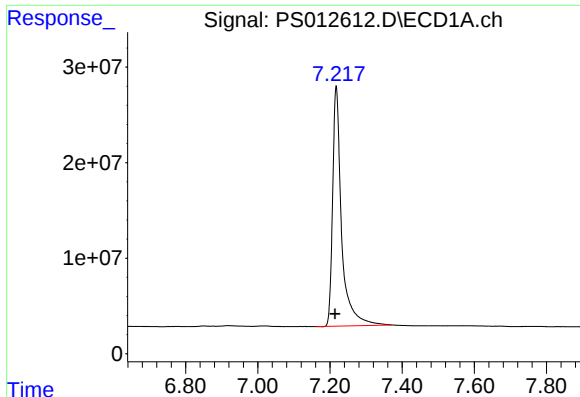

#4 2,4-DCAA


R.T.: 7.217 min
Delta R.T.: 0.003 min
Response: 434248356
Conc: 443.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

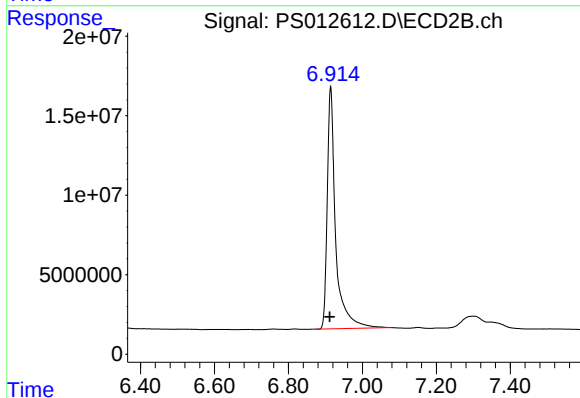


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.002 min
Response: 241281111
Conc: 524.51 ng/ml

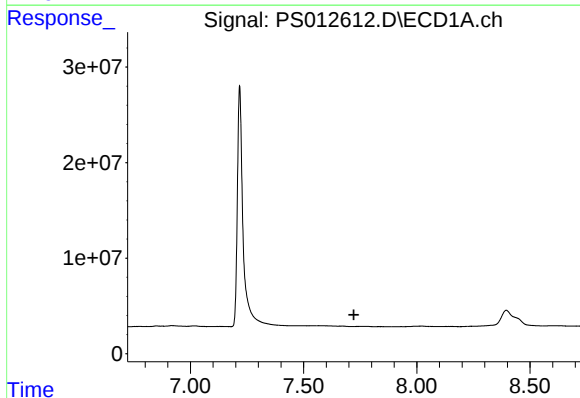


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.722 min
Response: 0
Conc: N.D.

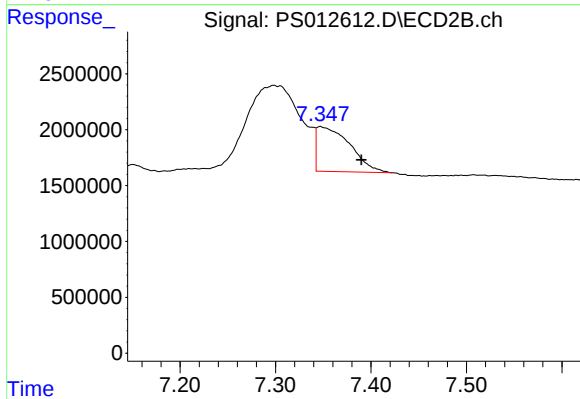

#7 MCPA


R.T.: 7.347 min
Delta R.T.: -0.043 min
Response: 9639814
Conc: 4.02 ug/ml

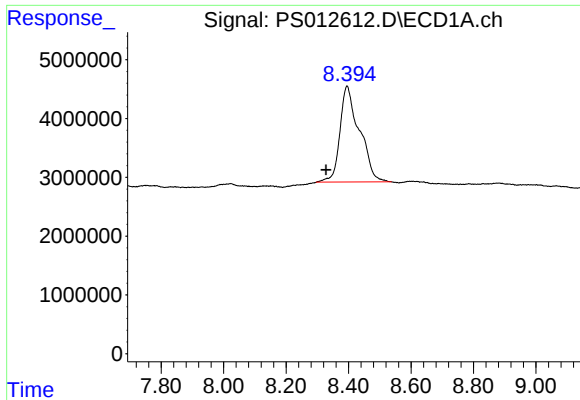

#9 2,4-D

R.T.: 8.395 min
Delta R.T.: 0.067 min
Response: 70753083
Conc: 62.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

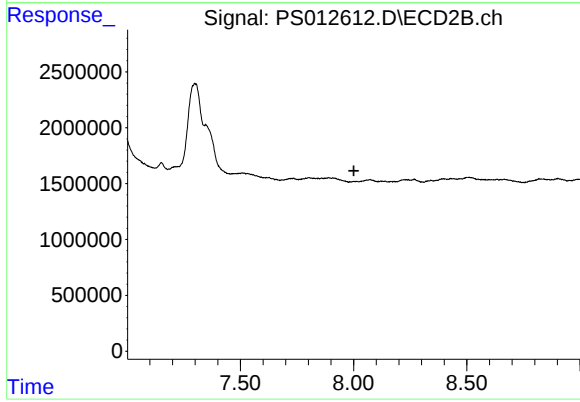

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.001 min
Response: 0
Conc: N.D.