

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100318\
 Data File : PS001892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2018 20:40
 Operator : EI\SJ
 Sample : J5211-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CB-1018-S-TCLP-GRID50-1

Manual Integrations
 APPROVED

Sohil
 10/4/2018 5:10:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:56:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	11.497	10.993	81420682	80510835	362.974m	316.951m
------	----------	--------	--------	----------	----------	----------	----------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100318\
Data File : PS001892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2018 20:40
Operator : EI\SJ
Sample : J5211-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
CB-1018-S-TCLP-GRID50-1


Manual Integrations
APPROVED

Sohil
10/4/2018 5:10:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:56:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

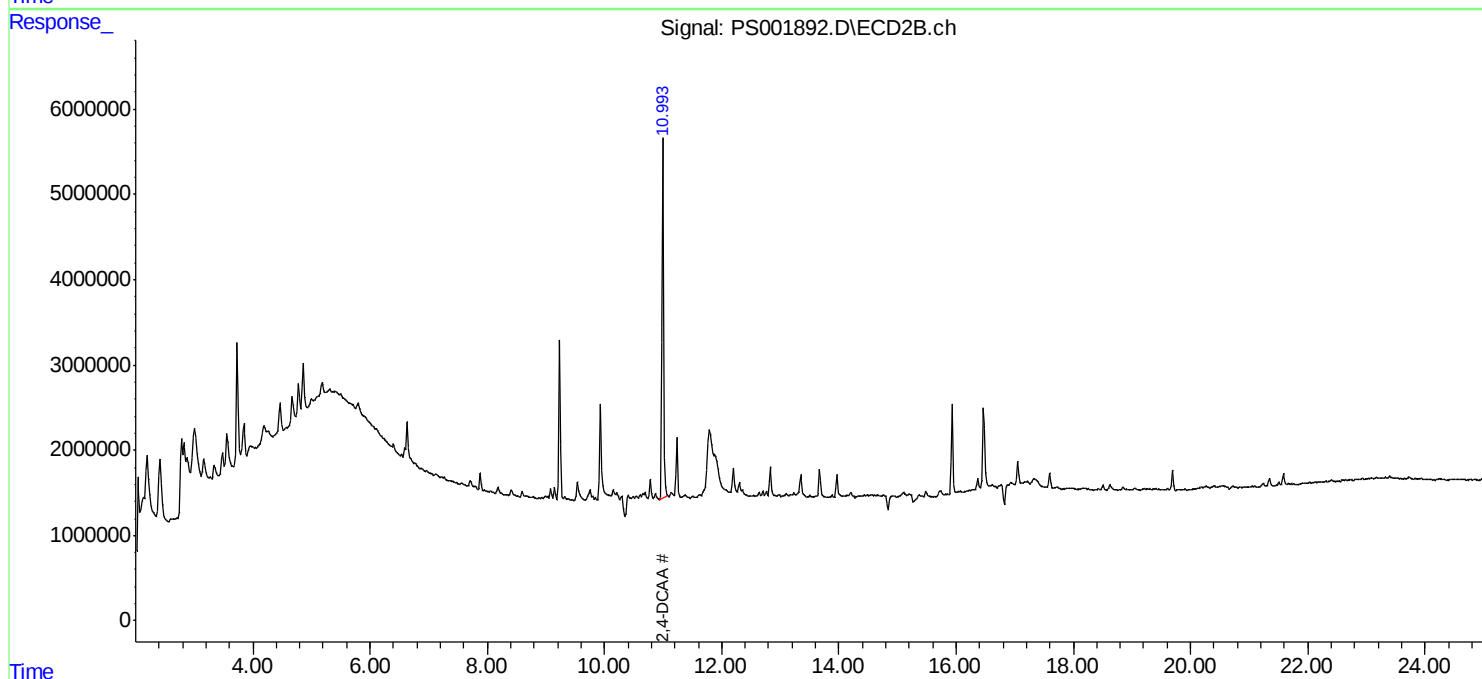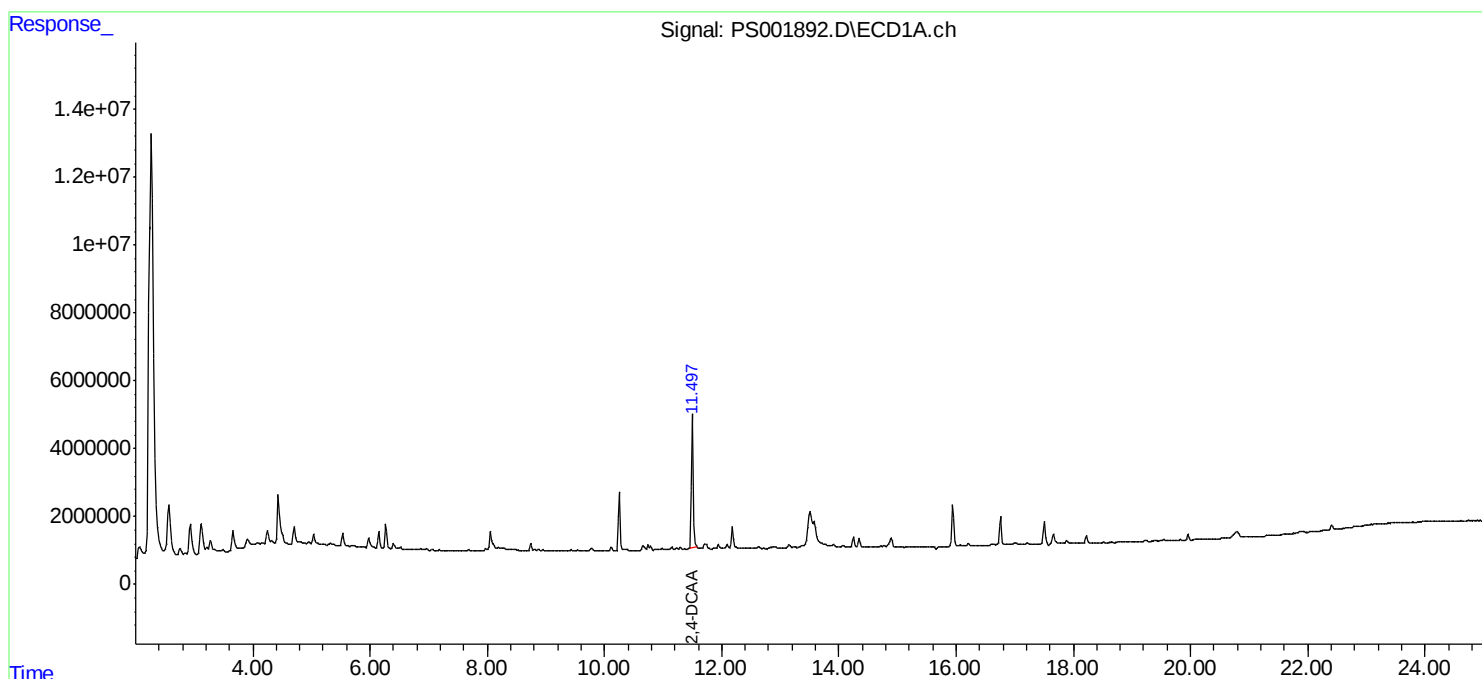

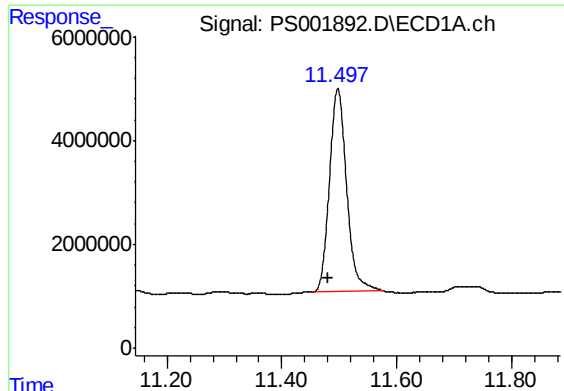


#4 2,4-DCAA

R.T.: 11.497 min
Delta R.T.: 0.017 min
Response: 81420682
Conc: 362.97 ng/ml m

Instrument :
ECD_S
ClientSampleId :
CB-1018-S-TCLP-GRID50-1

Manual Integrations
APPROVED

Sohil
10/4/2018 5:10:59 PM

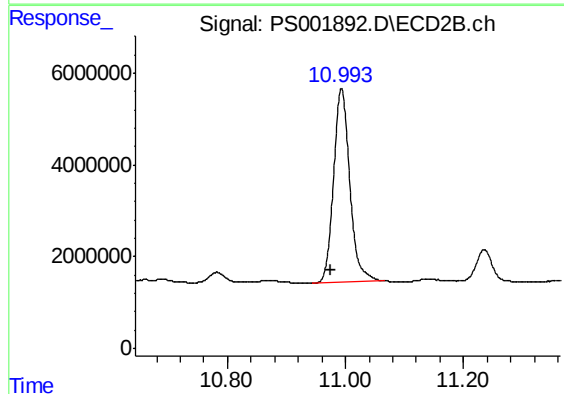

#4 2,4-DCAA

R.T.: 10.993 min
Delta R.T.: 0.017 min
Response: 80510835
Conc: 316.95 ng/ml m