

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100322\
 Data File : PS020707.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 09:46
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 22:39:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
1) T	Dalapon	3.039	0.000	879757	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.456f	0.000	316125	0	<MDL	N.D. #
3) T	4-Nitroph...	6.993	0.000	1876036	0	128.078	N.D. #
6) T	MCP	7.561	0.000	2129558	0	<MDL	N.D. #
7) T	MCPA	0.000	7.198	0	6464999	N.D.	1.497
8) T	DICHLORPROP	8.040	0.000	899231	0	<MDL	N.D. #
9) T	2,4-D	8.358f	0.000	41801545	0	8.993	N.D. #
10) T	Pentachlo...	8.610	0.000	498292	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.179	0.000	112504	0	<MDL	N.D. #
12) T	2,4,5-T	9.433	0.000	62539	0	<MDL	N.D. #
13) T	2,4-DB	9.986	0.000	187375	0	<MDL	N.D. #
14) T	DINOSEB	11.150	0.000	6618490	0	<MDL	N.D. #
15) T	Picloram	10.952	0.000	54416	0	<MDL	N.D. #
16) T	DCPA	11.401	0.000	1597199	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100322\
Data File : PS020707.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 09:46
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 22:39:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

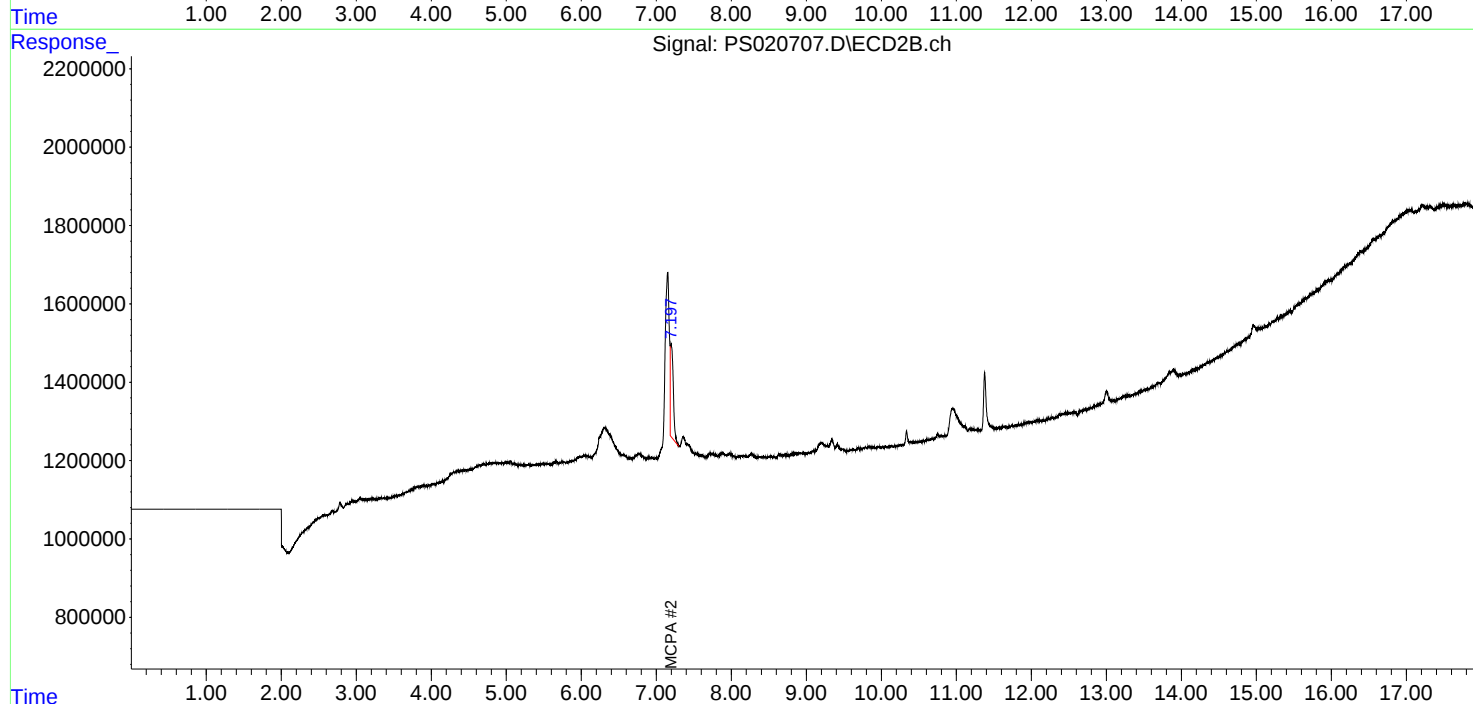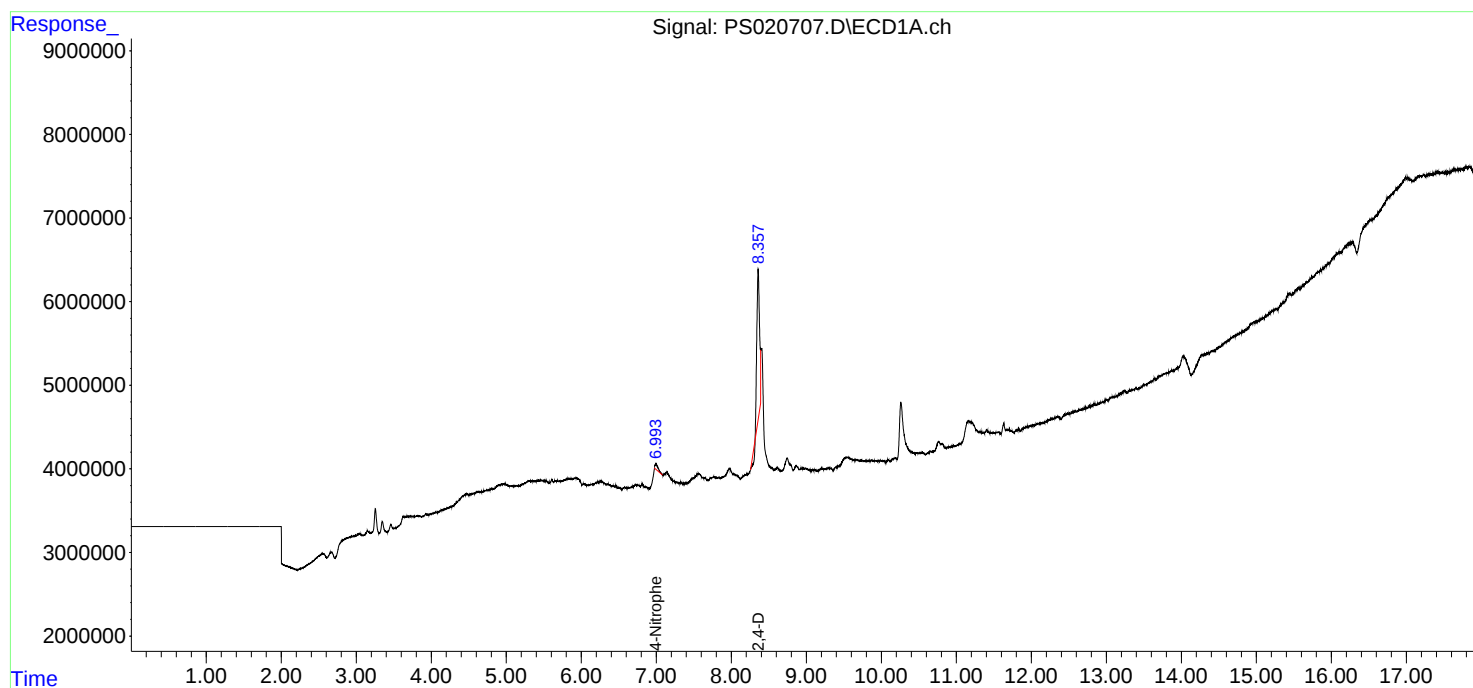


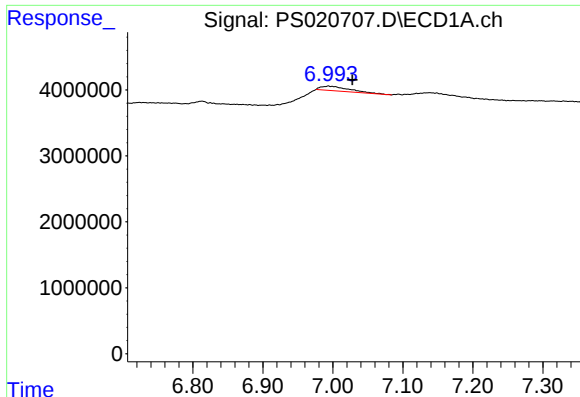

#3 4-Nitrophenol


R.T.: 6.993 min
Delta R.T.: -0.035 min
Response: 1876036
Conc: 128.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

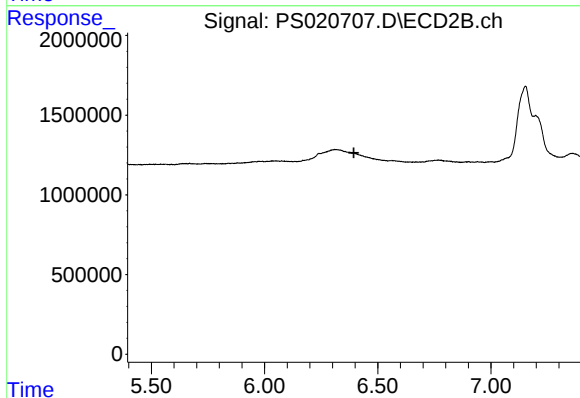


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

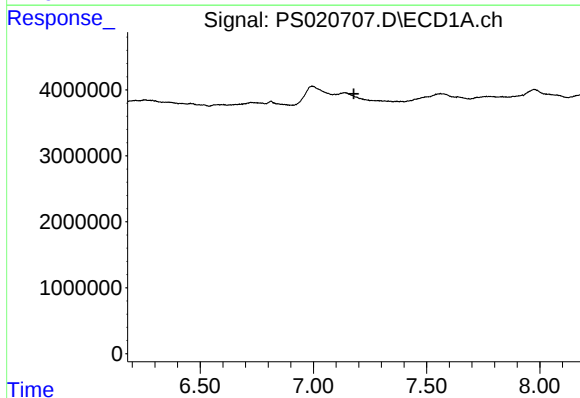


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.179 min
Response: 0
Conc: N.D.

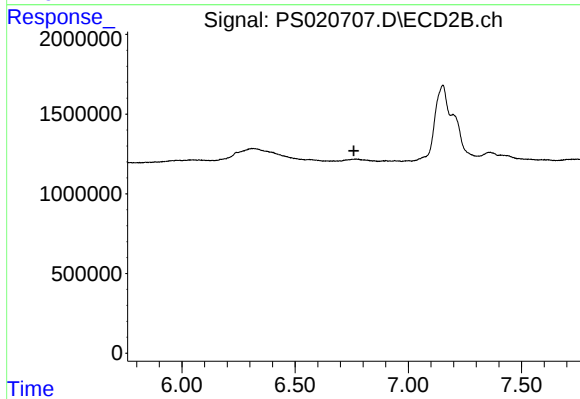

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.760 min
Response: 0
Conc: N.D.

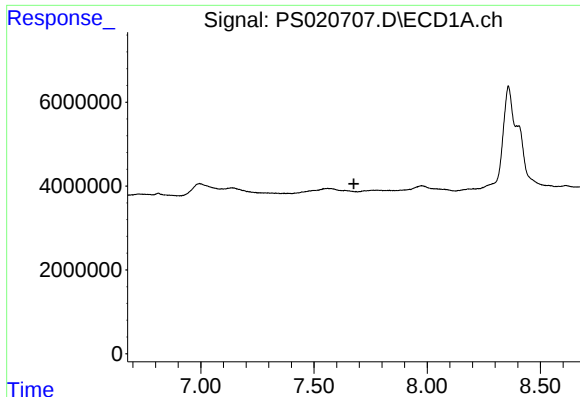

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.676 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

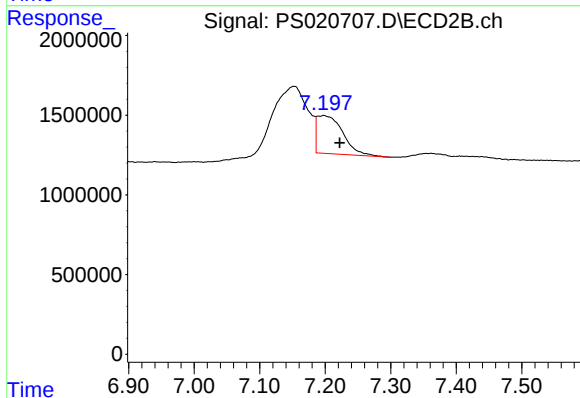


#7 MCPA

R.T.: 7.198 min
Delta R.T.: -0.024 min
Response: 6464999
Conc: 1.50 ug/ml

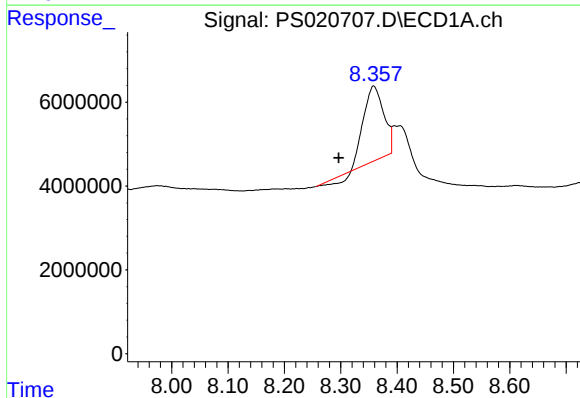

#9 2,4-D

R.T.: 8.358 min
Delta R.T.: 0.062 min
Response: 41801545
Conc: 8.99 ng/ml

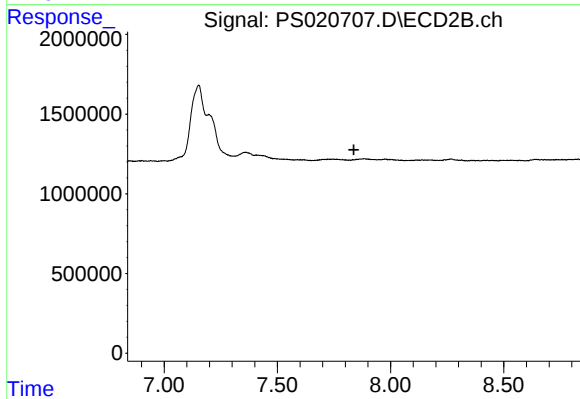

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.838 min
Response: 0
Conc: N.D.