

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100322\
 Data File : PS020718.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 16:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 22:43:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.183	6.763	1425.6E6	465.4E6	414.237	546.439 #
Target Compounds							
1) T	Dalapon	2.972	0.000	64438	0	<MDL	N.D. #
3) T	4-Nitroph...	6.993	0.000	-306053	0	126.943	N.D. #
7) T	MCPA	7.660	7.198	-1602	10909161	N.D.	2.527
9) T	2,4-D	8.354f	0.000	85308821	0	18.354	N.D. #
10) T	Pentachlo...	8.602	0.000	1129192	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.109	0.000	657771	0	<MDL	N.D. #
12) T	2,4,5-T	9.395	0.000	1095660	0	<MDL	N.D. #
13) T	2,4-DB	10.011	0.000	644637	0	<MDL	N.D. #
14) T	DINOSEB	11.130	0.000	16151837	0	<MDL	N.D. #
16) T	DCPA	11.399	0.000	2242213	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100322\
Data File : PS020718.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 16:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 22:43:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

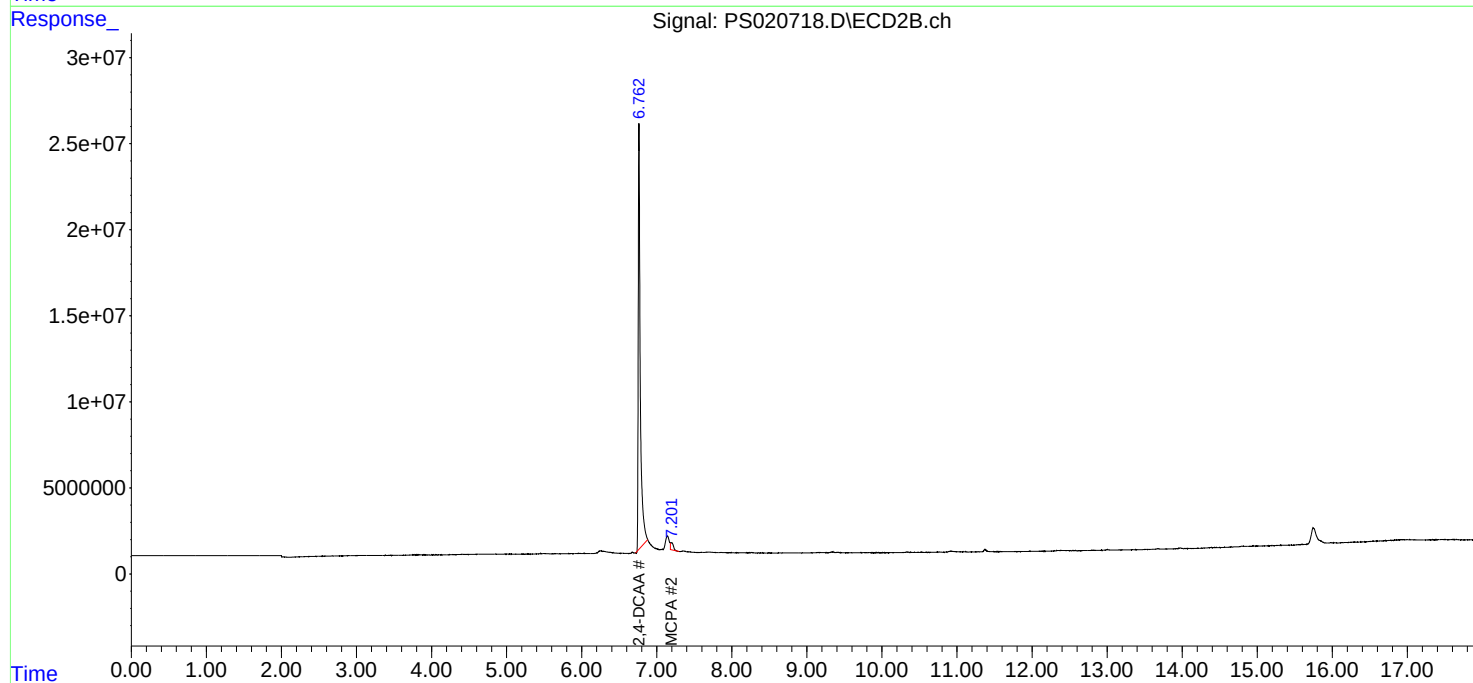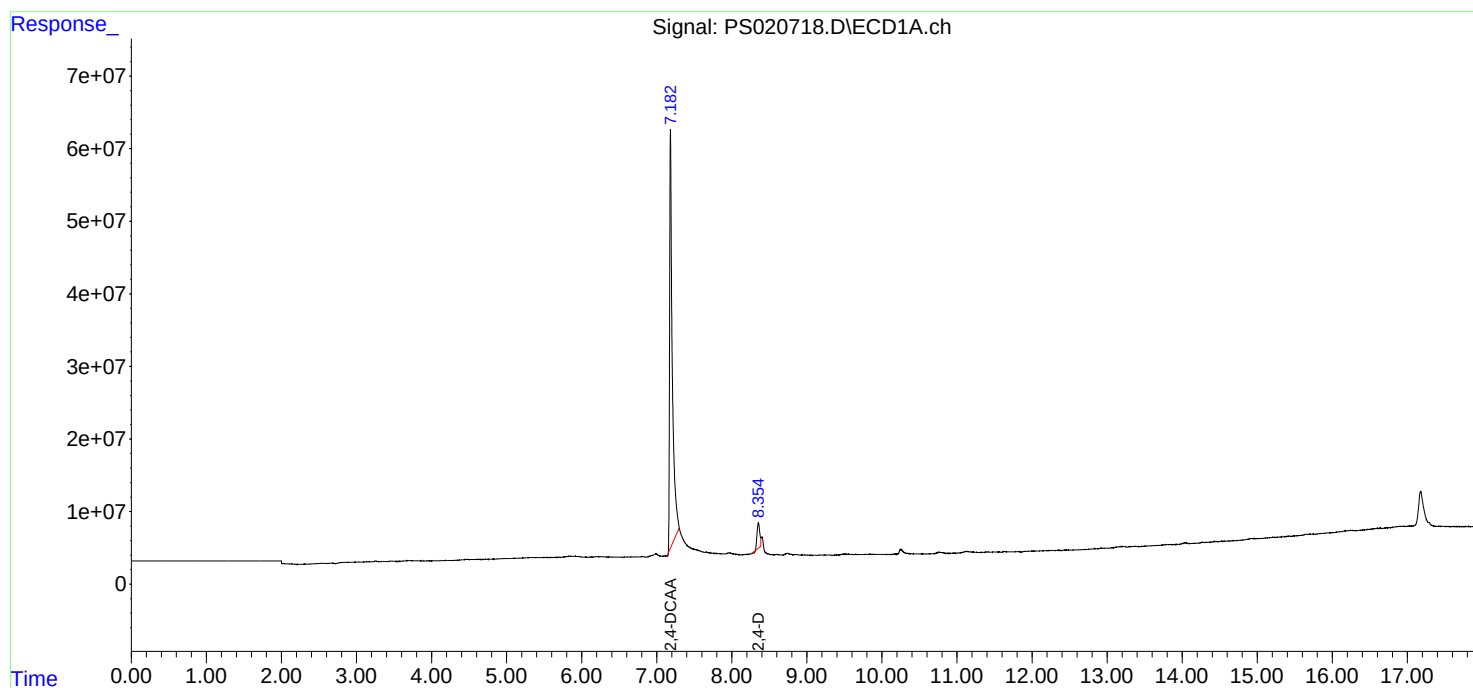


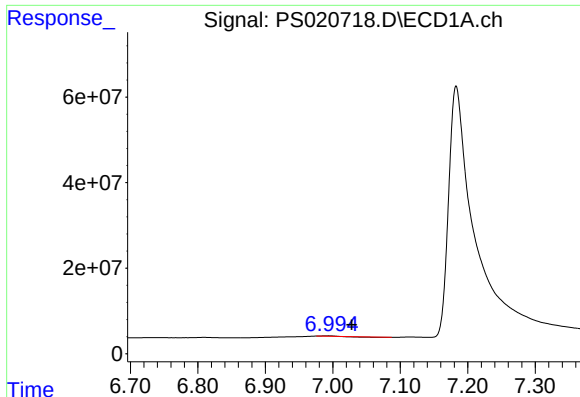

#3 4-Nitrophenol


R.T.: 6.993 min
Delta R.T.: -0.035 min
Response: -306053
Conc: 126.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

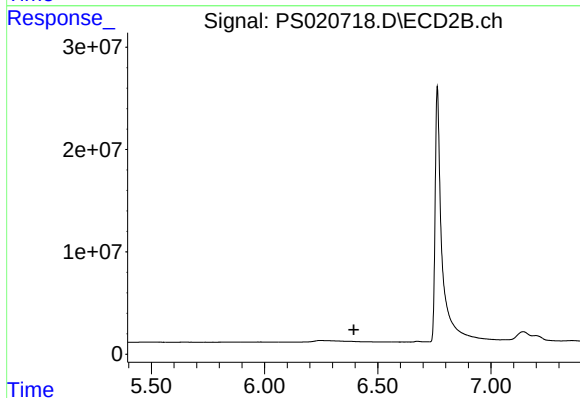


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

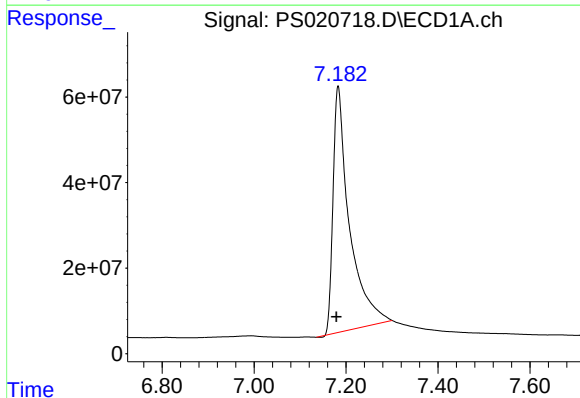


#4 2,4-DCAA

R.T.: 7.183 min
Delta R.T.: 0.004 min
Response: 1425590622
Conc: 414.24 ng/ml

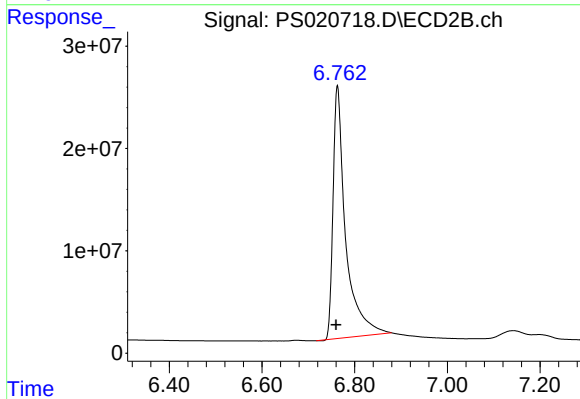

#4 2,4-DCAA


R.T.: 6.763 min
Delta R.T.: 0.003 min
Response: 465399251
Conc: 546.44 ng/ml

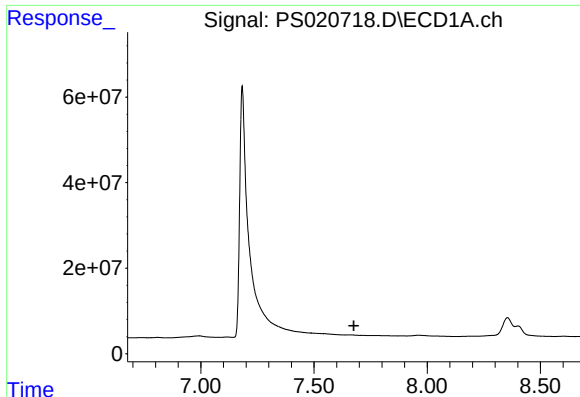

#7 MCPA


R.T.: 7.660 min
Delta R.T.: -0.016 min
Response: -1602
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

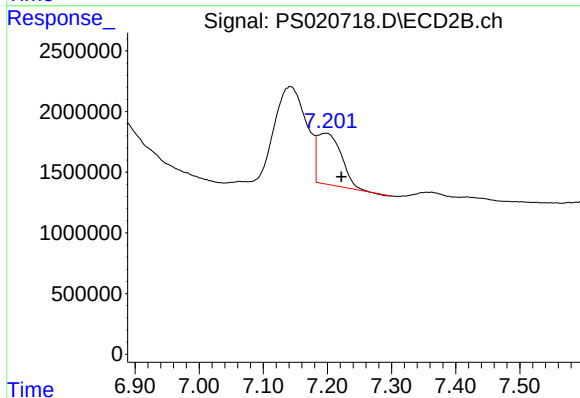


#7 MCPA

R.T.: 7.198 min
Delta R.T.: -0.024 min
Response: 10909161
Conc: 2.53 ug/ml

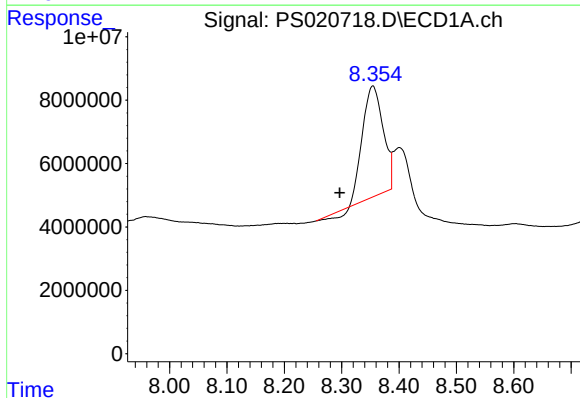

#9 2,4-D

R.T.: 8.354 min
Delta R.T.: 0.058 min
Response: 85308821
Conc: 18.35 ng/ml

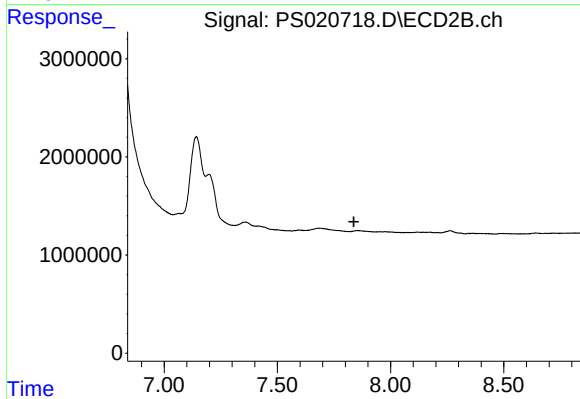

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.838 min
Response: 0
Conc: N.D.