

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100322\
 Data File : PS020728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 20:27
 Operator : AR\AJ
 Sample : N4898-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CRUSHED-MASONRY-PILE-11

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/04/2022
 Supervised By :Ankita Jodhani 10/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:57:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.172	6.756	857.9E6	273.3E6	249.296	320.911m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100322\
Data File : PS020728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 20:27
Operator : AR\AJ
Sample : N4898-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
CRUSHED-MASONRY-PILE-11


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/04/2022
Supervised By : Ankita Jodhani 10/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:57:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

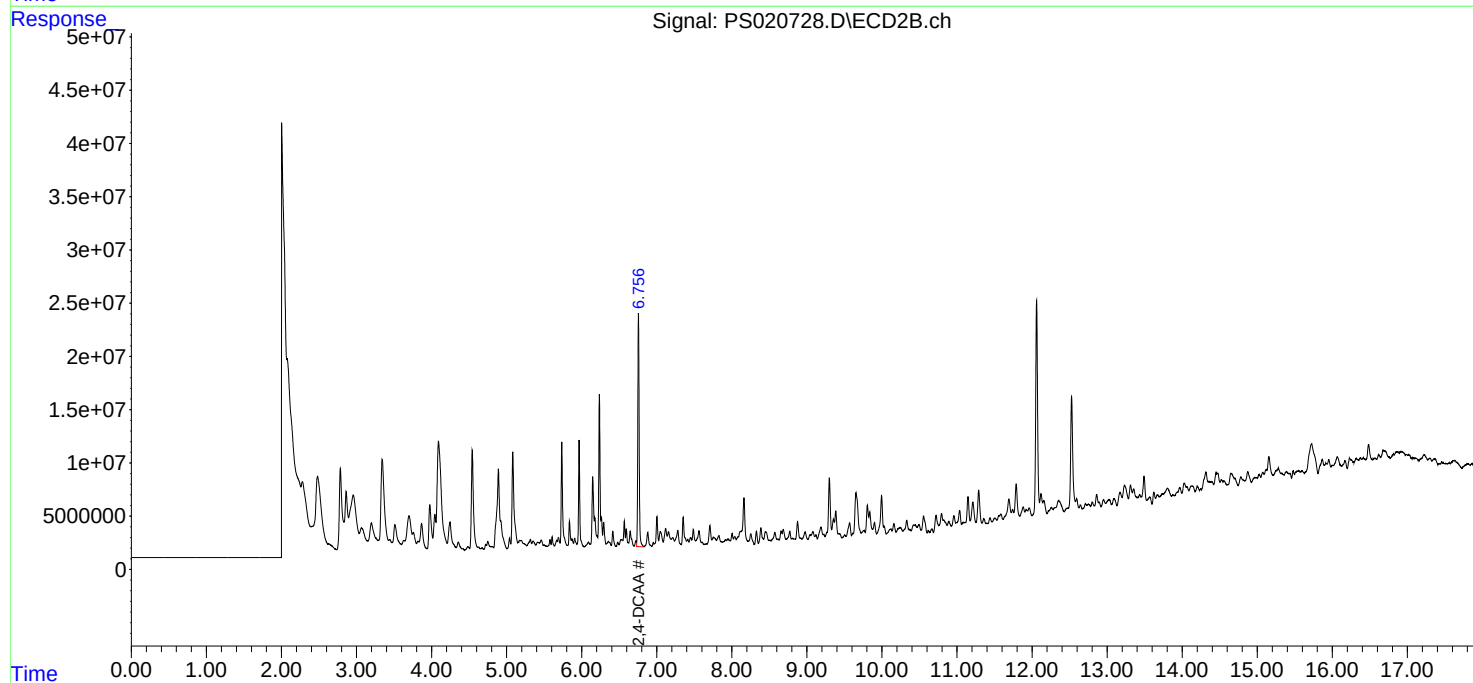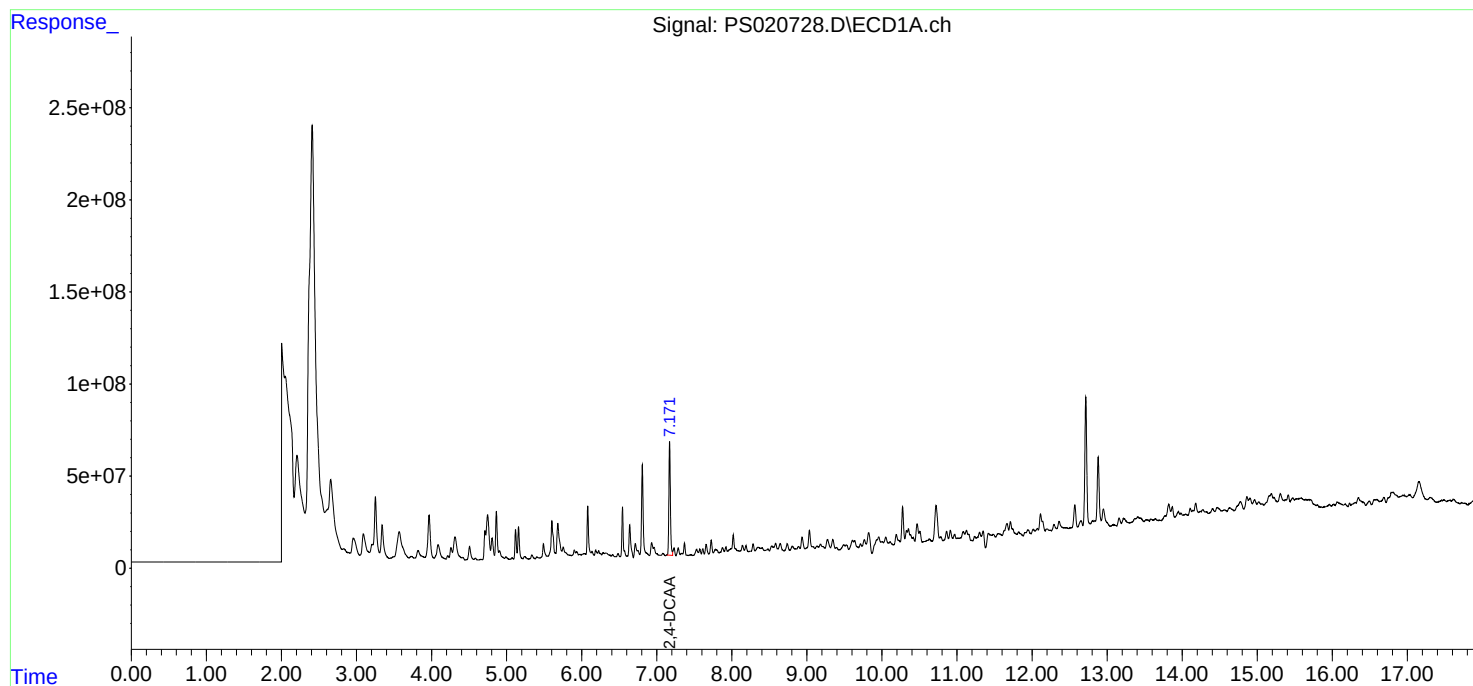

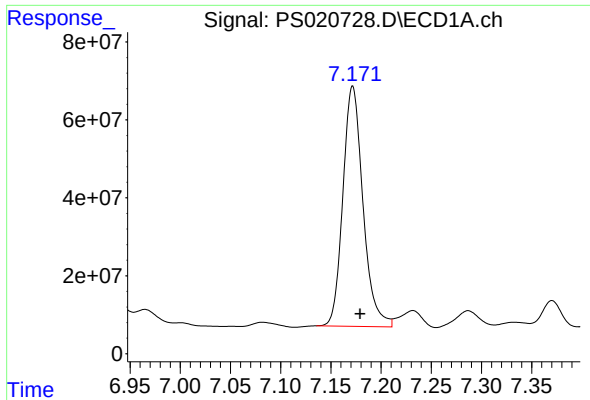


#4 2,4-DCAA

R.T.: 7.172 min
Delta R.T.: -0.007 min
Response: 857947314
Conc: 249.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
CRUSHED-MASONRY-PILE-11

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/04/2022
Supervised By :Ankita Jodhani 10/04/2022

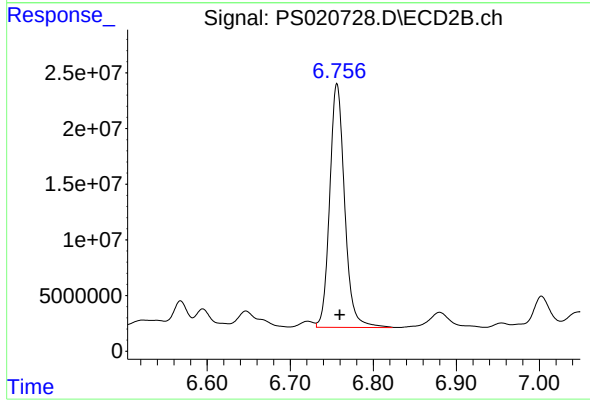

#4 2,4-DCAA

R.T.: 6.756 min
Delta R.T.: -0.004 min
Response: 273318429
Conc: 320.91 ng/ml m