

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100323\
 Data File : PS024484.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2023 15:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 16:01:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.359	6.783	1076.4E6	361.4E6	523.217	522.803
Target Compounds							
1) T	Dalapon	2.519f	2.575	9945240	5861669	4.026	5.238 #
5) T	DICAMBA	0.000	6.943	0	600753	N.D.	<MDL
7) T	MCPA	0.000	7.232	0	10340559	N.D.	3.227
8) T	DICHLORPROP	0.000	7.565	0	656498	N.D.	<MDL
9) T	2,4-D	7.354f	7.787f	221.1E6	586579	80.034	<MDL #
10) T	Pentachlo...	7.514	8.268	12023573	2193071	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.625	0	1489307	N.D.	<MDL
12) T	2,4,5-T	0.000	8.998	0	1671717	N.D.	<MDL
13) T	2,4-DB	0.000	9.503	0	945531	N.D.	1.856
14) T	DINOSEB	0.000	9.829	0	925551	N.D.	<MDL
15) T	Picloram	9.680	10.782	53980843	19577490	3.096	3.150
16) T	DCPA	0.000	10.782	0	19577490	N.D.	3.752



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100323\
Data File : PS024484.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2023 15:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 16:01:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

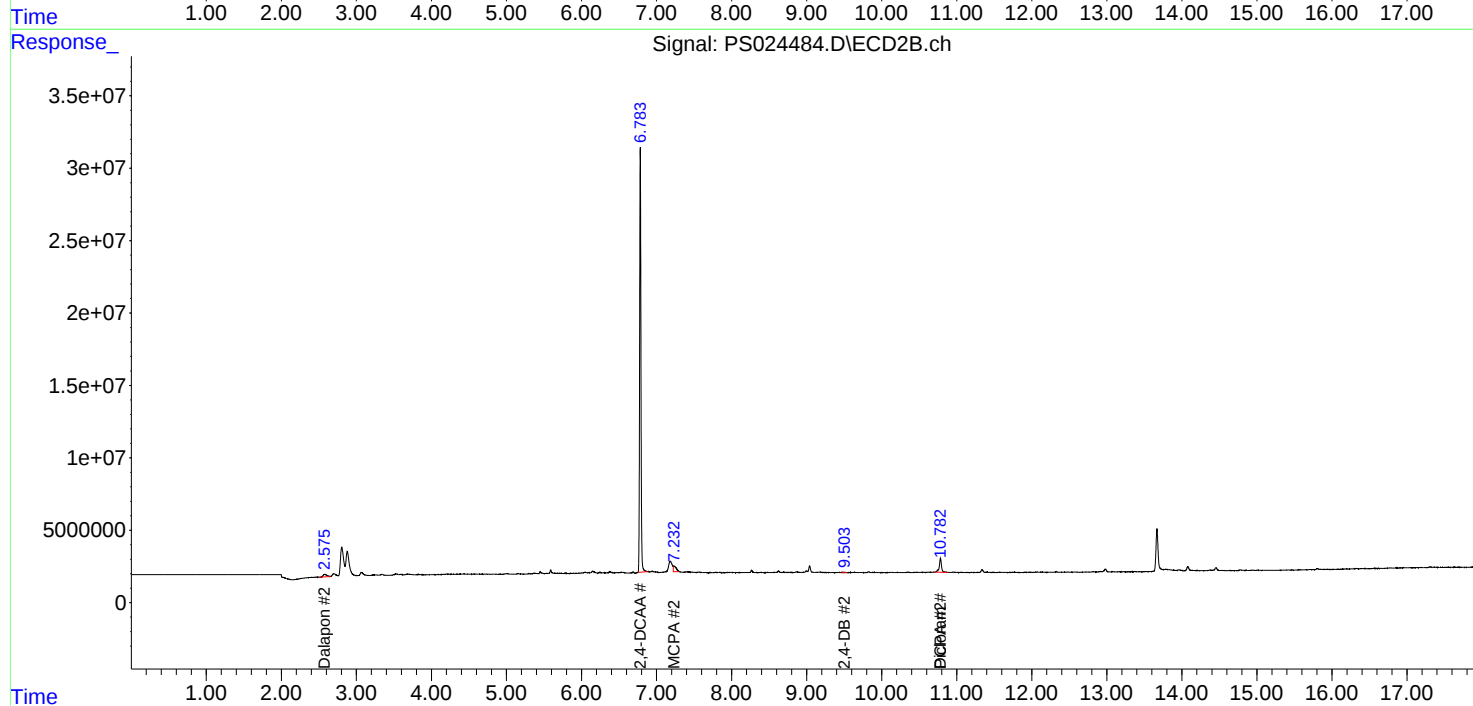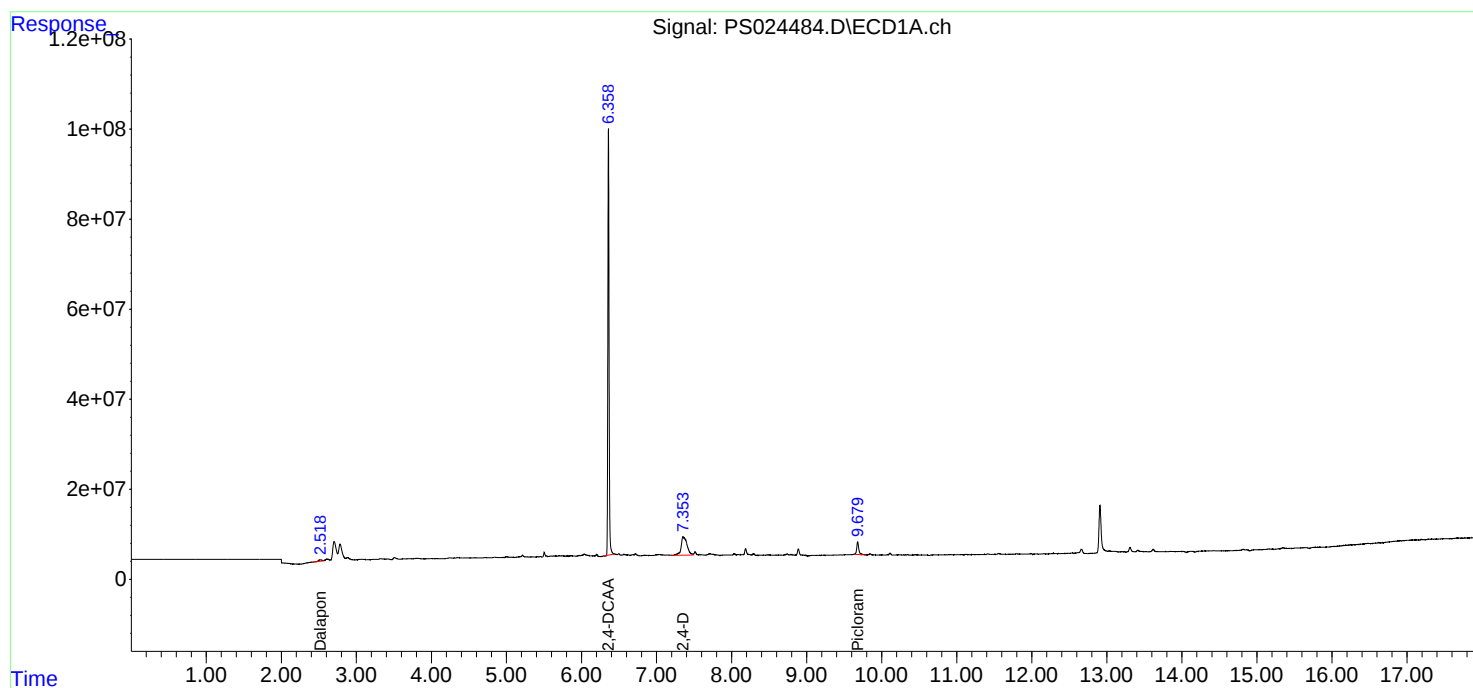


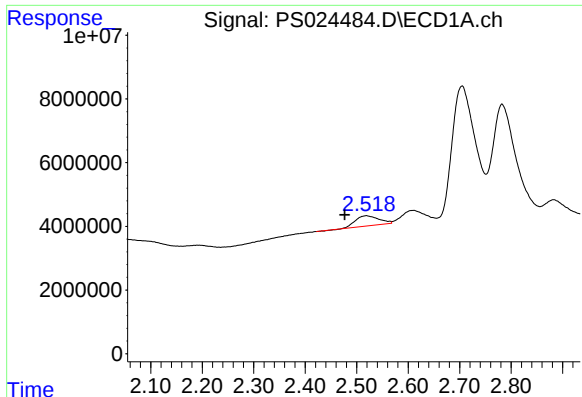

#1 Dalapon


R.T.: 2.519 min
Delta R.T.: 0.042 min
Response: 9945240
Conc: 4.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

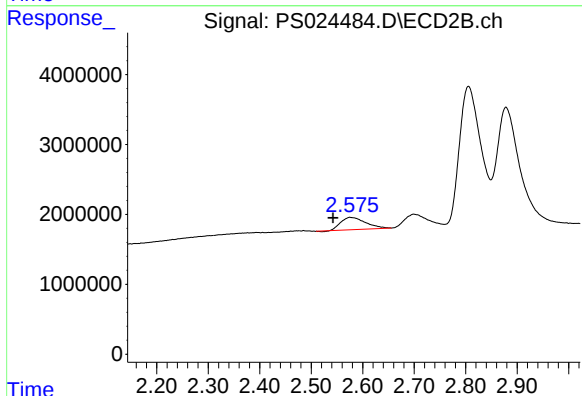


#1 Dalapon

R.T.: 2.575 min
Delta R.T.: 0.033 min
Response: 5861669
Conc: 5.24 ng/ml

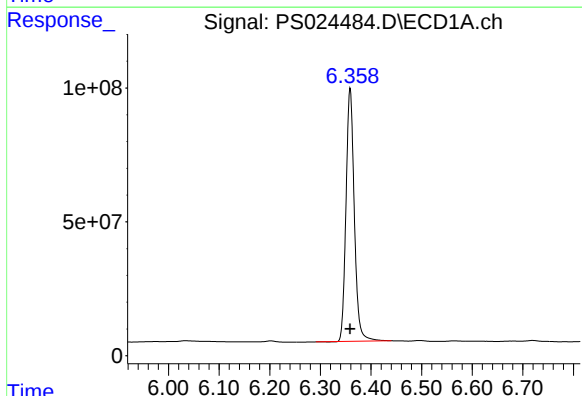


#4 2,4-DCAA

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 1076428954
Conc: 523.22 ng/ml

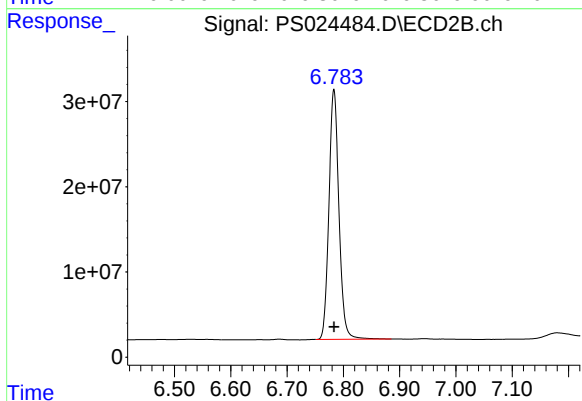

#4 2,4-DCAA


R.T.: 6.783 min
Delta R.T.: 0.000 min
Response: 361408977
Conc: 522.80 ng/ml

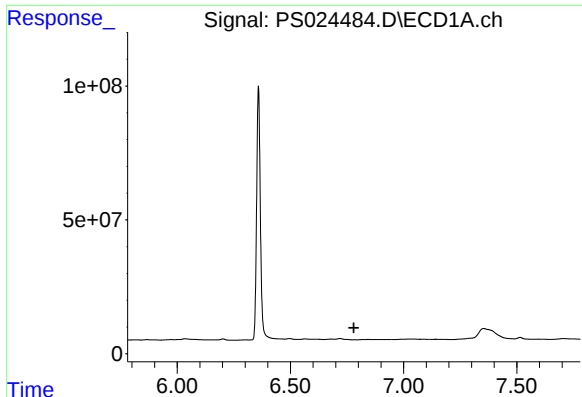

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

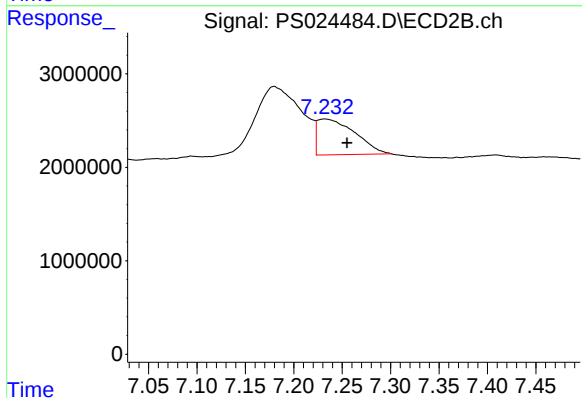


#7 MCPA

R.T.: 7.232 min
Delta R.T.: -0.023 min
Response: 10340559
Conc: 3.23 ug/ml

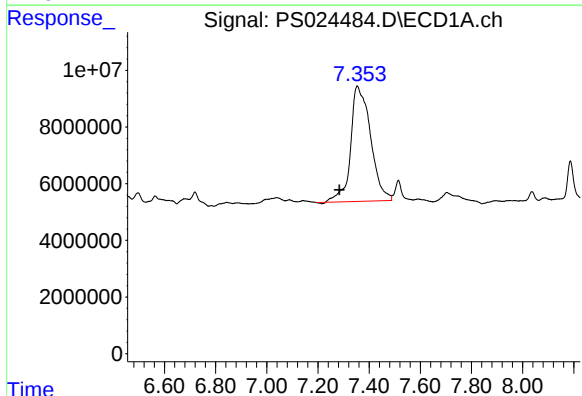


#9 2,4-D

R.T.: 7.354 min
Delta R.T.: 0.069 min
Response: 221132215
Conc: 80.03 ng/ml

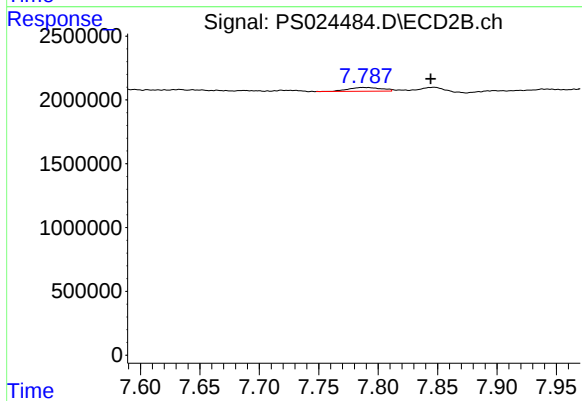

#9 2,4-D


R.T.: 7.787 min
Delta R.T.: -0.057 min
Response: 586579
Conc: N.D.

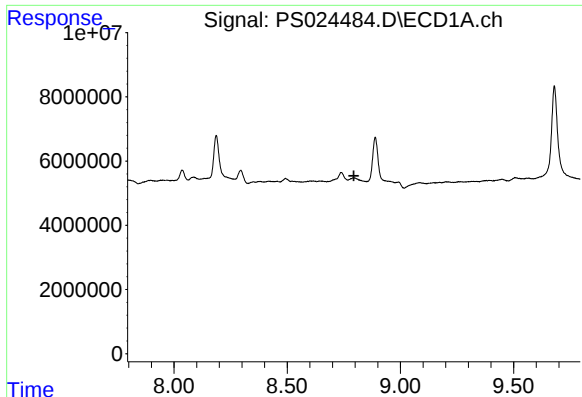

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

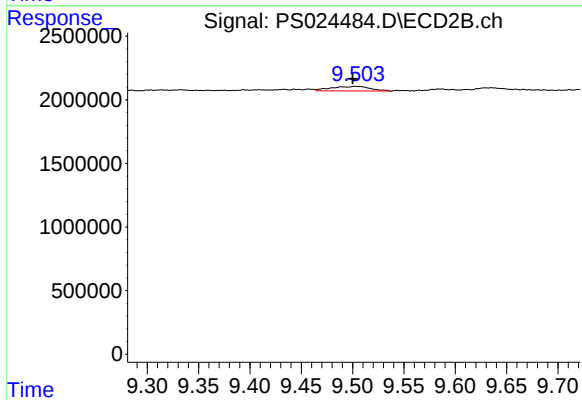


#13 2,4-DB

R.T.: 9.503 min
Delta R.T.: 0.003 min
Response: 945531
Conc: 1.86 ng/ml

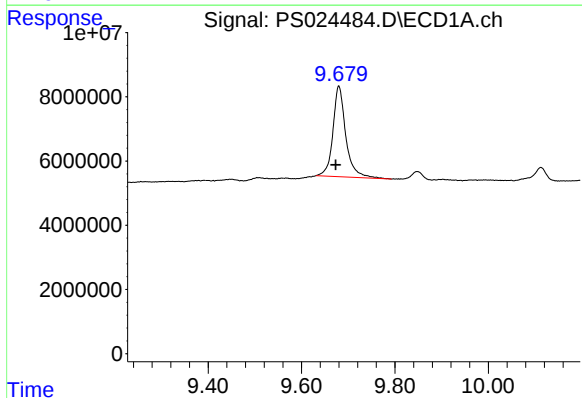


#15 Picloram

R.T.: 9.680 min
Delta R.T.: 0.007 min
Response: 53980843
Conc: 3.10 ng/ml

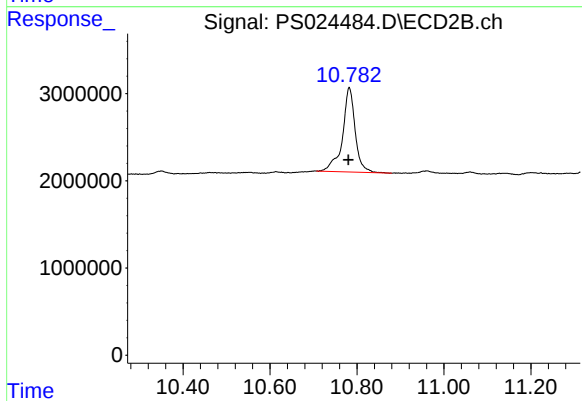

#15 Picloram


R.T.: 10.782 min
Delta R.T.: 0.002 min
Response: 19577490
Conc: 3.15 ng/ml

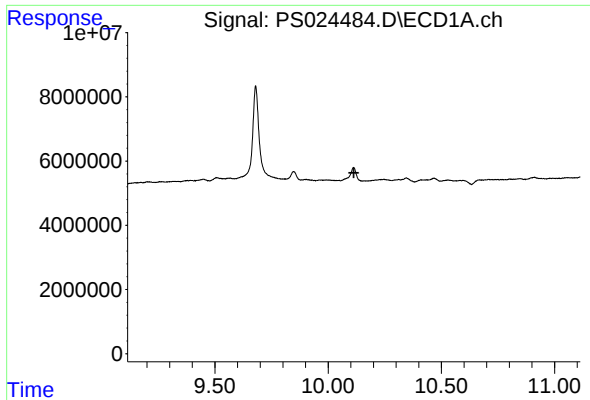

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

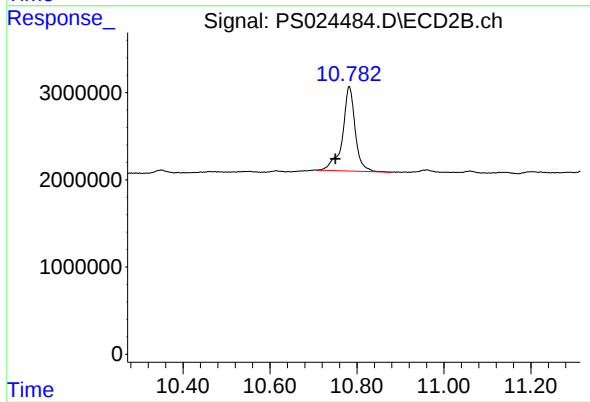

#16 DCPA

R.T.: 10.782 min
Delta R.T.: 0.032 min
Response: 19577490
Conc: 3.75 ng/ml