

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100323\
 Data File : PS024508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2023 01:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 03:29:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.358	6.783	1080.0E6	361.2E6	524.939	522.539
Target Compounds							
1) T	Dalapon	2.518f	2.576	7684496	4298678	3.110	3.841
2) T	3,5-DICHL...	0.000	5.970	0	433938	N.D.	<MDL
5) T	DICAMBA	6.499	6.944	6756069	1863807	<MDL	<MDL #
6) T	MCP	6.681	0.000	298713	0	<MDL	N.D. #
7) T	MCPA	0.000	7.229	0	9011389	N.D.	2.812
8) T	DICHLORPROP	0.000	7.570	0	2508112	N.D.	3.335
9) T	2,4-D	7.351f	7.847	196.3E6	639257	71.052	<MDL #
10) T	Pentachlo...	7.514	8.268	21885059	4848835	<MDL	<MDL #
11) T	2,4,5-TP ...	8.035	8.626	9574652	2768209	<MDL	<MDL #
12) T	2,4,5-T	8.294	8.998	9889569	2915522	<MDL	<MDL #
13) T	2,4-DB	0.000	9.495	0	912160	N.D.	1.790
14) T	DINOSEB	9.848	9.827	9469963	2433217	<MDL	<MDL #
15) T	Picloram	9.681	10.783	25581655	7720544	1.467	1.242
16) T	DCPA	10.112	10.748	14766273	3908501	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100323\
Data File : PS024508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2023 01:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 03:29:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

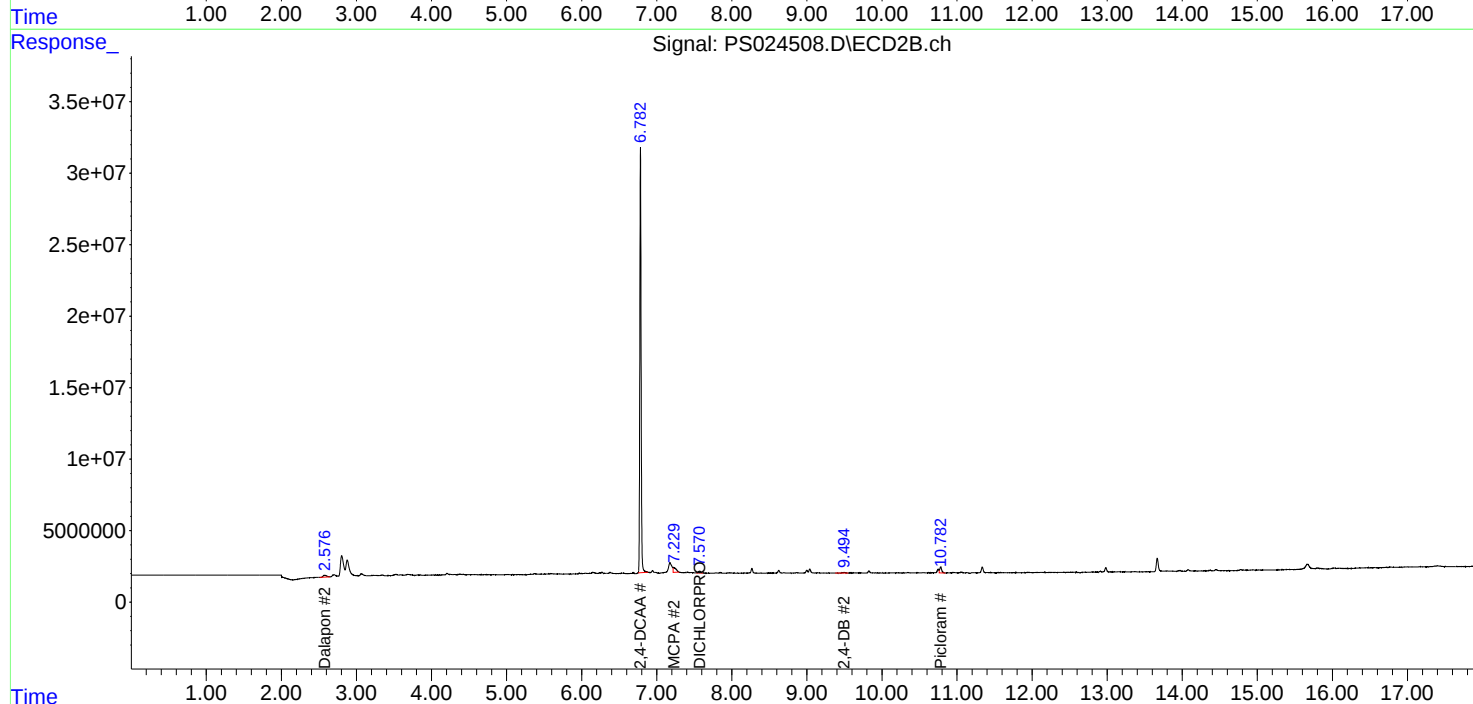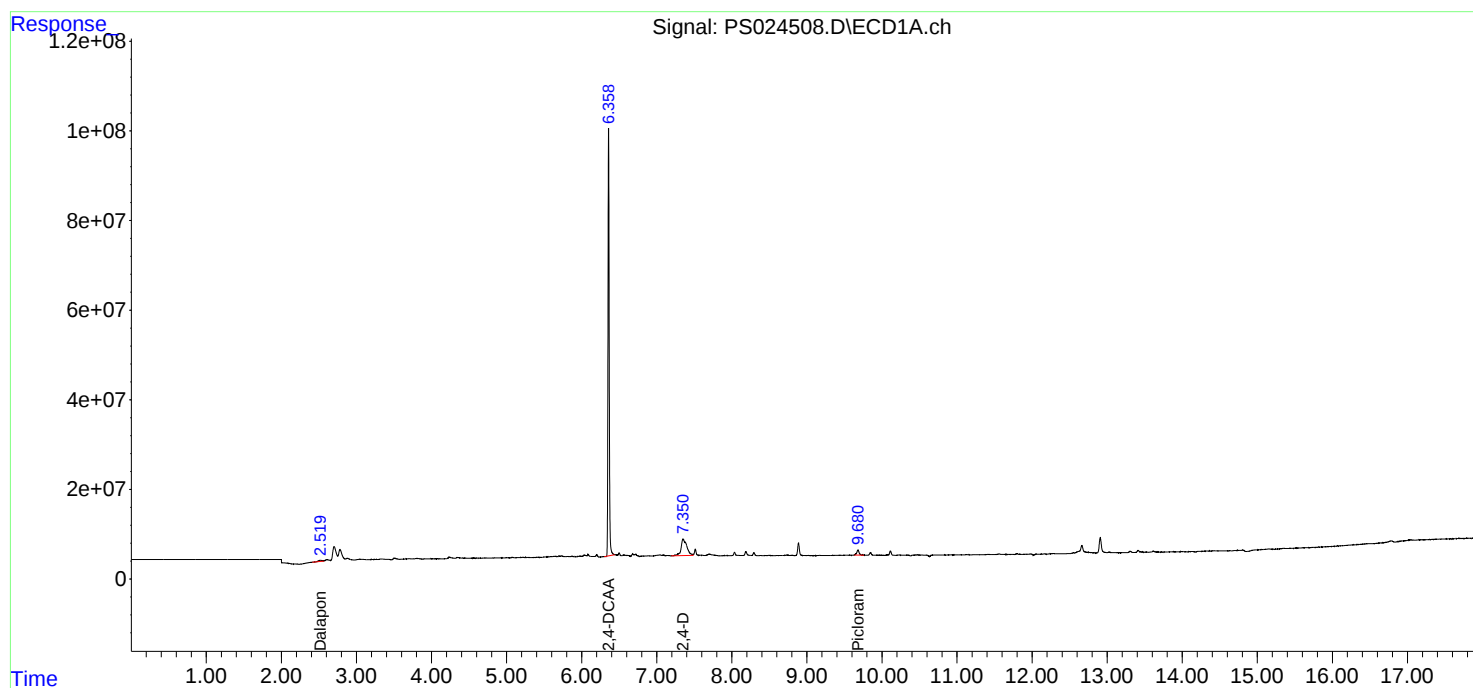


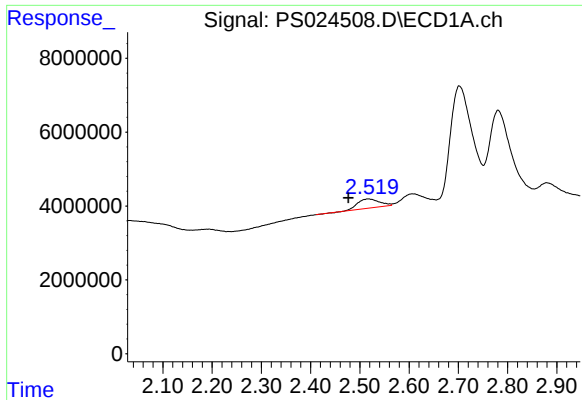

#1 Dalapon


R.T.: 2.518 min
Delta R.T.: 0.041 min
Response: 7684496
Conc: 3.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

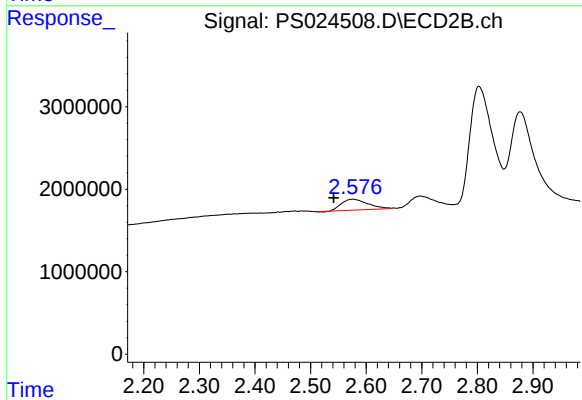


#1 Dalapon

R.T.: 2.576 min
Delta R.T.: 0.034 min
Response: 4298678
Conc: 3.84 ng/ml

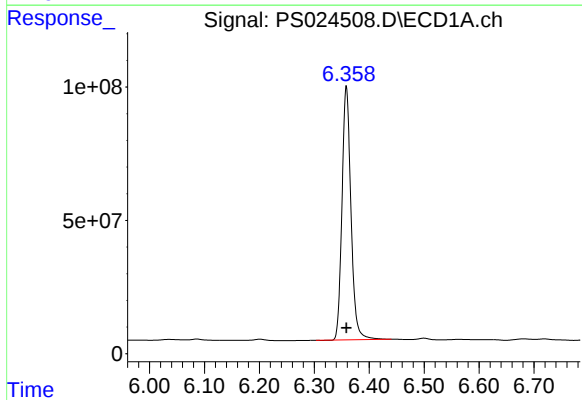


#4 2,4-DCAA

R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 1079971883
Conc: 524.94 ng/ml

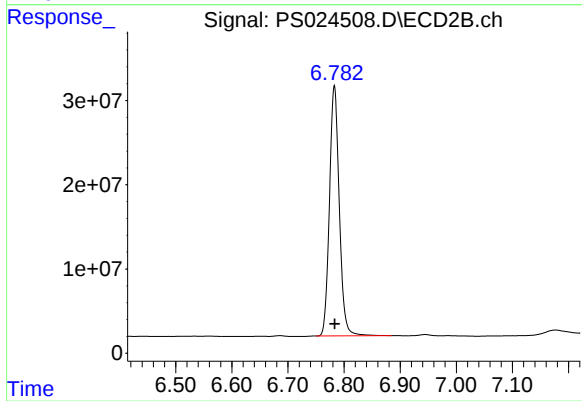

#4 2,4-DCAA


R.T.: 6.783 min
Delta R.T.: 0.000 min
Response: 361226553
Conc: 522.54 ng/ml

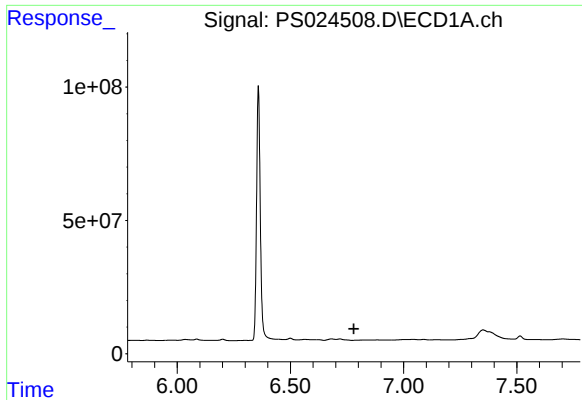

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

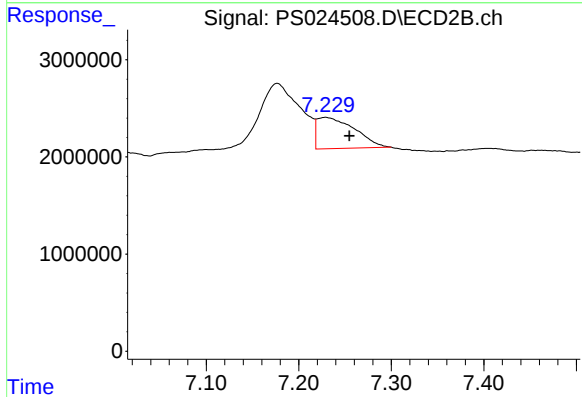


#7 MCPA

R.T.: 7.229 min
Delta R.T.: -0.026 min
Response: 9011389
Conc: 2.81 ug/ml

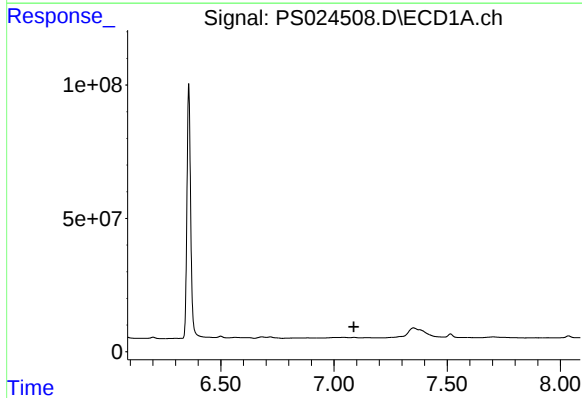


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

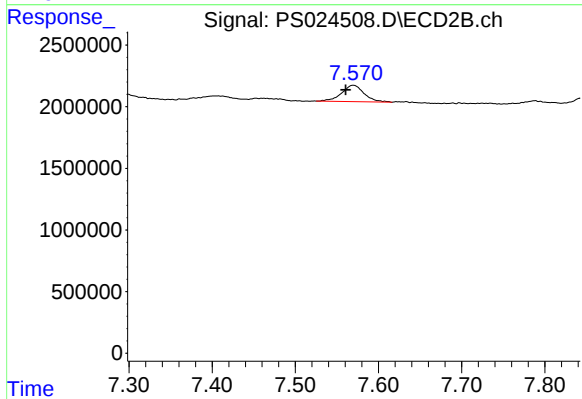

#8 DICHLORPROP


R.T.: 7.570 min
Delta R.T.: 0.009 min
Response: 2508112
Conc: 3.34 ng/ml

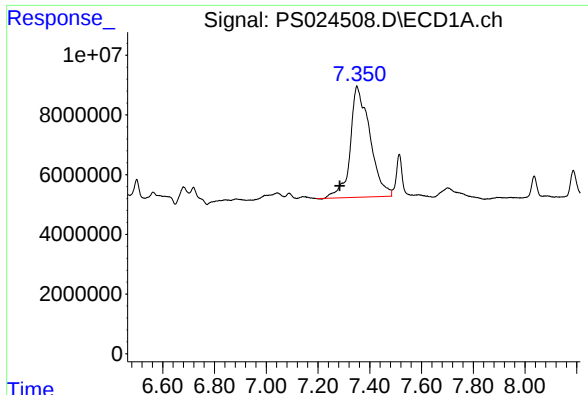

#9 2,4-D


R.T.: 7.351 min
Delta R.T.: 0.066 min
Response: 196316237
Conc: 71.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

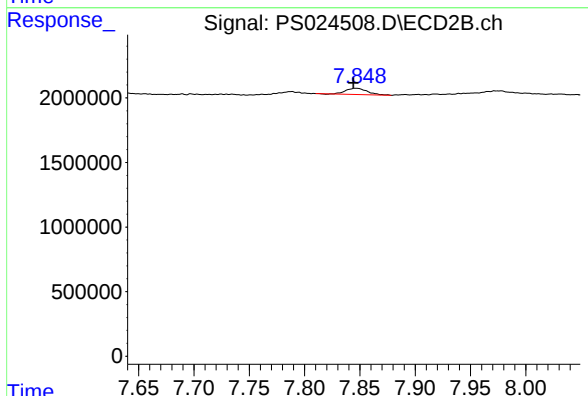


#9 2,4-D

R.T.: 7.847 min
Delta R.T.: 0.002 min
Response: 639257
Conc: N.D.

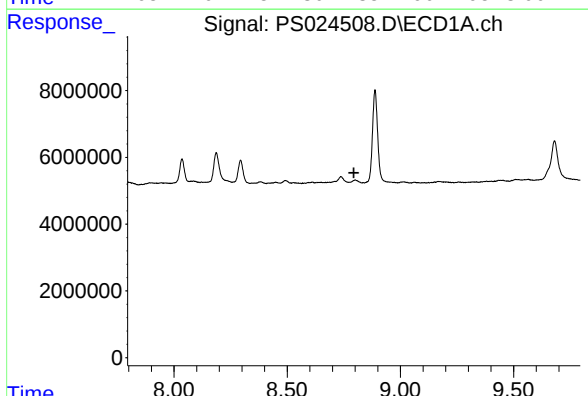


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.795 min
Response: 0
Conc: N.D.

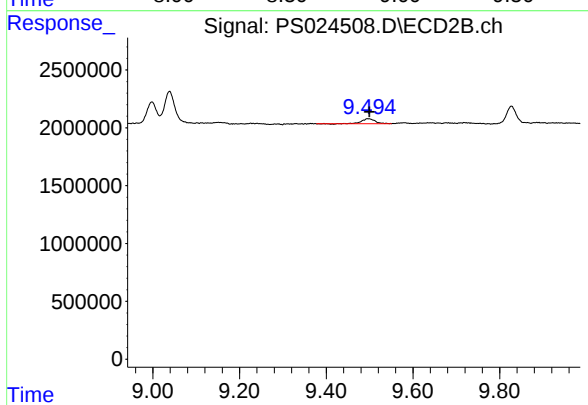

#13 2,4-DB


R.T.: 9.495 min
Delta R.T.: -0.005 min
Response: 912160
Conc: 1.79 ng/ml

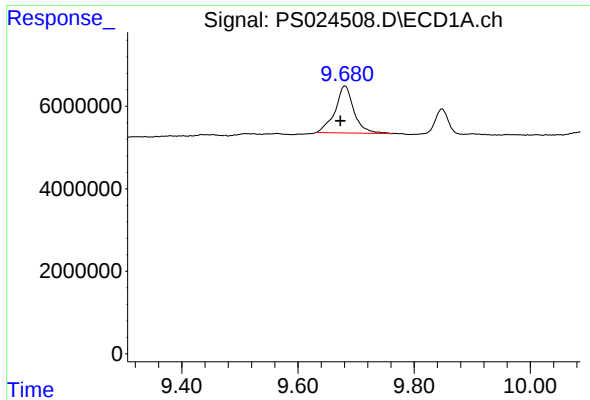

#15 Picloram

R.T.: 9.681 min
Delta R.T.: 0.008 min
Response: 25581655
Conc: 1.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

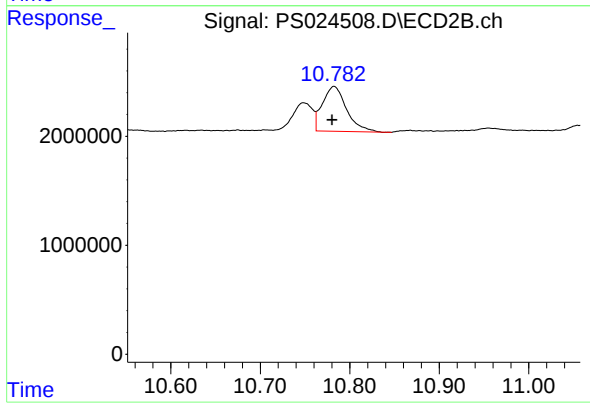

#15 Picloram

R.T.: 10.783 min
Delta R.T.: 0.002 min
Response: 7720544
Conc: 1.24 ng/ml