

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100323\
 Data File : PS024520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2023 06:39
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 07:04:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	6.358	6.782	1073.2E6	361.2E6	521.663	522.558
------	----------	-------	-------	----------	---------	---------	---------

Target Compounds

1) T	Dalapon	0.000	2.573	0	3186933	N.D.	2.848
5) T	DICAMBA	0.000	6.986f	0	466460	N.D.	<MDL
6) T	MCCP	6.680	6.986f	3498138	466460	<MDL	<MDL #
7) T	MCPA	0.000	7.234	0	9507196	N.D.	2.967
8) T	DICHLORPROP	0.000	7.571	0	2439731	N.D.	3.244
11) T	2,4,5-TP ...	0.000	8.623	0	416334	N.D.	<MDL
13) T	2,4-DB	0.000	9.495	0	624212	N.D.	1.225
15) T	Picloram	0.000	10.782	0	1616536	N.D.	<MDL
16) T	DCPA	0.000	10.782	0	1616536	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100323\
Data File : PS024520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2023 06:39
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 07:04:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

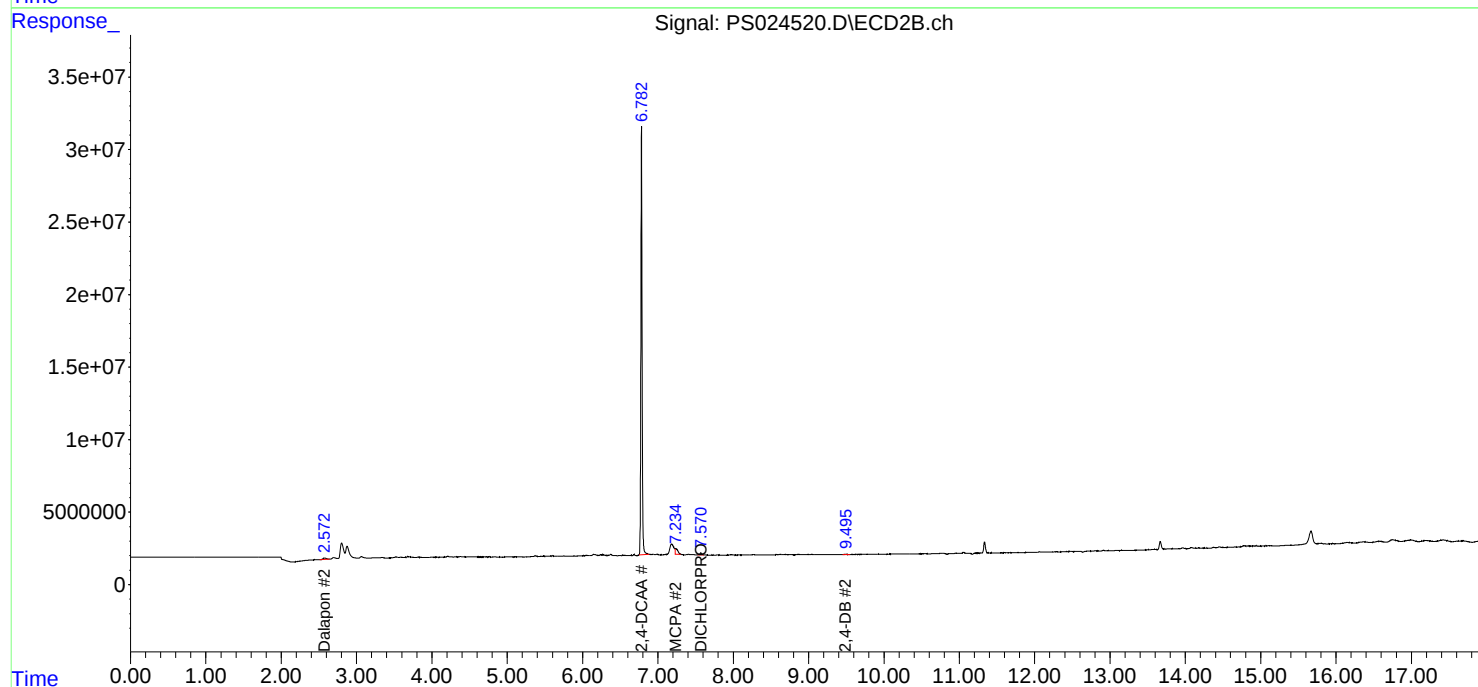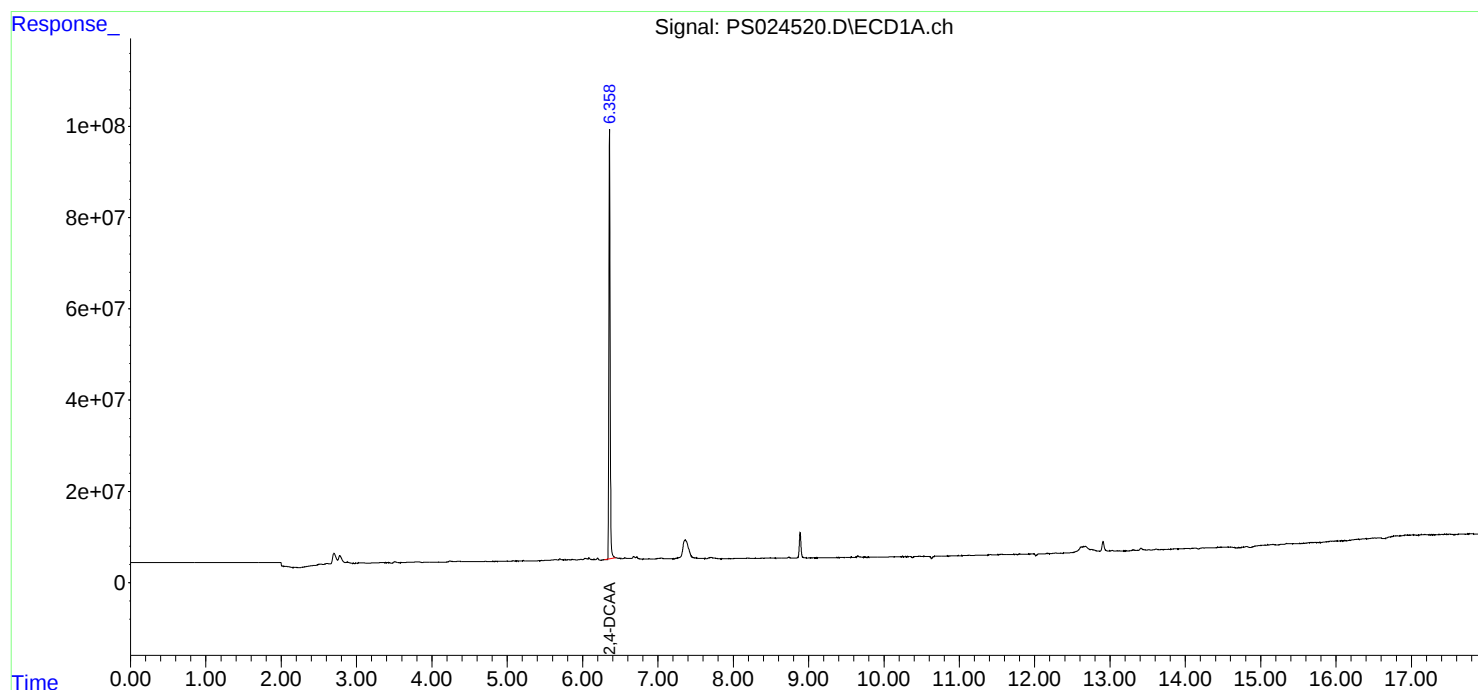


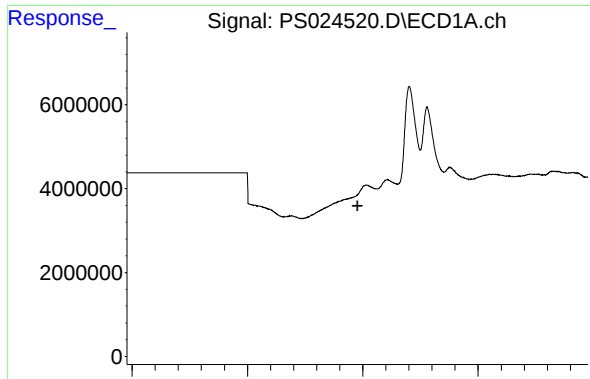

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

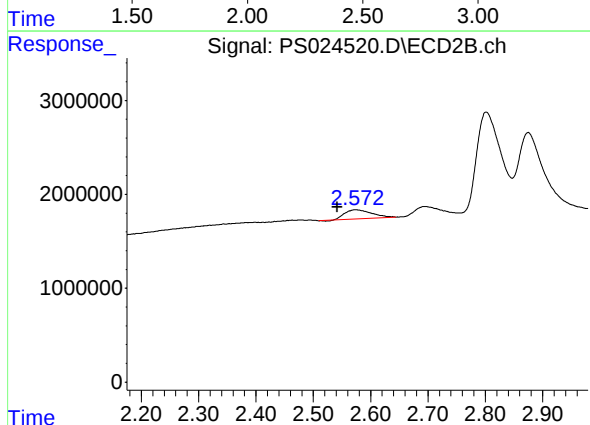


#1 Dalapon

R.T.: 2.573 min
Delta R.T.: 0.031 min
Response: 3186933
Conc: 2.85 ng/ml

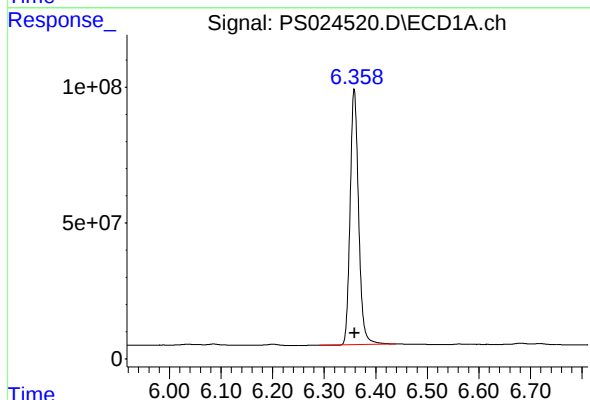


#4 2,4-DCAA

R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 1073231928
Conc: 521.66 ng/ml

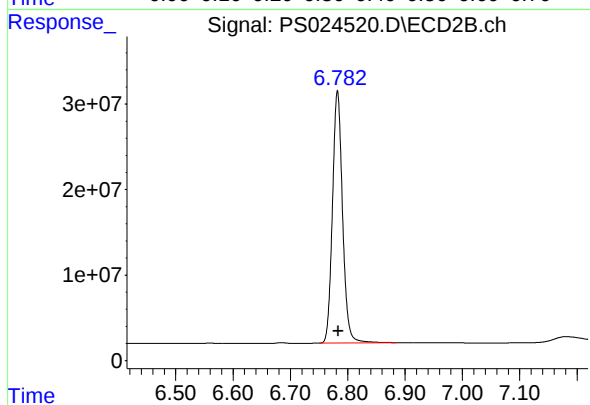

#4 2,4-DCAA


R.T.: 6.782 min
Delta R.T.: -0.002 min
Response: 361239147
Conc: 522.56 ng/ml

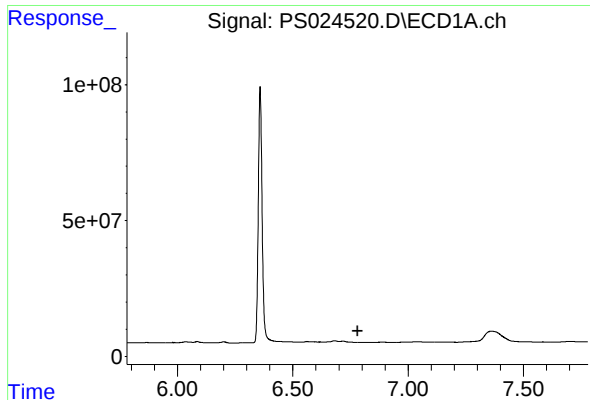

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

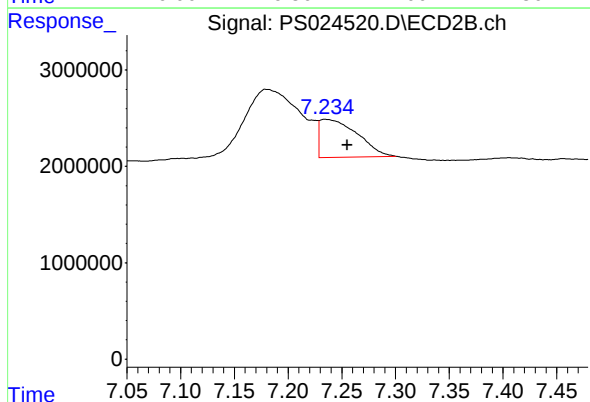


#7 MCPA

R.T.: 7.234 min
Delta R.T.: -0.021 min
Response: 9507196
Conc: 2.97 ug/ml

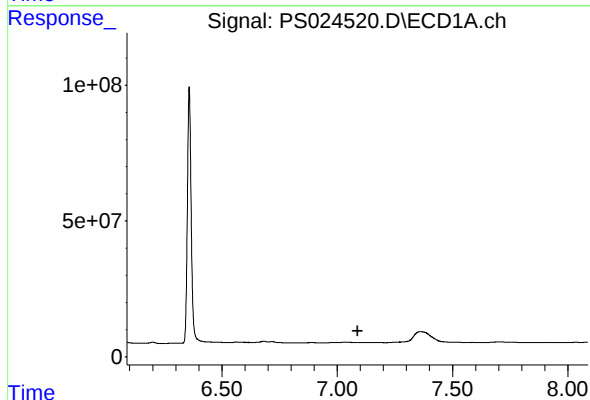


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

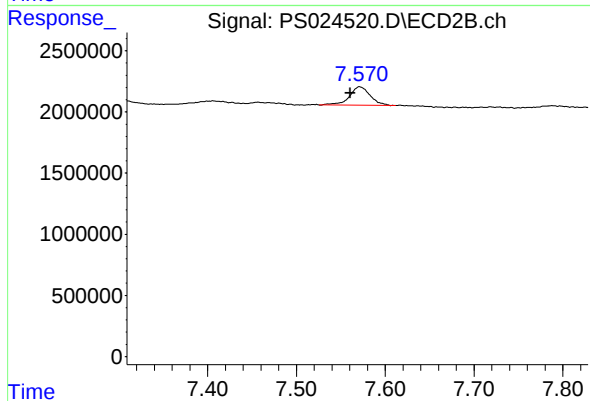

#8 DICHLORPROP


R.T.: 7.571 min
Delta R.T.: 0.010 min
Response: 2439731
Conc: 3.24 ng/ml

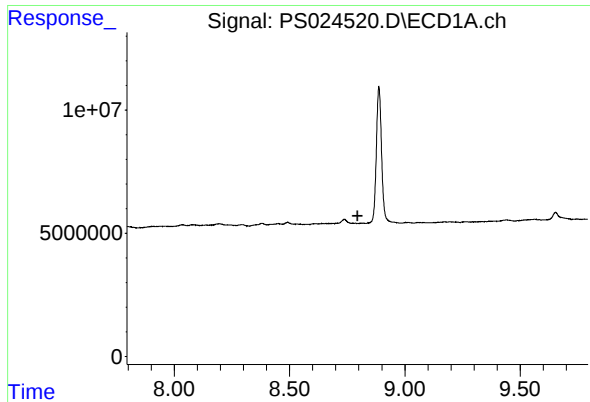

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

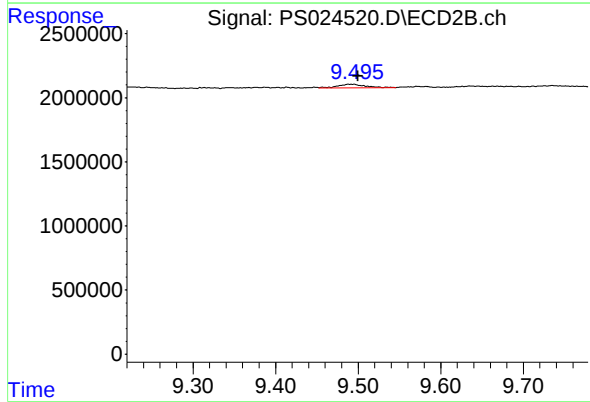

#13 2,4-DB

R.T.: 9.495 min
Delta R.T.: -0.005 min
Response: 624212
Conc: 1.22 ng/ml