

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100323\
 Data File : PS024528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2023 10:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 11:03:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.358	6.782	1081.3E6	363.4E6	525.591	525.667
Target Compounds							
1) T	Dalapon	0.000	2.572	0	3722452	N.D.	3.326
5) T	DICAMBA	0.000	6.943	0	741575	N.D.	<MDL
6) T	MCP	6.680	6.986f	5380289	763892	<MDL	<MDL #
7) T	MCPA	0.000	7.200f	0	18176033	N.D.	5.672
8) T	DICHLORPROP	0.000	7.571	0	3999798	N.D.	5.319
10) T	Pentachlo...	0.000	8.267	0	1047222	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.625	0	958660	N.D.	<MDL
12) T	2,4,5-T	0.000	8.999	0	774832	N.D.	<MDL
13) T	2,4-DB	0.000	9.489	0	977066	N.D.	1.917
15) T	Picloram	0.000	10.781	0	2345217	N.D.	<MDL
16) T	DCPA	0.000	10.747	0	1900154	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100323\
Data File : PS024528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2023 10:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 11:03:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

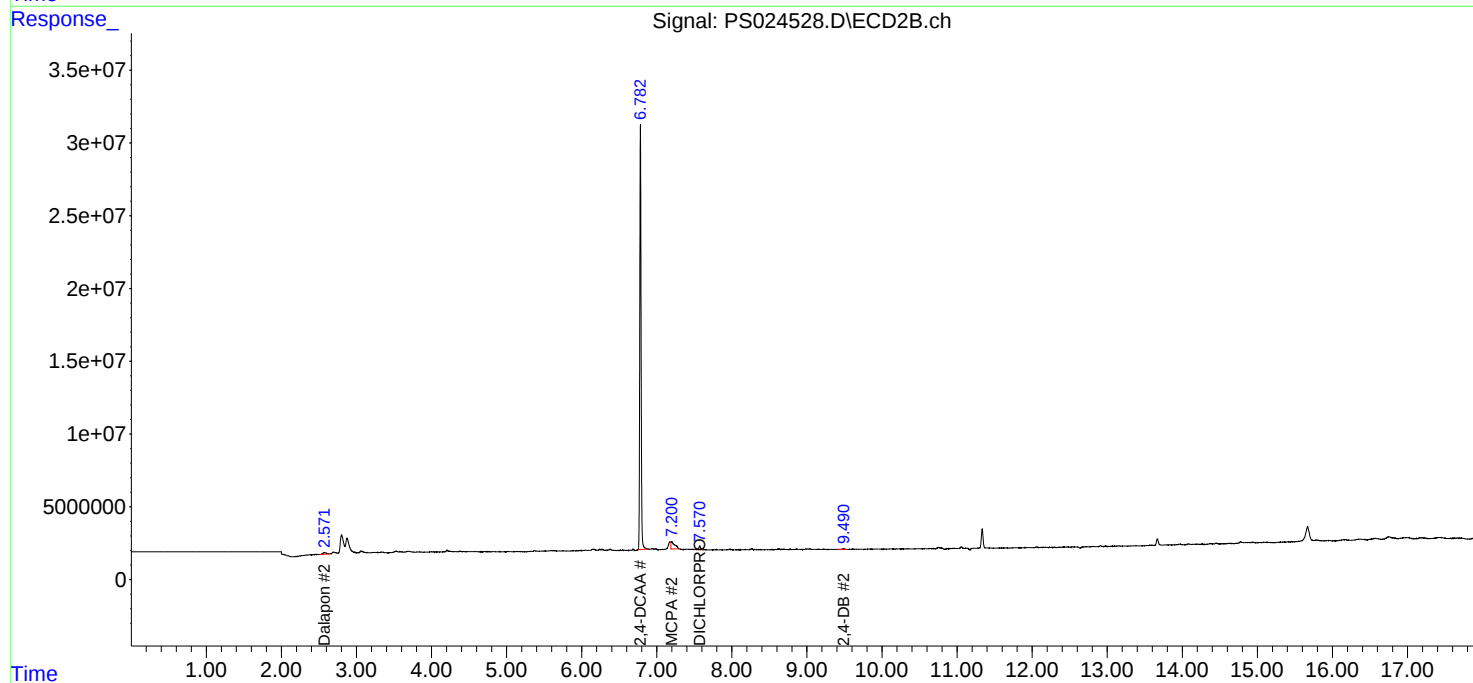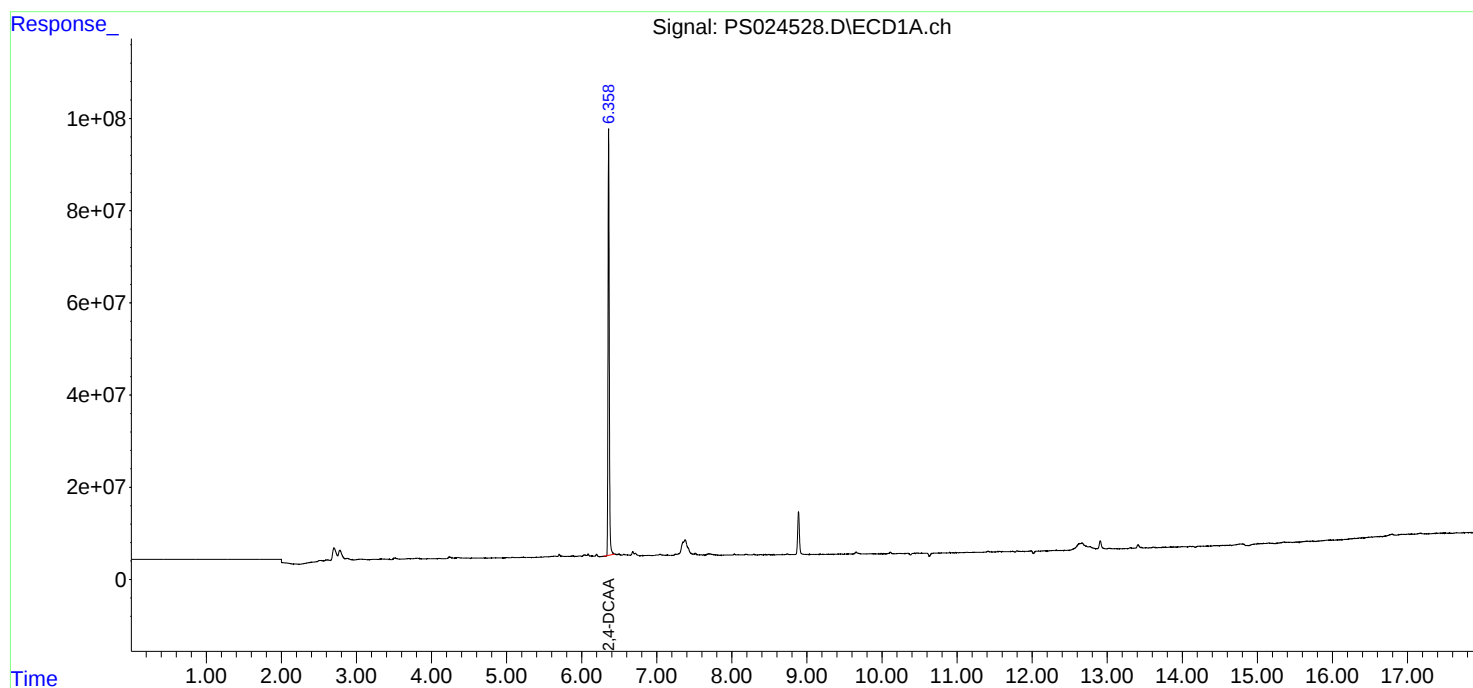


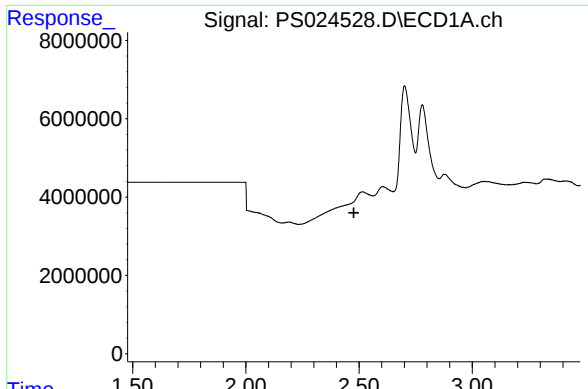

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

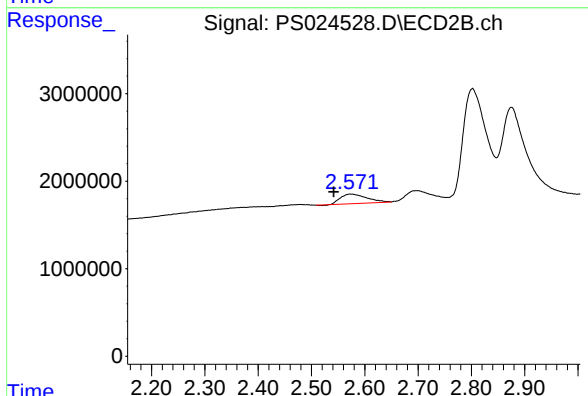


#1 Dalapon

R.T.: 2.572 min
Delta R.T.: 0.030 min
Response: 3722452
Conc: 3.33 ng/ml

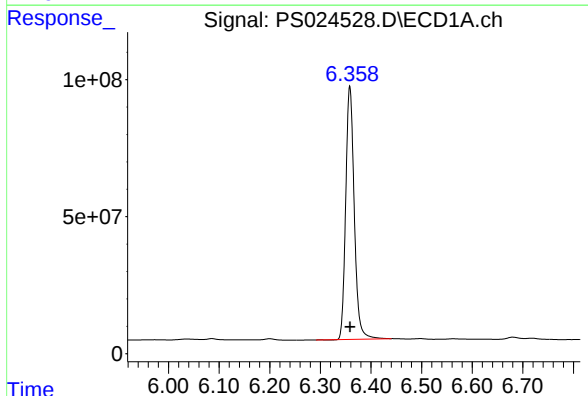


#4 2,4-DCAA

R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 1081313189
Conc: 525.59 ng/ml

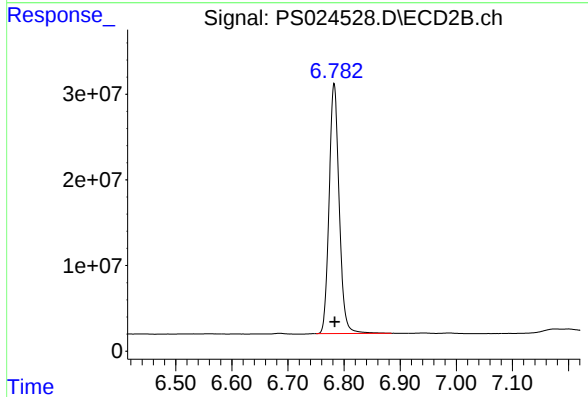

#4 2,4-DCAA


R.T.: 6.782 min
Delta R.T.: -0.001 min
Response: 363388637
Conc: 525.67 ng/ml

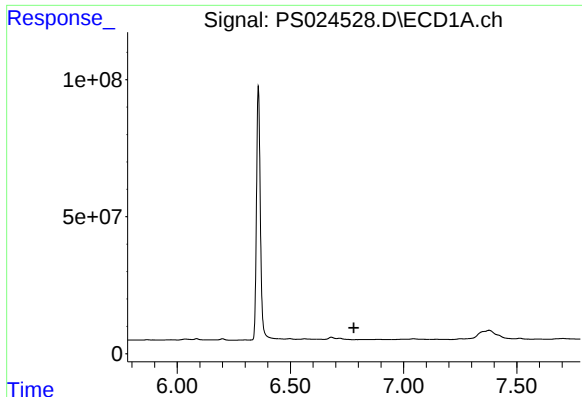

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

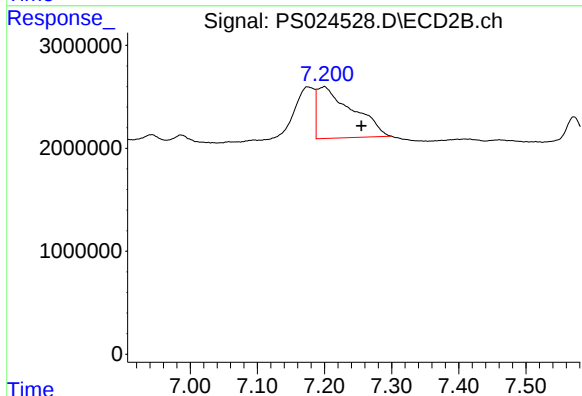


#7 MCPA

R.T.: 7.200 min
Delta R.T.: -0.055 min
Response: 18176033
Conc: 5.67 ug/ml

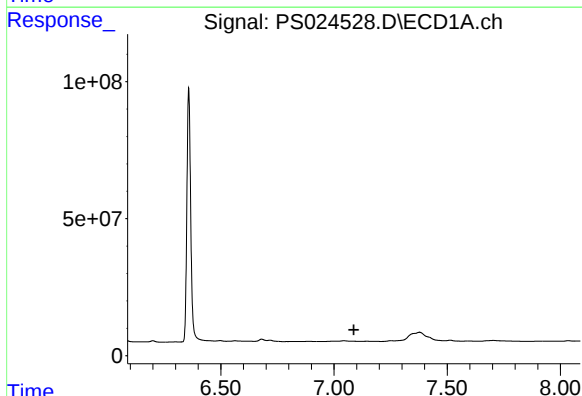


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

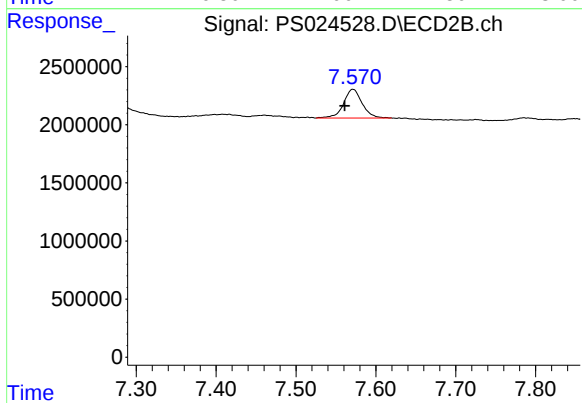

#8 DICHLORPROP


R.T.: 7.571 min
Delta R.T.: 0.010 min
Response: 3999798
Conc: 5.32 ng/ml

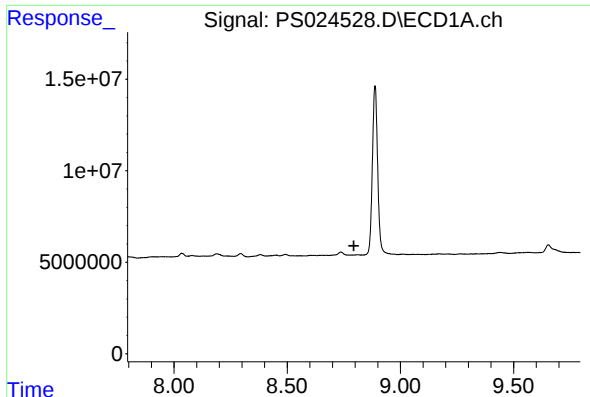

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

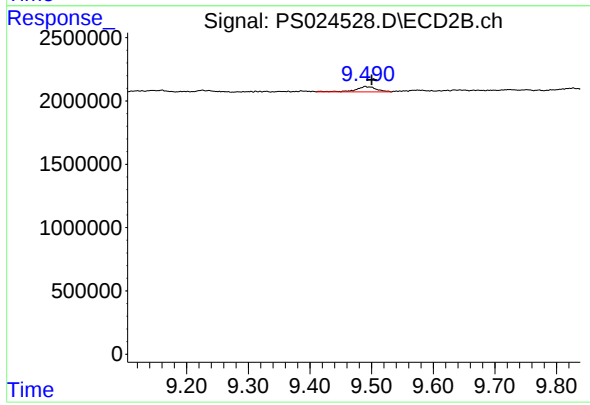

#13 2,4-DB

R.T.: 9.489 min
Delta R.T.: -0.011 min
Response: 977066
Conc: 1.92 ng/ml