

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100324\
 Data File : PS027814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2024 11:13
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 00:54:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.114	7.643	455449	881515	<MDL	<MDL #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.591	0	967839	N.D.	<MDL
3) T	4-Nitroph...	6.890	7.138f	18192958	1940572	10.745	2.707 #
5) T	DICAMBA	7.308	7.838	-871555	1269856	N.D.	<MDL
6) T	MCP	0.000	7.936	0	696524	N.D.	<MDL
8) T	DICHLORPROP	7.985	8.572f	401309	6723305	<MDL	6.018 #
10) T	Pentachlo...	0.000	9.358	0	924983	N.D.	<MDL
11) T	2,4,5-TP ...	9.050	9.790f	2067222	487519	<MDL	<MDL #
12) T	2,4,5-T	9.337	10.155	1563142	1689996	<MDL	<MDL #
13) T	2,4-DB	9.878f	0.000	659779	0	<MDL	N.D. #
14) T	DINOSEB	11.066	0.000	1953519	0	<MDL	N.D. #
15) T	Picloram	10.900	12.190	27868959	6029496	1.490	1.297
16) T	DCPA	11.362	12.113f	5457677	6084423	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100324\
Data File : PS027814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2024 11:13
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 00:54:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

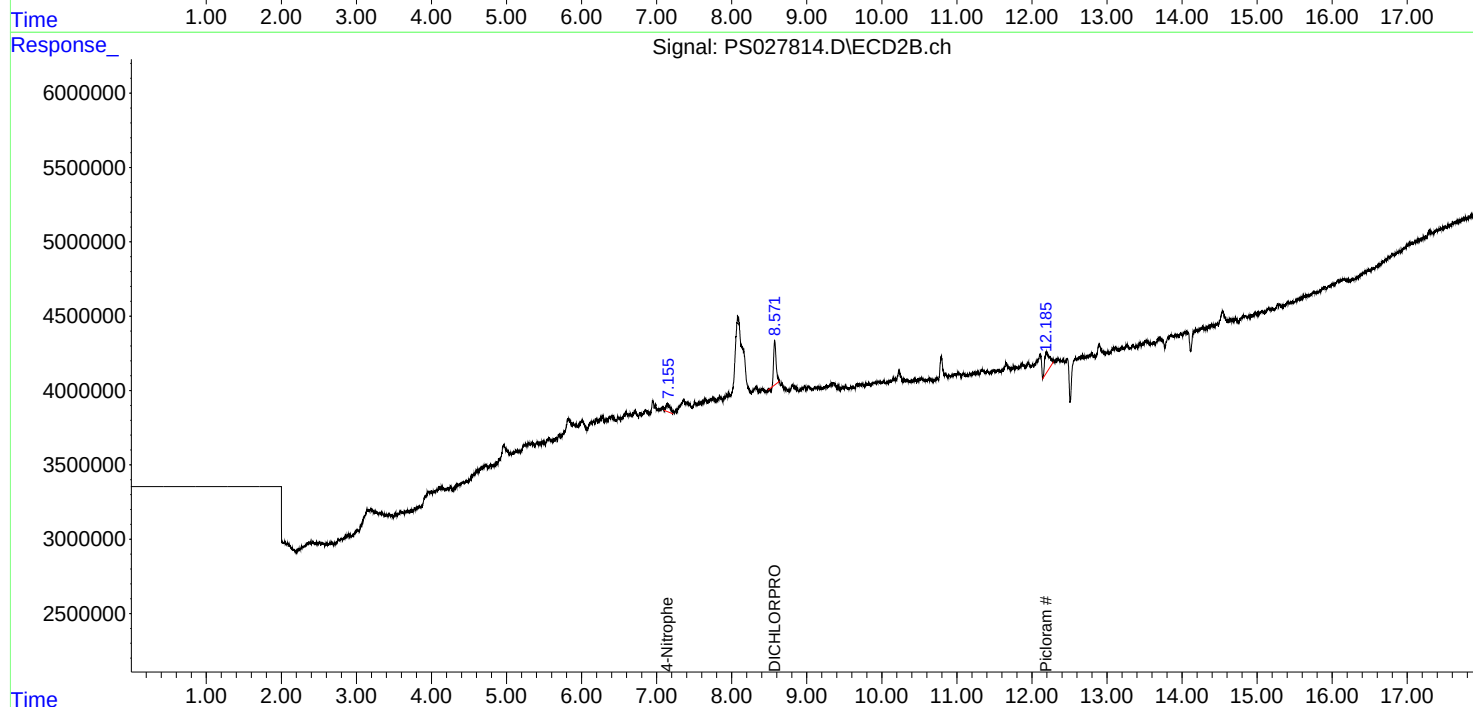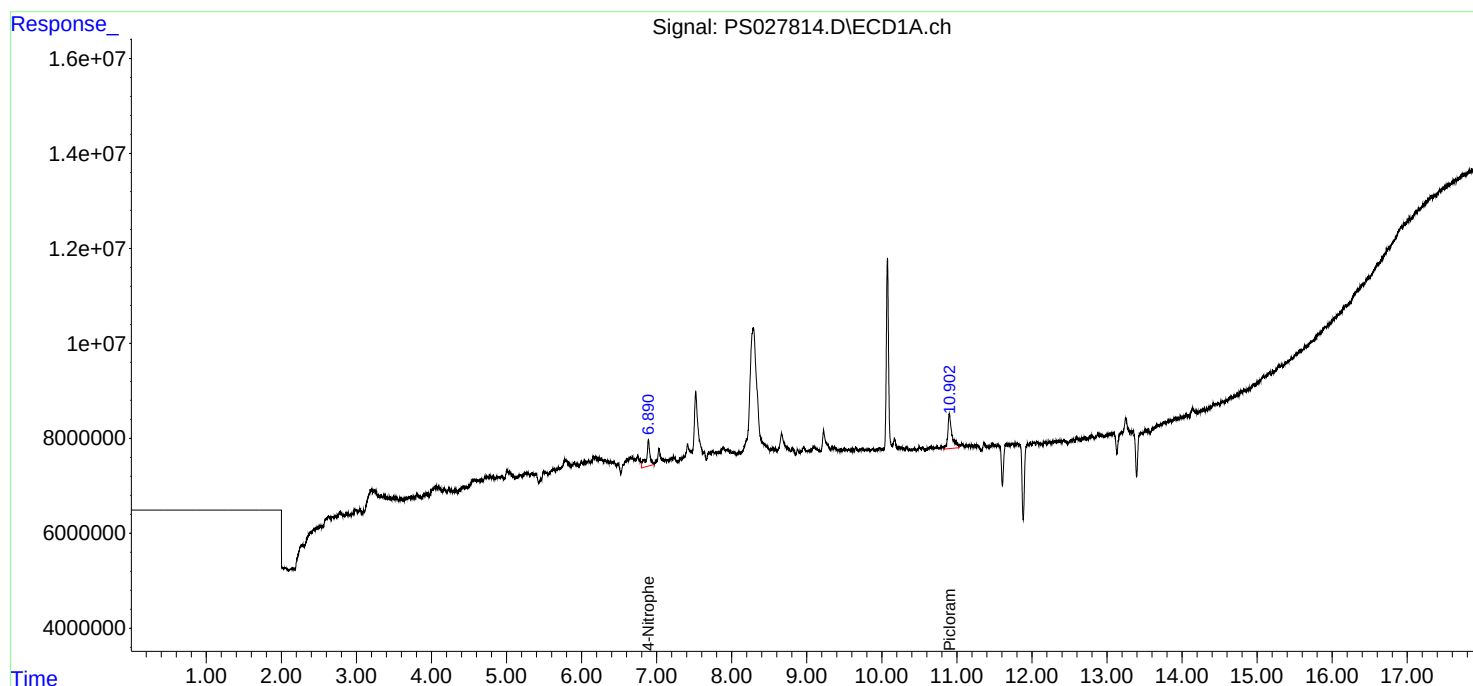


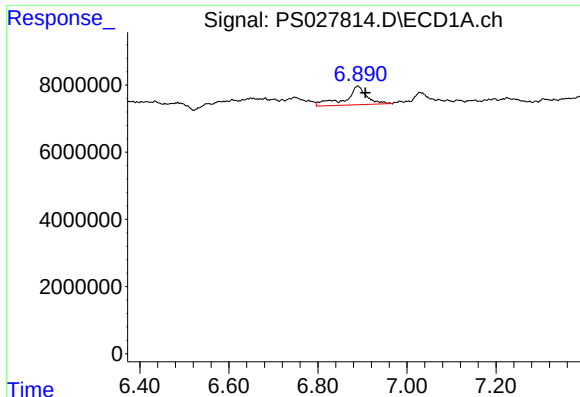

#3 4-Nitrophenol


R.T.: 6.890 min
Delta R.T.: -0.017 min
Response: 18192958
Conc: 10.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

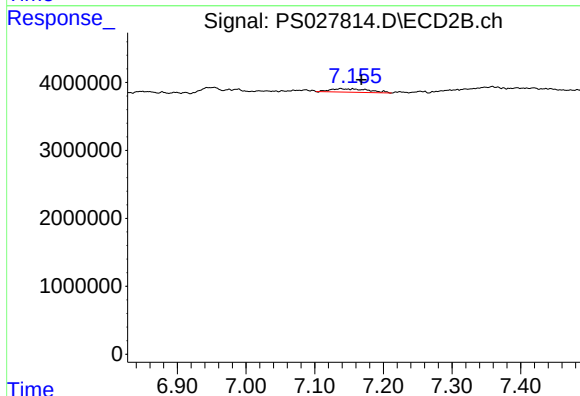


#3 4-Nitrophenol

R.T.: 7.138 min
Delta R.T.: -0.030 min
Response: 1940572
Conc: 2.71 ng/ml

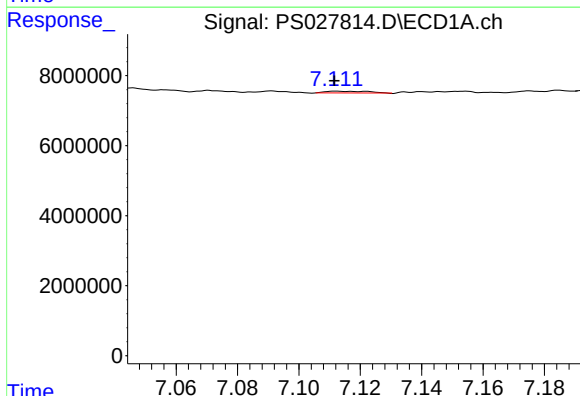


#4 2,4-DCAA

R.T.: 7.114 min
Delta R.T.: 0.002 min
Response: 455449
Conc: N.D.

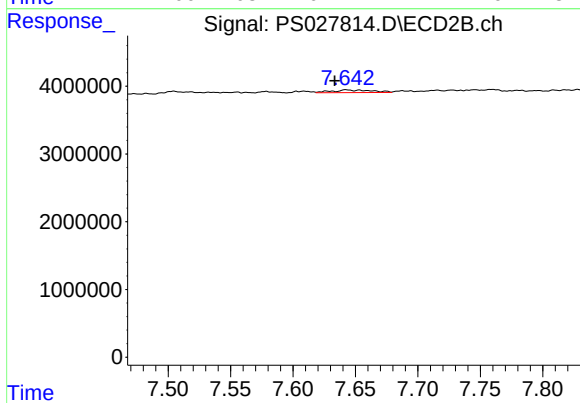

#4 2,4-DCAA


R.T.: 7.643 min
Delta R.T.: 0.010 min
Response: 881515
Conc: N.D.

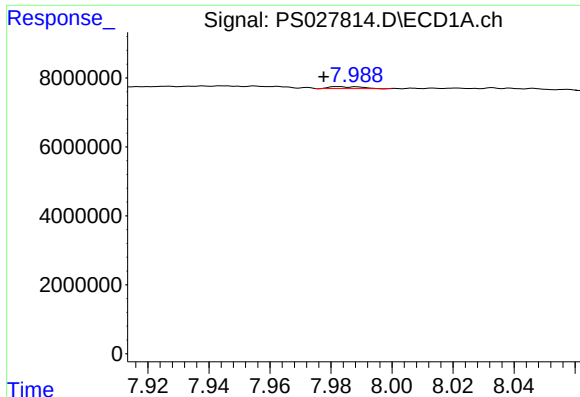

#8 DICHLORPROP


R.T.: 7.985 min
Delta R.T.: 0.007 min
Response: 401309
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

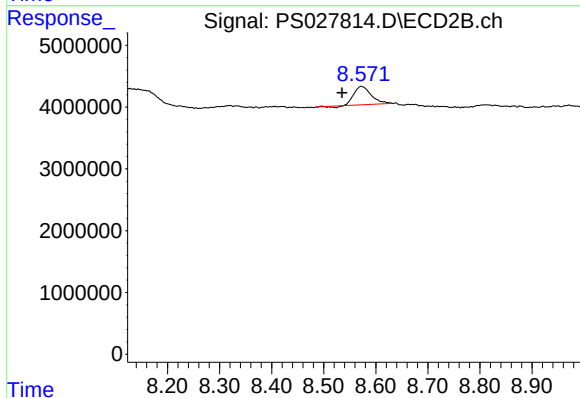


#8 DICHLORPROP

R.T.: 8.572 min
Delta R.T.: 0.037 min
Response: 6723305
Conc: 6.02 ng/ml

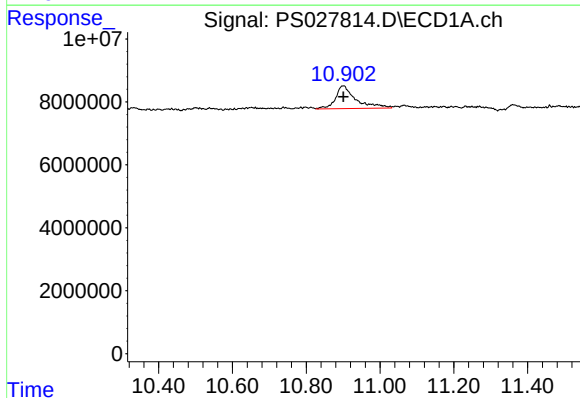

#15 Picloram

R.T.: 10.900 min
Delta R.T.: 0.000 min
Response: 27868959
Conc: 1.49 ng/ml

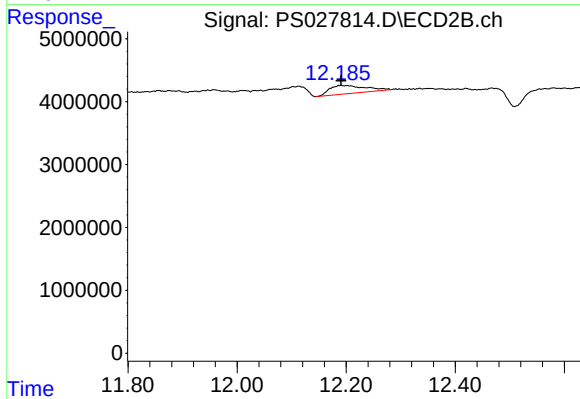

#15 Picloram

R.T.: 12.190 min
Delta R.T.: 0.000 min
Response: 6029496
Conc: 1.30 ng/ml