

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100324\
 Data File : PS027815.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2024 11:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 00:55:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.101	7.624	1334.5E6	545.8E6	536.465	550.756
Target Compounds							
1) T	Dalapon	2.522f	0.000	15062234	0	3.636	N.D. #
3) T	4-Nitroph...	6.900	0.000	10516672	0	6.211	N.D. #
5) T	DICAMBA	7.334f	7.851	272660	2601845	<MDL	<MDL #
6) T	MCP	0.000	7.912	0	1605251	N.D.	<MDL
8) T	DICHLORPROP	0.000	8.575f	0	3436587	N.D.	3.076
9) T	2,4-D	0.000	8.830f	0	1509572	N.D.	1.354
10) T	Pentachlo...	8.534f	0.000	1783212	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.016f	9.778	3826669	413357	<MDL	<MDL #
12) T	2,4,5-T	9.348	10.169	2364099	1102661	<MDL	<MDL #
13) T	2,4-DB	9.920	0.000	2387004	0	1.028	N.D. #
14) T	DINOSEB	11.058f	0.000	2239348	0	<MDL	N.D. #
15) T	Picloram	10.886	12.181	46816028	2404984	2.502	<MDL #
16) T	DCPA	11.364	12.124	2826689	2249675	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100324\
Data File : PS027815.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2024 11:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 00:55:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

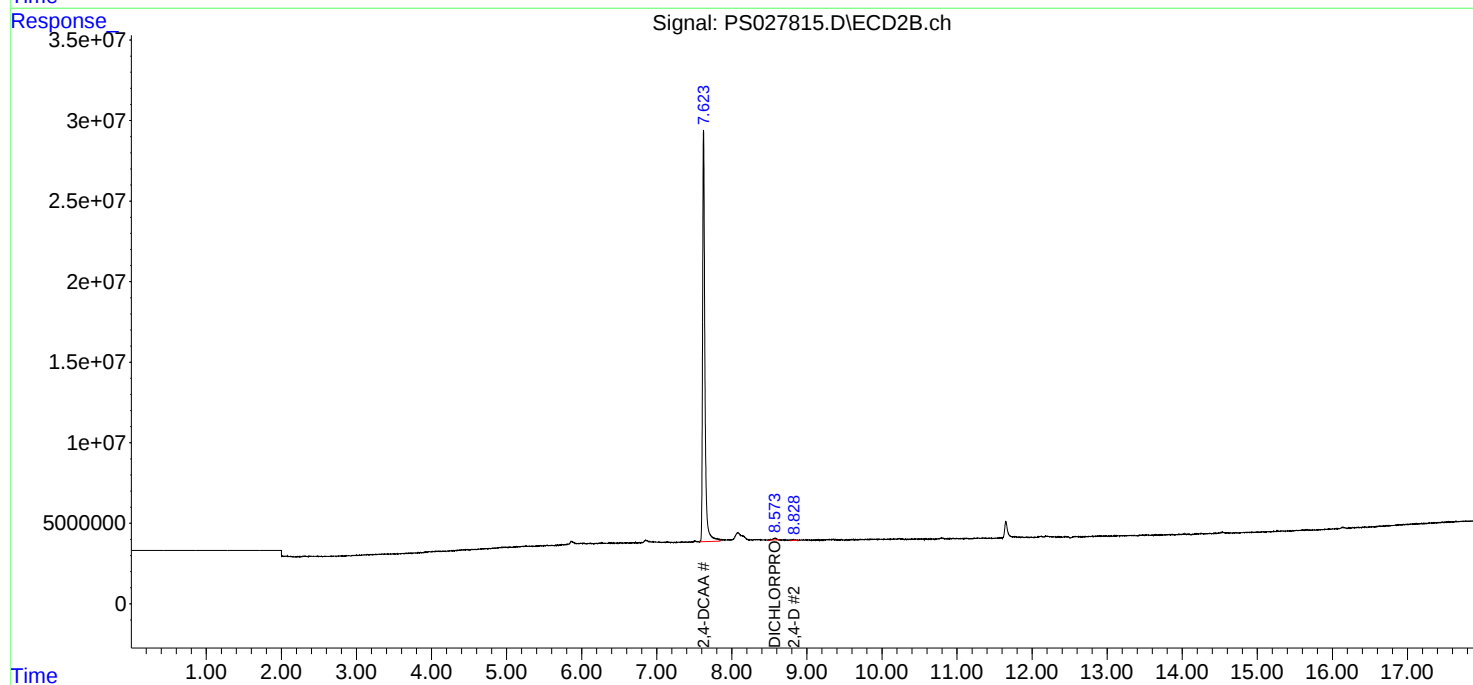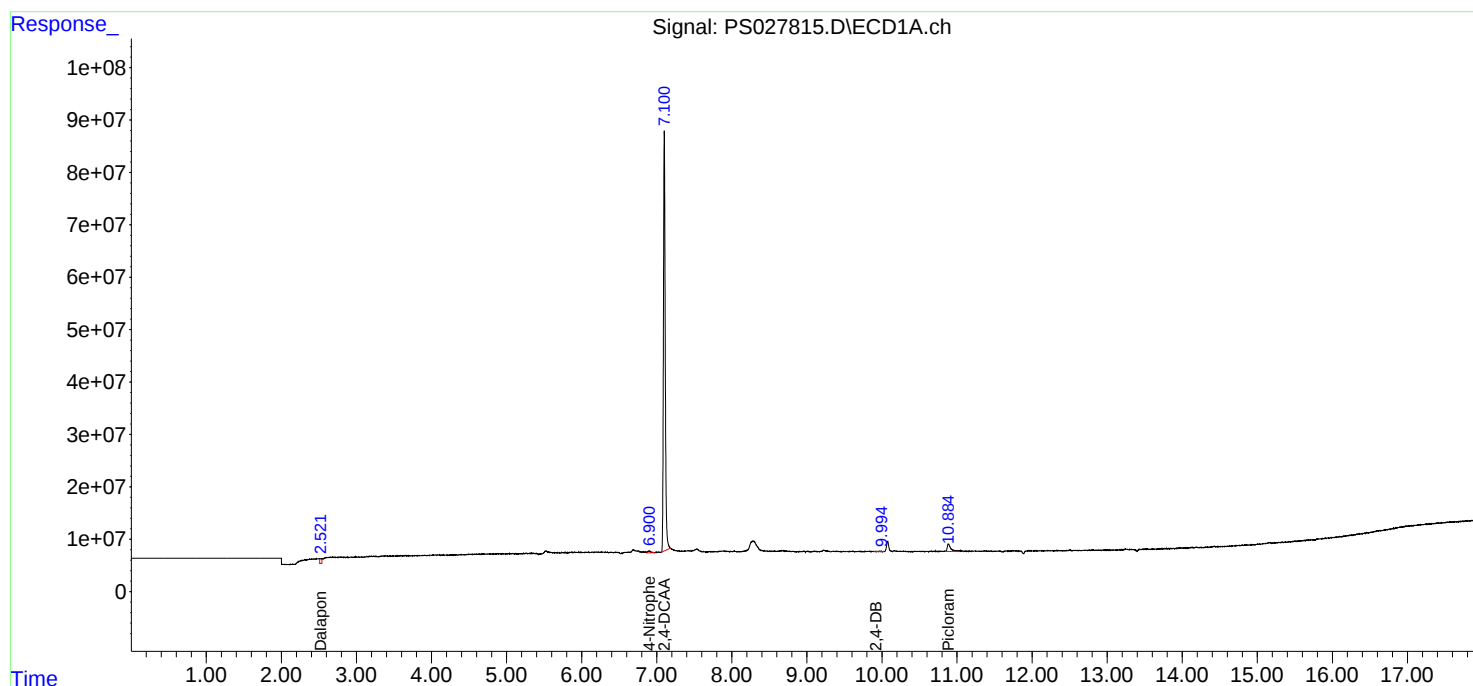


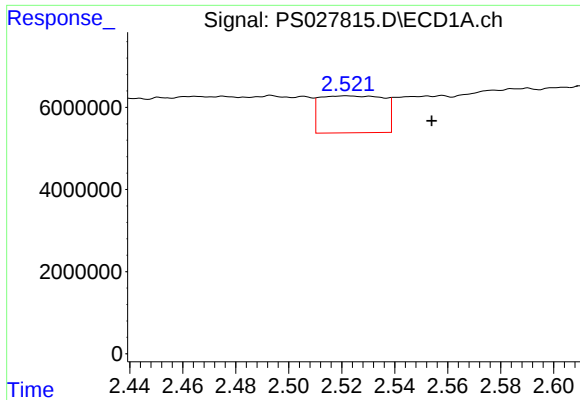

#1 Dalapon


R.T.: 2.522 min
Delta R.T.: -0.032 min
Response: 15062234
Conc: 3.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

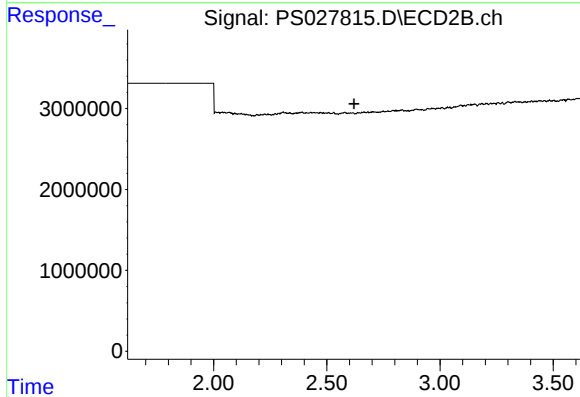


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.620 min
Response: 0
Conc: N.D.

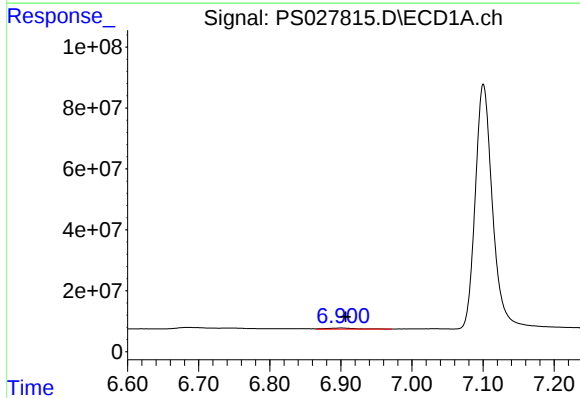


#3 4-Nitrophenol

R.T.: 6.900 min
Delta R.T.: -0.007 min
Response: 10516672
Conc: 6.21 ng/ml

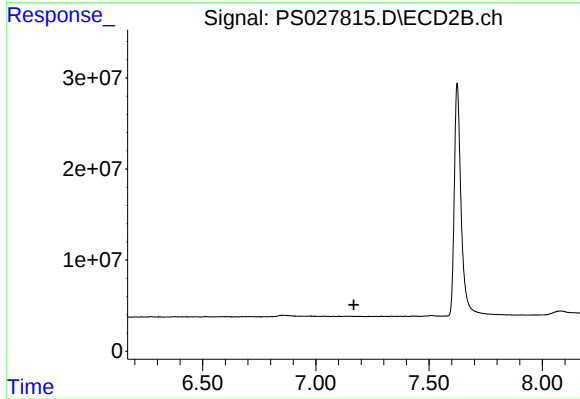

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.168 min
Response: 0
Conc: N.D.

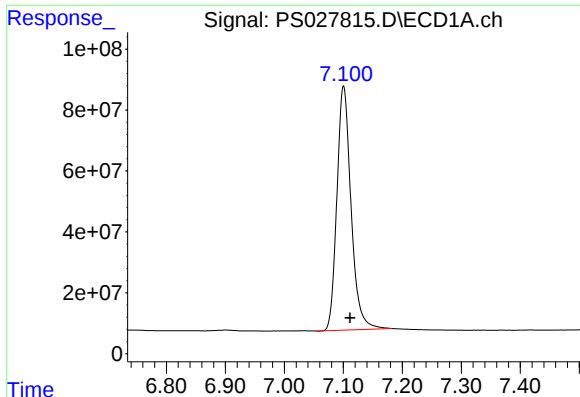

#4 2,4-DCAA


R.T.: 7.101 min
Delta R.T.: -0.011 min
Response: 1334512810
Conc: 536.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

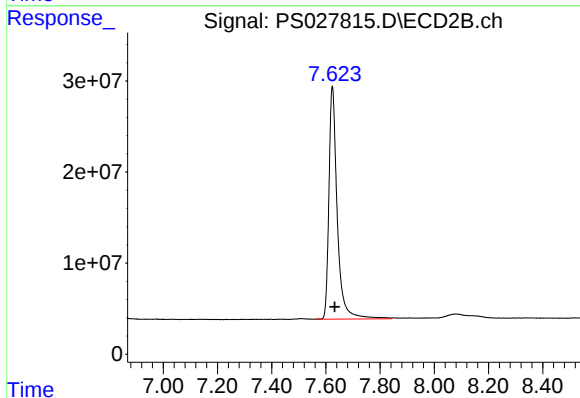


#4 2,4-DCAA

R.T.: 7.624 min
Delta R.T.: -0.009 min
Response: 545817735
Conc: 550.76 ng/ml

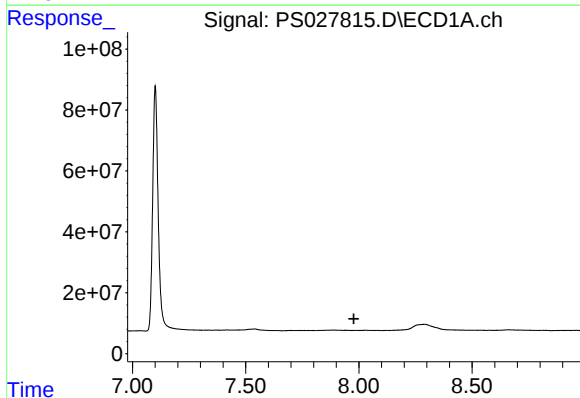


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.978 min
Response: 0
Conc: N.D.

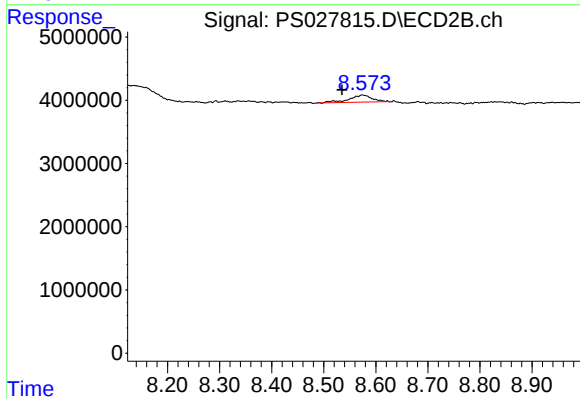

#8 DICHLORPROP


R.T.: 8.575 min
Delta R.T.: 0.040 min
Response: 3436587
Conc: 3.08 ng/ml

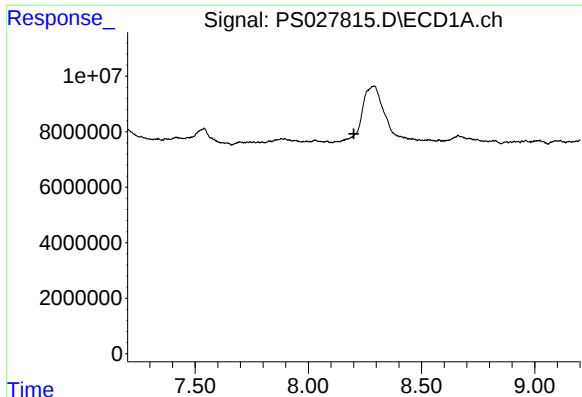

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.201 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

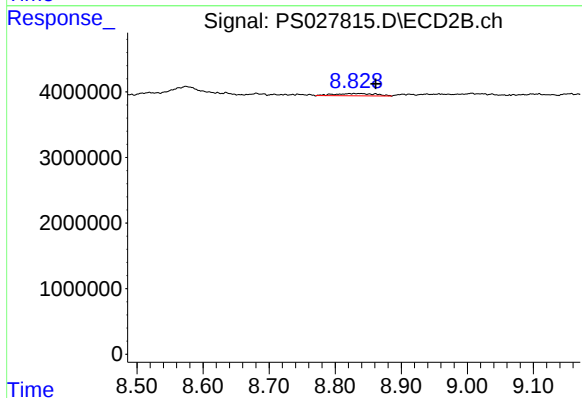


#9 2,4-D

R.T.: 8.830 min
Delta R.T.: -0.031 min
Response: 1509572
Conc: 1.35 ng/ml

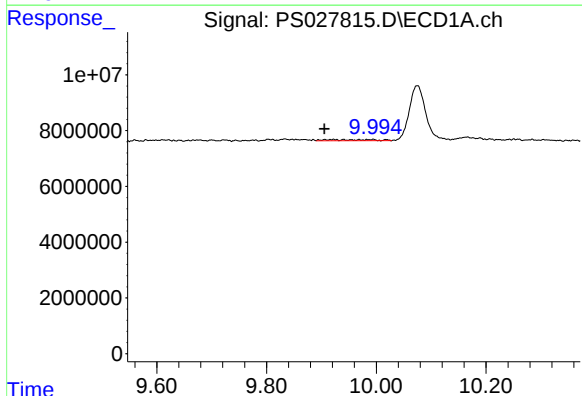


#13 2,4-DB

R.T.: 9.920 min
Delta R.T.: 0.015 min
Response: 2387004
Conc: 1.03 ng/ml

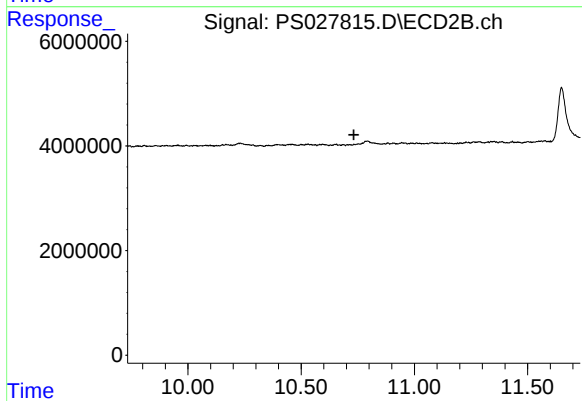

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.733 min
Response: 0
Conc: N.D.

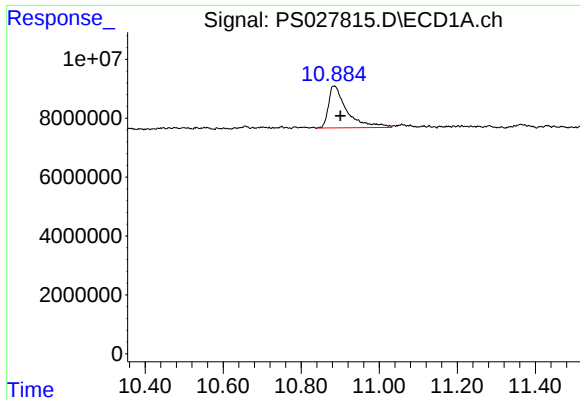

#15 Picloram

R.T.: 10.886 min
Delta R.T.: -0.015 min
Response: 46816028
Conc: 2.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

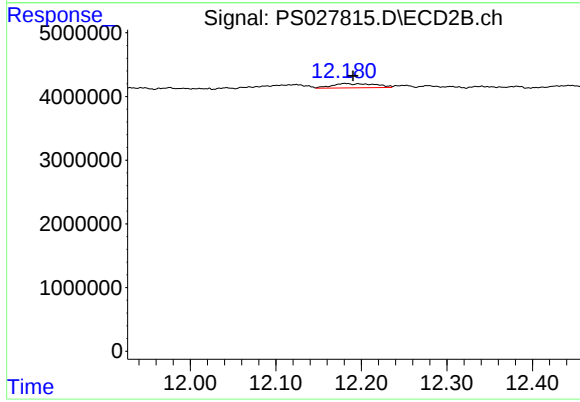

#15 Picloram

R.T.: 12.181 min
Delta R.T.: -0.009 min
Response: 2404984
Conc: N.D.