

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100324\
 Data File : PS027822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2024 19:00
 Operator : AR\AJ
 Sample : P4232-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:04:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.102	7.625	137.2E6	34543971	55.154	34.857 #
Target Compounds							
1) T	Dalapon	2.512f	0.000	58628716	0	14.151	N.D. #
2) T	3,5-DICHL...	0.000	6.598	0	959380	N.D.	<MDL
3) T	4-Nitroph...	6.902	7.171	36008954	15450807	21.268	21.556
5) T	DICAMBA	7.332f	7.795f	1653895	12968496	<MDL	2.943 #
6) T	MCP	7.506f	7.908	280.8E6	4505292	40.735	1.373 #
7) T	MCPA	7.620	8.162	6754993	24882555	<MDL	4.700 #
8) T	DICHLORPROP	0.000	8.565f	0	70575264	N.D.	63.170
9) T	2,4-D	8.192	8.847	19074759	1717522	6.223	1.540 #
10) T	Pentachlo...	8.473	9.359	15790387	2557851	<MDL	<MDL #
11) T	2,4,5-TP ...	9.032	9.800f	1499909	6374661	<MDL	1.063 #
12) T	2,4,5-T	9.329	10.157	24233789	20655894	1.619	3.952 #
13) T	2,4-DB	9.911	0.000	111.5E6	0	48.031	N.D. #
14) T	DINOSEB	11.075	11.102	4152182	6828132	<MDL	1.624 #
15) T	Picloram	10.892	12.177	88707320	20719499	4.742	4.458
16) T	DCPA	11.358	12.116f	70038725	17263599	4.220	2.679 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100324\
Data File : PS027822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2024 19:00
Operator : AR\AJ
Sample : P4232-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:04:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

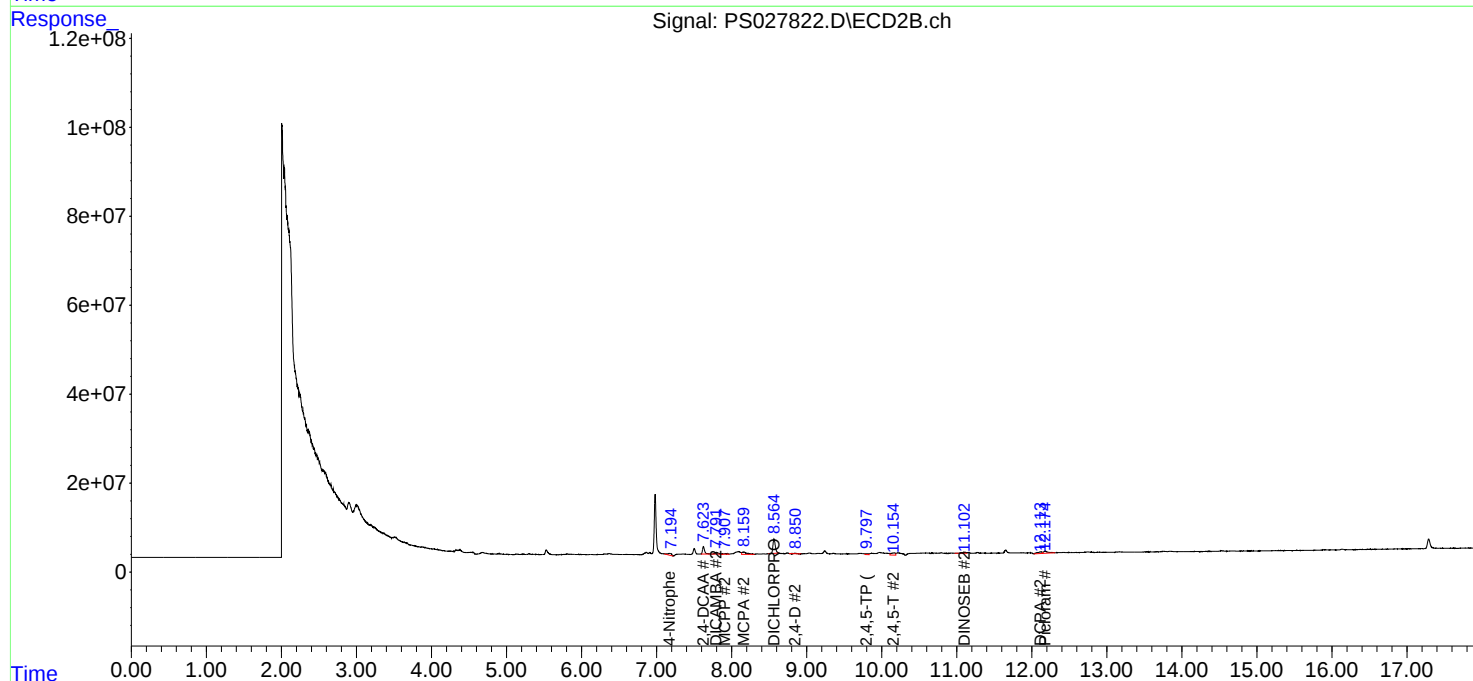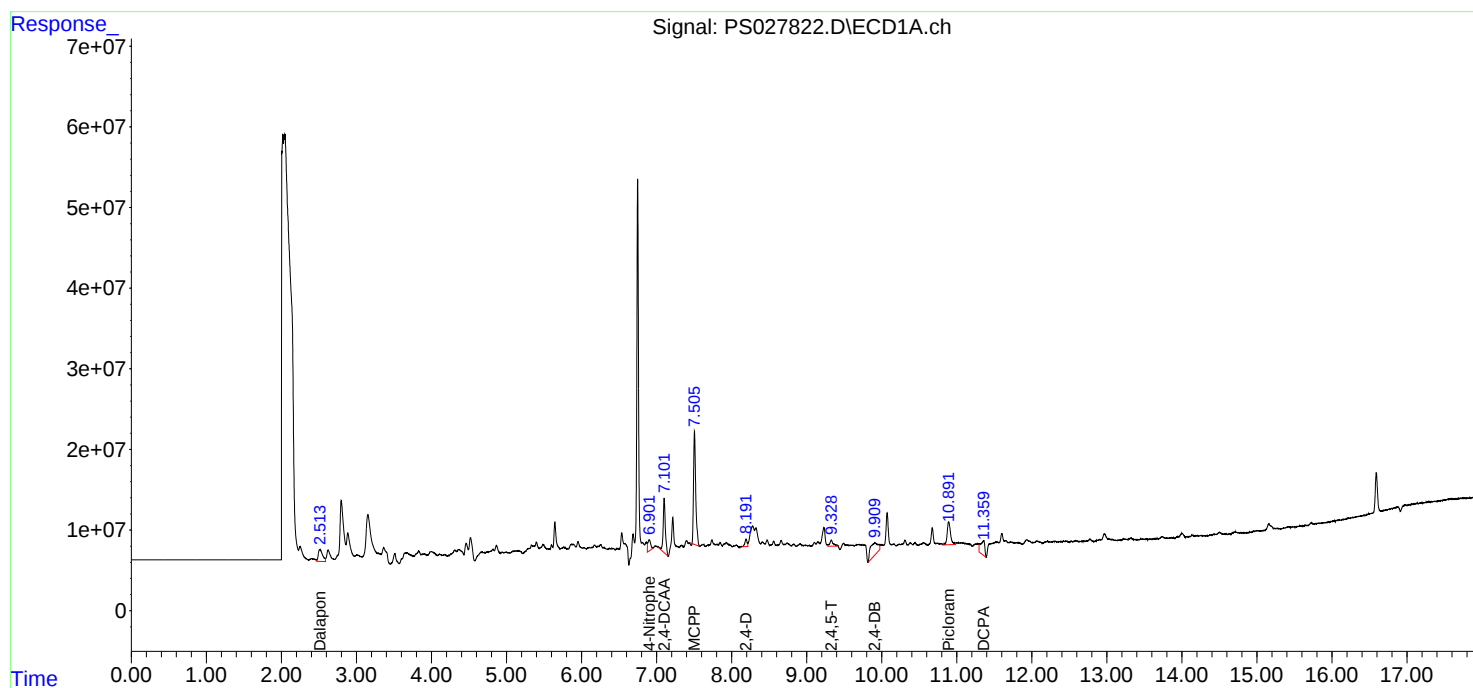


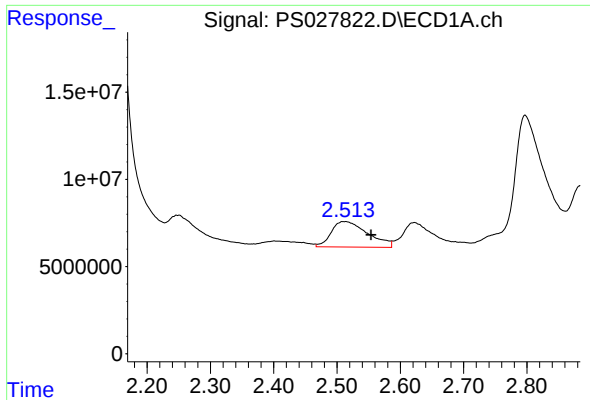

#1 Dalapon


R.T.: 2.512 min
Delta R.T.: -0.042 min
Response: 58628716
Conc: 14.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

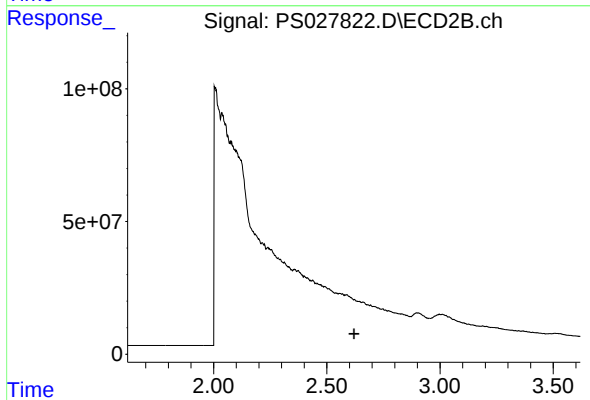


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.620 min
Response: 0
Conc: N.D.

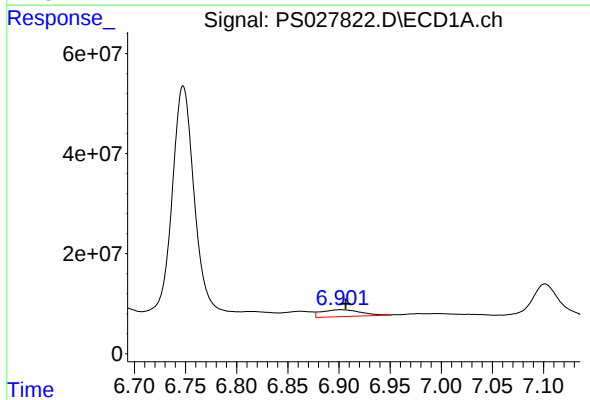


#3 4-Nitrophenol

R.T.: 6.902 min
Delta R.T.: -0.005 min
Response: 36008954
Conc: 21.27 ng/ml

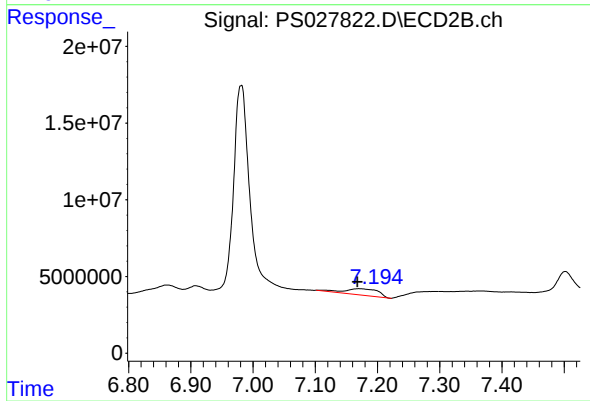

#3 4-Nitrophenol


R.T.: 7.171 min
Delta R.T.: 0.003 min
Response: 15450807
Conc: 21.56 ng/ml

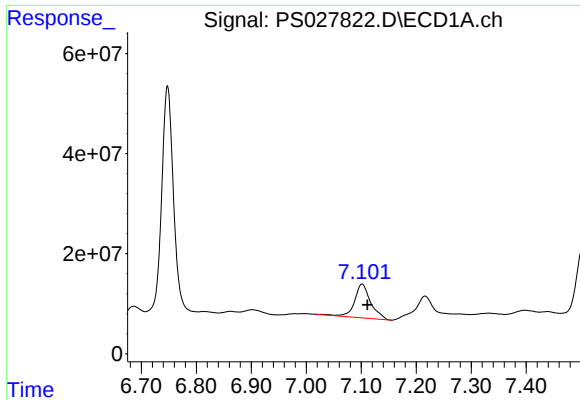

#4 2,4-DCAA


R.T.: 7.102 min
Delta R.T.: -0.010 min
Response: 137201395
Conc: 55.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

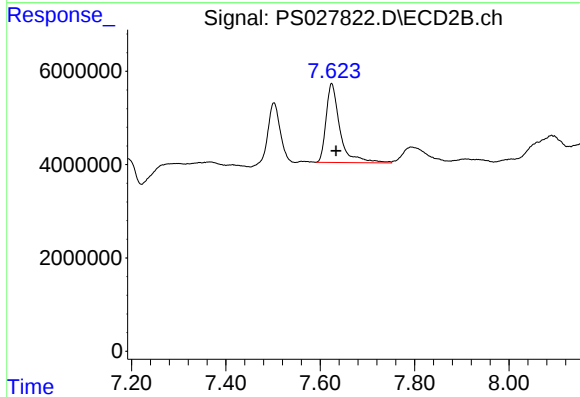


#4 2,4-DCAA

R.T.: 7.625 min
Delta R.T.: -0.009 min
Response: 34543971
Conc: 34.86 ng/ml

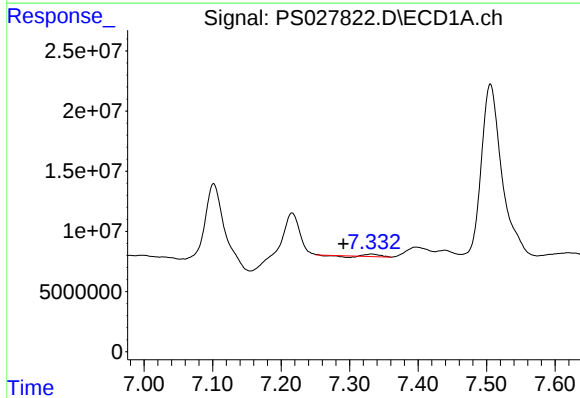


#5 DICAMBA

R.T.: 7.332 min
Delta R.T.: 0.041 min
Response: 1653895
Conc: N.D.

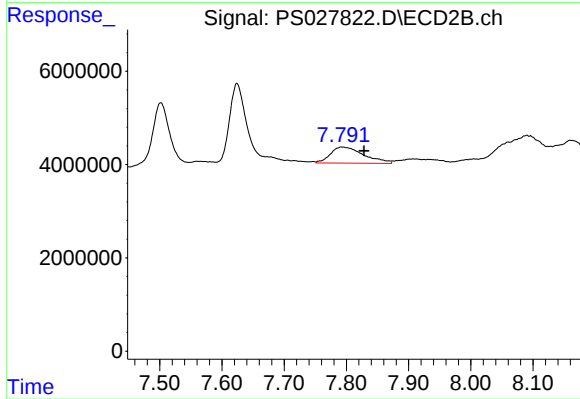

#5 DICAMBA


R.T.: 7.795 min
Delta R.T.: -0.033 min
Response: 12968496
Conc: 2.94 ng/ml

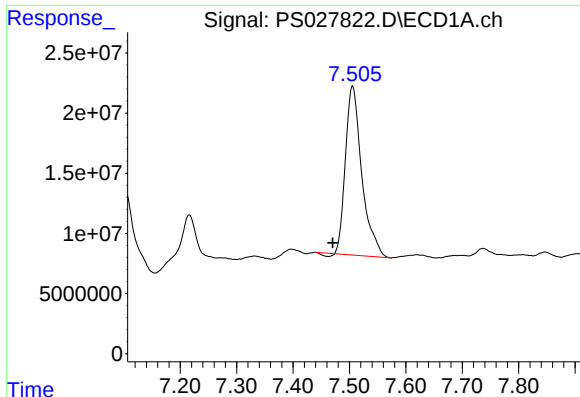

#6 MCPP


R.T.: 7.506 min
Delta R.T.: 0.035 min
Response: 280809225
Conc: 40.73 ug/ml

Instrument :
ECD_S
ClientSampleId :

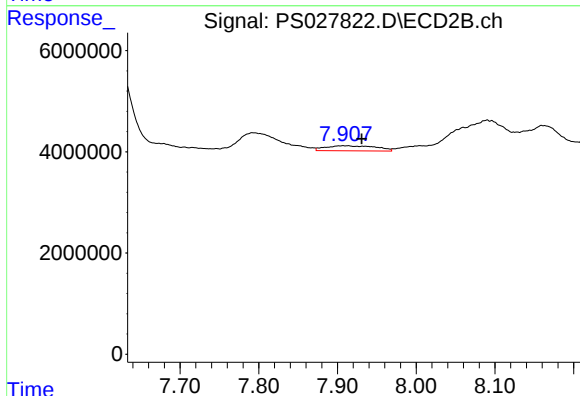


#6 MCPP

R.T.: 7.908 min
Delta R.T.: -0.023 min
Response: 4505292
Conc: 1.37 ug/ml

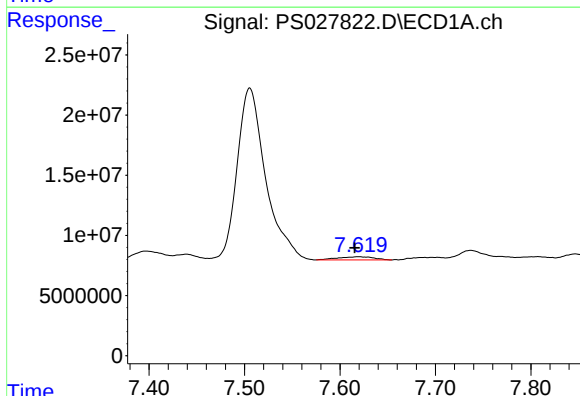


#7 MCPA

R.T.: 7.620 min
Delta R.T.: 0.004 min
Response: 6754993
Conc: N.D.

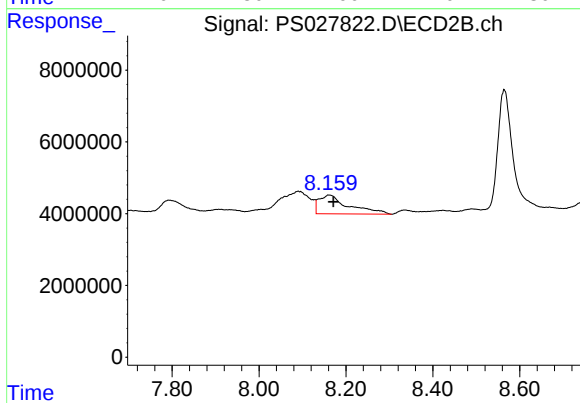

#7 MCPA


R.T.: 8.162 min
Delta R.T.: -0.009 min
Response: 24882555
Conc: 4.70 ug/ml

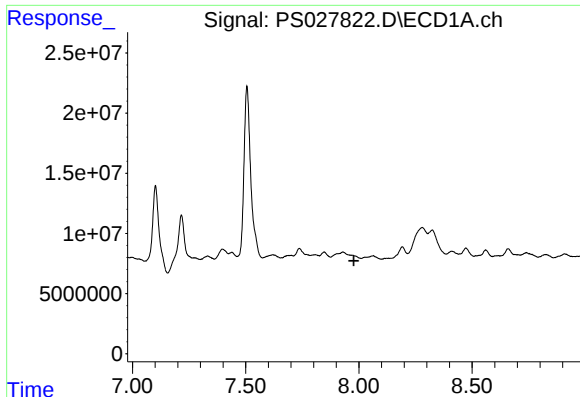

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

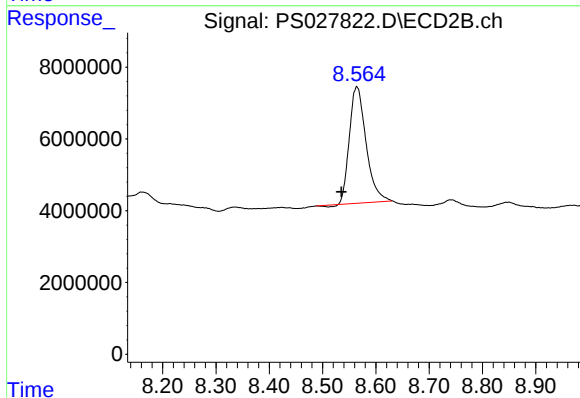


#8 DICHLORPROP

R.T.: 8.565 min
Delta R.T.: 0.029 min
Response: 70575264
Conc: 63.17 ng/ml

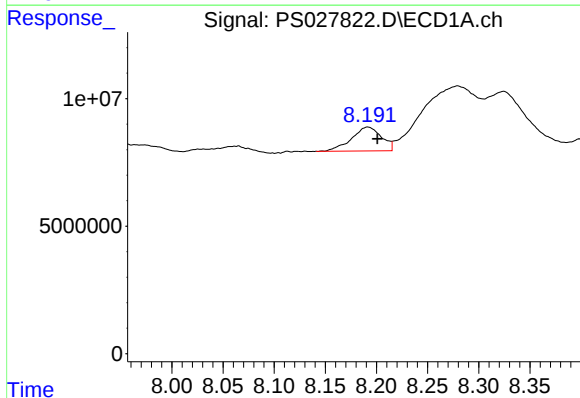


#9 2,4-D

R.T.: 8.192 min
Delta R.T.: -0.009 min
Response: 19074759
Conc: 6.22 ng/ml

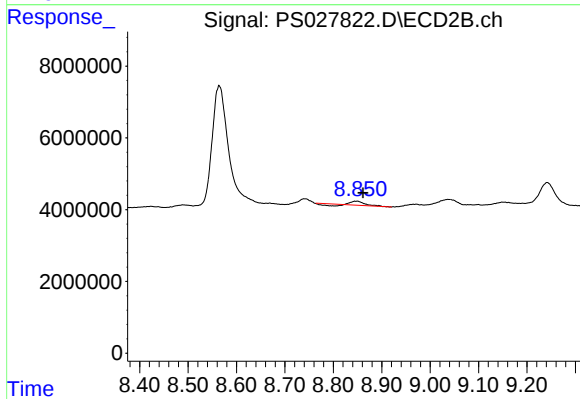

#9 2,4-D


R.T.: 8.847 min
Delta R.T.: -0.014 min
Response: 1717522
Conc: 1.54 ng/ml

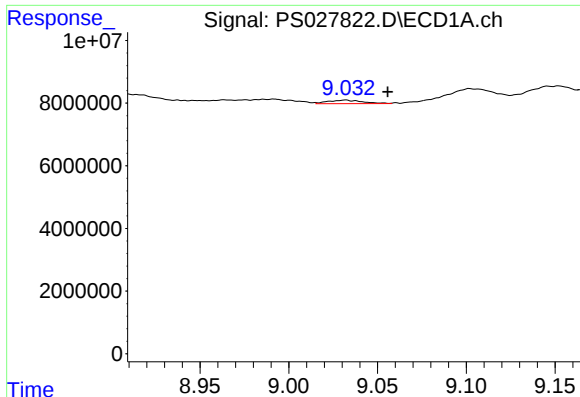

#11 2,4,5-TP (SILVEX)


R.T.: 9.032 min
Delta R.T.: -0.024 min
Response: 1499909
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

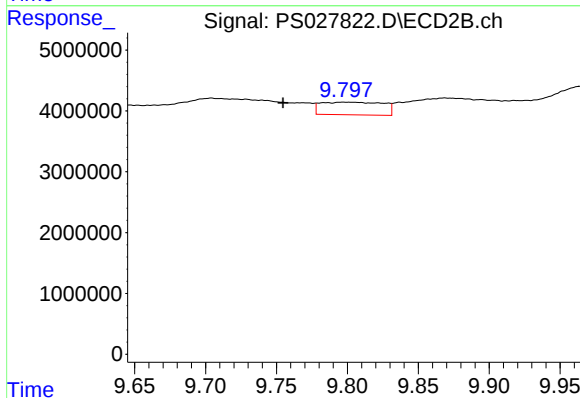


#11 2,4,5-TP (SILVEX)

R.T.: 9.800 min
Delta R.T.: 0.045 min
Response: 6374661
Conc: 1.06 ng/ml

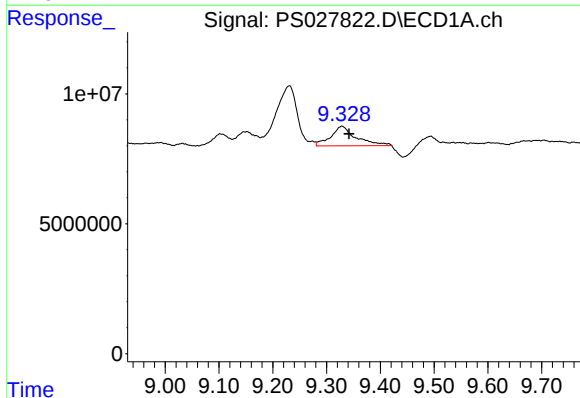


#12 2,4,5-T

R.T.: 9.329 min
Delta R.T.: -0.013 min
Response: 24233789
Conc: 1.62 ng/ml

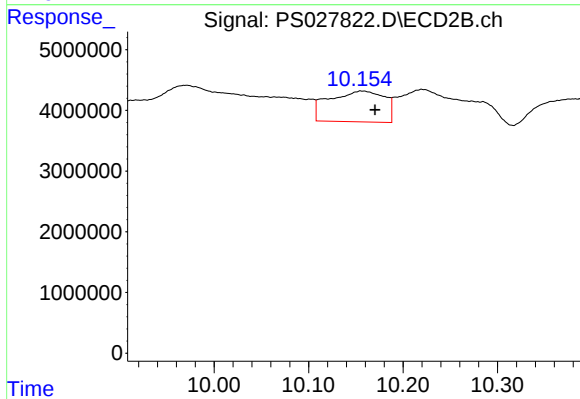

#12 2,4,5-T


R.T.: 10.157 min
Delta R.T.: -0.013 min
Response: 20655894
Conc: 3.95 ng/ml

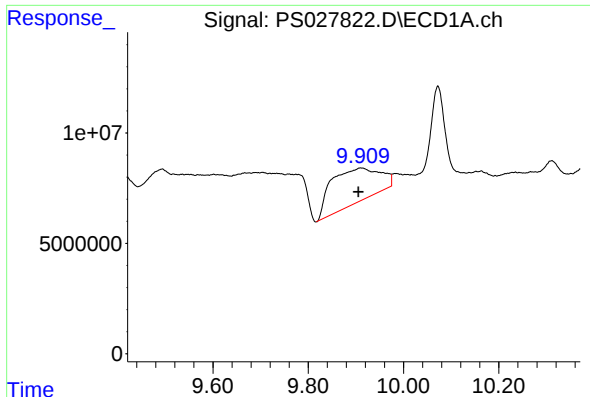

#13 2,4-DB


R.T.: 9.911 min
Delta R.T.: 0.006 min
Response: 111538346
Conc: 48.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

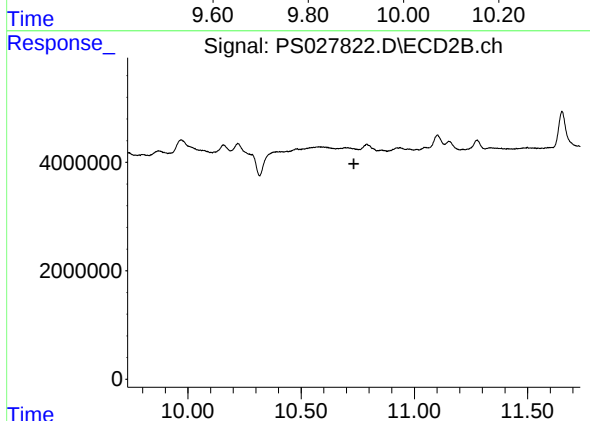


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.733 min
Response: 0
Conc: N.D.

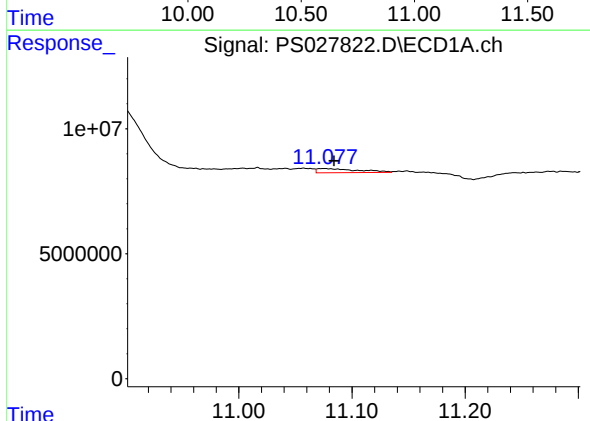


#14 DINOSEB

R.T.: 11.075 min
Delta R.T.: -0.009 min
Response: 4152182
Conc: N.D.

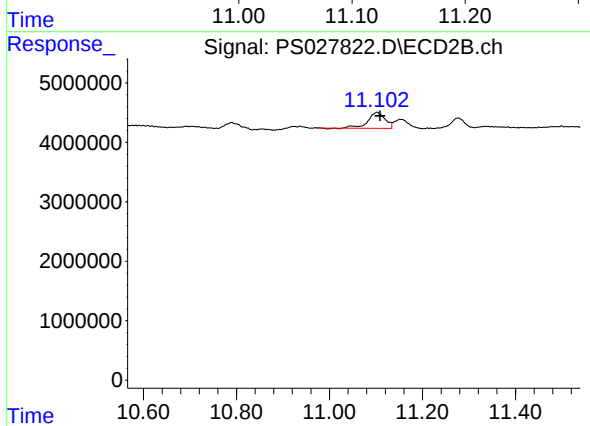

#14 DINOSEB


R.T.: 11.102 min
Delta R.T.: -0.007 min
Response: 6828132
Conc: 1.62 ng/ml

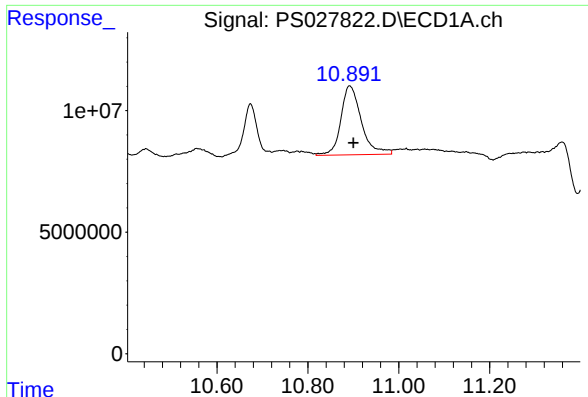

#15 Picloram


R.T.: 10.892 min
Delta R.T.: -0.009 min
Response: 88707320
Conc: 4.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

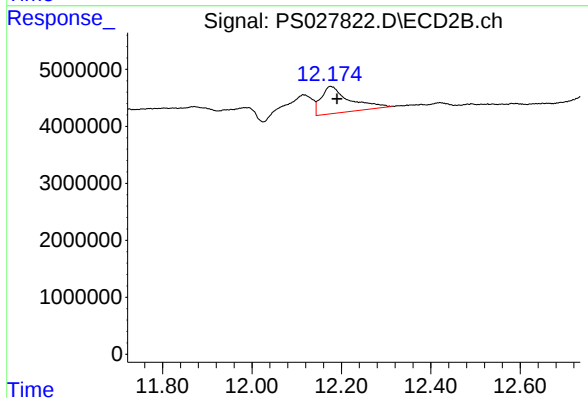


#15 Picloram

R.T.: 12.177 min
Delta R.T.: -0.013 min
Response: 20719499
Conc: 4.46 ng/ml

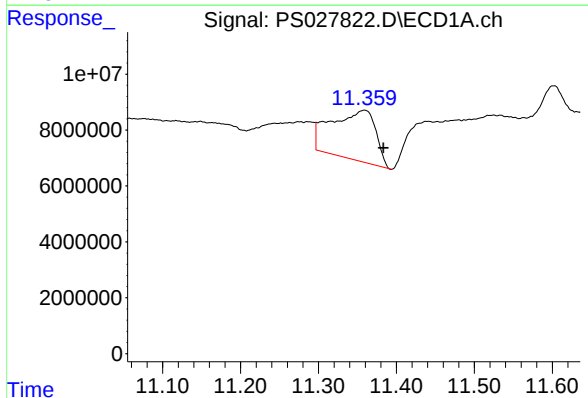

#16 DCPA

R.T.: 11.358 min
Delta R.T.: -0.025 min
Response: 70038725
Conc: 4.22 ng/ml

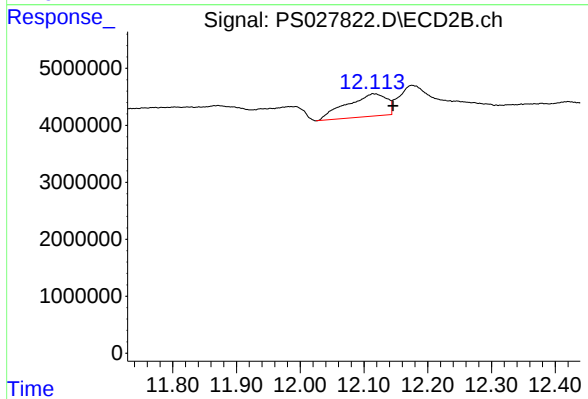

#16 DCPA

R.T.: 12.116 min
Delta R.T.: -0.029 min
Response: 17263599
Conc: 2.68 ng/ml