

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100324\
 Data File : PS027827.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2024 20:59
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:09:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
 Quant Title : 8080.M
 QLast Update : Sat Sep 14 02:36:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.099	7.623	1324.8E6	537.0E6	532.574	541.879
Target Compounds							
2) T	3,5-DICHL...	0.000	6.614	0	217403	N.D.	<MDL
3) T	4-Nitroph...	6.898	0.000	10329661	0	6.101	N.D. #
5) T	DICAMBA	0.000	7.801f	0	7802718	N.D.	1.771
6) T	MCP	7.518f	7.939	41185809	870443	5.974	<MDL #
8) T	DICHLORPROP	7.989	8.516	275146	152629	<MDL	<MDL #
10) T	Pentachlo...	0.000	9.361	0	1282746	N.D.	<MDL
11) T	2,4,5-TP ...	9.023f	9.771	2489055	612147	<MDL	<MDL #
12) T	2,4,5-T	9.378f	10.176	2231591	1613528	<MDL	<MDL #
13) T	2,4-DB	9.881	0.000	4267949	0	1.838	N.D. #
15) T	Picloram	10.911	12.208	9007708	2079069	<MDL	<MDL #
16) T	DCPA	11.356f	12.115f	3947016	1990447	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100324\
Data File : PS027827.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2024 20:59
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:09:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091224.M
Quant Title : 8080.M
QLast Update : Sat Sep 14 02:36:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

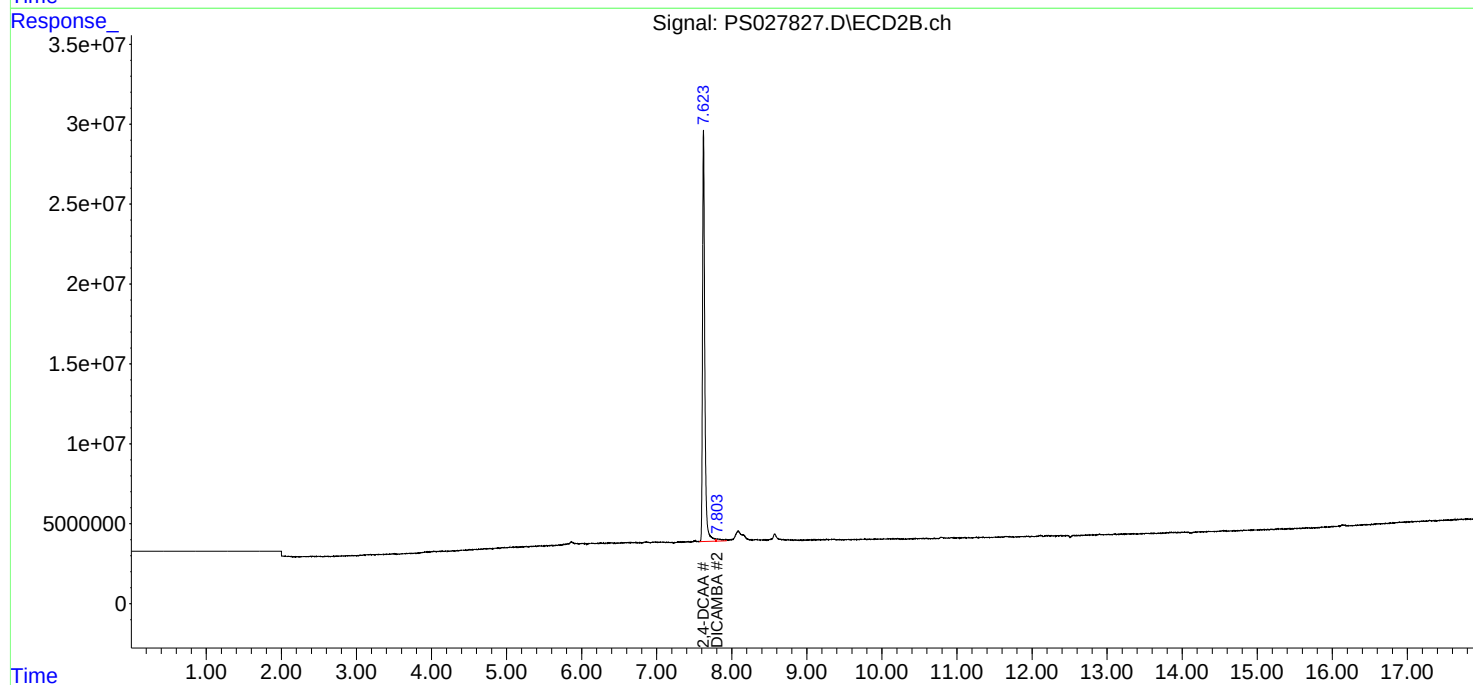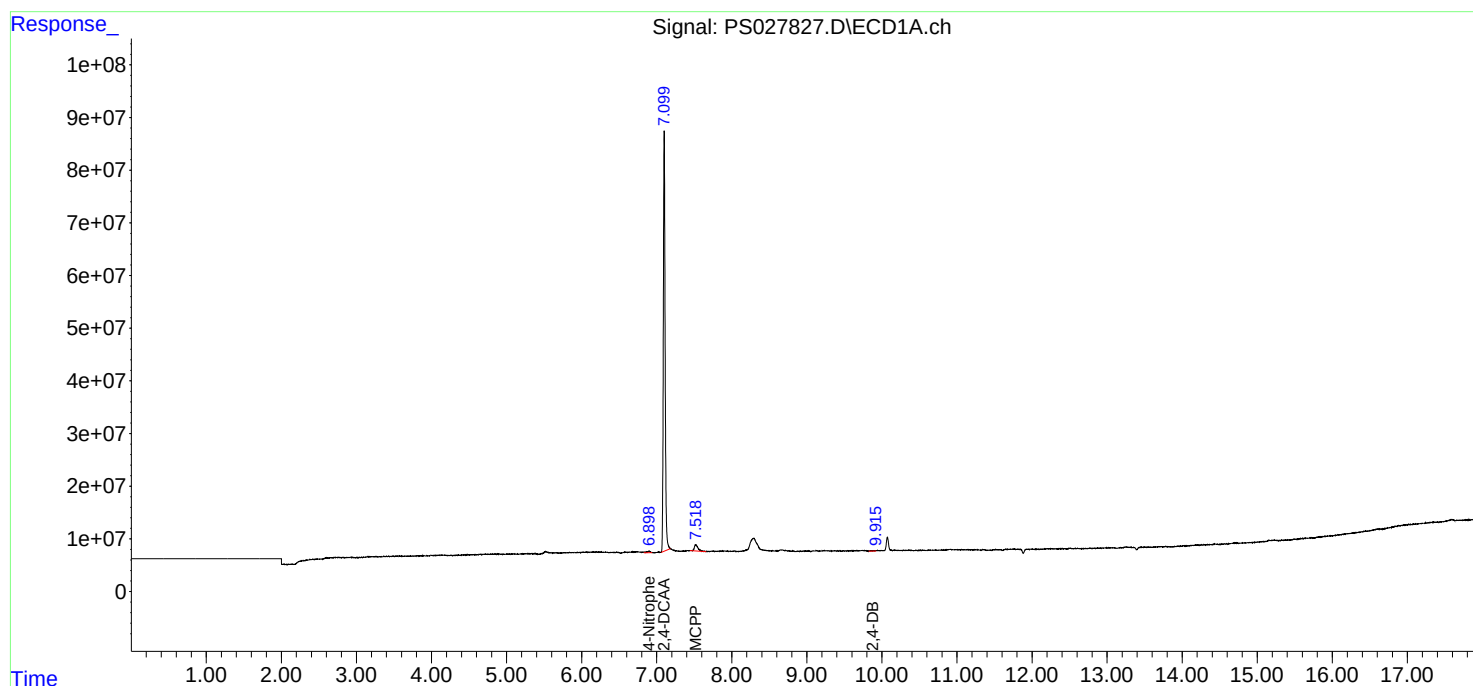


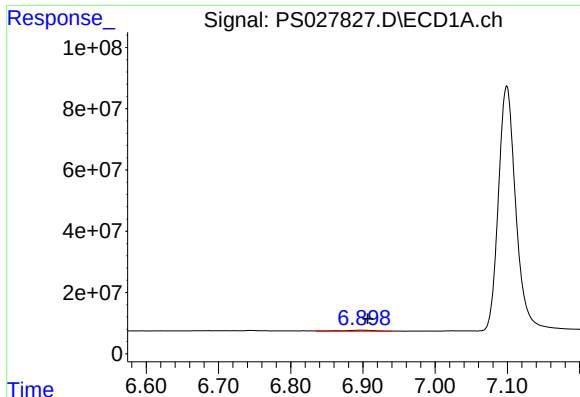

#3 4-Nitrophenol


R.T.: 6.898 min
Delta R.T.: -0.009 min
Response: 10329661
Conc: 6.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

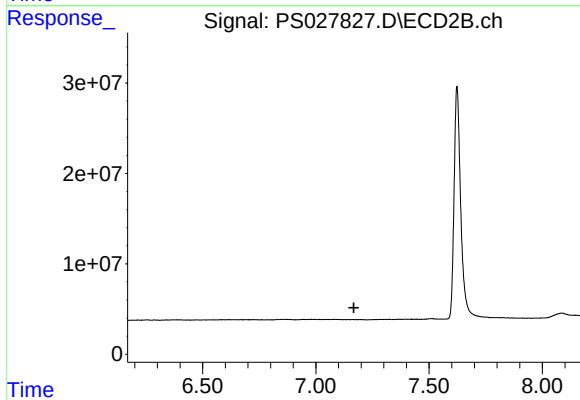


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.168 min
Response: 0
Conc: N.D.

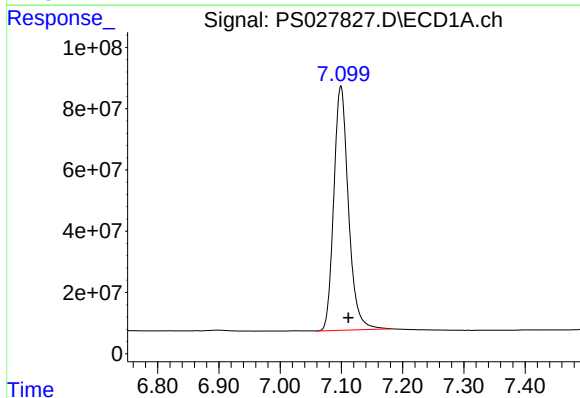


#4 2,4-DCAA

R.T.: 7.099 min
Delta R.T.: -0.012 min
Response: 1324835654
Conc: 532.57 ng/ml

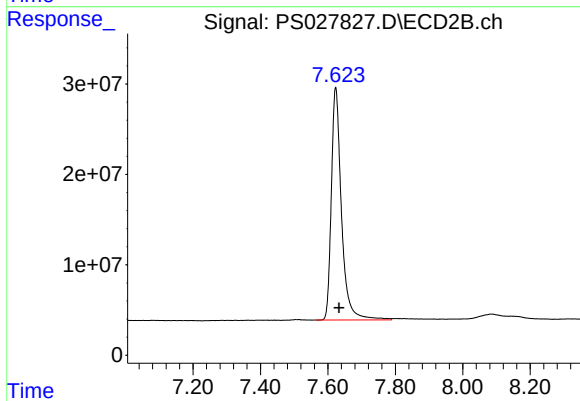

#4 2,4-DCAA


R.T.: 7.623 min
Delta R.T.: -0.010 min
Response: 537020349
Conc: 541.88 ng/ml

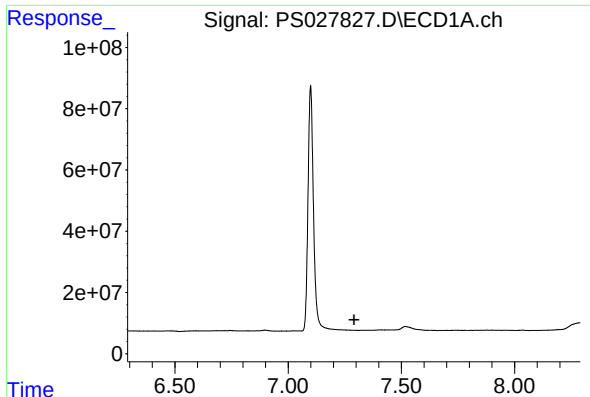

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

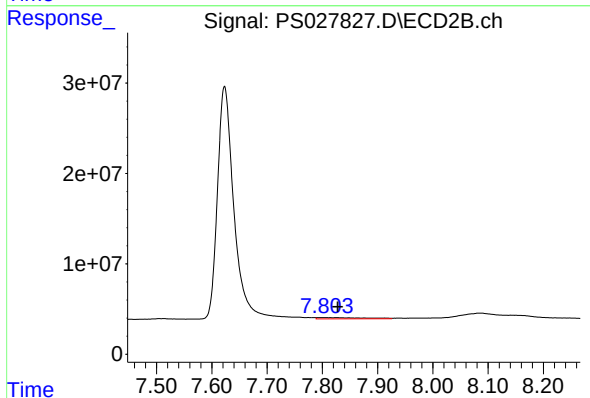


#5 DICAMBA

R.T.: 7.801 min
Delta R.T.: -0.027 min
Response: 7802718
Conc: 1.77 ng/ml

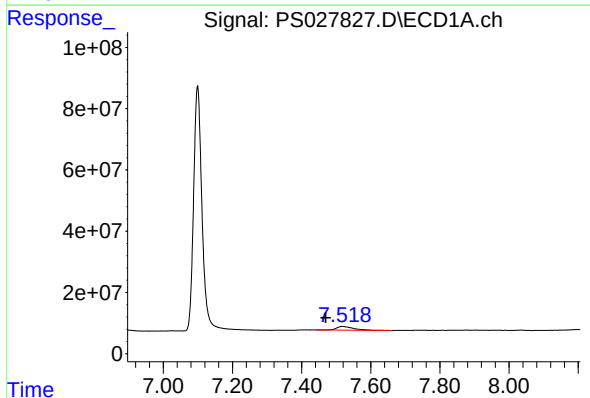


#6 MCP

R.T.: 7.518 min
Delta R.T.: 0.047 min
Response: 41185809
Conc: 5.97 ug/ml

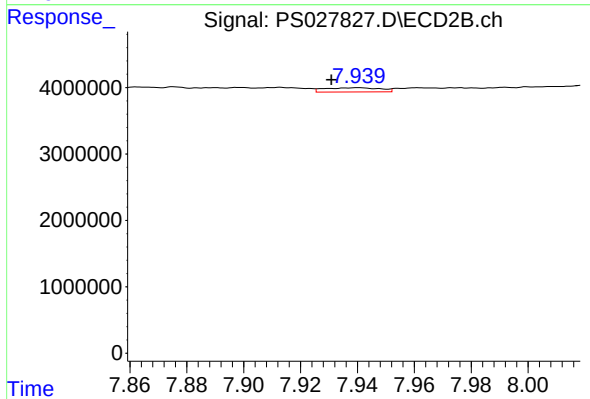

#6 MCP


R.T.: 7.939 min
Delta R.T.: 0.008 min
Response: 870443
Conc: N.D.

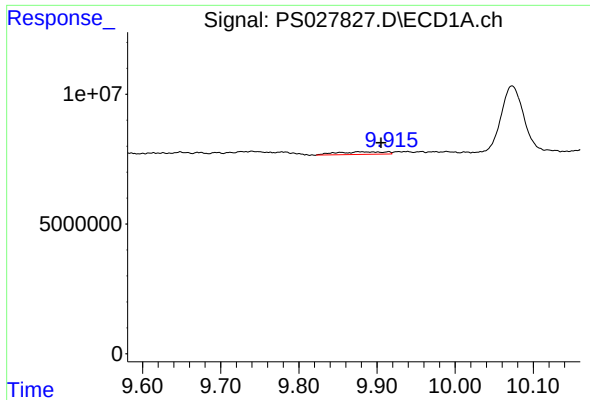

#13 2,4-DB

R.T.: 9.881 min
Delta R.T.: -0.024 min
Response: 4267949
Conc: 1.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

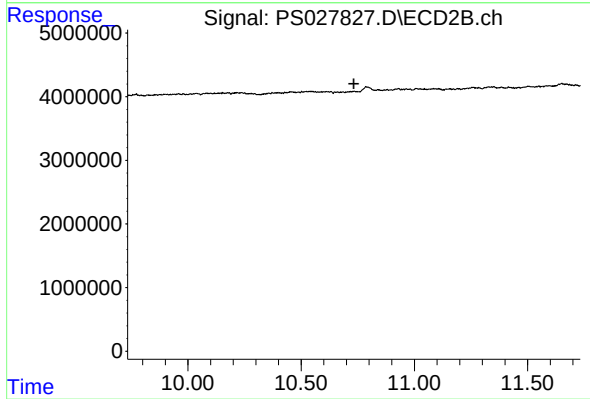

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.733 min
Response: 0
Conc: N.D.