

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100325\
 Data File : PS031944.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2025 13:40
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:29:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.283	7.745	1720.8E6	494.2E6	477.792	543.701
Target Compounds							
1) T	Dalapon	0.000	2.646f	0	38708110	N.D.	13.738
2) T	3,5-DICHL...	6.442	0.000	5468079	0	1.025	N.D. #
3) T	4-Nitroph...	7.071	0.000	4941948	0	4.480	N.D. #
7) T	MCPA	7.757f	8.241f	12659795	21785838	1.139	7.777 #
8) T	DICHLORPROP	8.184	8.700f	532269	2126172	<MDL	1.461 #
10) T	Pentachlo...	8.703	9.511	9276302	8850183	<MDL	<MDL #
11) T	2,4,5-TP ...	9.295	9.913	6170133	3470501	<MDL	<MDL #
12) T	2,4,5-T	9.628f	0.000	6872909	0	<MDL	N.D. #
13) T	2,4-DB	10.173	0.000	7850520	0	3.365	N.D. #
14) T	DINOSEB	11.347	0.000	11489208	0	<MDL	N.D. #
15) T	Picloram	11.190	0.000	5904020	0	<MDL	N.D. #
16) T	DCPA	11.652	0.000	3149780	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100325\
Data File : PS031944.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2025 13:40
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:29:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

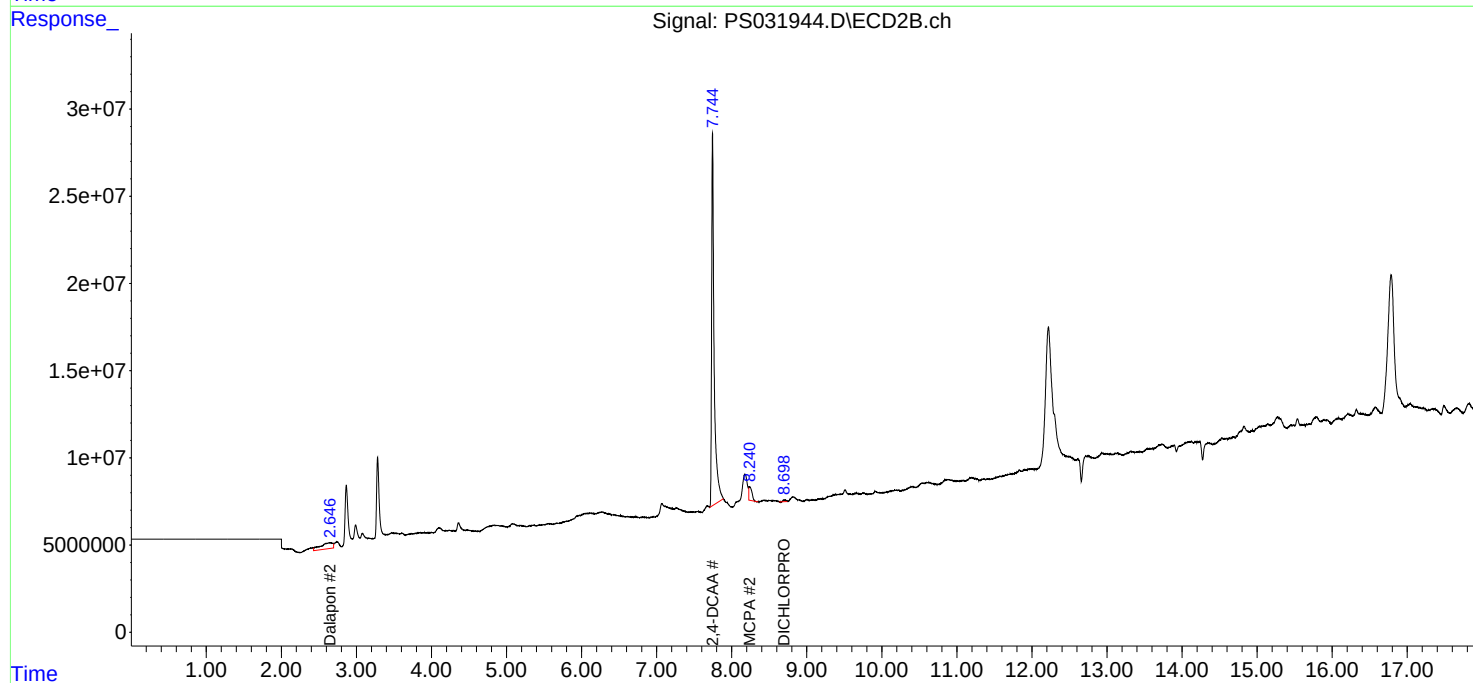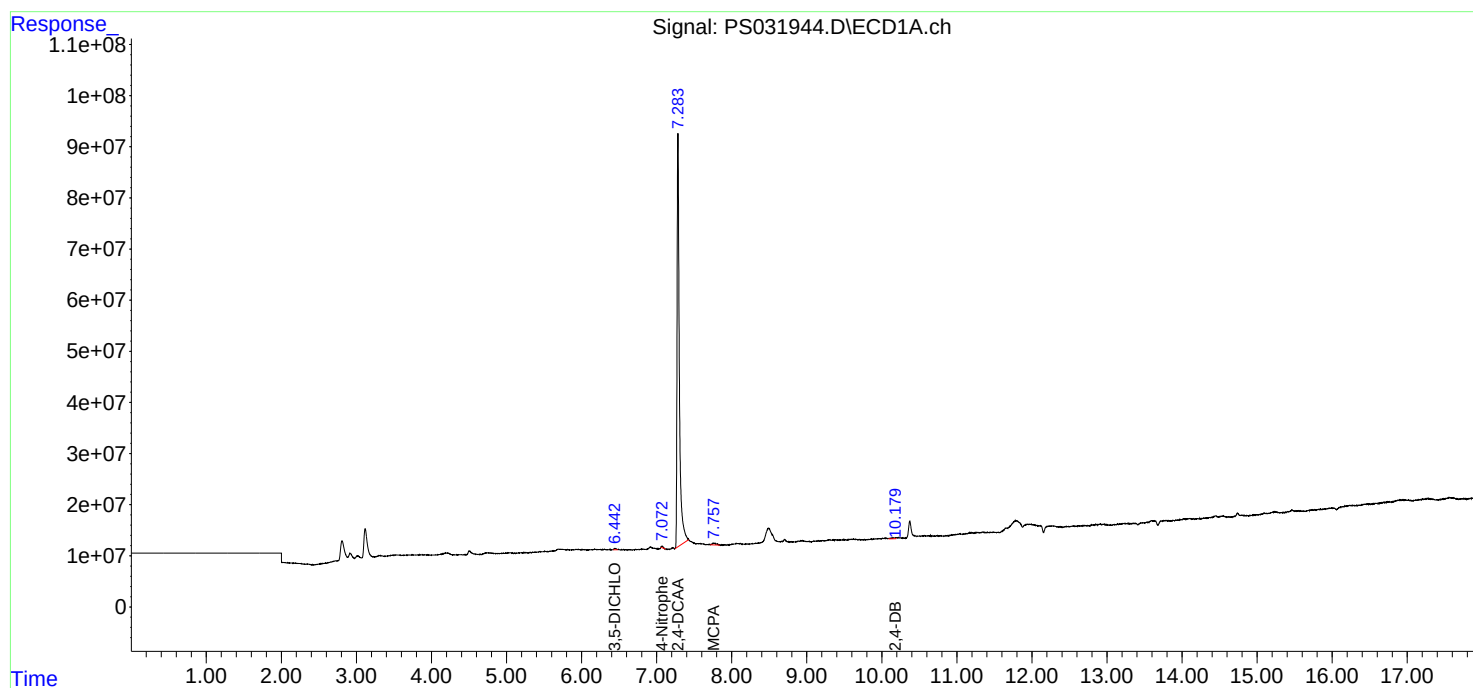


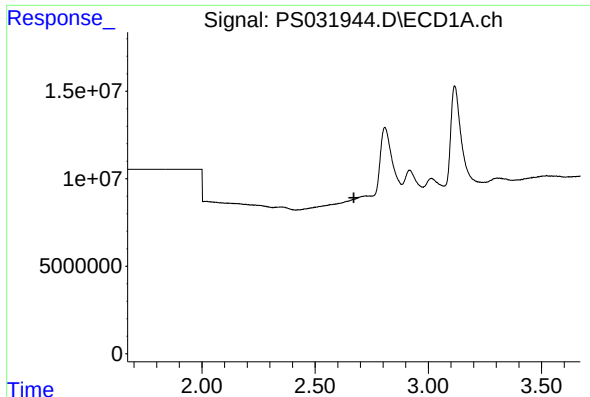

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

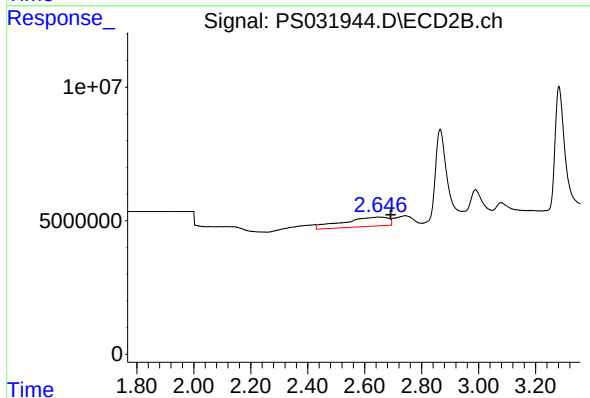


#1 Dalapon

R.T.: 2.646 min
Delta R.T.: -0.046 min
Response: 38708110
Conc: 13.74 ng/ml

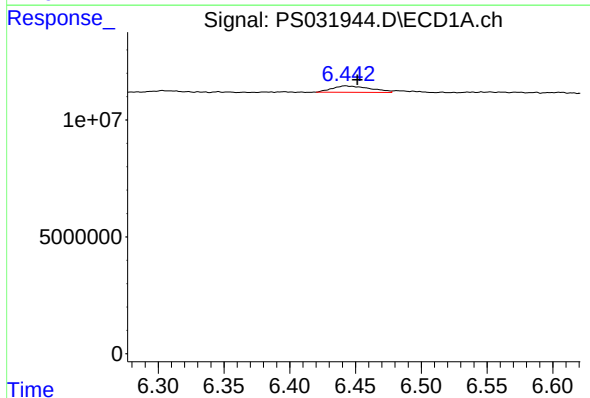


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.442 min
Delta R.T.: -0.009 min
Response: 5468079
Conc: 1.03 ng/ml

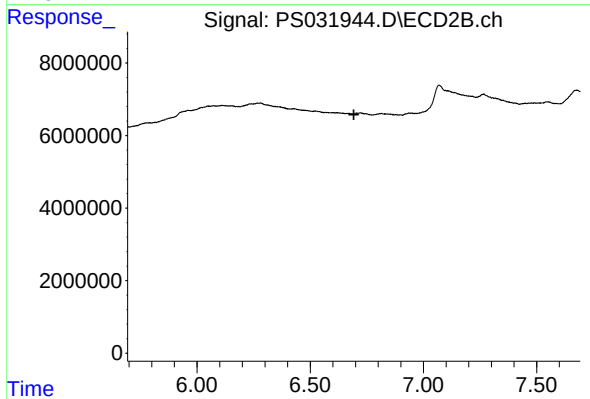

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.693 min
Response: 0
Conc: N.D.

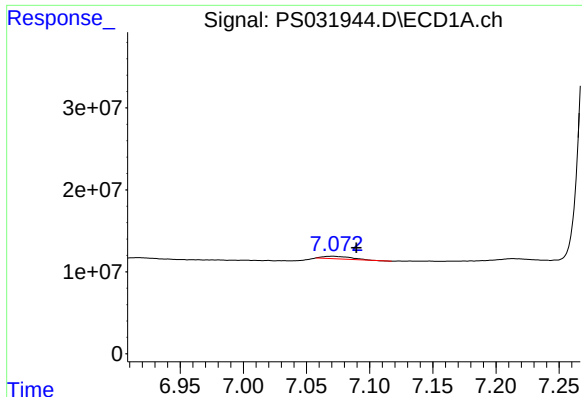

#3 4-Nitrophenol


R.T.: 7.071 min
Delta R.T.: -0.019 min
Response: 4941948
Conc: 4.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

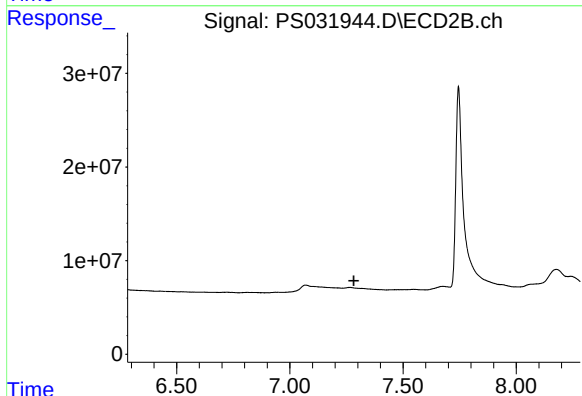


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

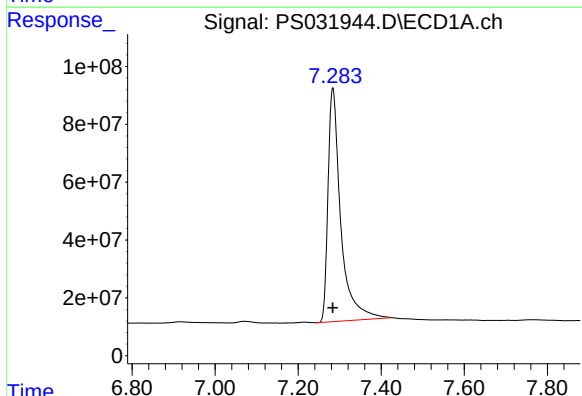


#4 2,4-DCAA

R.T.: 7.283 min
Delta R.T.: 0.000 min
Response: 1720780931
Conc: 477.79 ng/ml

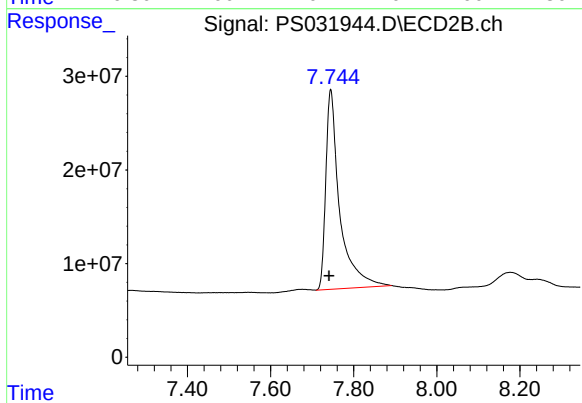

#4 2,4-DCAA


R.T.: 7.745 min
Delta R.T.: 0.004 min
Response: 494169989
Conc: 543.70 ng/ml

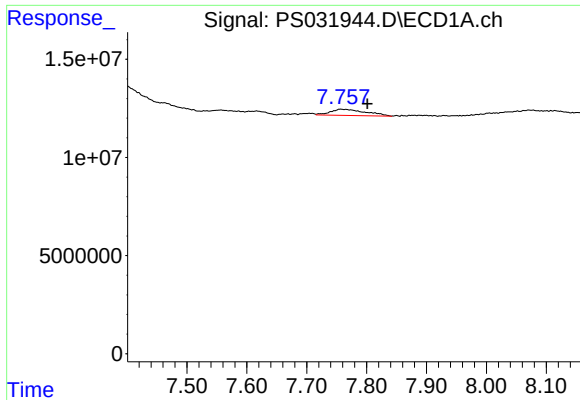

#7 MCPA


R.T.: 7.757 min
Delta R.T.: -0.045 min
Response: 12659795
Conc: 1.14 ug/ml

Instrument :
ECD_S
ClientSampleId :

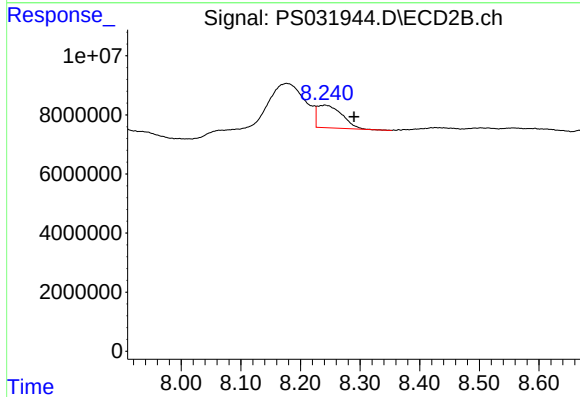


#7 MCPA

R.T.: 8.241 min
Delta R.T.: -0.049 min
Response: 21785838
Conc: 7.78 ug/ml

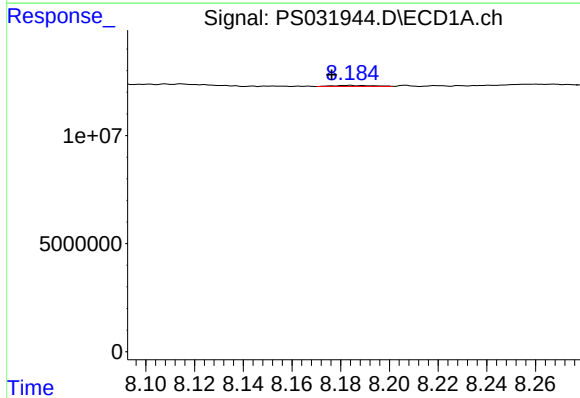


#8 DICHLORPROP

R.T.: 8.184 min
Delta R.T.: 0.007 min
Response: 532269
Conc: N.D.

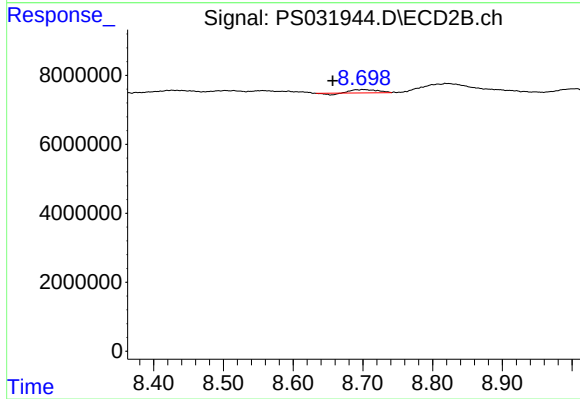

#8 DICHLORPROP


R.T.: 8.700 min
Delta R.T.: 0.043 min
Response: 2126172
Conc: 1.46 ng/ml

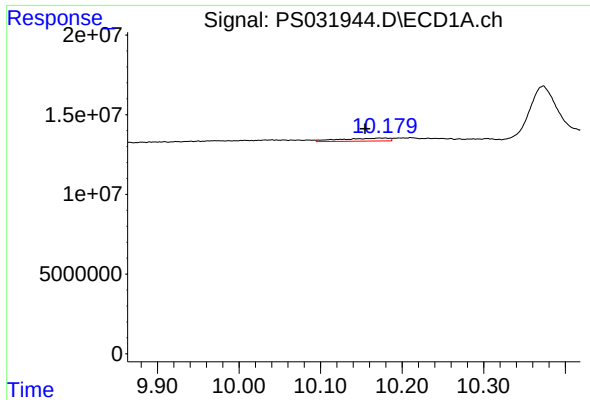

#13 2,4-DB

R.T.: 10.173 min
Delta R.T.: 0.019 min
Response: 7850520
Conc: 3.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

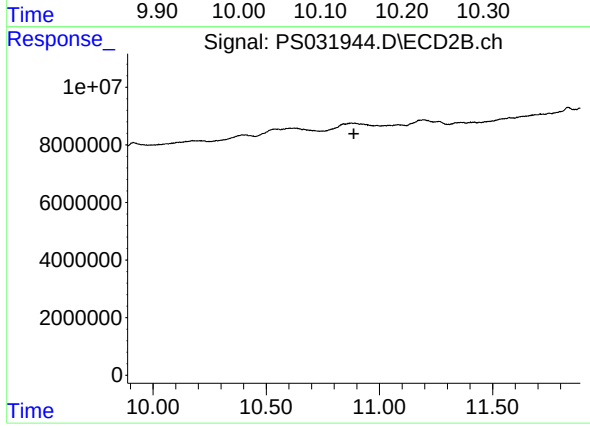

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.887 min
Response: 0
Conc: N.D.