

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100325\
 Data File : PS031946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2025 16:21
 Operator : AR\AJ
 Sample : PB169975BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:30:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.283	7.737	1466.2E6	437.1E6	407.101	480.950
Target Compounds							
1) T	Dalapon	0.000	2.649f	0	1328.0E6	N.D.	471.311
3) T	4-Nitroph...	0.000	7.246f	0	6069642	N.D.	4.807
5) T	DICAMBA	7.447	0.000	96437	0	<MDL	N.D. #
8) T	DICHLORPROP	8.170	8.650	18760040	5820362	5.267	4.000
9) T	2,4-D	8.452f	9.045f	31126532	2027992	9.086	1.233 #
10) T	Pentachlo...	8.706	9.466f	1640492	27754502	<MDL	<MDL #
11) T	2,4,5-TP ...	9.331f	9.876	216.8E6	230.9E6	10.338	15.338 #
12) T	2,4,5-T	9.600	10.339	128.6E6	116.2E6	7.028	8.635
13) T	2,4-DB	10.186f	10.918f	196.1E6	10630473	84.073	9.935 #
14) T	DINOSEB	11.325f	0.000	53515061	0	3.710	N.D. #
15) T	Picloram	11.163	12.420f	18082225	147.0E6	1.004	6.208 #
16) T	DCPA	11.621f	12.303	35910862	18258620	1.333	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100325\
Data File : PS031946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2025 16:21
Operator : AR\AJ
Sample : PB169975BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:30:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

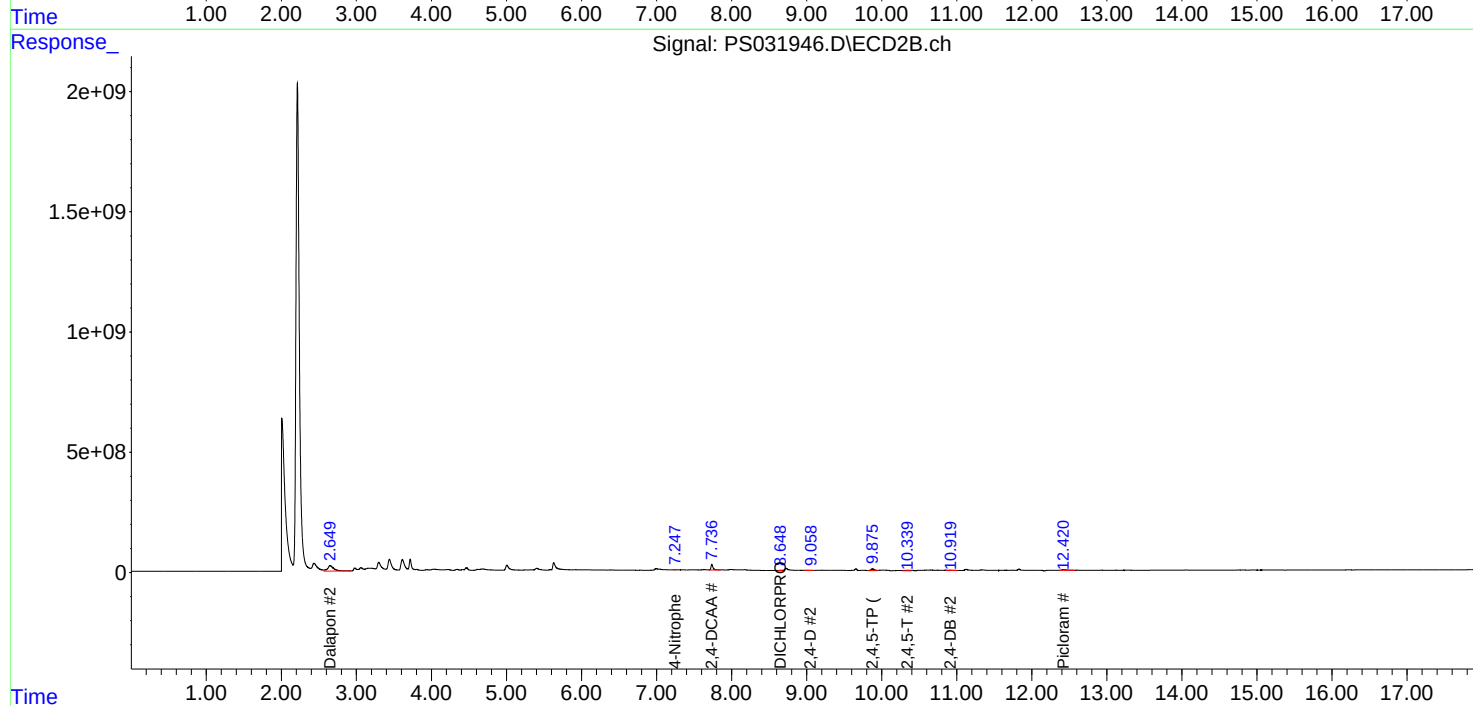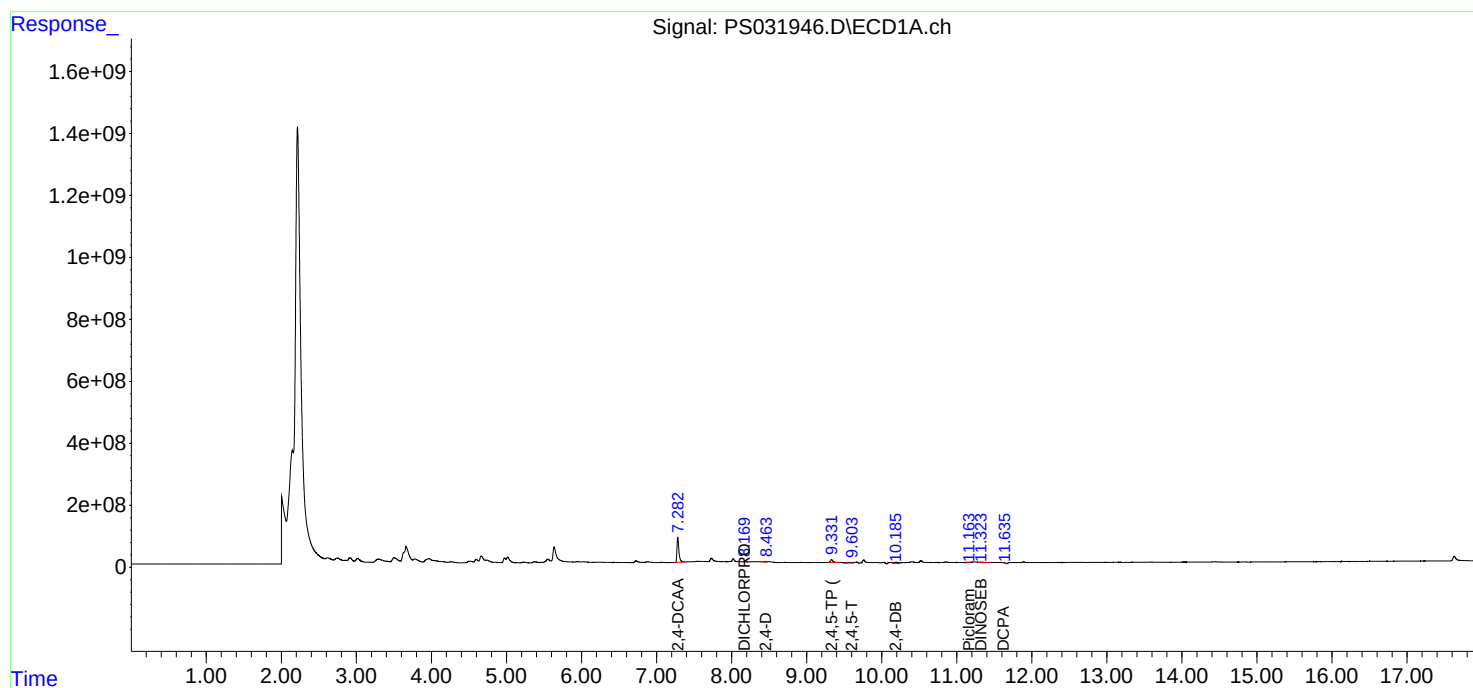


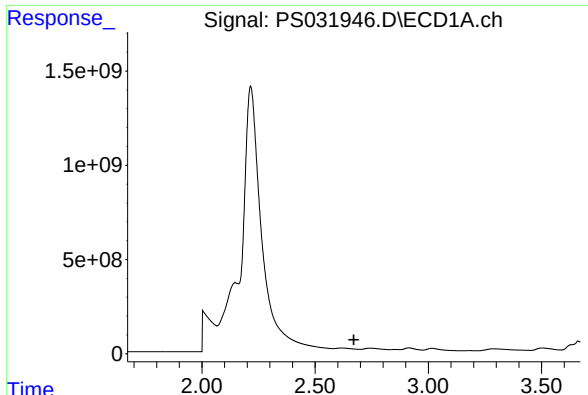

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

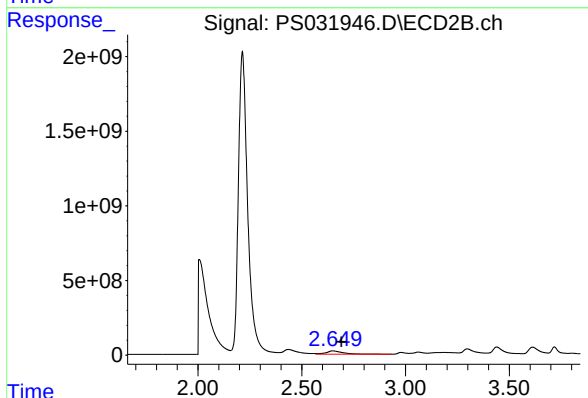


#1 Dalapon

R.T.: 2.649 min
Delta R.T.: -0.043 min
Response: 1327978220
Conc: 471.31 ng/ml

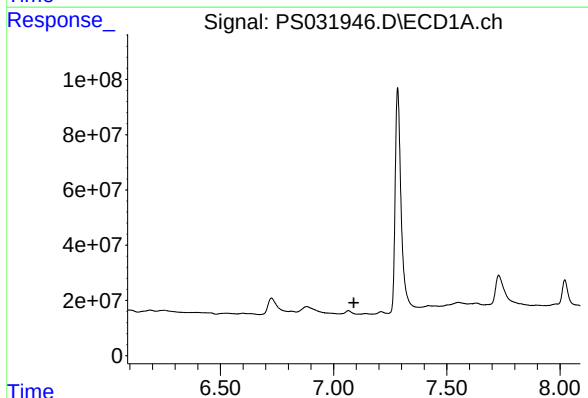


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

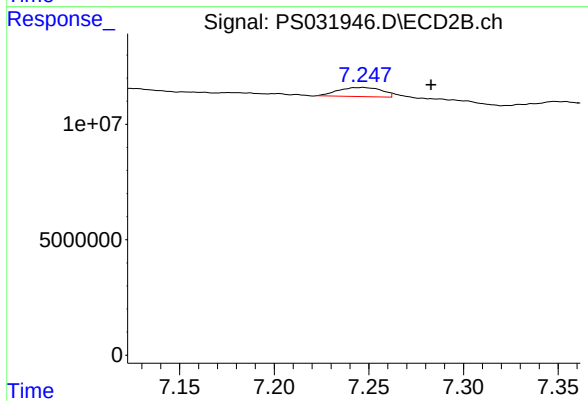

#3 4-Nitrophenol


R.T.: 7.246 min
Delta R.T.: -0.037 min
Response: 6069642
Conc: 4.81 ng/ml

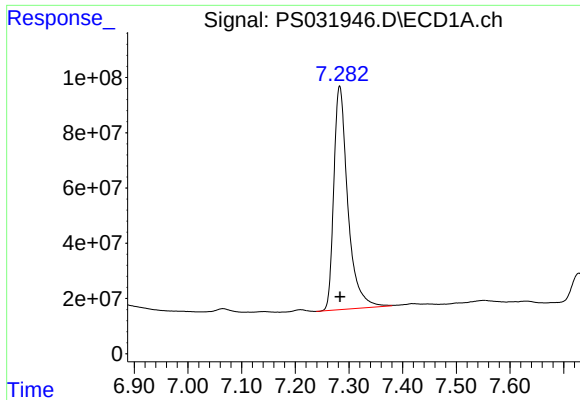

#4 2,4-DCAA


R.T.: 7.283 min
Delta R.T.: 0.000 min
Response: 1466184992
Conc: 407.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

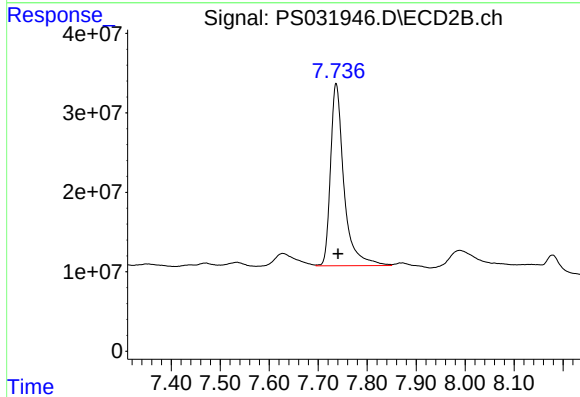


#4 2,4-DCAA

R.T.: 7.737 min
Delta R.T.: -0.004 min
Response: 437135275
Conc: 480.95 ng/ml

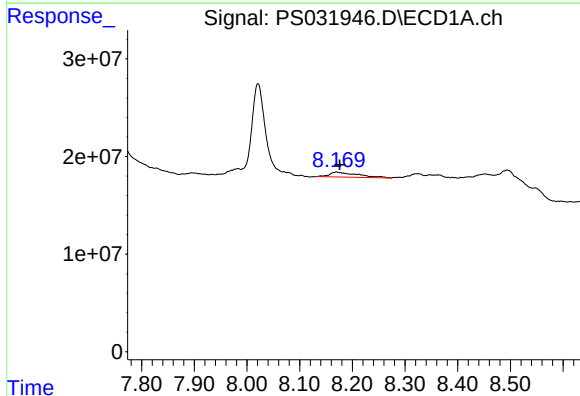


#8 DICHLORPROP

R.T.: 8.170 min
Delta R.T.: -0.006 min
Response: 18760040
Conc: 5.27 ng/ml

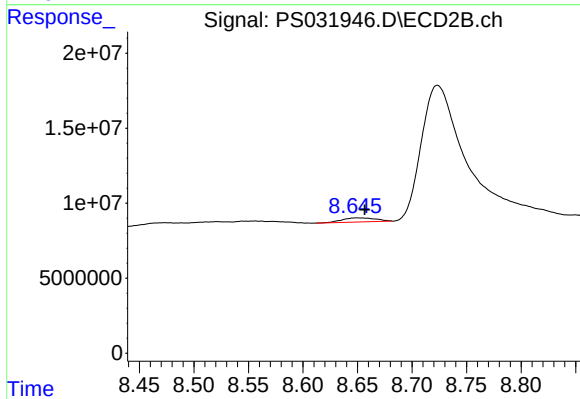

#8 DICHLORPROP


R.T.: 8.650 min
Delta R.T.: -0.006 min
Response: 5820362
Conc: 4.00 ng/ml

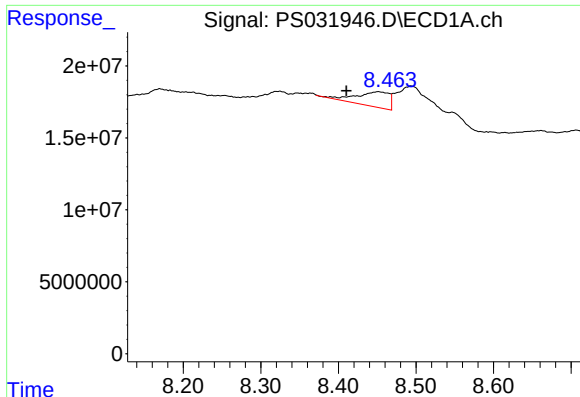

#9 2,4-D


R.T.: 8.452 min
Delta R.T.: 0.041 min
Response: 31126532
Conc: 9.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

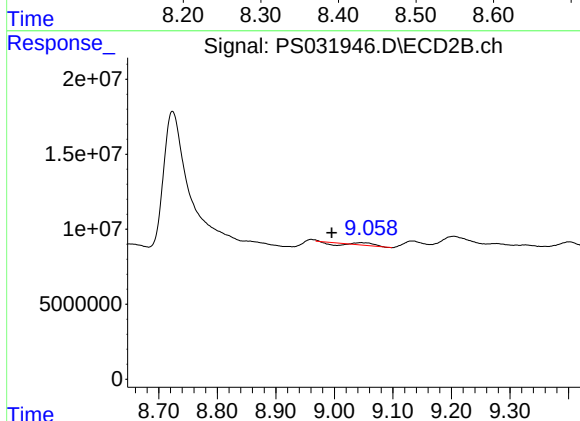


#9 2,4-D

R.T.: 9.045 min
Delta R.T.: 0.050 min
Response: 2027992
Conc: 1.23 ng/ml

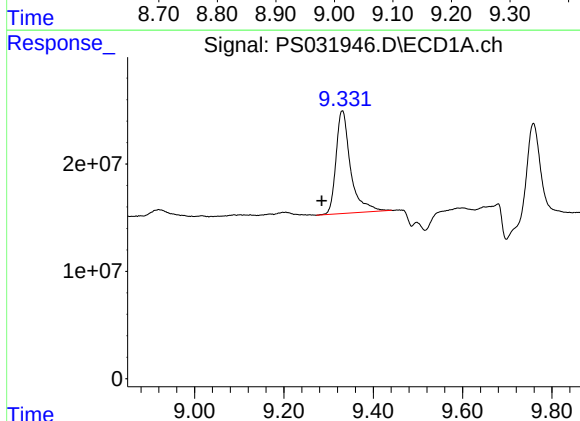


#11 2,4,5-TP (SILVEX)

R.T.: 9.331 min
Delta R.T.: 0.046 min
Response: 216827633
Conc: 10.34 ng/ml

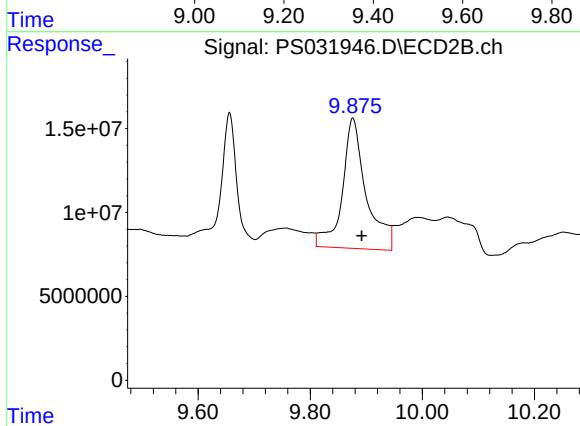

#11 2,4,5-TP (SILVEX)


R.T.: 9.876 min
Delta R.T.: -0.016 min
Response: 230898334
Conc: 15.34 ng/ml

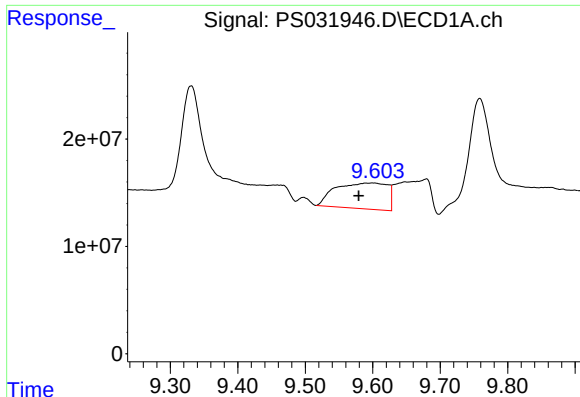

#12 2,4,5-T


R.T.: 9.600 min
Delta R.T.: 0.021 min
Response: 128608394
Conc: 7.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

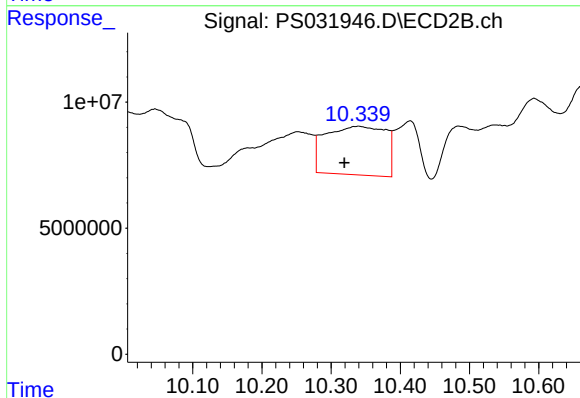


#12 2,4,5-T

R.T.: 10.339 min
Delta R.T.: 0.020 min
Response: 116206231
Conc: 8.64 ng/ml

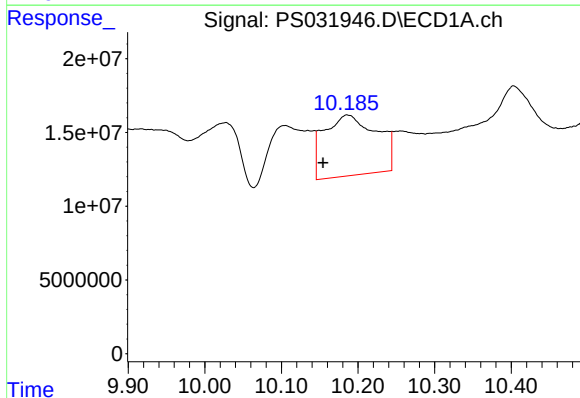


#13 2,4-DB

R.T.: 10.186 min
Delta R.T.: 0.032 min
Response: 196123211
Conc: 84.07 ng/ml

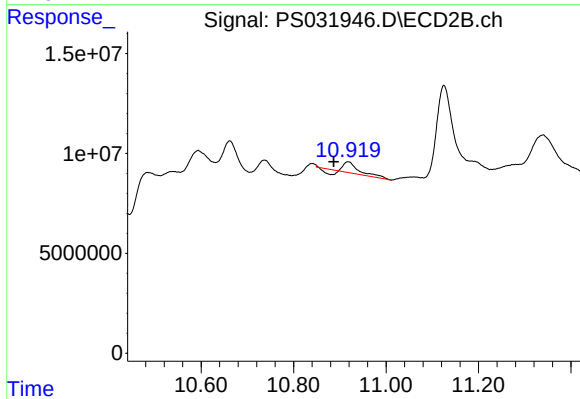

#13 2,4-DB


R.T.: 10.918 min
Delta R.T.: 0.031 min
Response: 10630473
Conc: 9.93 ng/ml

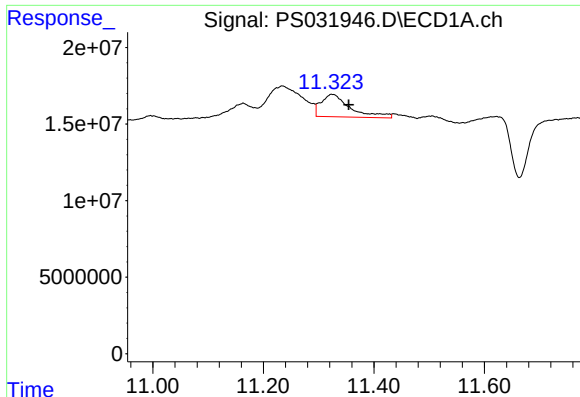

#14 DINOSEB


R.T.: 11.325 min
Delta R.T.: -0.030 min
Response: 53515061
Conc: 3.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

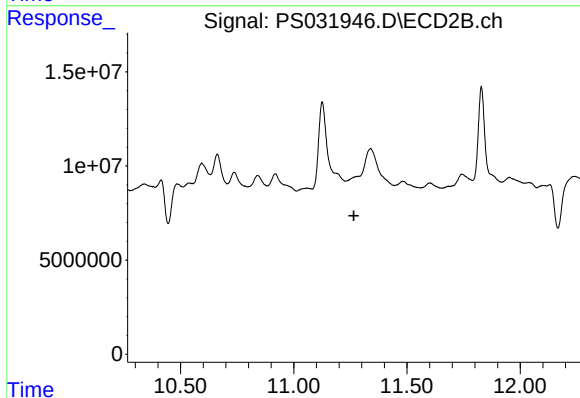


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.265 min
Response: 0
Conc: N.D.

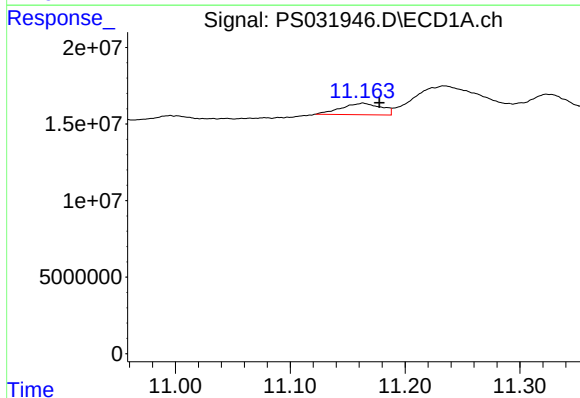


#15 Picloram

R.T.: 11.163 min
Delta R.T.: -0.014 min
Response: 18082225
Conc: 1.00 ng/ml

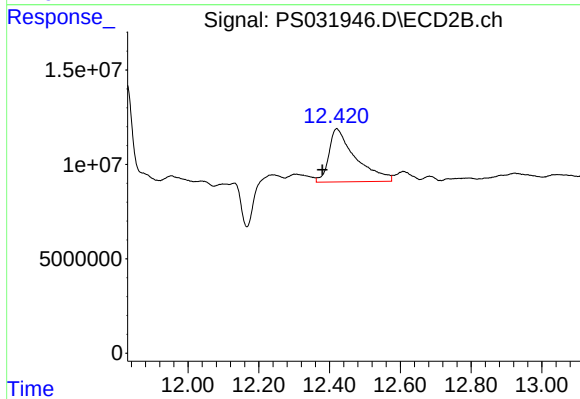

#15 Picloram


R.T.: 12.420 min
Delta R.T.: 0.040 min
Response: 147028369
Conc: 6.21 ng/ml

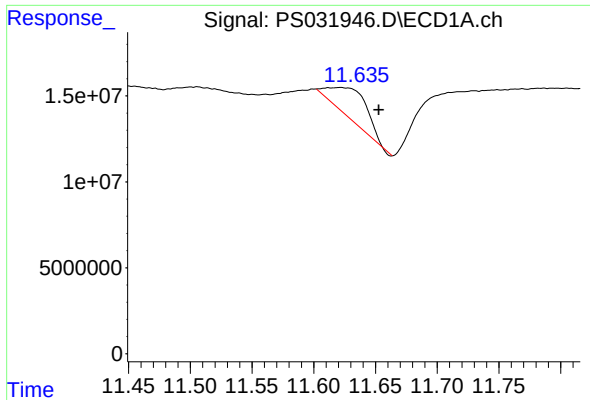

#16 DCPA

R.T.: 11.621 min
Delta R.T.: -0.032 min
Response: 35910862
Conc: 1.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

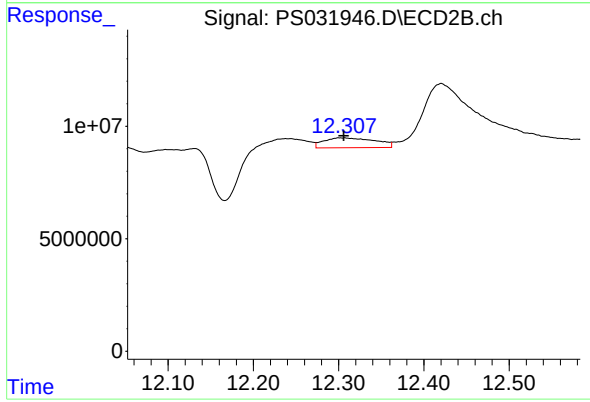

#16 DCPA

R.T.: 12.303 min
Delta R.T.: -0.003 min
Response: 18258620
Conc: N.D.