

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100325\
 Data File : PS031951.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2025 18:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:32:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.284	7.747	1708.9E6	494.1E6	474.491	543.662
Target Compounds							
1) T	Dalapon	0.000	2.654f	0	49349584	N.D.	17.515
2) T	3,5-DICHL...	6.447	0.000	5497698	0	1.031	N.D. #
3) T	4-Nitroph...	7.072	0.000	3266715	0	2.961	N.D. #
7) T	MCPA	7.816	8.242f	1245965	34071644	<MDL	12.163 #
8) T	DICHLORPROP	8.186	0.000	183715	0	<MDL	N.D. #
10) T	Pentachlo...	8.707	9.514	8682802	5997970	<MDL	<MDL #
11) T	2,4,5-TP ...	9.299	9.921f	3166186	2561417	<MDL	<MDL #
12) T	2,4,5-T	9.596	0.000	3234335	0	<MDL	N.D. #
13) T	2,4-DB	10.136	0.000	780738	0	<MDL	N.D. #
14) T	DINOSEB	11.349	0.000	4209879	0	<MDL	N.D. #
15) T	Picloram	11.195	0.000	2770987	0	<MDL	N.D. #
16) T	DCPA	11.651	0.000	4274783	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100325\
Data File : PS031951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2025 18:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:32:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

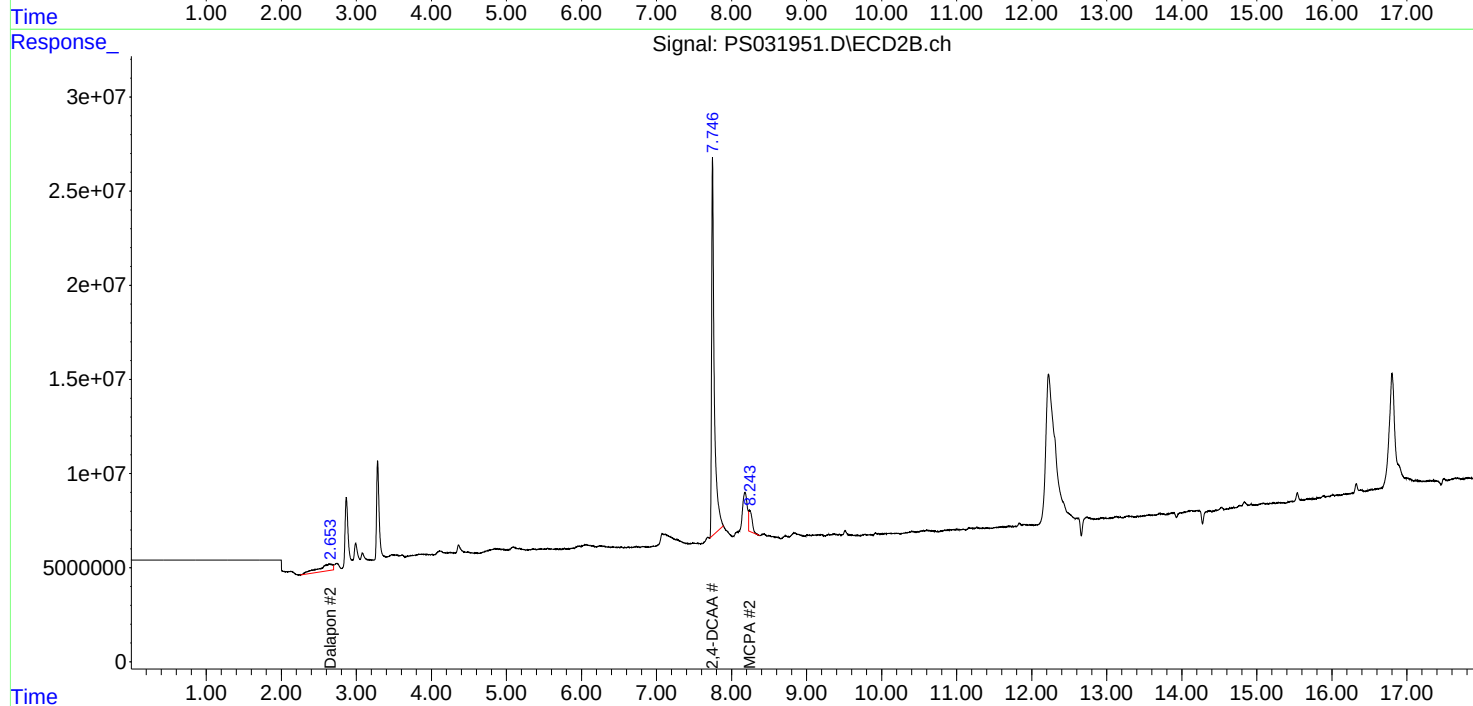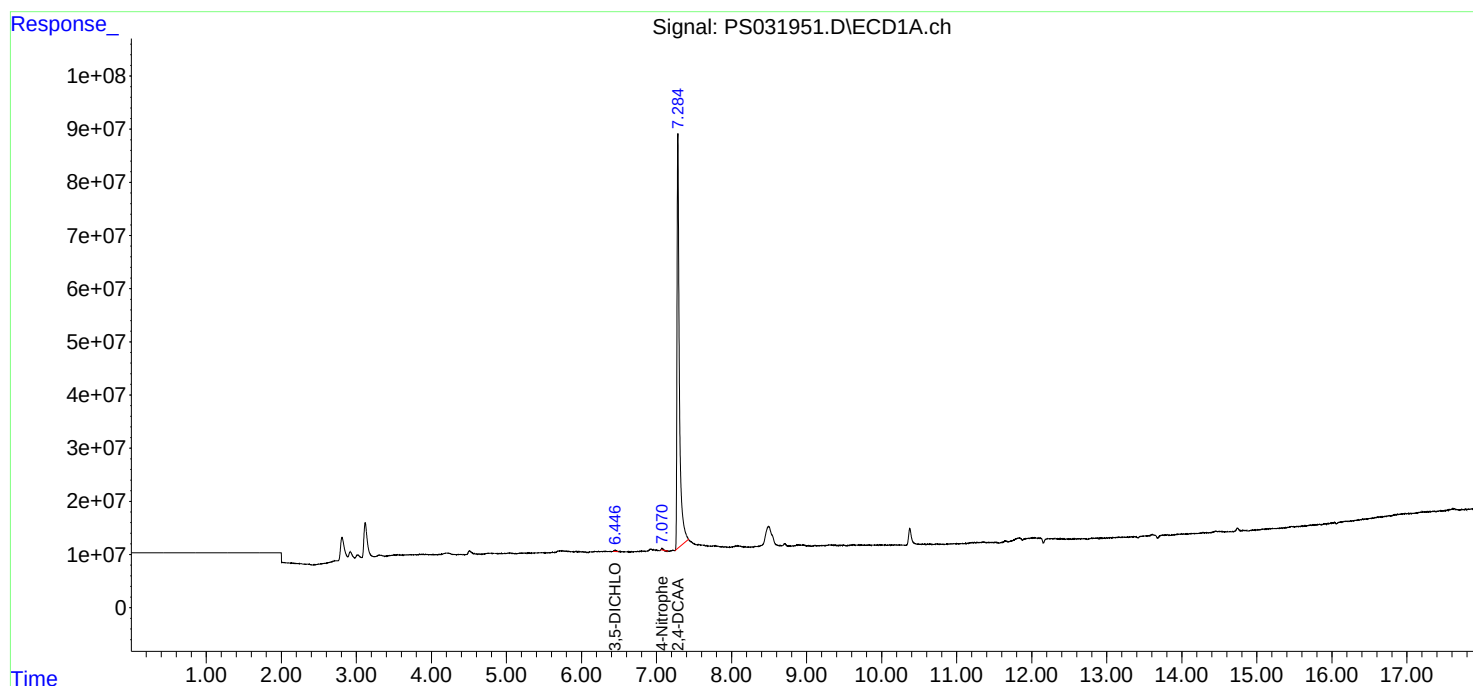


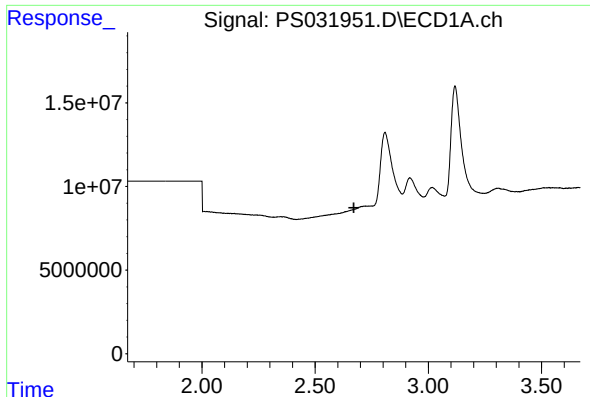

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

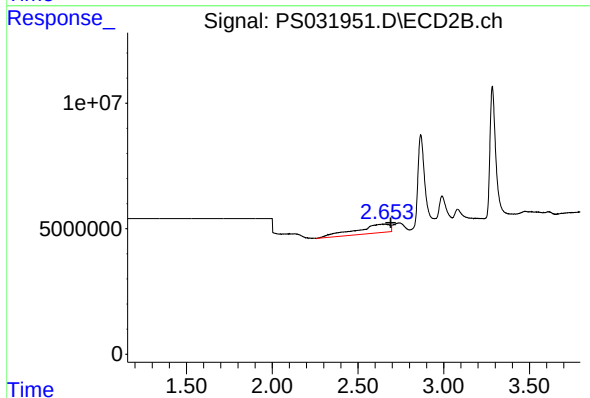


#1 Dalapon

R.T.: 2.654 min
Delta R.T.: -0.038 min
Response: 49349584
Conc: 17.51 ng/ml

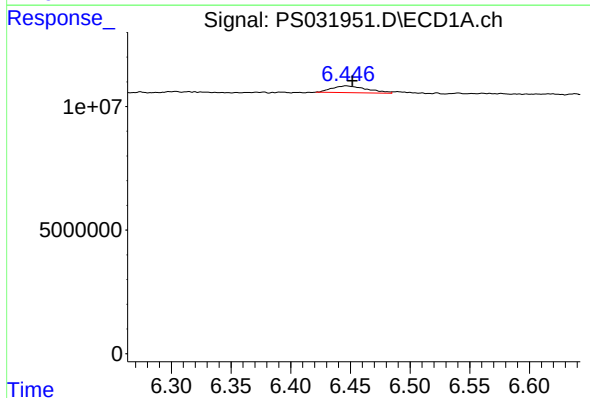


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.447 min
Delta R.T.: -0.005 min
Response: 5497698
Conc: 1.03 ng/ml

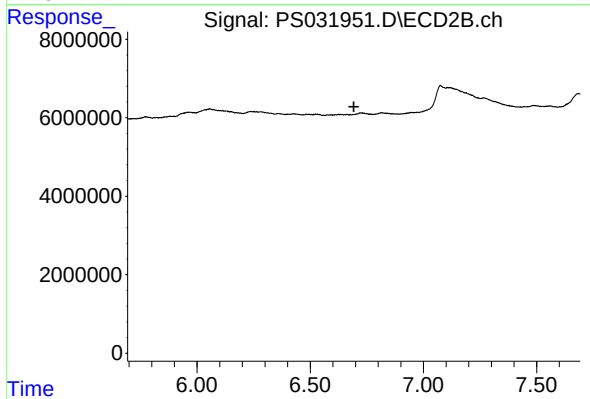

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.693 min
Response: 0
Conc: N.D.

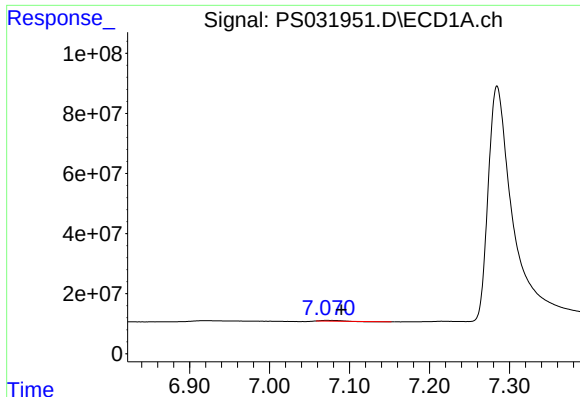

#3 4-Nitrophenol


R.T.: 7.072 min
Delta R.T.: -0.018 min
Response: 3266715
Conc: 2.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

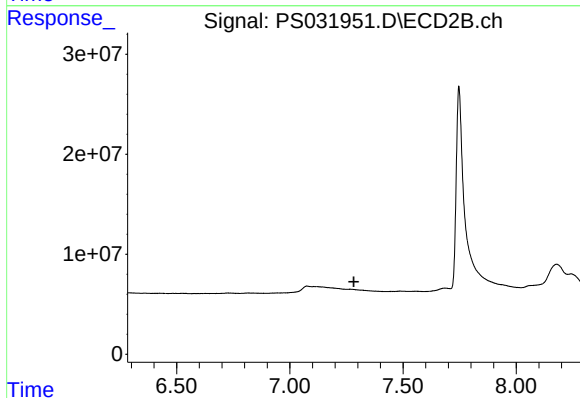


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

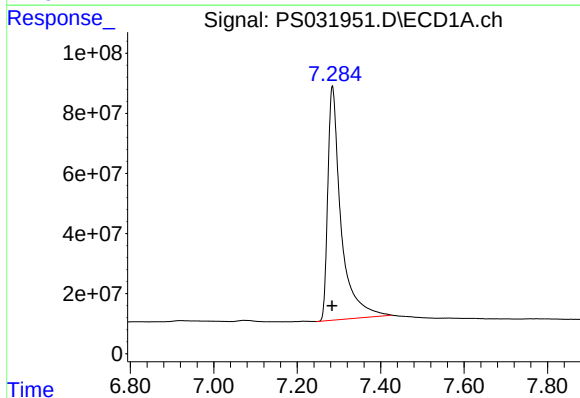


#4 2,4-DCAA

R.T.: 7.284 min
Delta R.T.: 0.001 min
Response: 1708893293
Conc: 474.49 ng/ml

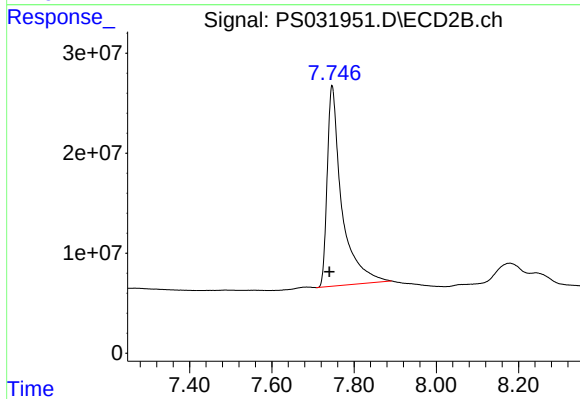

#4 2,4-DCAA


R.T.: 7.747 min
Delta R.T.: 0.006 min
Response: 494133662
Conc: 543.66 ng/ml

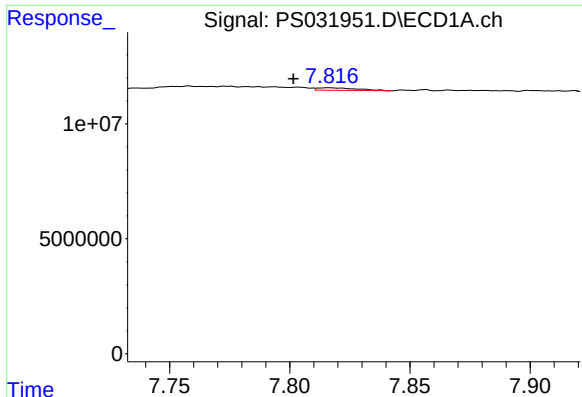

#7 MCPA

R.T.: 7.816 min
Delta R.T.: 0.015 min
Response: 1245965
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

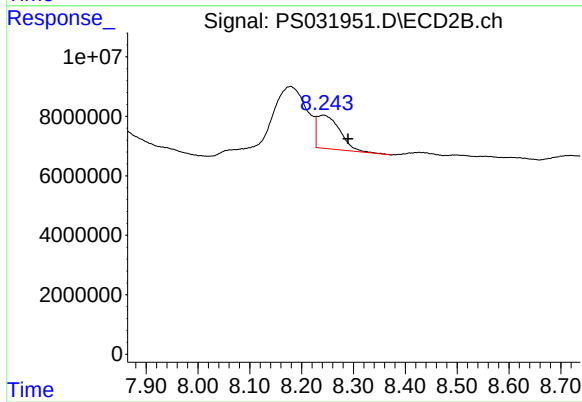

#7 MCPA

R.T.: 8.242 min
Delta R.T.: -0.048 min
Response: 34071644
Conc: 12.16 ug/ml