

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100419\
 Data File : PS007031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2019 15:58
 Operator : SM\AJ
 Sample : PB123645BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB123645BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 00:45:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.496	5.223	584.0E6	302.4E6	639.098	657.588
Target Compounds							
1) T	Dalapon	2.043	1.754	142.1E6	124.0E6	132.984	232.686 #
2) T	3,5-DICHL...	0.000	4.551	0	25322484	N.D.	44.050
3) T	4-Nitroph...	5.354	0.000	94114254	0	246.826	N.D. #
5) T	DICAMBA	5.592	0.000	80160635	0	24.810	N.D. #
7) T	MCPA	5.975	0.000	9590690	0	3.083	N.D. #
9) T	2,4-D	0.000	6.145	0	10907593	N.D.	21.384
10) T	Pentachlo...	0.000	6.535	0	9045042	N.D.	1.438
11) T	2,4,5-TP ...	0.000	6.843	0	14305526	N.D.	5.972
12) T	2,4,5-T	0.000	7.303	0	15017379	N.D.	6.948
15) T	Picloram	9.040	8.997	87876665	49252793	13.105	13.532
16) T	DCPA	0.000	8.997	0	49252793	N.D.	15.501



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100419\
Data File : PS007031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2019 15:58
Operator : SM\AJ
Sample : PB123645BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB123645BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 00:45:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

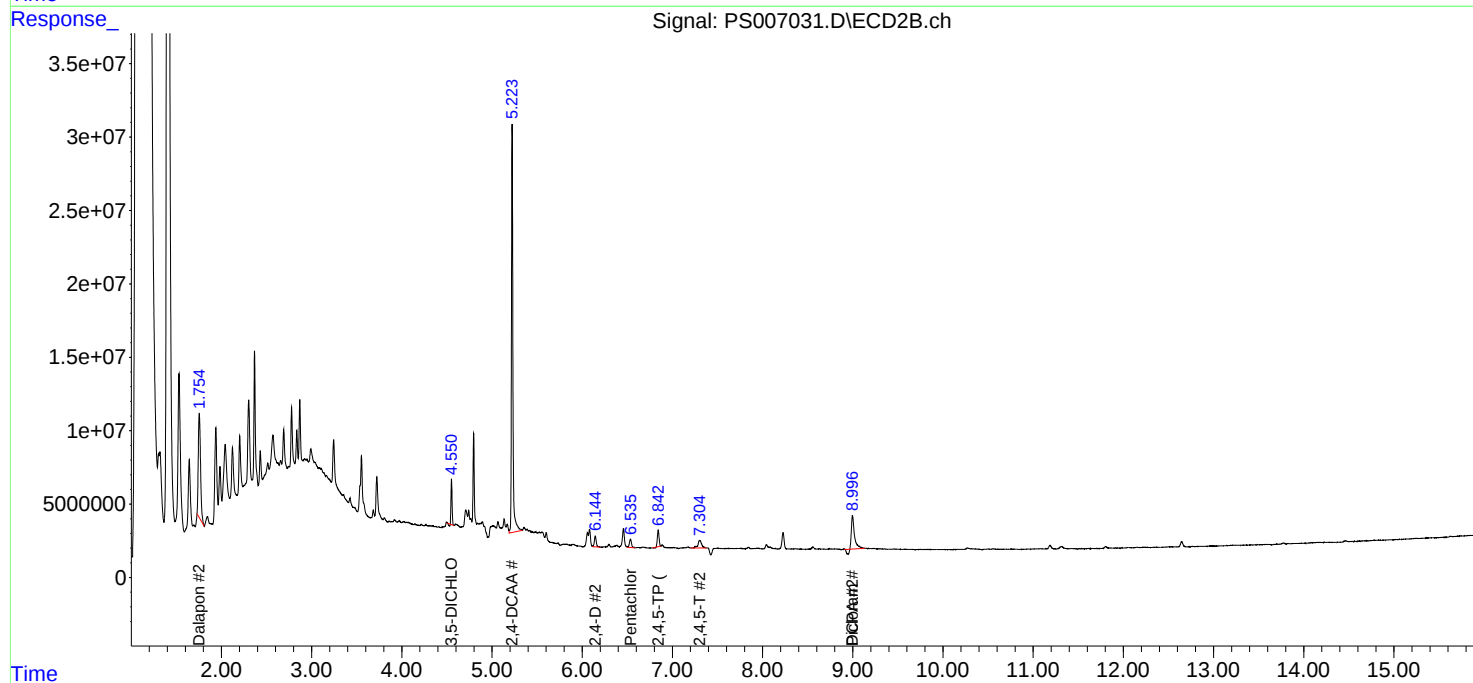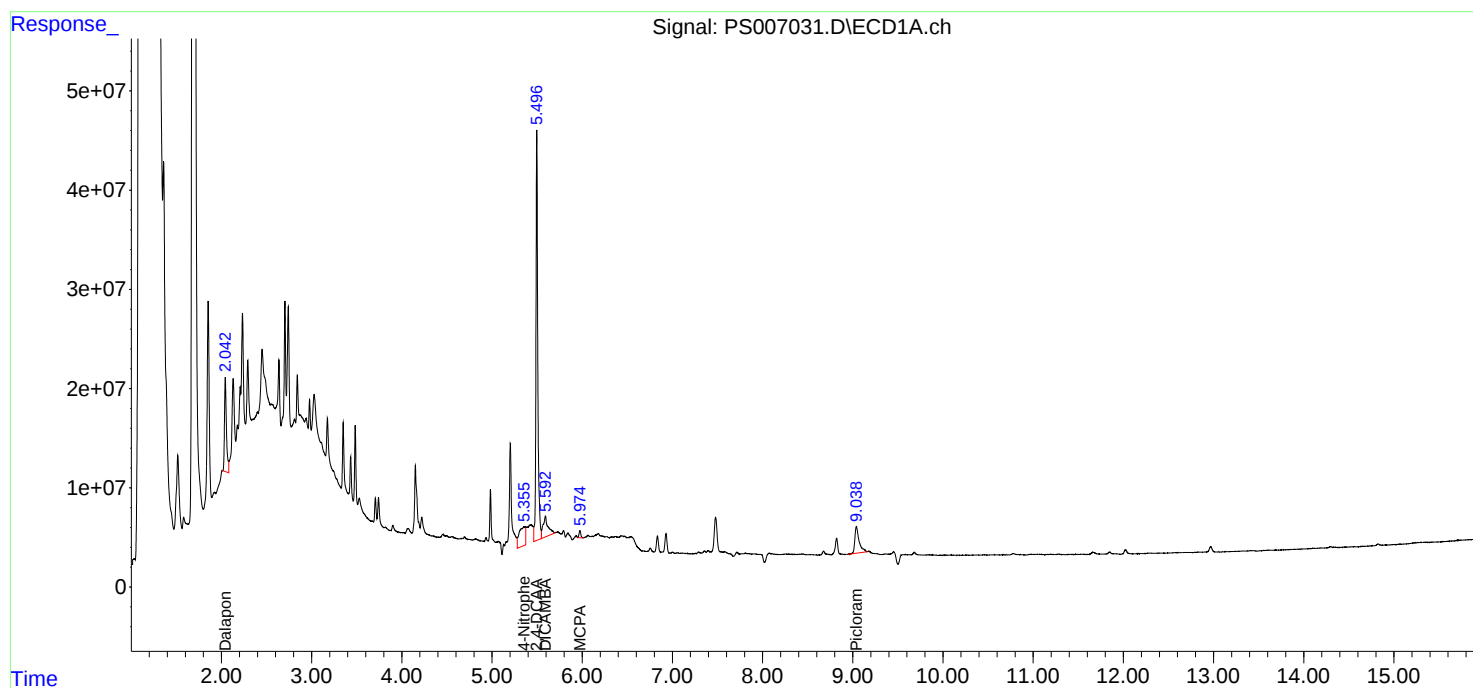


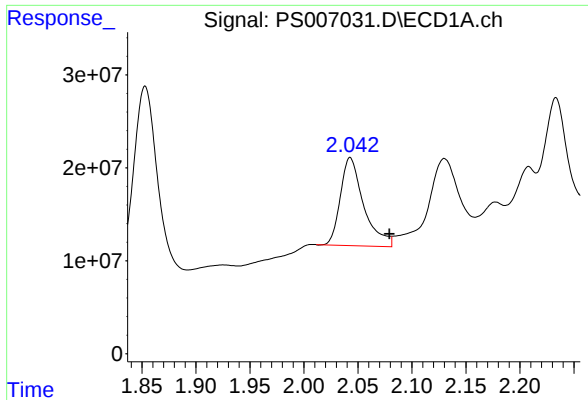

#1 Dalapon


R.T.: 2.043 min
Delta R.T.: -0.036 min
Response: 142080837
Conc: 132.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123645BL

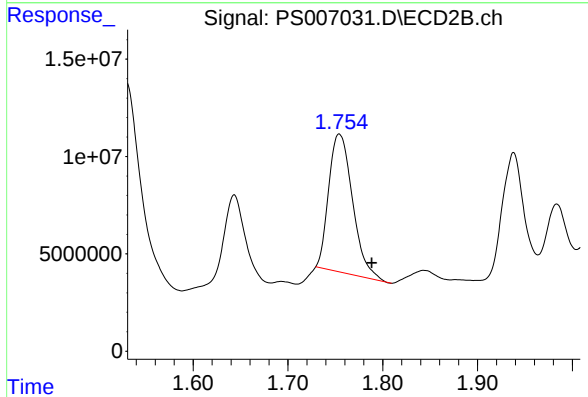


#1 Dalapon

R.T.: 1.754 min
Delta R.T.: -0.034 min
Response: 124037493
Conc: 232.69 ng/ml

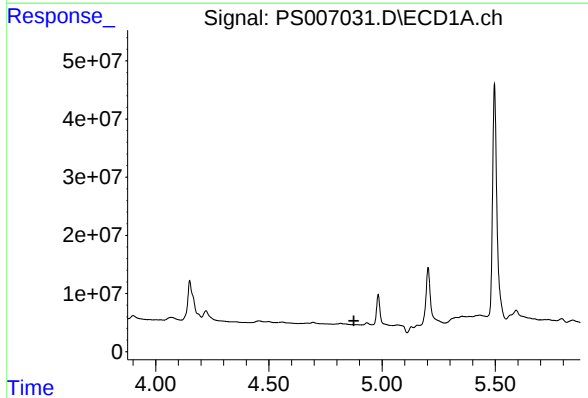


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.876 min
Response: 0
Conc: N.D.

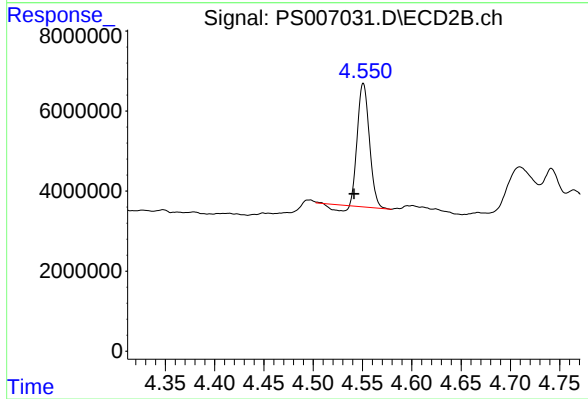

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.551 min
Delta R.T.: 0.009 min
Response: 25322484
Conc: 44.05 ng/ml

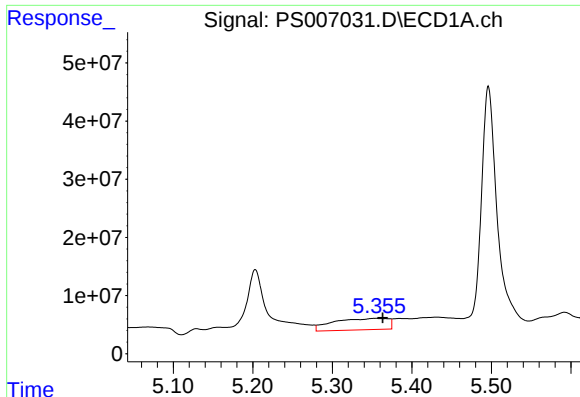

#3 4-Nitrophenol


R.T.: 5.354 min
Delta R.T.: -0.010 min
Response: 94114254
Conc: 246.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123645BL

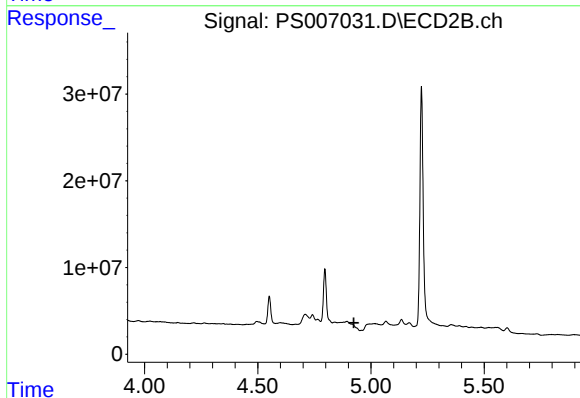


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

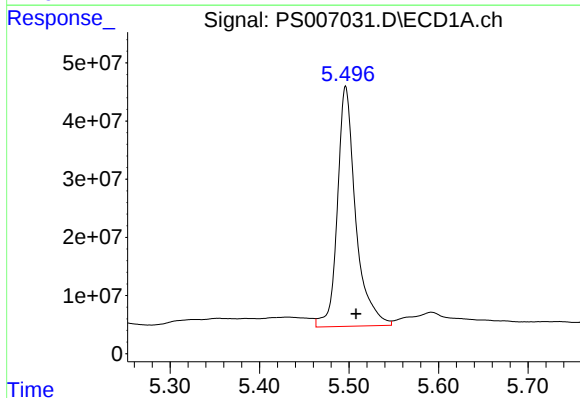


#4 2,4-DCAA

R.T.: 5.496 min
Delta R.T.: -0.011 min
Response: 584016801
Conc: 639.10 ng/ml

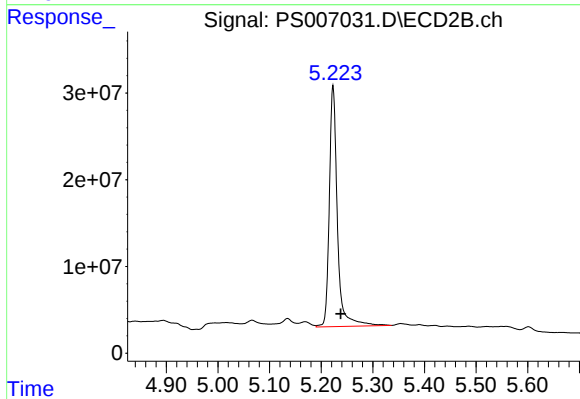

#4 2,4-DCAA


R.T.: 5.223 min
Delta R.T.: -0.015 min
Response: 302386123
Conc: 657.59 ng/ml

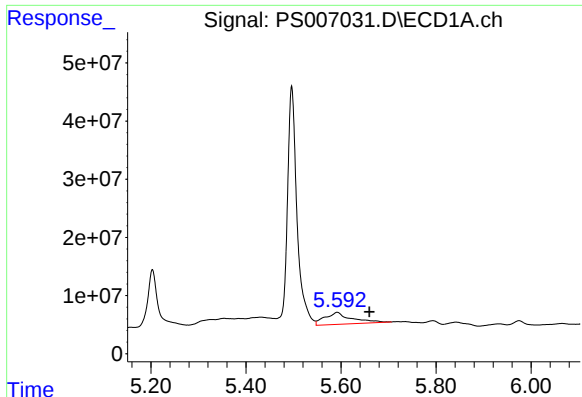

#5 DICAMBA


R.T.: 5.592 min
Delta R.T.: -0.068 min
Response: 80160635
Conc: 24.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123645BL

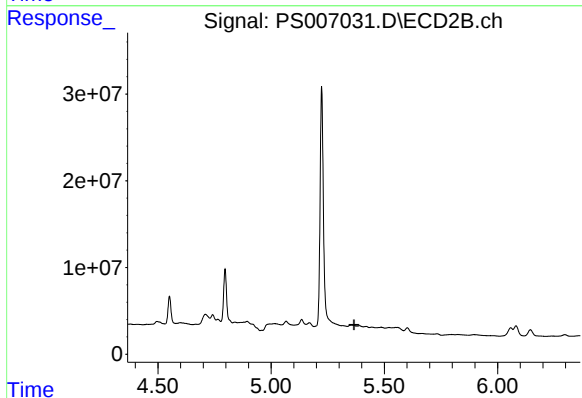


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.366 min
Response: 0
Conc: N.D.

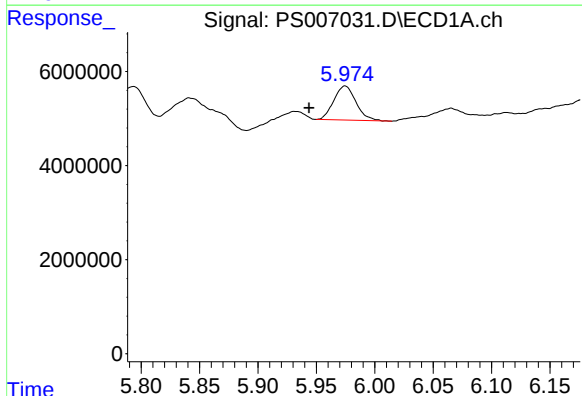


#7 MCPA

R.T.: 5.975 min
Delta R.T.: 0.031 min
Response: 9590690
Conc: 3.08 ug/ml

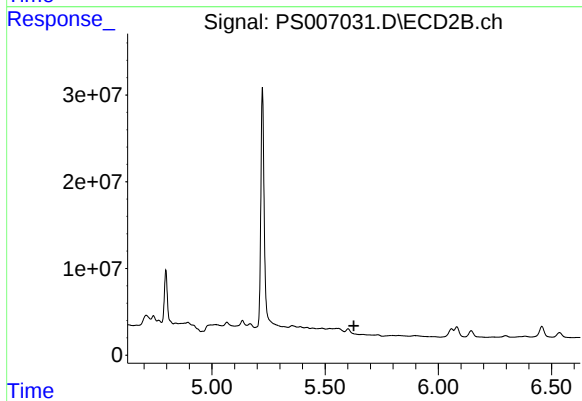

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 5.627 min
Response: 0
Conc: N.D.

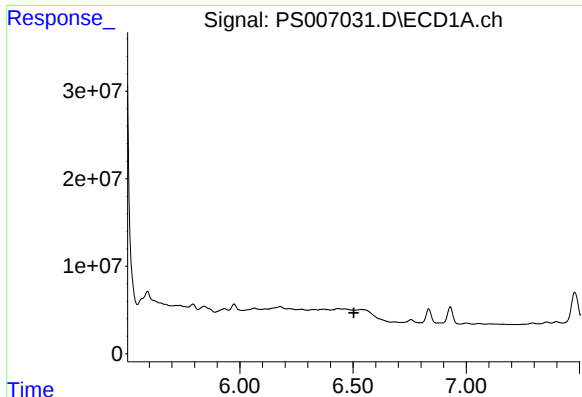

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.504 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB123645BL

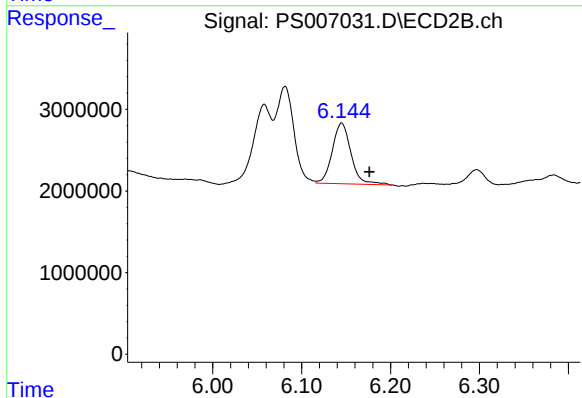


#9 2,4-D

R.T.: 6.145 min
Delta R.T.: -0.031 min
Response: 10907593
Conc: 21.38 ng/ml

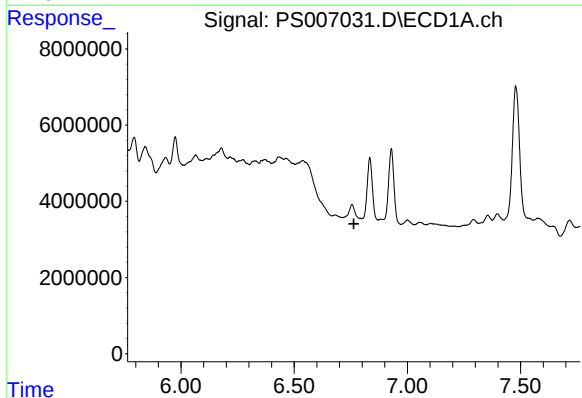


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.763 min
Response: 0
Conc: N.D.

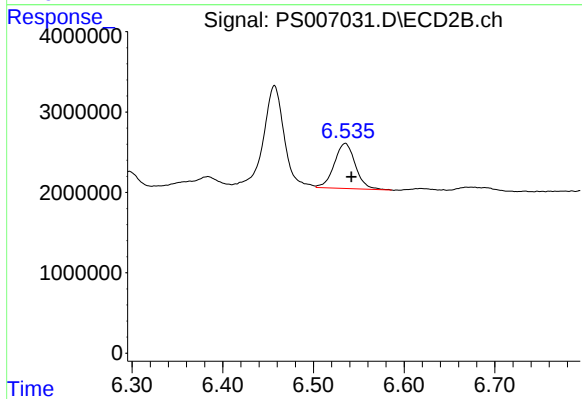

#10 Pentachlorophenol


R.T.: 6.535 min
Delta R.T.: -0.007 min
Response: 9045042
Conc: 1.44 ng/ml

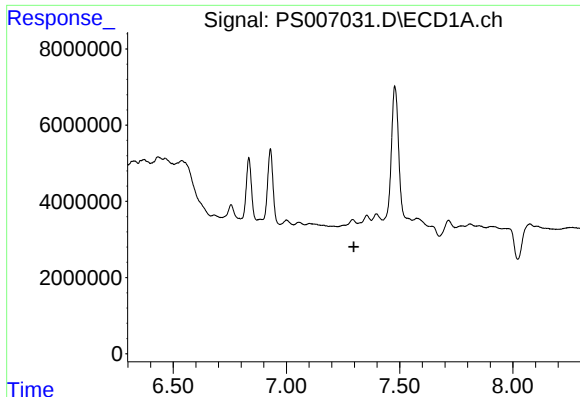

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB123645BL

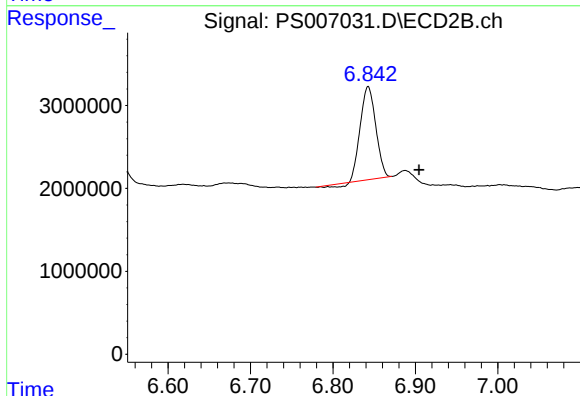


#11 2,4,5-TP (SILVEX)

R.T.: 6.843 min
Delta R.T.: -0.062 min
Response: 14305526
Conc: 5.97 ng/ml

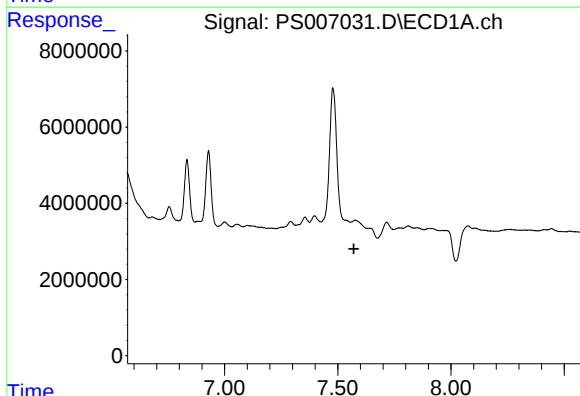


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.572 min
Response: 0
Conc: N.D.

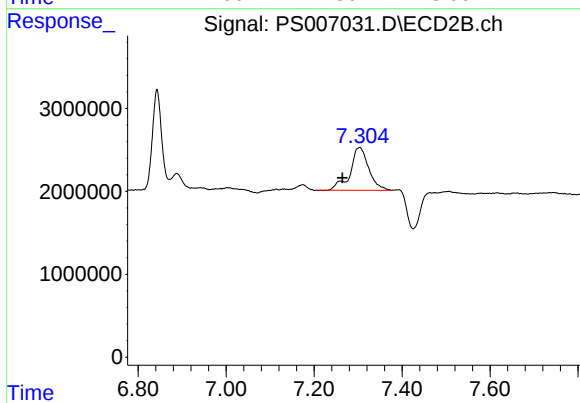

#12 2,4,5-T


R.T.: 7.303 min
Delta R.T.: 0.038 min
Response: 15017379
Conc: 6.95 ng/ml

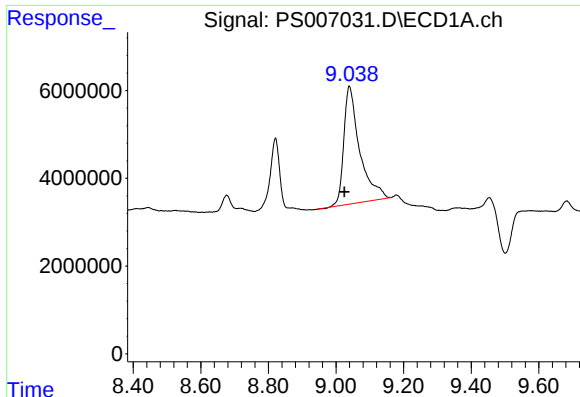

#15 Picloram


R.T.: 9.040 min
Delta R.T.: 0.015 min
Response: 87876665
Conc: 13.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123645BL

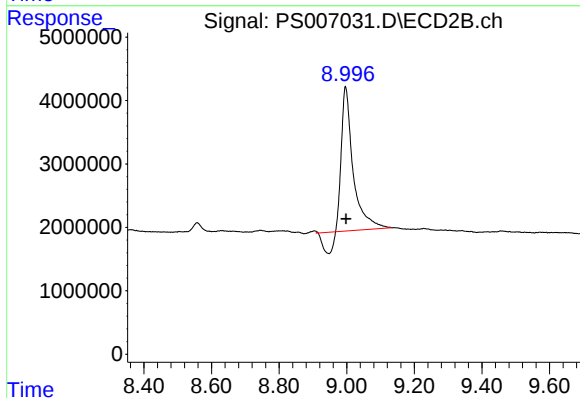


#15 Picloram

R.T.: 8.997 min
Delta R.T.: -0.002 min
Response: 49252793
Conc: 13.53 ng/ml

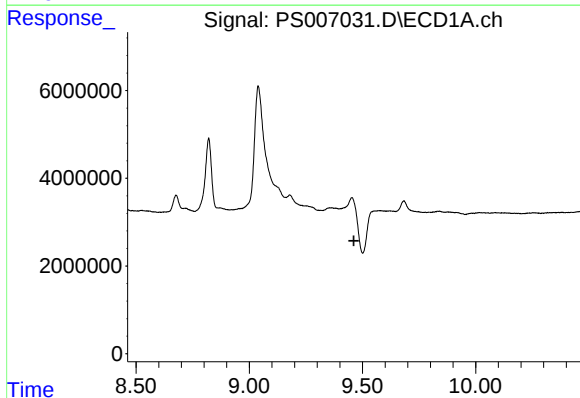

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.462 min
Response: 0
Conc: N.D.

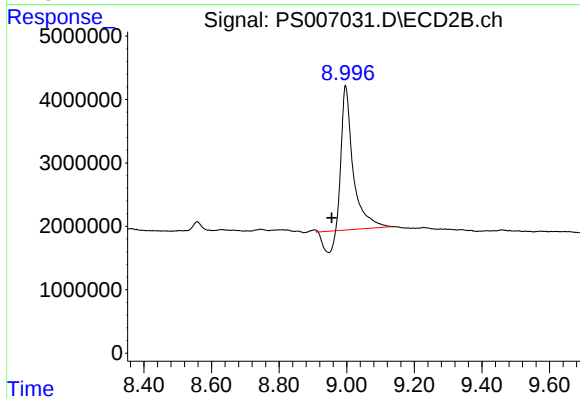

#16 DCPA

R.T.: 8.997 min
Delta R.T.: 0.041 min
Response: 49252793
Conc: 15.50 ng/ml