

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100421\
 Data File : PS016946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2021 14:03
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 14:54:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.162	6.749	702.4E6	303.0E6	461.014	516.680
Target Compounds							
2) T	3,5-DICHL...	6.418	0.000	619.1E6	0	290.925	N.D. #
5) T	DICAMBA	0.000	6.966f	0	324.1E6	N.D.	127.212
6) T	MCP	0.000	6.966f	0	324.1E6	N.D.	158.194
9) T	2,4-D	8.333f	0.000	711.8E6	0	404.841	N.D. #
10) T	Pentachlo...	8.578	0.000	10773766	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.131	0.000	4757535	0	<MDL	N.D. #
12) T	2,4,5-T	9.439	0.000	3978332	0	<MDL	N.D. #
14) T	DINOSEB	11.108	0.000	5890787	0	<MDL	N.D. #
15) T	Picloram	10.906	0.000	30105897	0	2.530	N.D. #
16) T	DCPA	11.375	0.000	6918096	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100421\
Data File : PS016946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2021 14:03
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 14:54:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

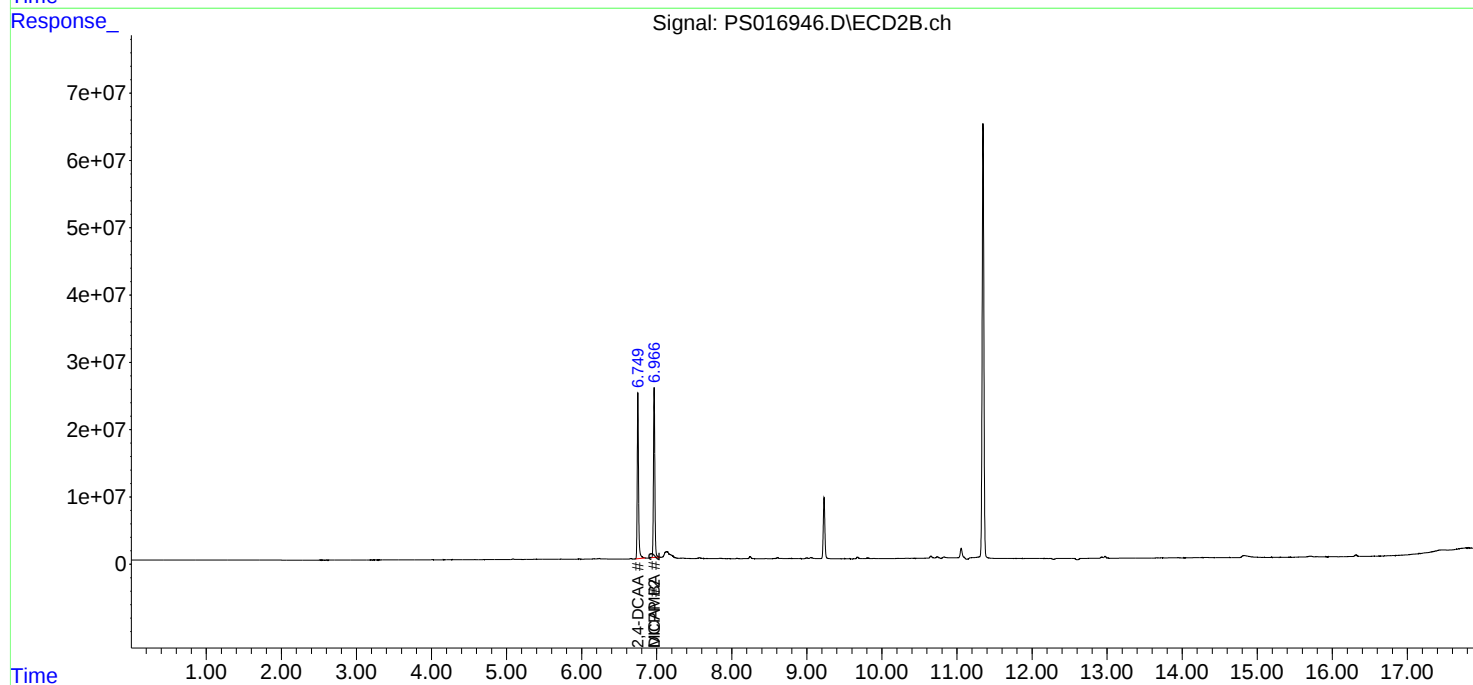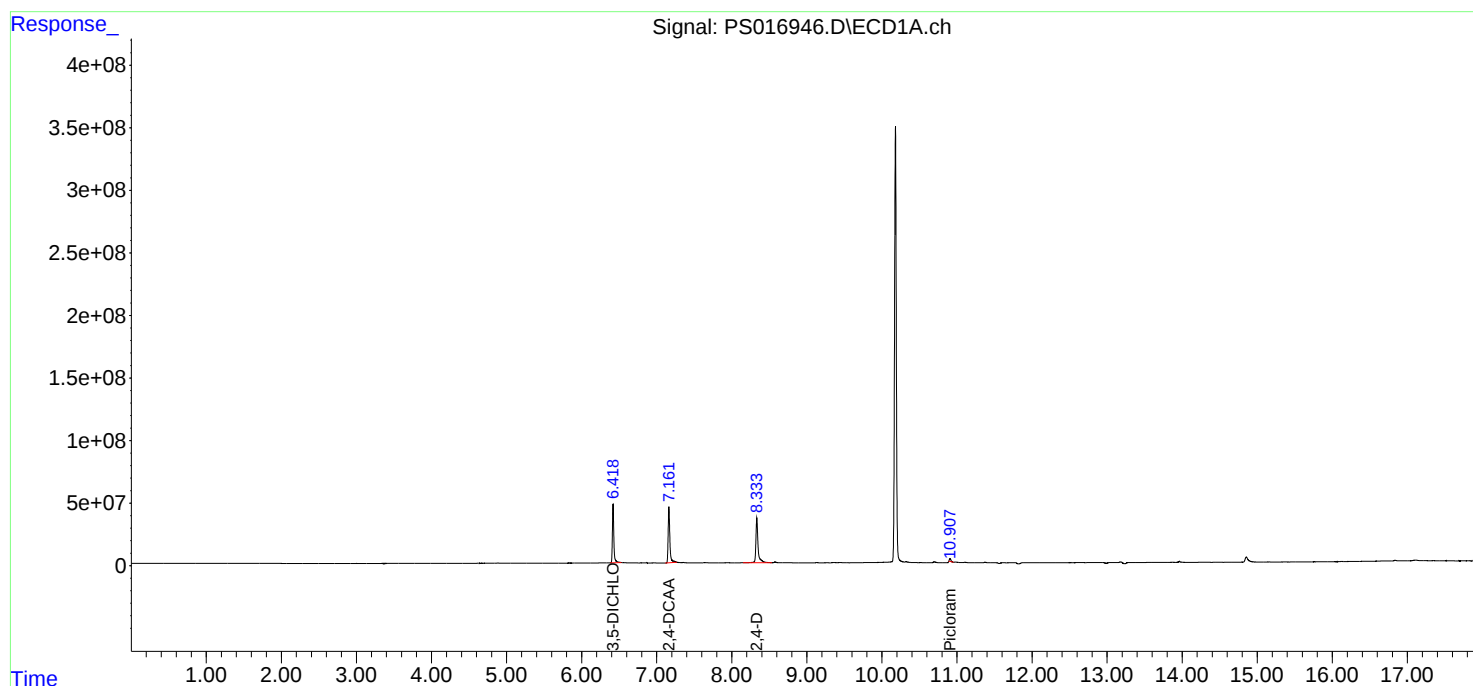


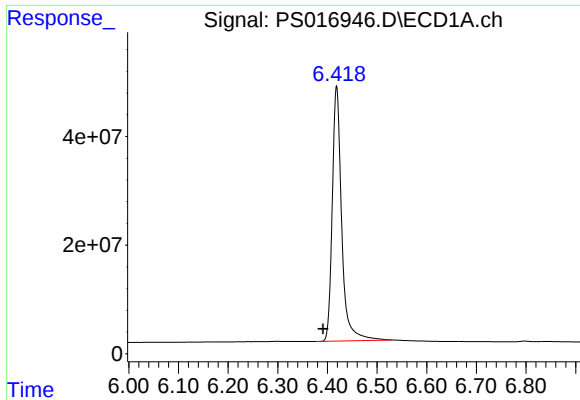

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.418 min
Delta R.T.: 0.027 min
Response: 619116875
Conc: 290.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

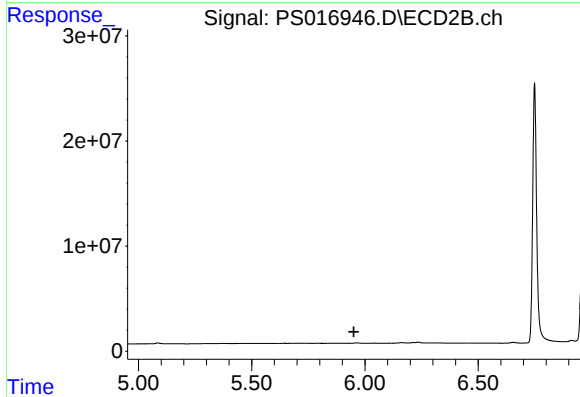


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.951 min
Response: 0
Conc: N.D.

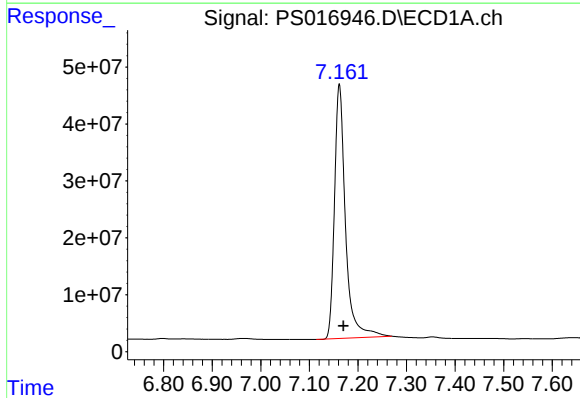


#4 2,4-DCAA

R.T.: 7.162 min
Delta R.T.: -0.009 min
Response: 702378431
Conc: 461.01 ng/ml

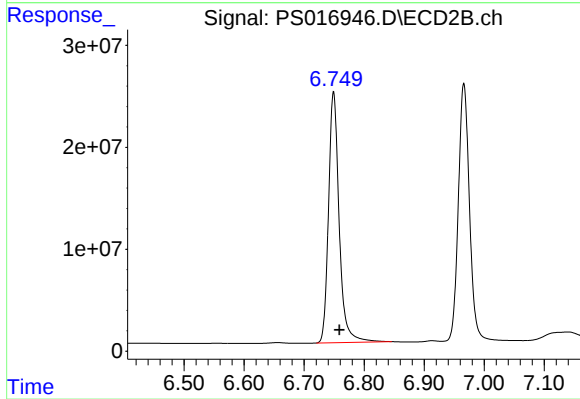

#4 2,4-DCAA


R.T.: 6.749 min
Delta R.T.: -0.010 min
Response: 302962193
Conc: 516.68 ng/ml

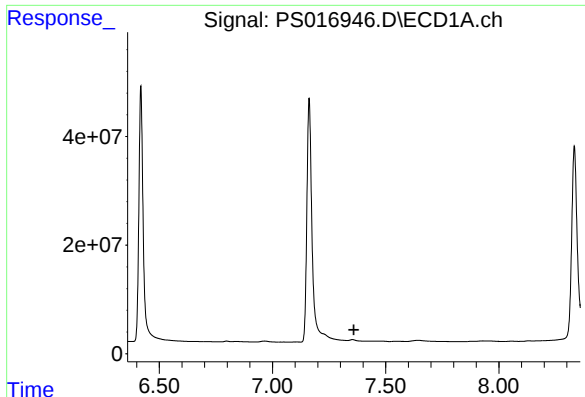

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.360 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

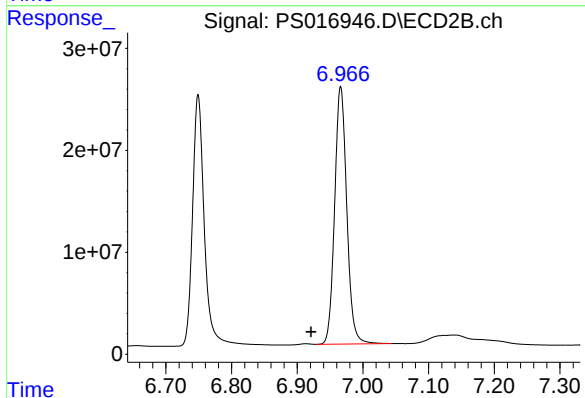


#5 DICAMBA

R.T.: 6.966 min
Delta R.T.: 0.045 min
Response: 324065464
Conc: 127.21 ng/ml

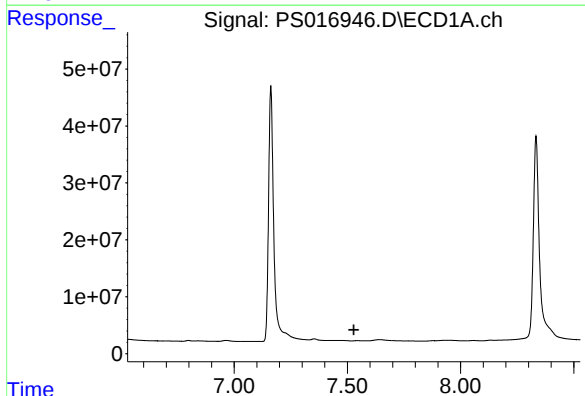


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.529 min
Response: 0
Conc: N.D.

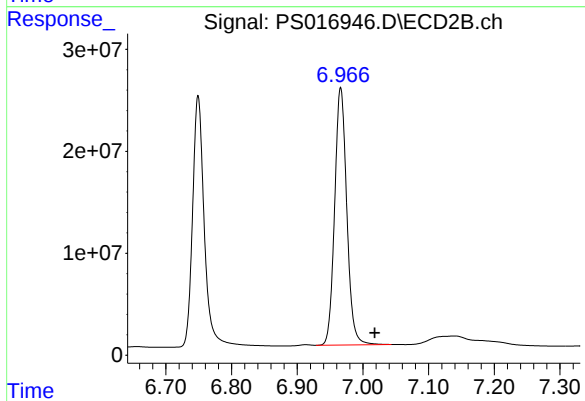

#6 MCP


R.T.: 6.966 min
Delta R.T.: -0.052 min
Response: 324065464
Conc: 158.19 ug/ml

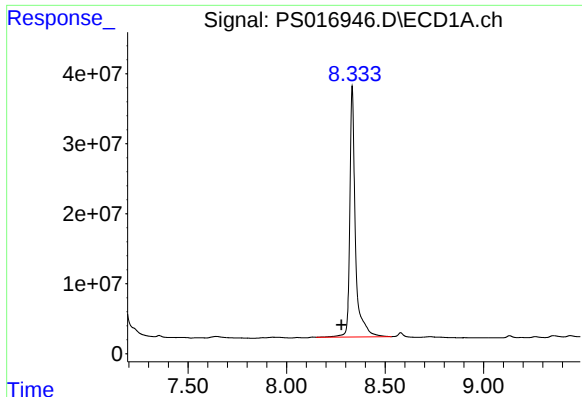

#9 2,4-D


R.T.: 8.333 min
Delta R.T.: 0.055 min
Response: 711813293
Conc: 404.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

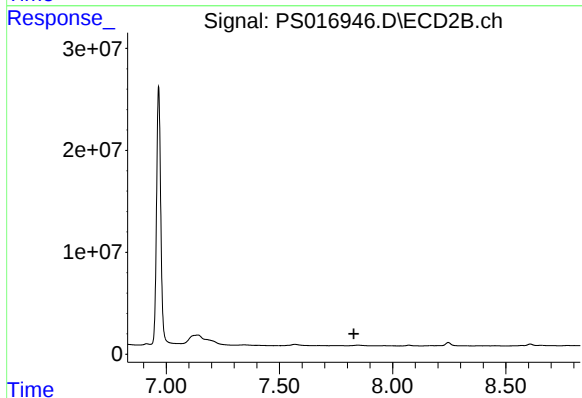


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.829 min
Response: 0
Conc: N.D.

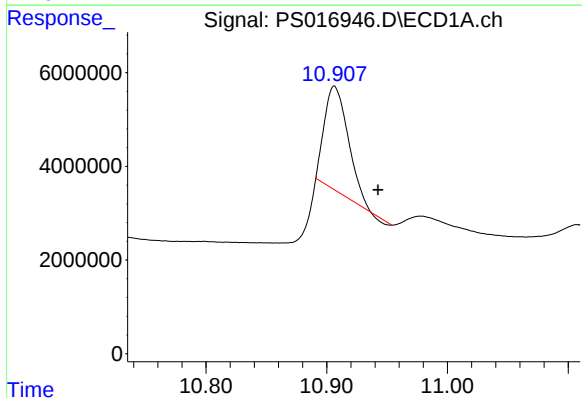

#15 Picloram

R.T.: 10.906 min
Delta R.T.: -0.036 min
Response: 30105897
Conc: 2.53 ng/ml

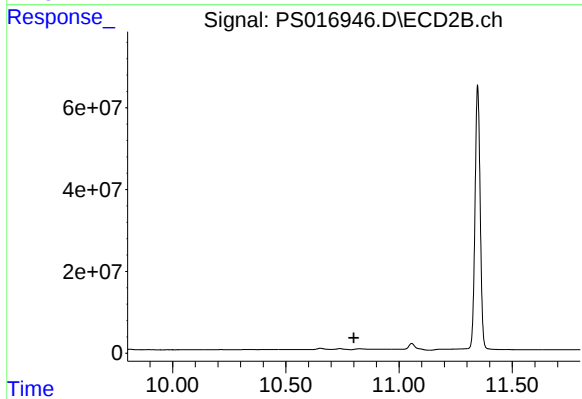

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.801 min
Response: 0
Conc: N.D.