

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100421\
 Data File : PS016957.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2021 18:29
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 01:54:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.160	6.748	688.0E6	303.1E6	451.545	516.902
Target Compounds							
2) T	3,5-DICHL...	6.417	0.000	722.0E6	0	339.291	N.D. #
3) T	4-Nitroph...	6.947f	0.000	6294962	0	7.267	N.D. #
5) T	DICAMBA	0.000	6.966f	0	331.5E6	N.D.	130.113
6) T	MCP	0.000	6.966f	0	331.5E6	N.D.	161.801
7) T	MCPA	7.614f	0.000	18816976	0	3.043	N.D. #
9) T	2,4-D	8.331f	0.000	689.0E6	0	391.888	N.D. #
15) T	Picloram	10.899f	0.000	12024319	0	1.010	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100421\
Data File : PS016957.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2021 18:29
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 01:54:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

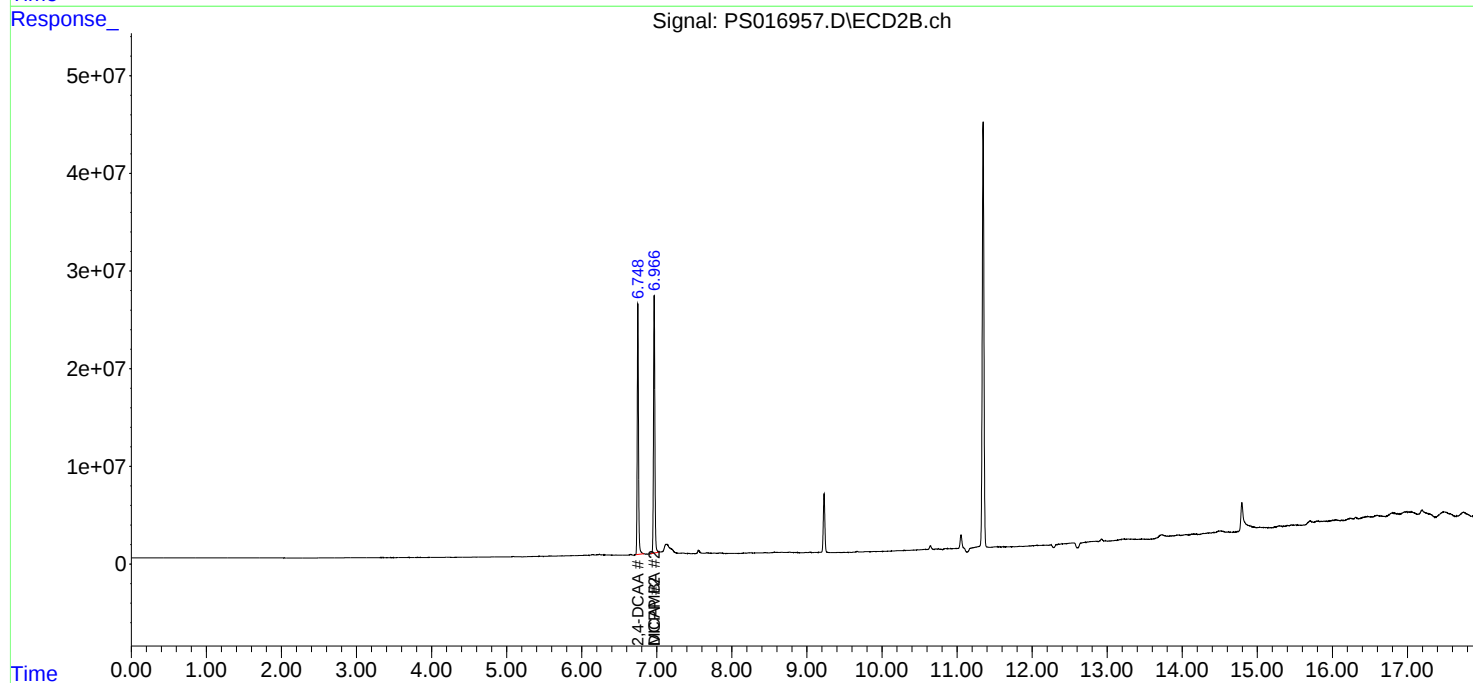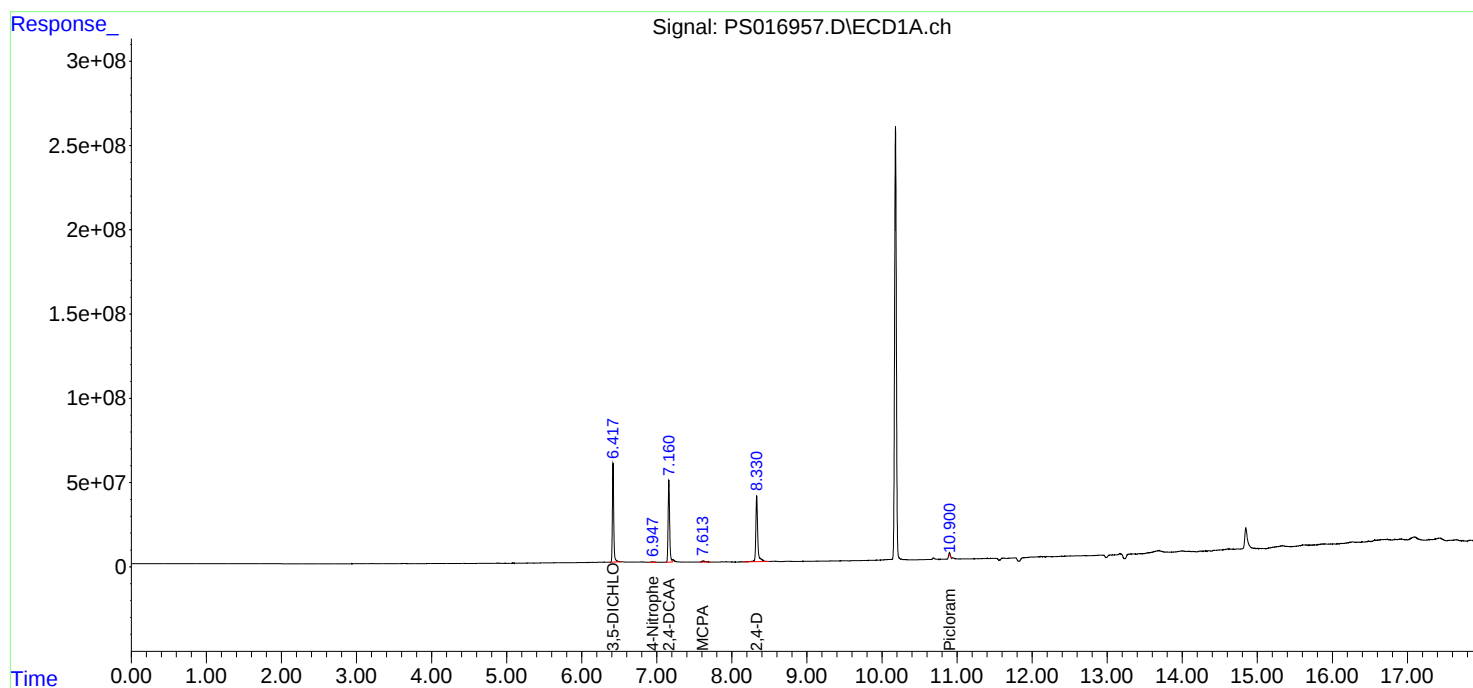


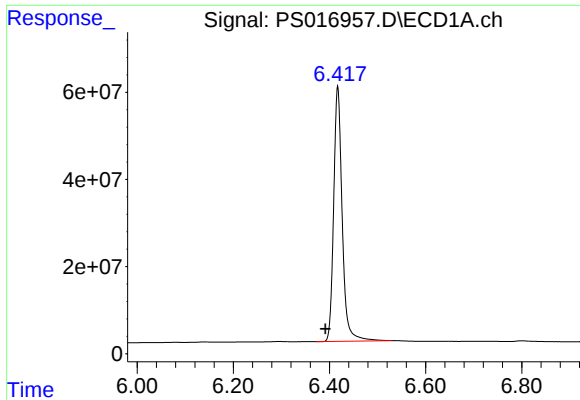

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.417 min
Delta R.T.: 0.026 min
Response: 722043431
Conc: 339.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

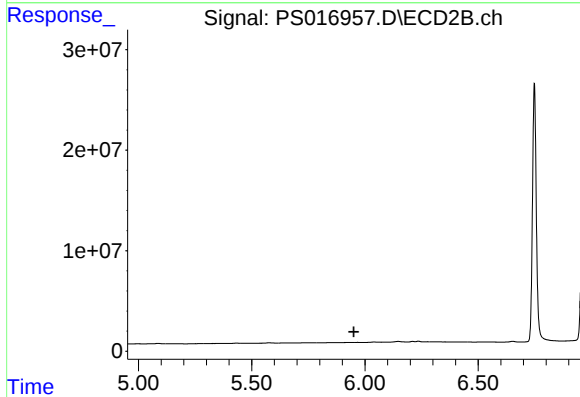


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.951 min
Response: 0
Conc: N.D.

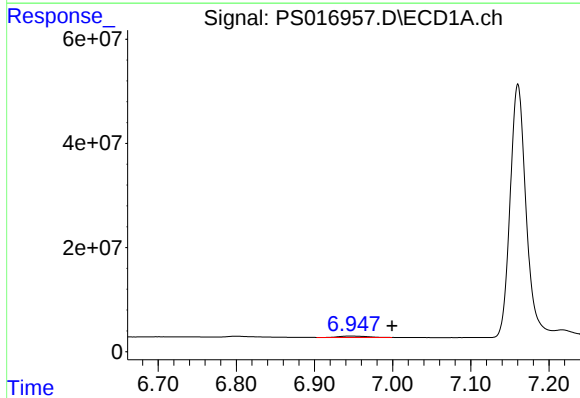


#3 4-Nitrophenol

R.T.: 6.947 min
Delta R.T.: -0.052 min
Response: 6294962
Conc: 7.27 ng/ml

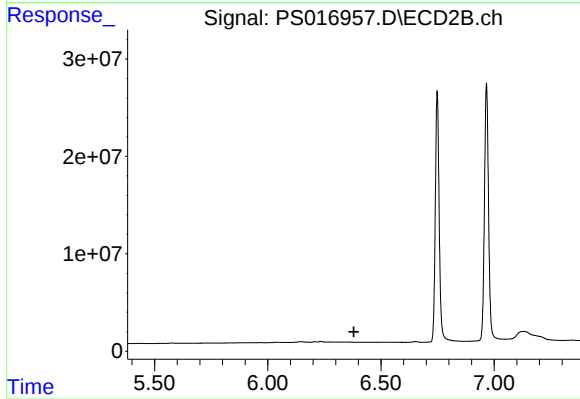

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.381 min
Response: 0
Conc: N.D.

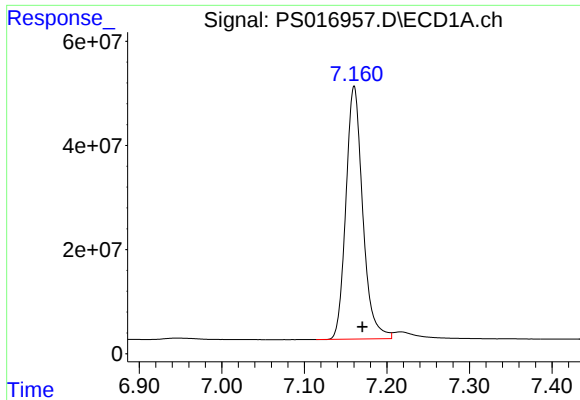

#4 2,4-DCAA


R.T.: 7.160 min
Delta R.T.: -0.010 min
Response: 687950885
Conc: 451.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

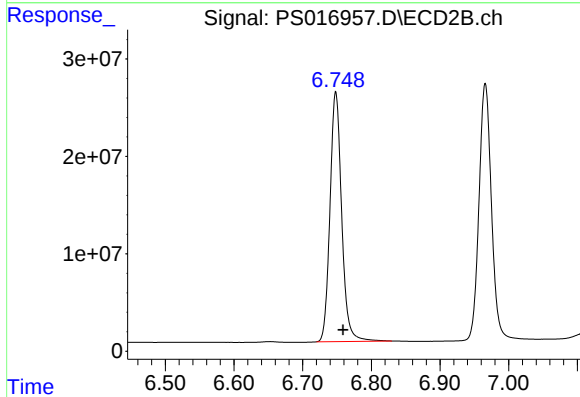


#4 2,4-DCAA

R.T.: 6.748 min
Delta R.T.: -0.011 min
Response: 303092259
Conc: 516.90 ng/ml

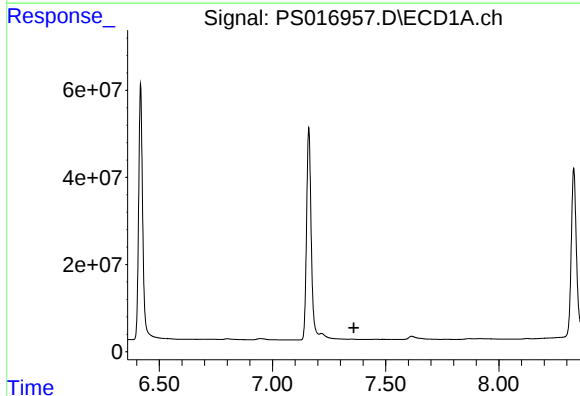


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.360 min
Response: 0
Conc: N.D.

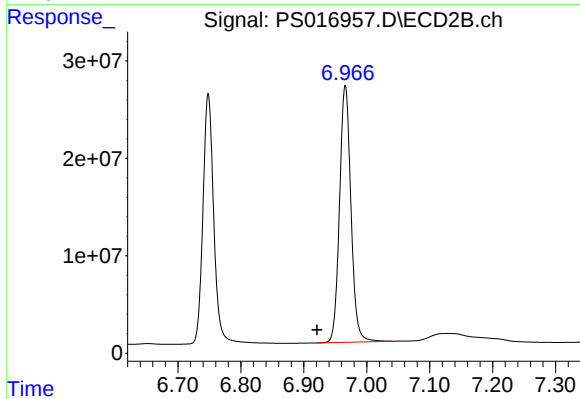

#5 DICAMBA


R.T.: 6.966 min
Delta R.T.: 0.045 min
Response: 331454726
Conc: 130.11 ng/ml

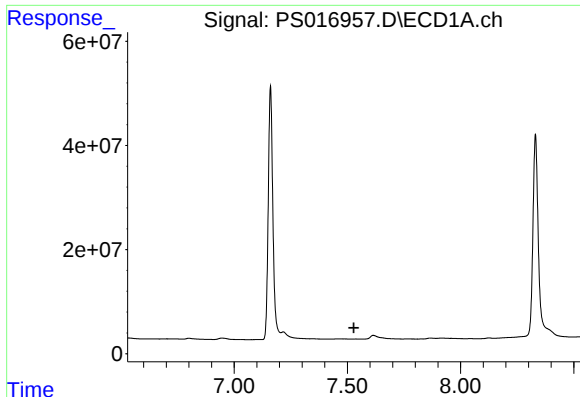

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

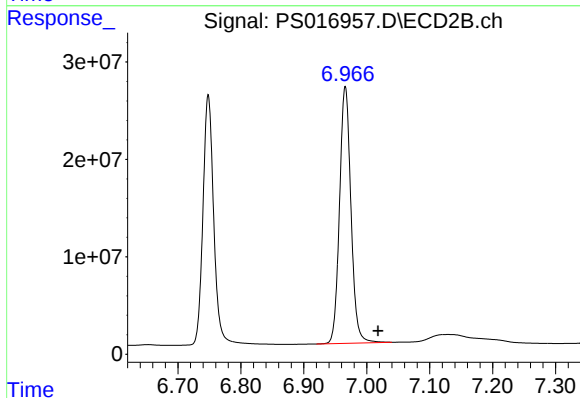


#6 MCPP

R.T.: 6.966 min
Delta R.T.: -0.052 min
Response: 331454726
Conc: 161.80 ug/ml

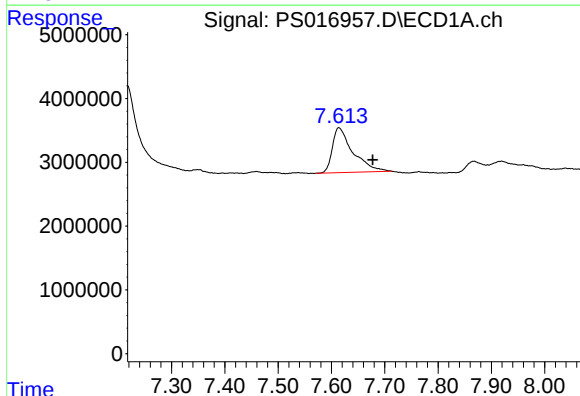


#7 MCPA

R.T.: 7.614 min
Delta R.T.: -0.064 min
Response: 18816976
Conc: 3.04 ug/ml

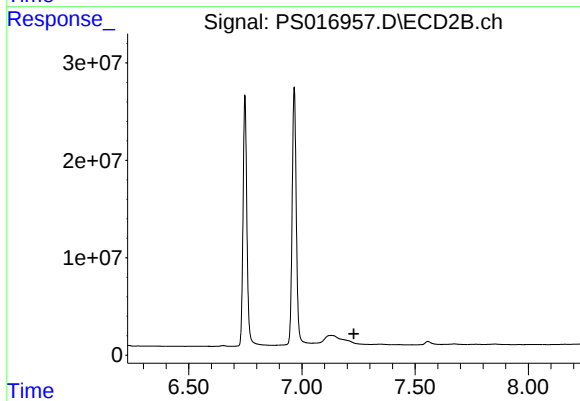

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.229 min
Response: 0
Conc: N.D.

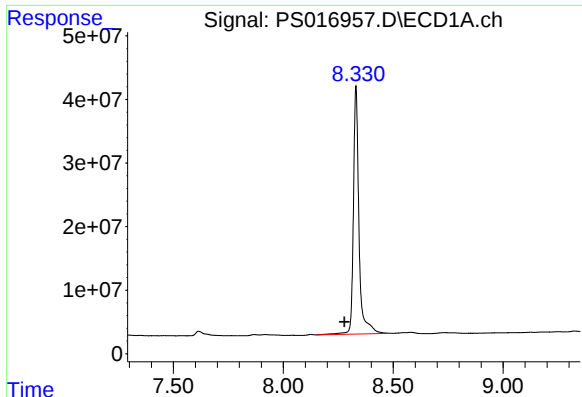

#9 2,4-D


R.T.: 8.331 min
Delta R.T.: 0.052 min
Response: 689038586
Conc: 391.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

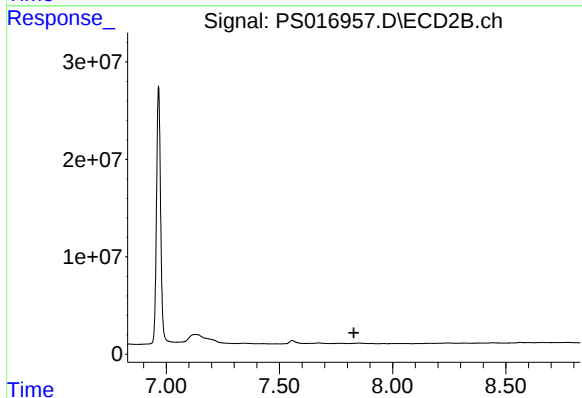


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.829 min
Response: 0
Conc: N.D.

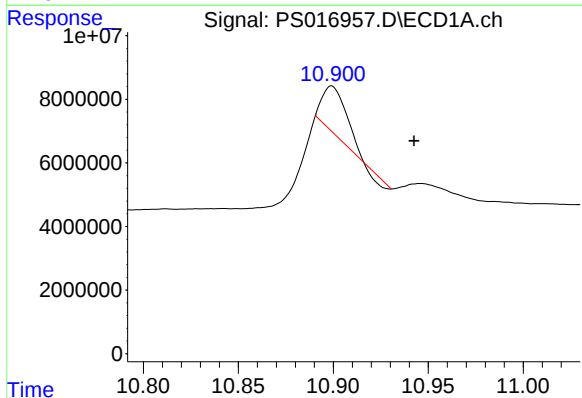

#15 Picloram

R.T.: 10.899 min
Delta R.T.: -0.043 min
Response: 12024319
Conc: 1.01 ng/ml

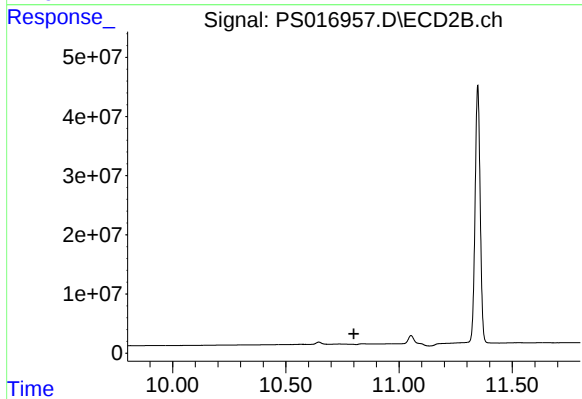

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.801 min
Response: 0
Conc: N.D.