

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100423\
 Data File : PS024531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2023 12:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 00:17:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.359	6.782	1083.1E6	362.9E6	526.439	525.003
Target Compounds							
1) T	Dalapon	2.517f	2.580	8663604	4620014	3.507	4.128
3) T	4-Nitroph...	6.200	6.378	9516892	590046	7.030	1.294 #
5) T	DICAMBA	0.000	6.943	0	1162835	N.D.	<MDL
6) T	MCP	0.000	6.986f	0	1055937	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.569	0	1847788	N.D.	2.457
9) T	2,4-D	0.000	7.846	0	782652	N.D.	<MDL
10) T	Pentachlo...	0.000	8.266	0	1459402	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.625	0	1448939	N.D.	<MDL
12) T	2,4,5-T	8.295	8.997	10472032	2311916	<MDL	<MDL #
13) T	2,4-DB	0.000	9.498	0	900951	N.D.	1.768
14) T	DINOSEB	9.848	9.828	6834544	1220969	<MDL	<MDL #
15) T	Picloram	9.680	10.781	224.6E6	64188080	12.880	10.329
16) T	DCPA	10.113	10.781	7018118	64188080	<MDL	12.303 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100423\
Data File : PS024531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2023 12:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 00:17:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

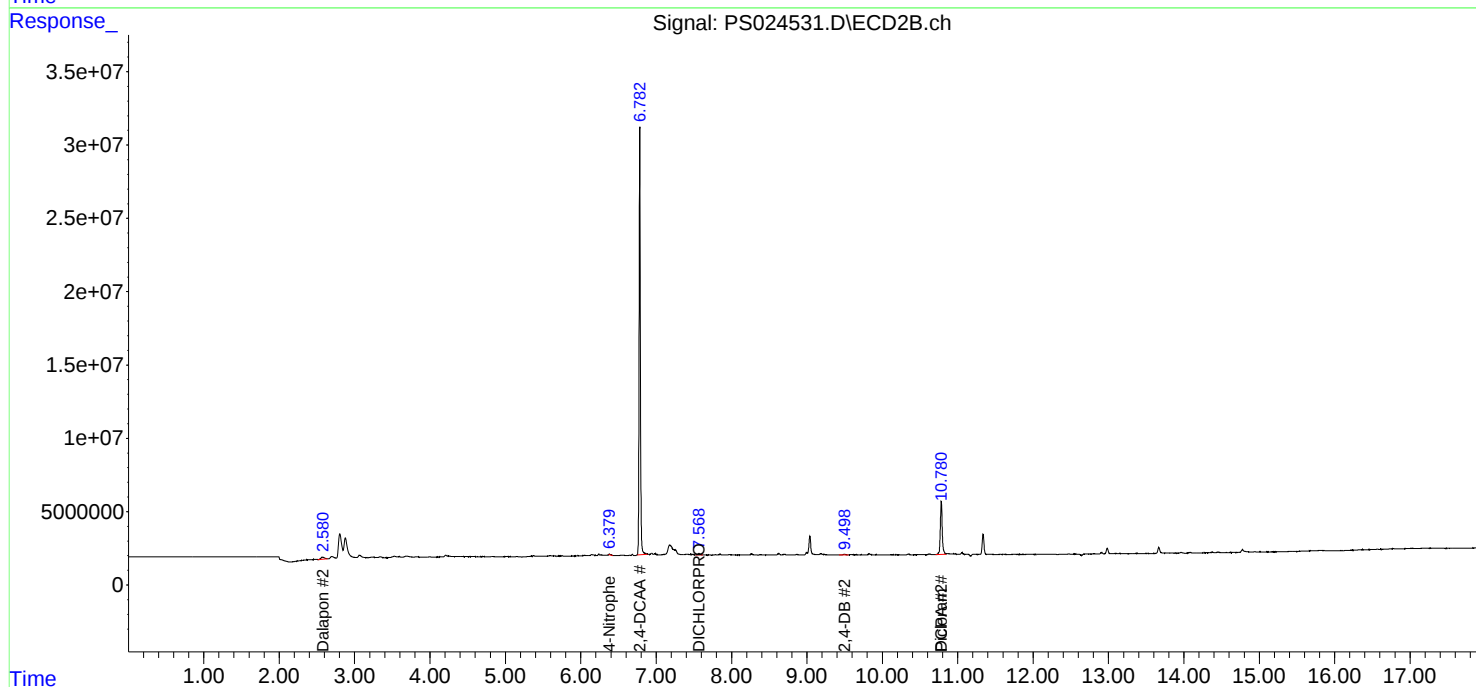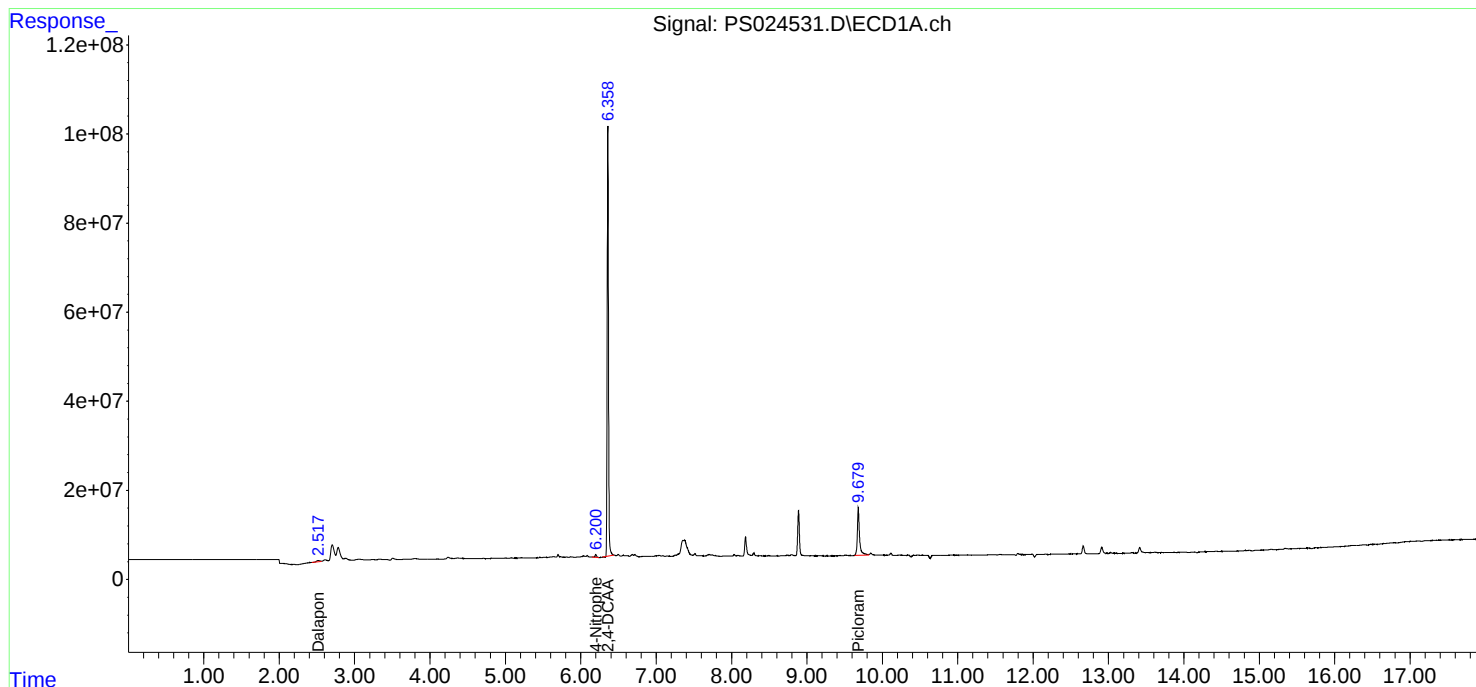


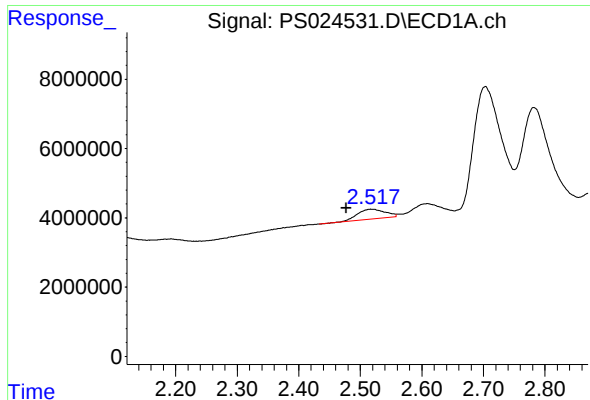

#1 Dalapon


R.T.: 2.517 min
Delta R.T.: 0.040 min
Response: 8663604
Conc: 3.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

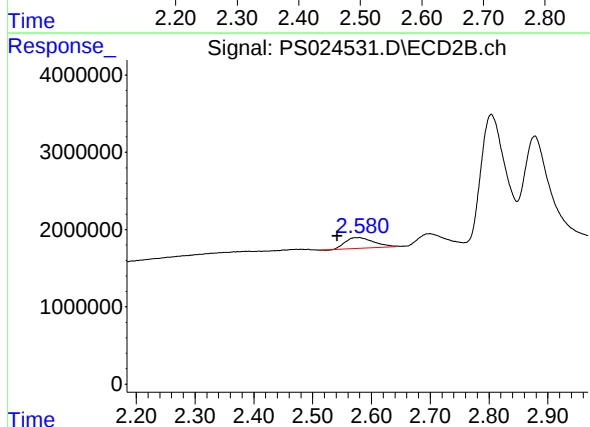


#1 Dalapon

R.T.: 2.580 min
Delta R.T.: 0.038 min
Response: 4620014
Conc: 4.13 ng/ml

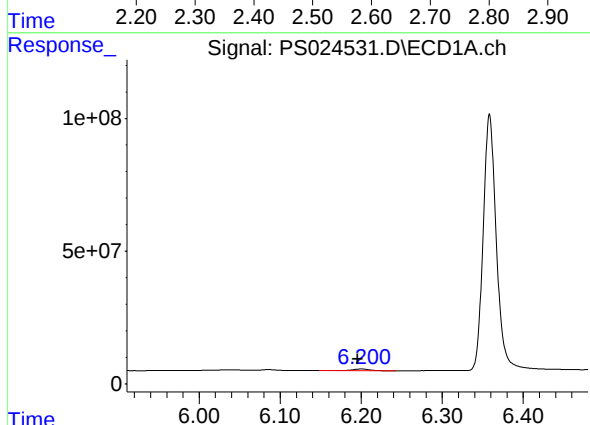


#3 4-Nitrophenol

R.T.: 6.200 min
Delta R.T.: 0.004 min
Response: 9516892
Conc: 7.03 ng/ml

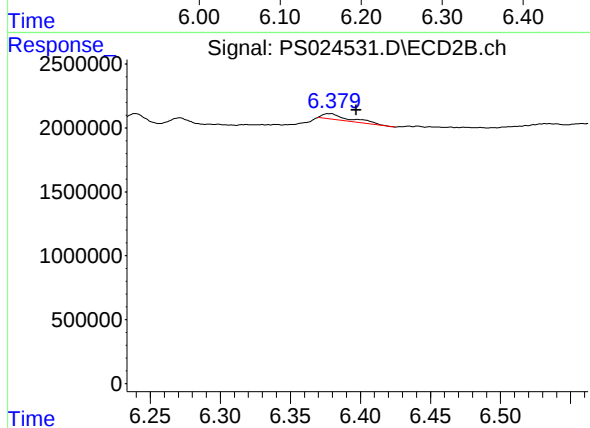

#3 4-Nitrophenol


R.T.: 6.378 min
Delta R.T.: -0.019 min
Response: 590046
Conc: 1.29 ng/ml

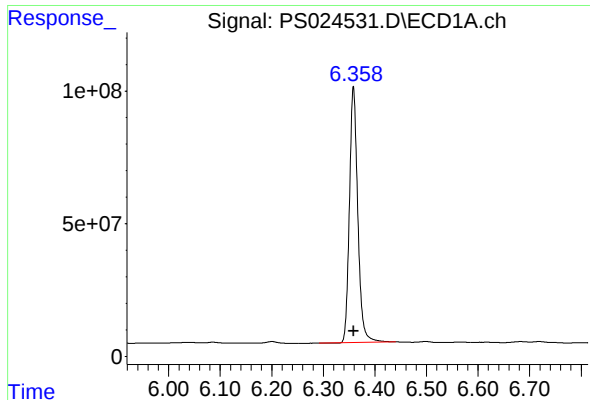

#4 2,4-DCAA


R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 1083059232
Conc: 526.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

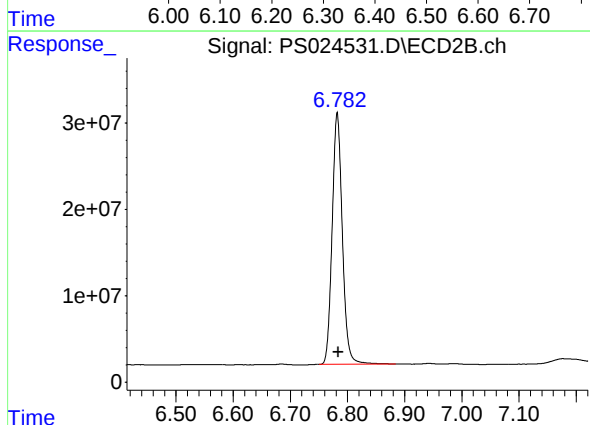


#4 2,4-DCAA

R.T.: 6.782 min
Delta R.T.: -0.002 min
Response: 362929762
Conc: 525.00 ng/ml

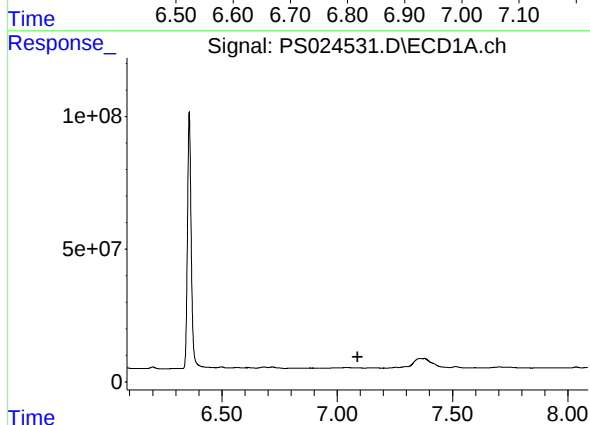


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

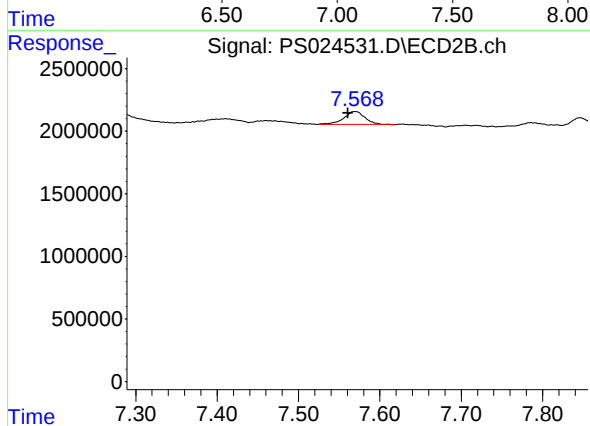

#8 DICHLORPROP


R.T.: 7.569 min
Delta R.T.: 0.009 min
Response: 1847788
Conc: 2.46 ng/ml

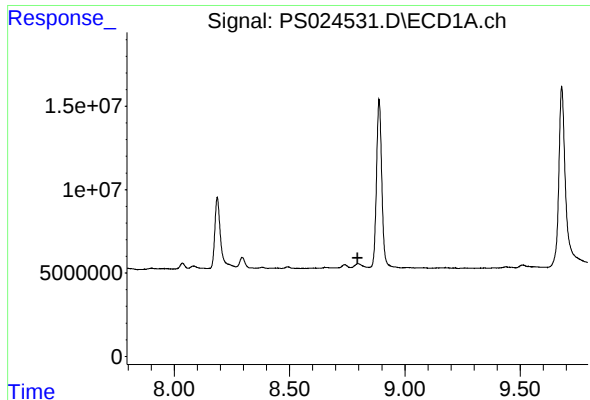

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

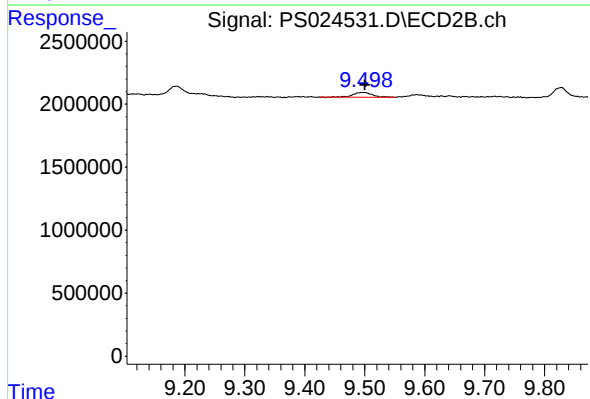


#13 2,4-DB

R.T.: 9.498 min
Delta R.T.: -0.002 min
Response: 900951
Conc: 1.77 ng/ml

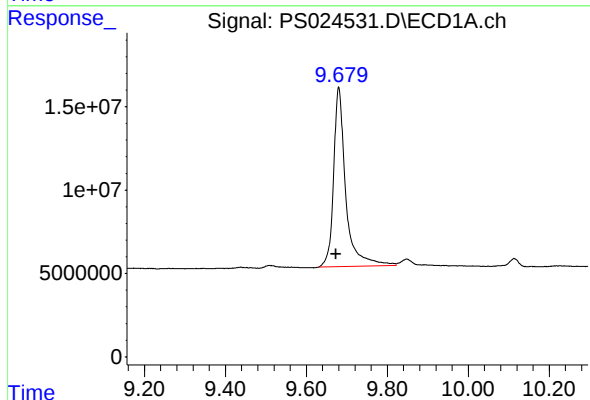


#15 Picloram

R.T.: 9.680 min
Delta R.T.: 0.007 min
Response: 224586210
Conc: 12.88 ng/ml

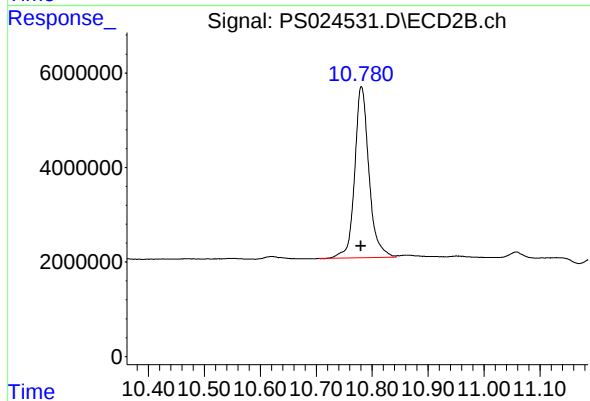

#15 Picloram


R.T.: 10.781 min
Delta R.T.: 0.000 min
Response: 64188080
Conc: 10.33 ng/ml

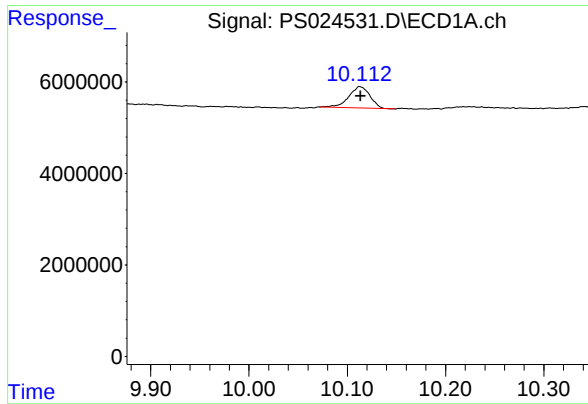

#16 DCPA

R.T.: 10.113 min
Delta R.T.: 0.000 min
Response: 7018118
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

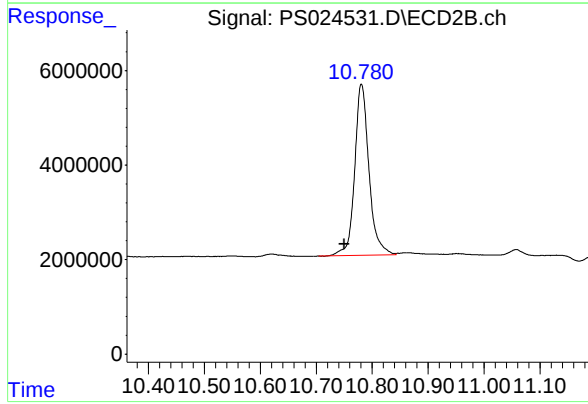

#16 DCPA

R.T.: 10.781 min
Delta R.T.: 0.031 min
Response: 64188080
Conc: 12.30 ng/ml