

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100423\
 Data File : PS024552.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2023 02:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 04:49:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.358	6.782	1115.1E6	375.7E6	541.991	543.527
Target Compounds							
1) T	Dalapon	0.000	2.572	0	4275261	N.D.	3.820
3) T	4-Nitroph...	6.199	6.377	8615369	181072	6.364	<MDL #
5) T	DICAMBA	0.000	6.942	0	986481	N.D.	<MDL
6) T	MCP	6.681	6.985f	2822797	897046	<MDL	<MDL #
8) T	DICHLORPROP	0.000	7.571	0	3183544	N.D.	4.233
9) T	2,4-D	7.353f	7.845	192.9E6	432269	69.812	<MDL #
10) T	Pentachlo...	7.513	8.265	10397766	1765140	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.625	0	1252003	N.D.	<MDL
12) T	2,4,5-T	0.000	8.997	0	1568561	N.D.	<MDL
13) T	2,4-DB	0.000	9.490	0	695979	N.D.	1.366
14) T	DINOSEB	0.000	9.825	0	783246	N.D.	<MDL
15) T	Picloram	9.681	10.782	26944173	7955368	1.545	1.280
16) T	DCPA	0.000	10.749	0	1707441	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100423\
Data File : PS024552.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2023 02:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 04:49:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

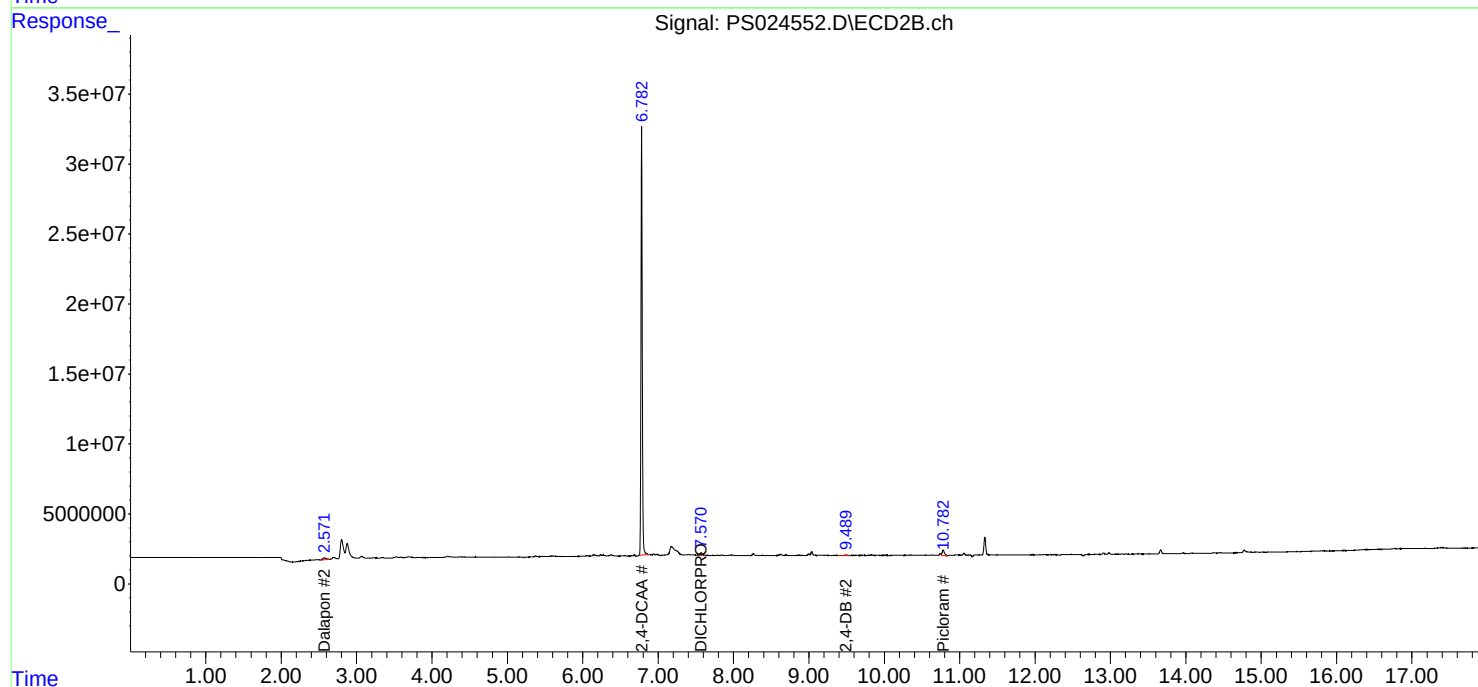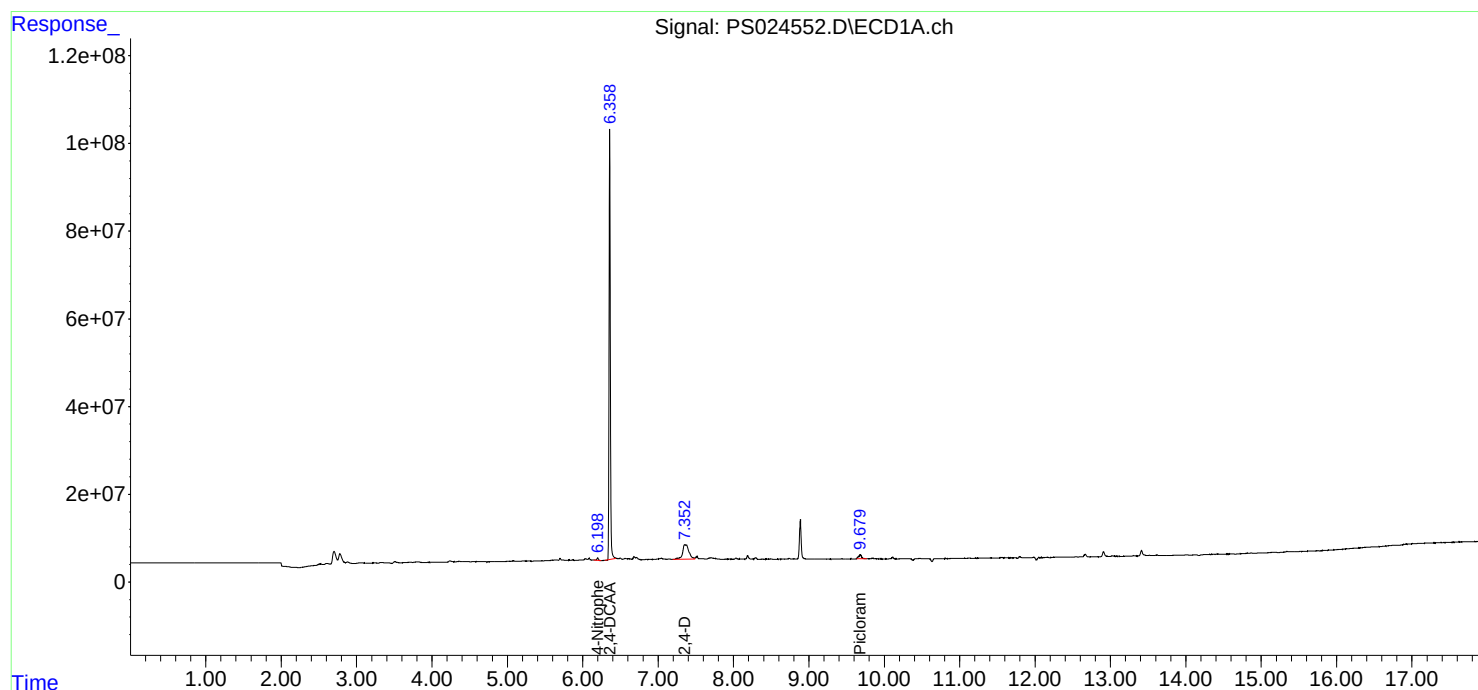


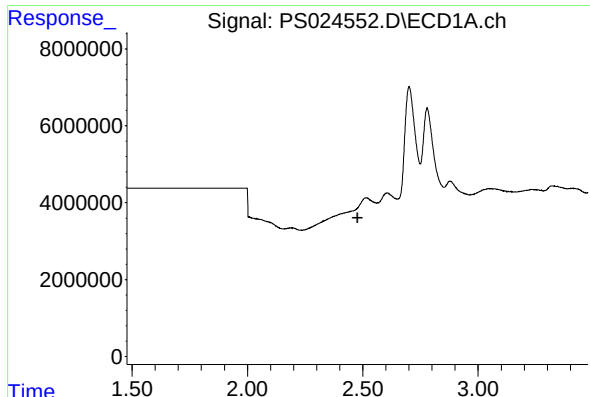

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

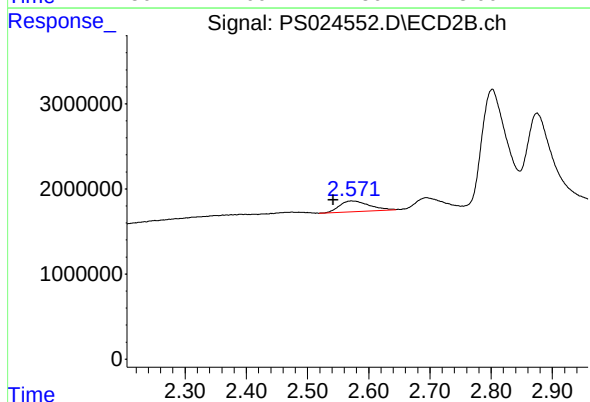


#1 Dalapon

R.T.: 2.572 min
Delta R.T.: 0.030 min
Response: 4275261
Conc: 3.82 ng/ml

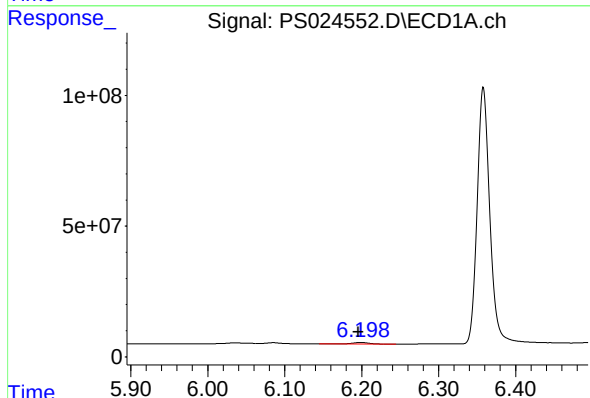


#3 4-Nitrophenol

R.T.: 6.199 min
Delta R.T.: 0.003 min
Response: 8615369
Conc: 6.36 ng/ml

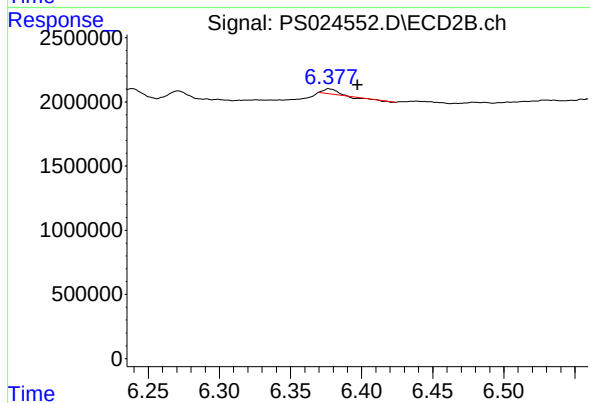

#3 4-Nitrophenol


R.T.: 6.377 min
Delta R.T.: -0.020 min
Response: 181072
Conc: N.D.

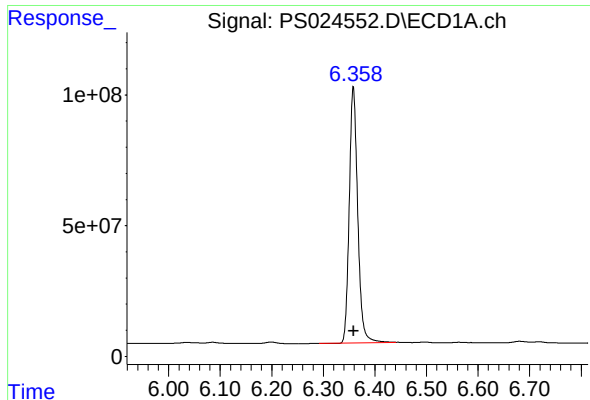

#4 2,4-DCAA


R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 1115054431
Conc: 541.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

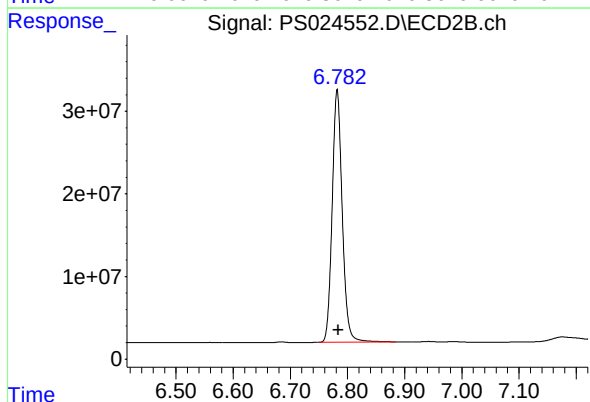


#4 2,4-DCAA

R.T.: 6.782 min
Delta R.T.: -0.002 min
Response: 375734823
Conc: 543.53 ng/ml

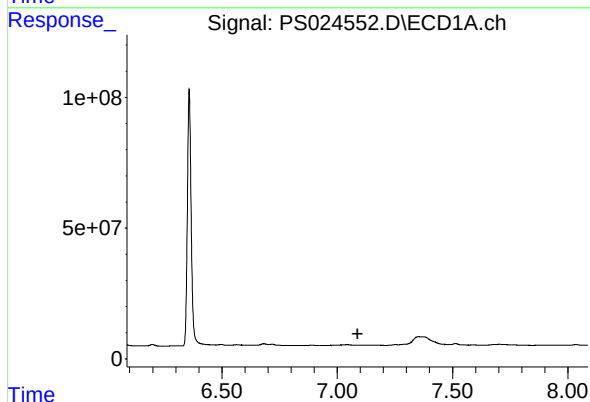


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

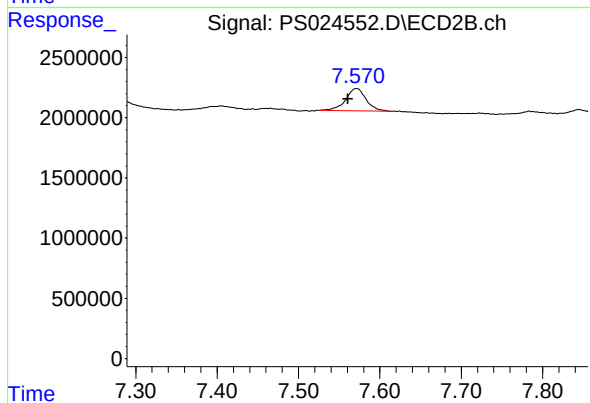

#8 DICHLORPROP


R.T.: 7.571 min
Delta R.T.: 0.010 min
Response: 3183544
Conc: 4.23 ng/ml

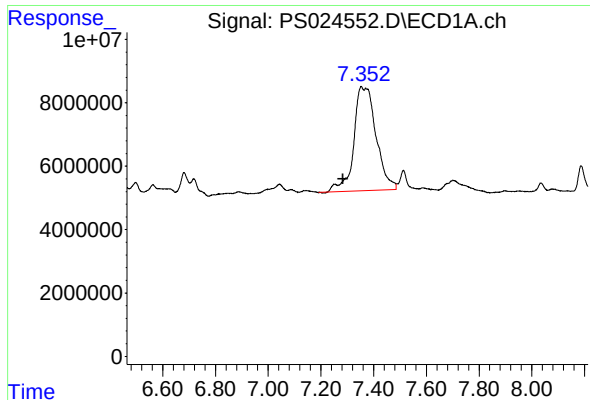

#9 2,4-D


R.T.: 7.353 min
Delta R.T.: 0.069 min
Response: 192891336
Conc: 69.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

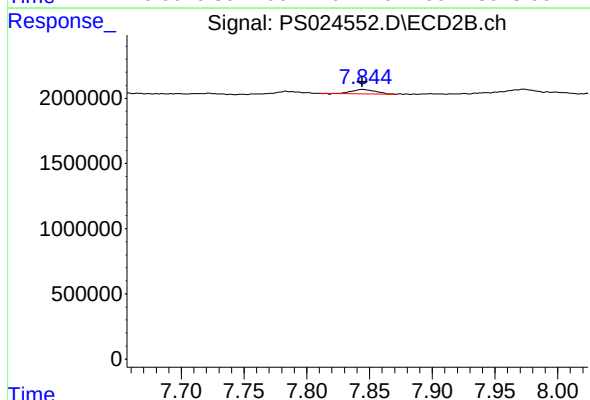


#9 2,4-D

R.T.: 7.845 min
Delta R.T.: 0.000 min
Response: 432269
Conc: N.D.

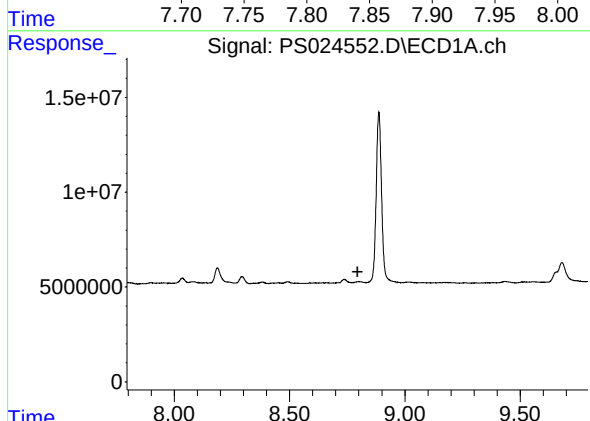


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

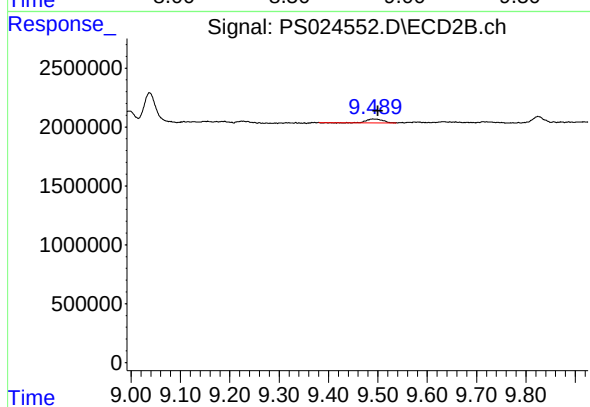

#13 2,4-DB


R.T.: 9.490 min
Delta R.T.: -0.010 min
Response: 695979
Conc: 1.37 ng/ml

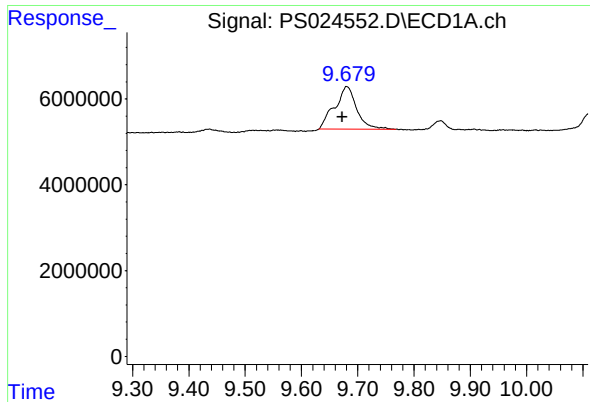

#15 Picloram

R.T.: 9.681 min
Delta R.T.: 0.008 min
Response: 26944173
Conc: 1.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

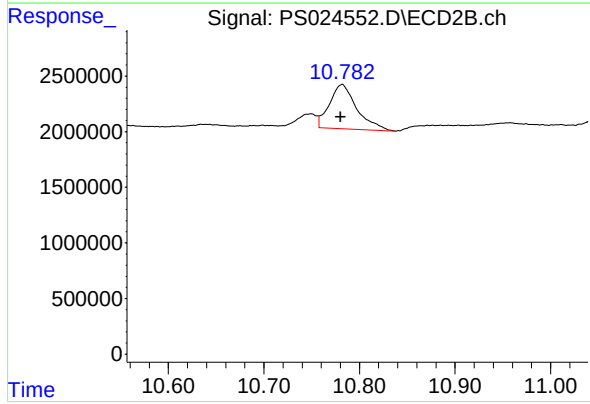

#15 Picloram

R.T.: 10.782 min
Delta R.T.: 0.002 min
Response: 7955368
Conc: 1.28 ng/ml