

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100520\
 Data File : PS012620.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2020 12:54
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 15:50:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.222	6.913	390.5E6	211.3E6	398.725	459.321
Target Compounds							
2) T	3,5-DICHL...	0.000	6.007	0	8463065	N.D.	11.870
6) T	MCP	7.620	0.000	14412720	0	4.940	N.D. #
7) T	MCPA	7.693	0.000	32585071	0	7.813	N.D. #
12) T	2,4,5-T	9.444	0.000	10595880	0	1.885	N.D. #
15) T	Picloram	0.000	11.053	0	37307952	N.D.	9.466



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100520\
Data File : PS012620.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2020 12:54
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 15:50:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

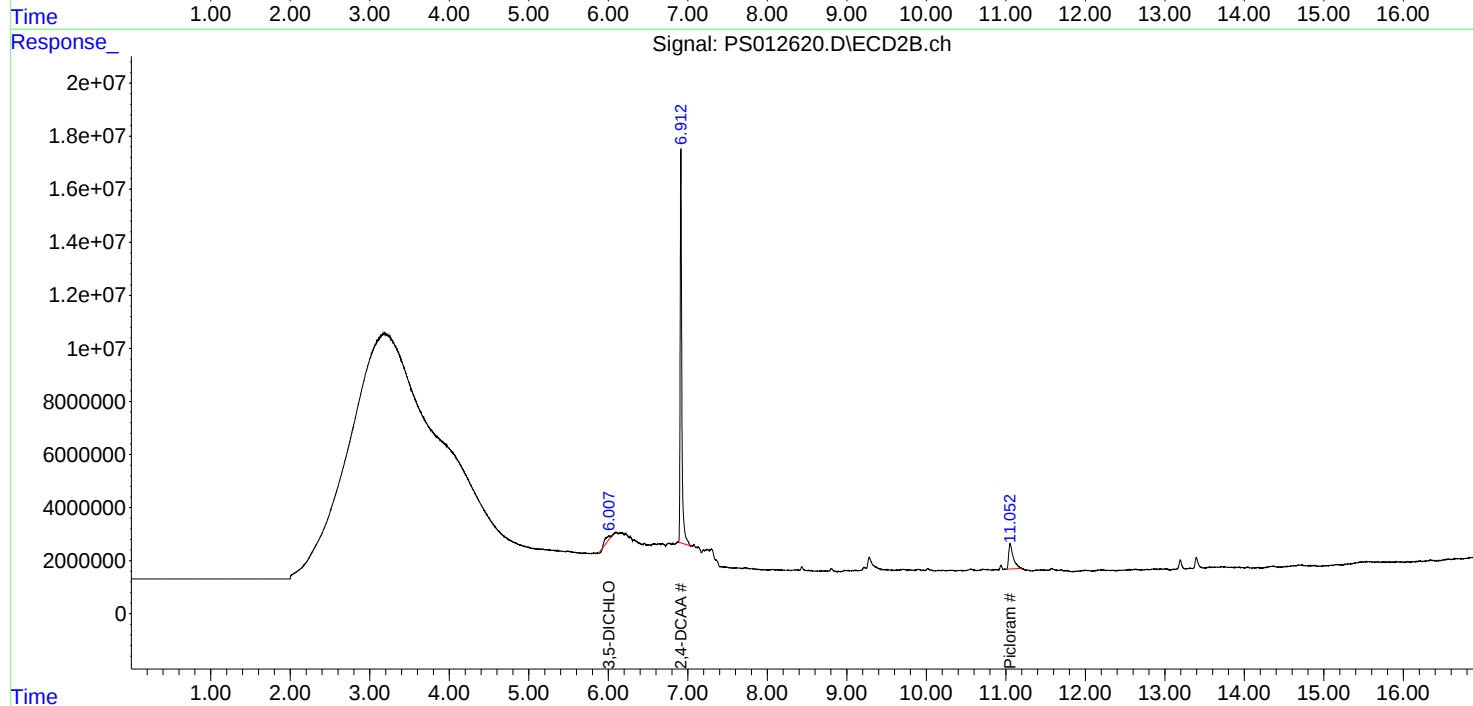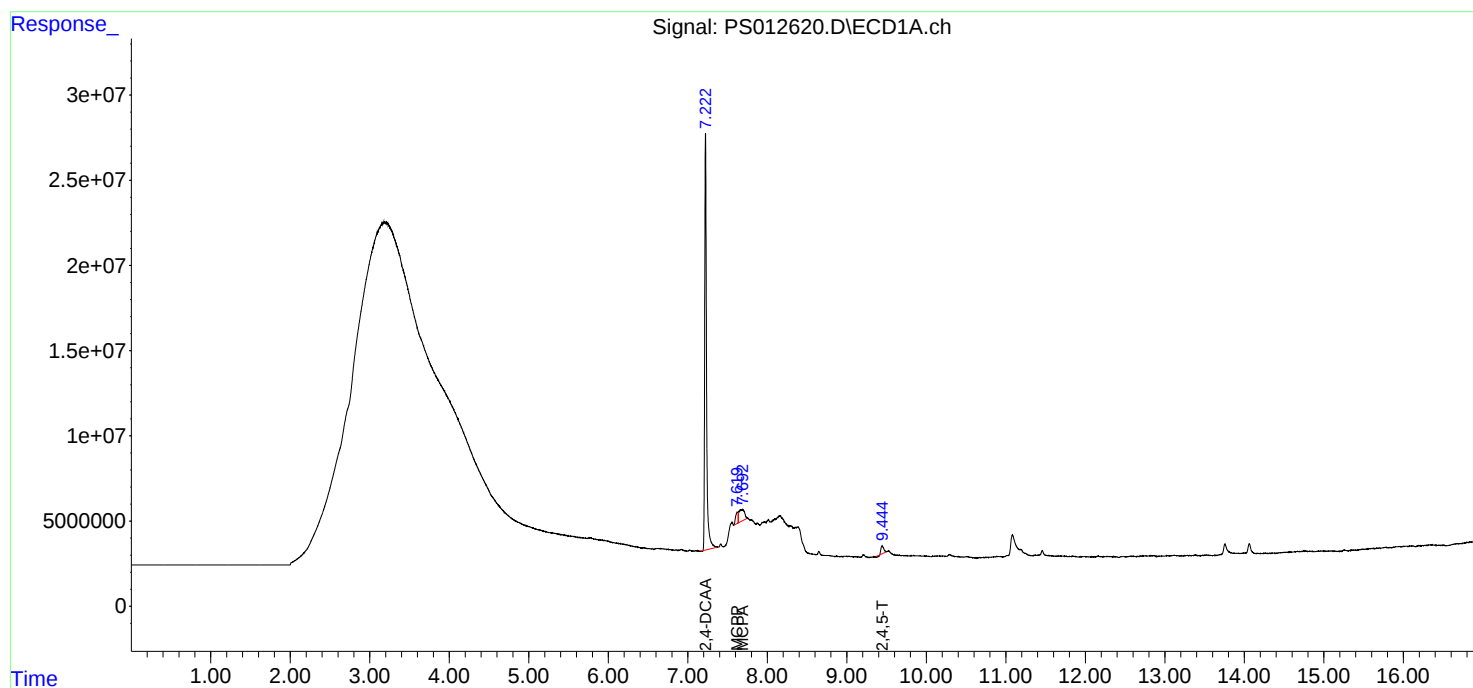


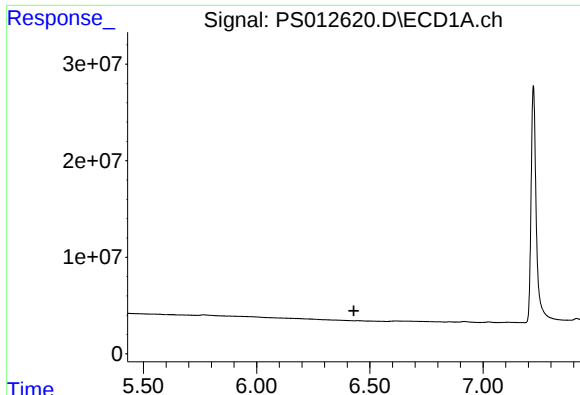

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

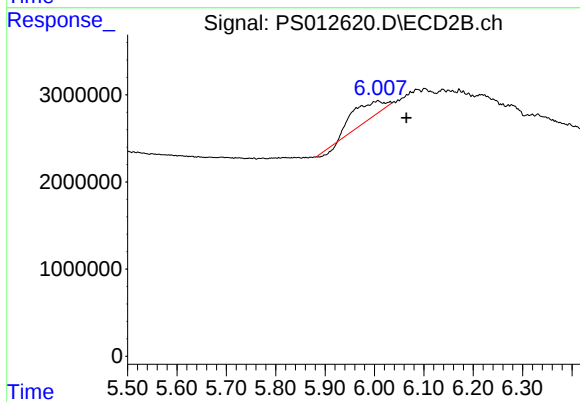


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.007 min
Delta R.T.: -0.057 min
Response: 8463065
Conc: 11.87 ng/ml

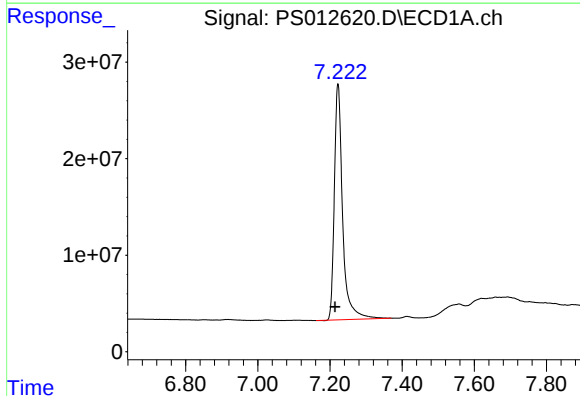


#4 2,4-DCAA

R.T.: 7.222 min
Delta R.T.: 0.008 min
Response: 390530571
Conc: 398.72 ng/ml

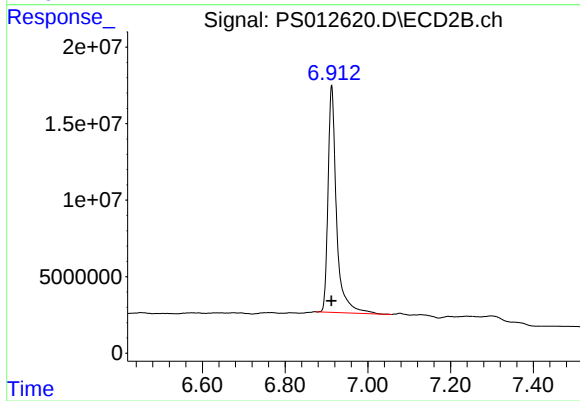

#4 2,4-DCAA


R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 211295357
Conc: 459.32 ng/ml

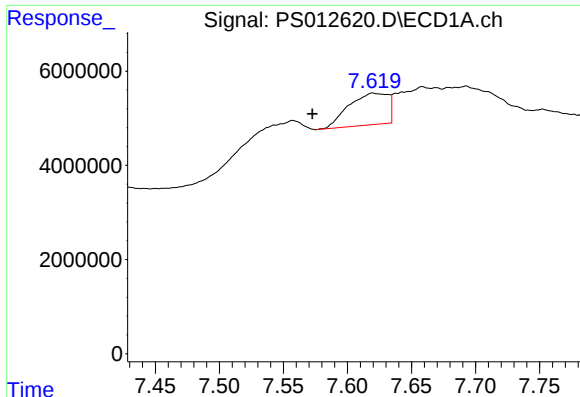

#6 MCPP


R.T.: 7.620 min
Delta R.T.: 0.047 min
Response: 14412720
Conc: 4.94 ug/ml

Instrument :
ECD_S
ClientSampleId :

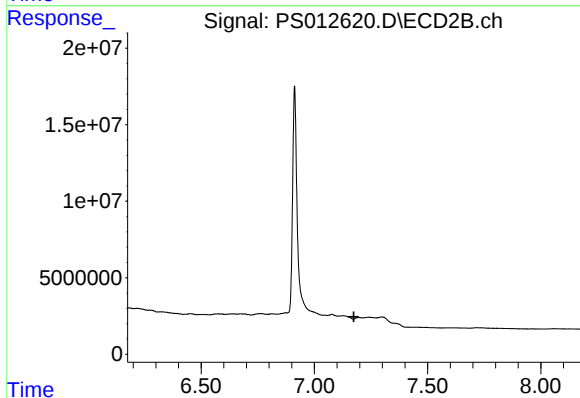


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.175 min
Response: 0
Conc: N.D.

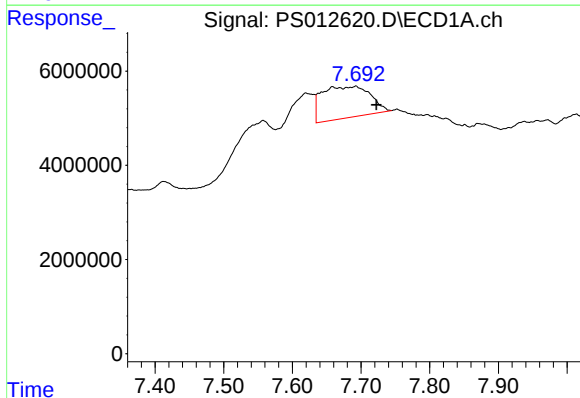


#7 MCPA

R.T.: 7.693 min
Delta R.T.: -0.030 min
Response: 32585071
Conc: 7.81 ug/ml

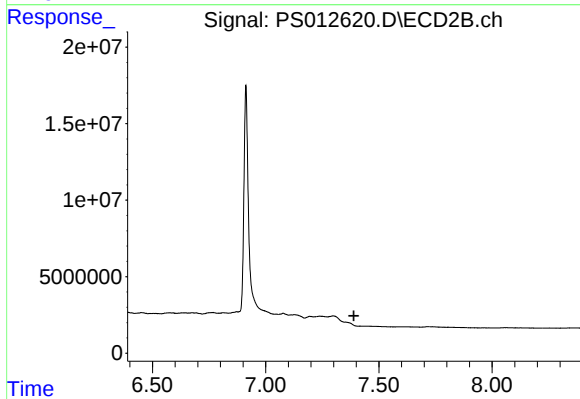

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.390 min
Response: 0
Conc: N.D.

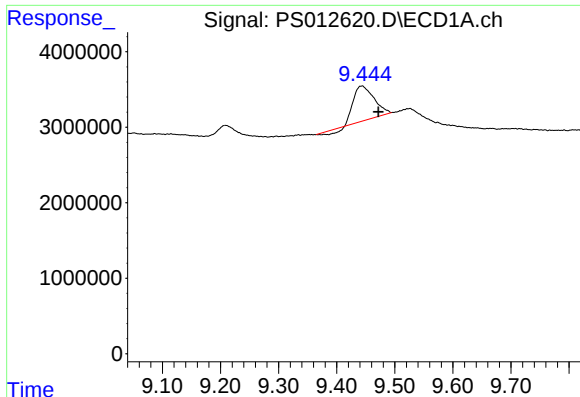

#12 2,4,5-T


R.T.: 9.444 min
Delta R.T.: -0.028 min
Response: 10595880
Conc: 1.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

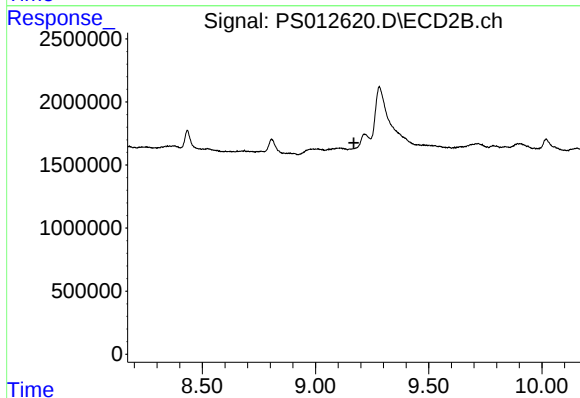


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.169 min
Response: 0
Conc: N.D.

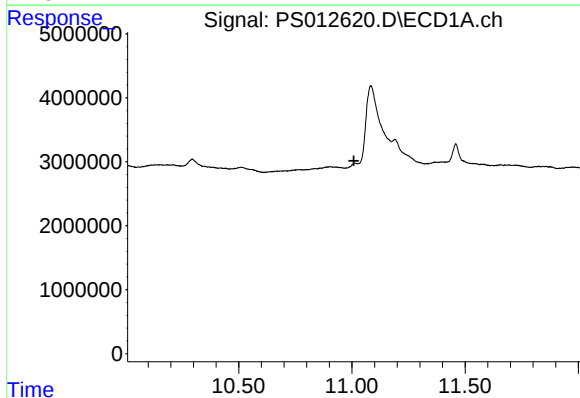

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

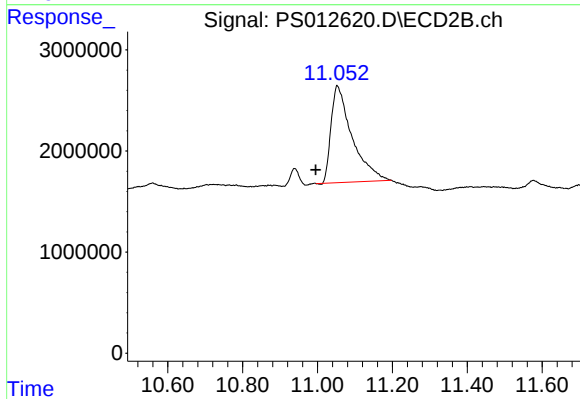

#15 Picloram

R.T.: 11.053 min
Delta R.T.: 0.057 min
Response: 37307952
Conc: 9.47 ng/ml