

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100621\
 Data File : PS016995.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2021 19:52
 Operator : DD\AJ
 Sample : PB139665BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 01:59:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.181	0.000	4700575	0	3.085	N.D. #
Target Compounds							
7) T	MCPA	7.649	0.000	242.8E6	0	39.257	N.D. #
9) T	2,4-D	8.339f	0.000	96845358	0	55.080	N.D. #
12) T	2,4,5-T	0.000	9.042f	0	8224561	N.D.	2.527
15) T	Picloram	10.952	10.796	119.6E6	38372280	10.045	8.945
16) T	DCPA	0.000	10.796f	0	38372280	N.D.	8.803



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100621\
Data File : PS016995.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2021 19:52
Operator : DD\AJ
Sample : PB139665BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 01:59:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

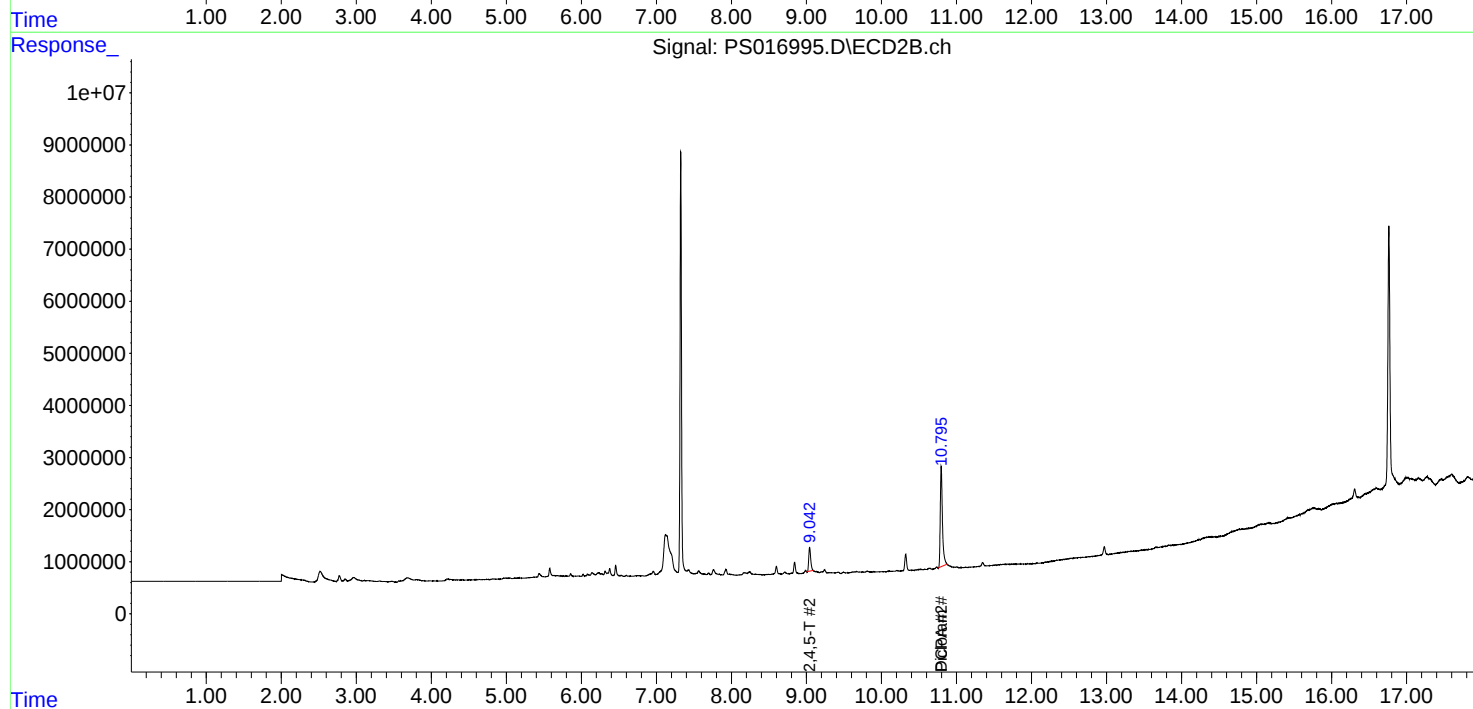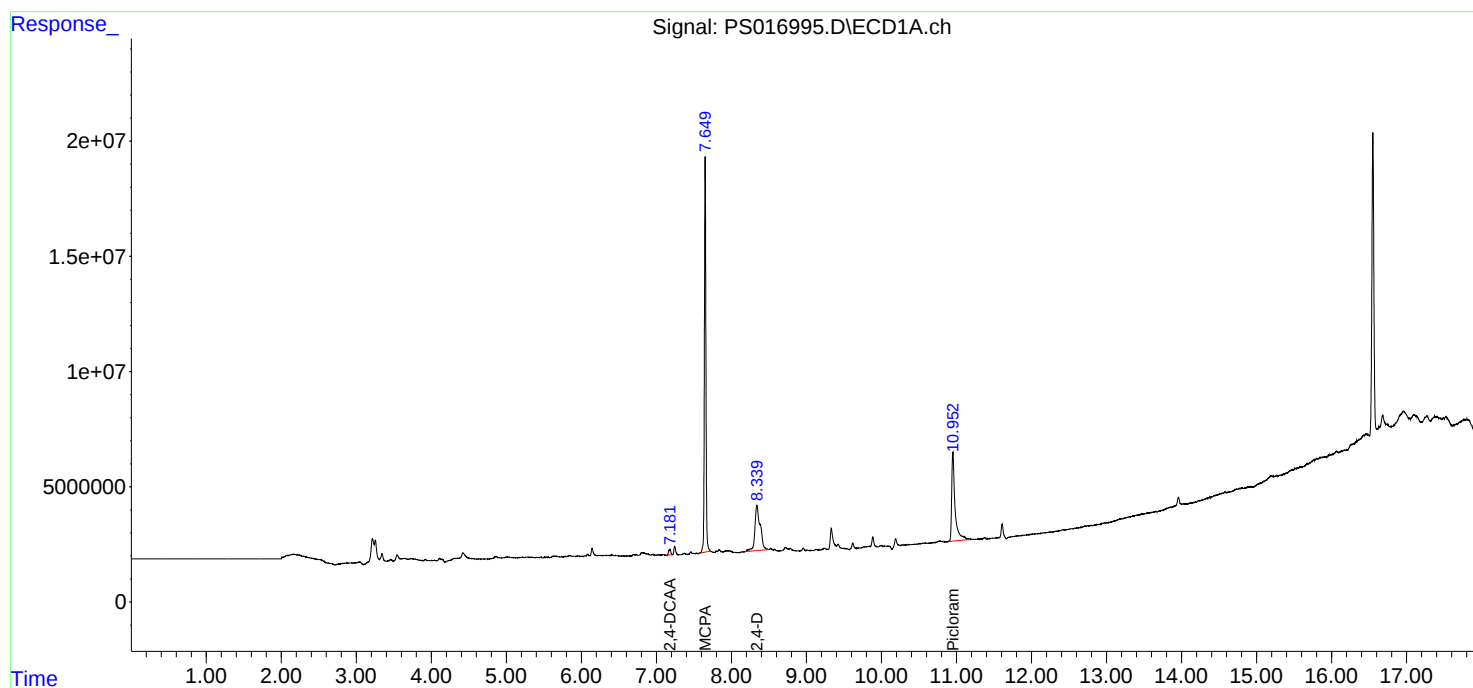


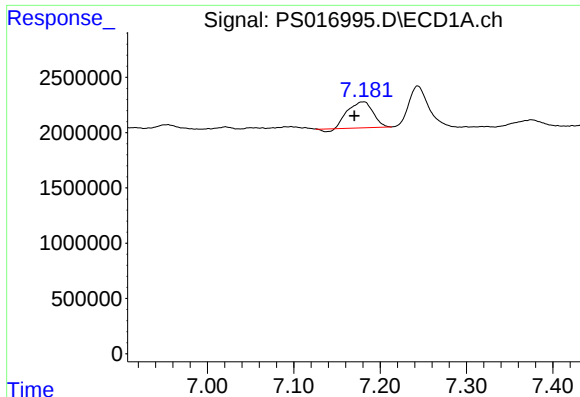

#4 2,4-DCAA


R.T.: 7.181 min
Delta R.T.: 0.010 min
Response: 4700575
Conc: 3.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

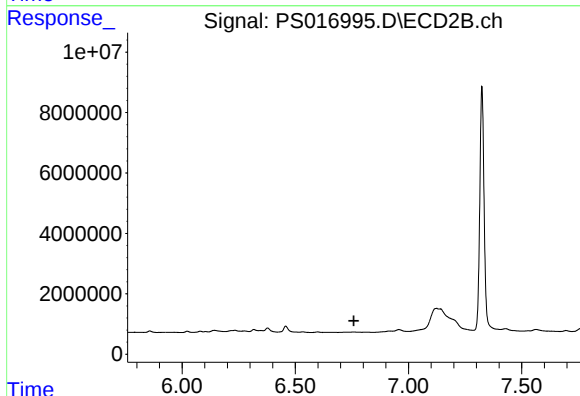


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

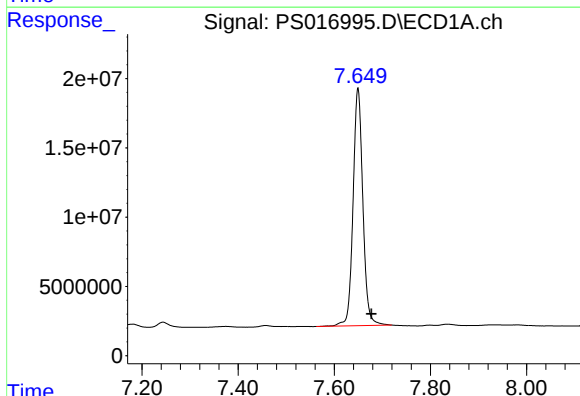


#7 MCPA

R.T.: 7.649 min
Delta R.T.: -0.028 min
Response: 242787277
Conc: 39.26 ug/ml

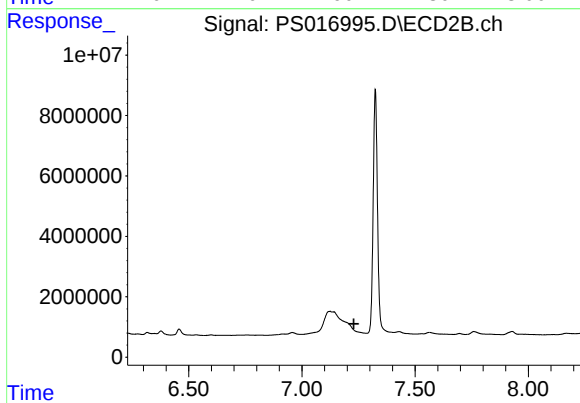

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.229 min
Response: 0
Conc: N.D.

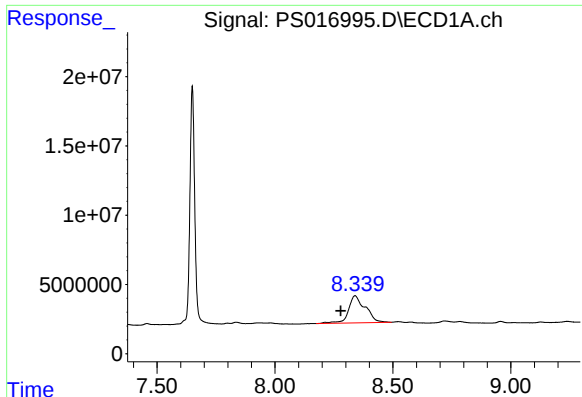

#9 2,4-D


R.T.: 8.339 min
Delta R.T.: 0.061 min
Response: 96845358
Conc: 55.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

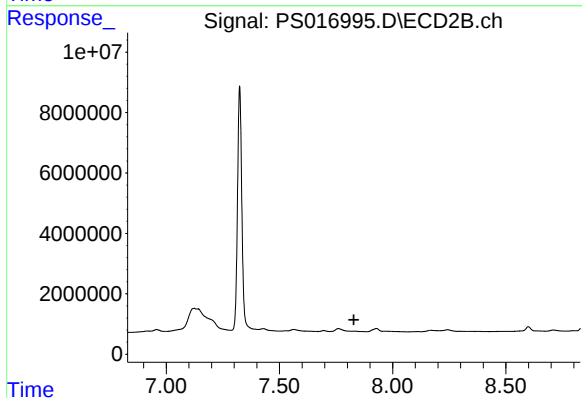


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.829 min
Response: 0
Conc: N.D.

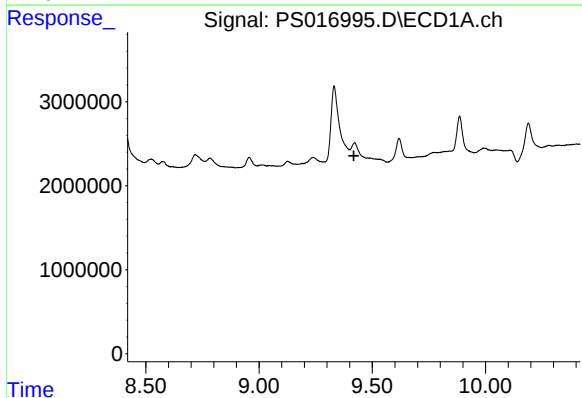


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.418 min
Response: 0
Conc: N.D.

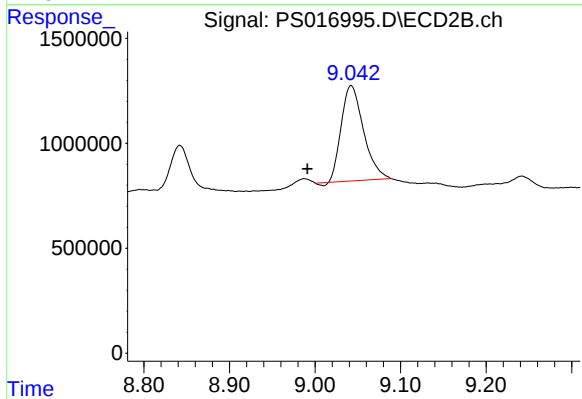

#12 2,4,5-T


R.T.: 9.042 min
Delta R.T.: 0.051 min
Response: 8224561
Conc: 2.53 ng/ml

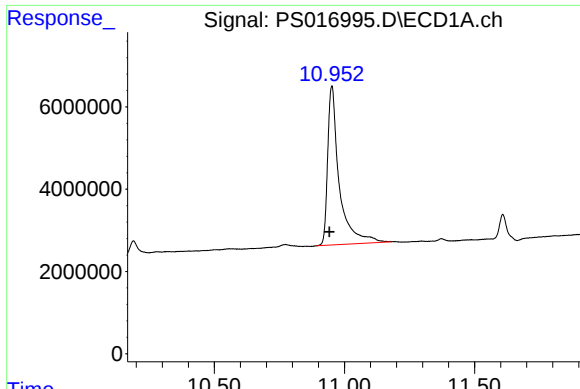

#15 Picloram


R.T.: 10.952 min
Delta R.T.: 0.009 min
Response: 119550194
Conc: 10.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

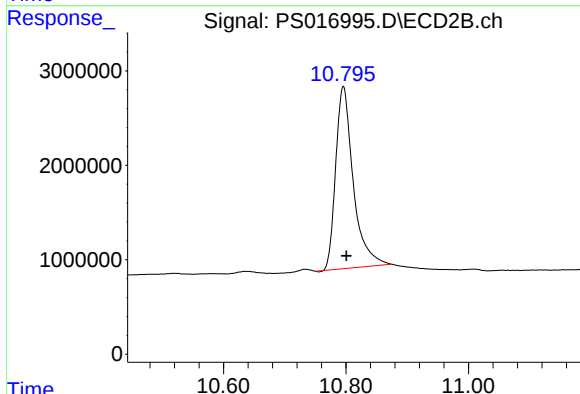


#15 Picloram

R.T.: 10.796 min
Delta R.T.: -0.005 min
Response: 38372280
Conc: 8.95 ng/ml

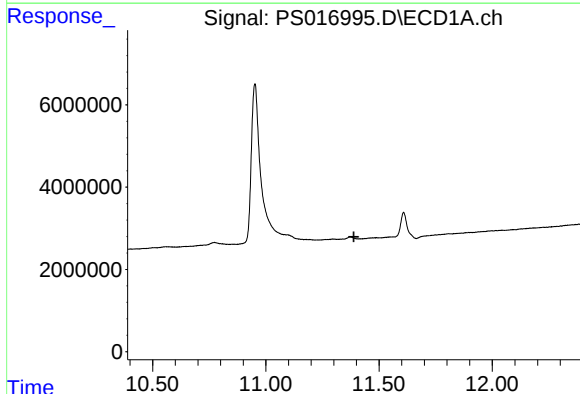

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.389 min
Response: 0
Conc: N.D.

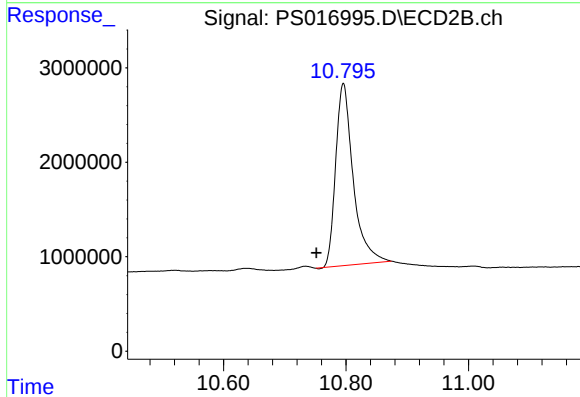

#16 DCPA

R.T.: 10.796 min
Delta R.T.: 0.044 min
Response: 38372280
Conc: 8.80 ng/ml