

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100621\
 Data File : PS016997.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2021 20:40
 Operator : DD\AJ
 Sample : PB139665TB
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 02:00:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.181	0.000	4691715	0	3.079	N.D.	#
Target Compounds								
7) T	MCPA	7.650	0.000	241.3E6	0	39.023	N.D.	#
9) T	2,4-D	8.340f	0.000	92447012	0	52.579	N.D.	#
15) T	Picloram	10.971	0.000	7781786	0	<MDL	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100621\
Data File : PS016997.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2021 20:40
Operator : DD\AJ
Sample : PB139665TB
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 02:00:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

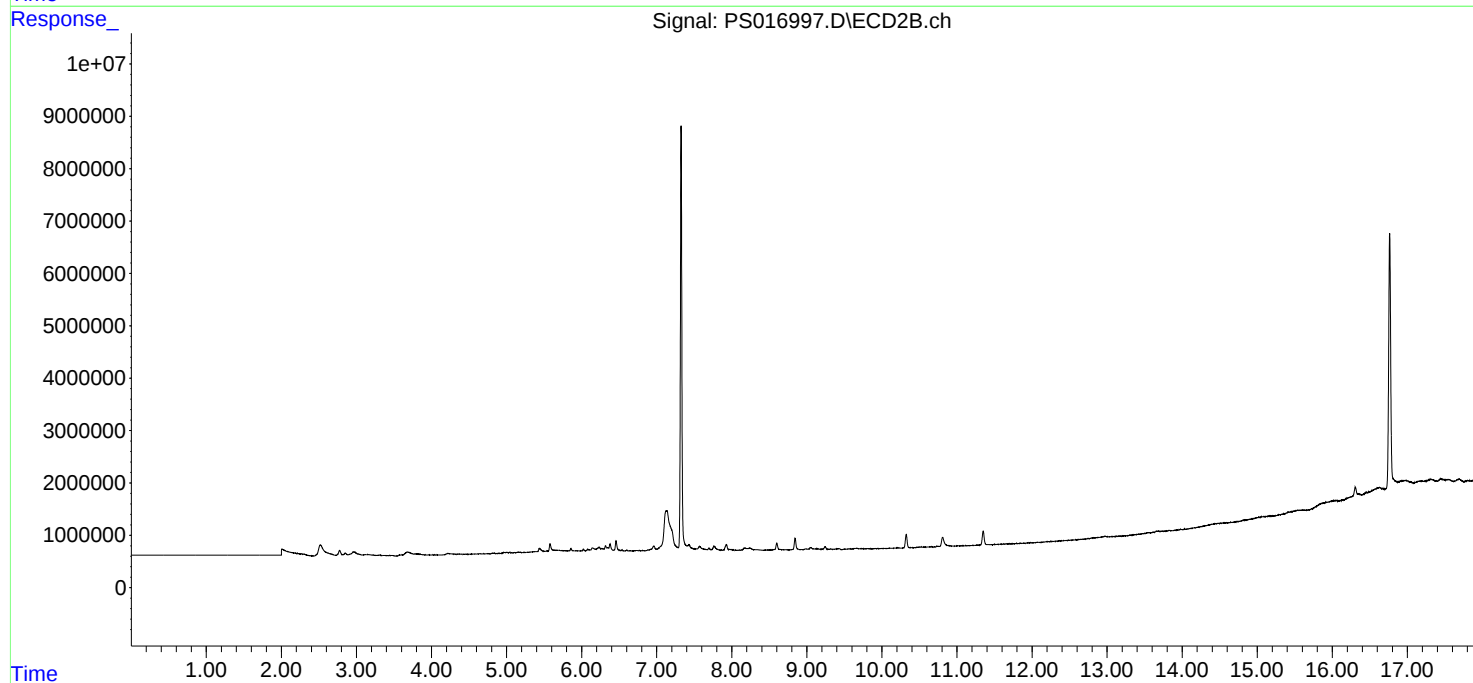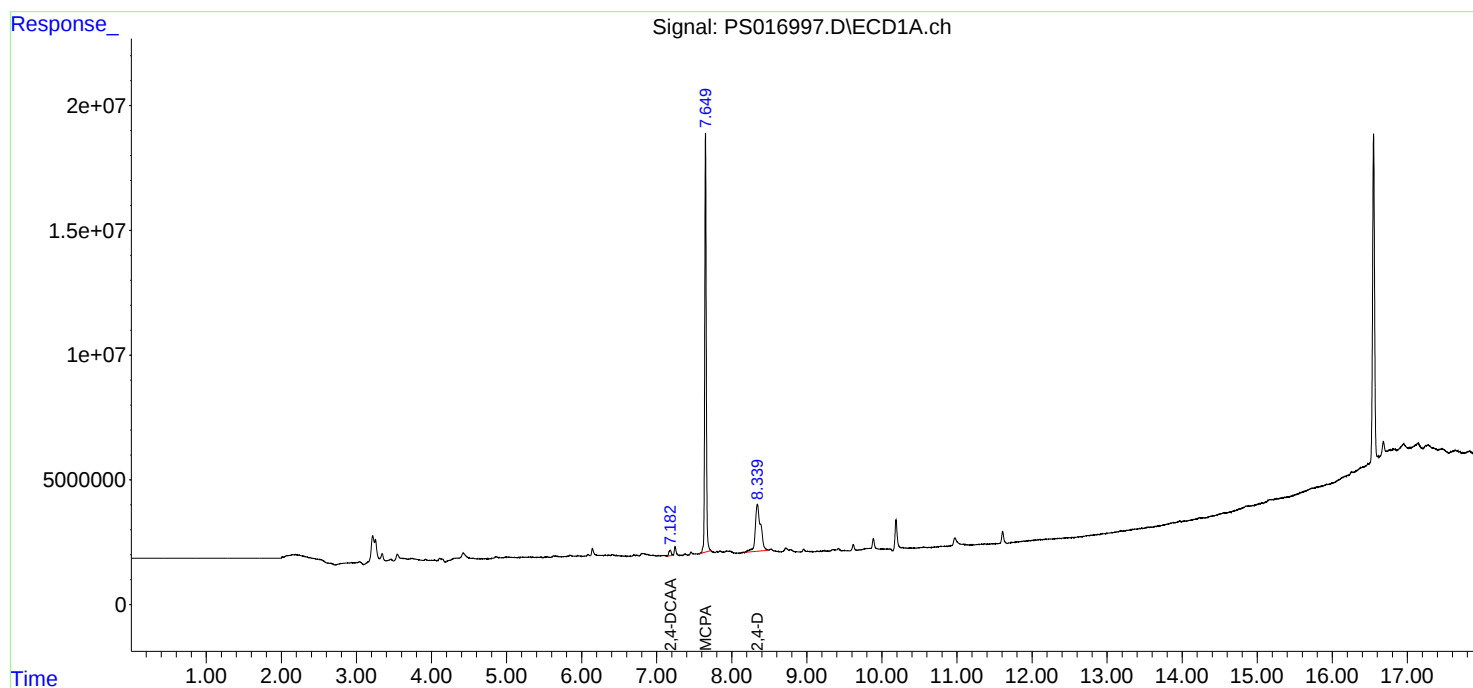


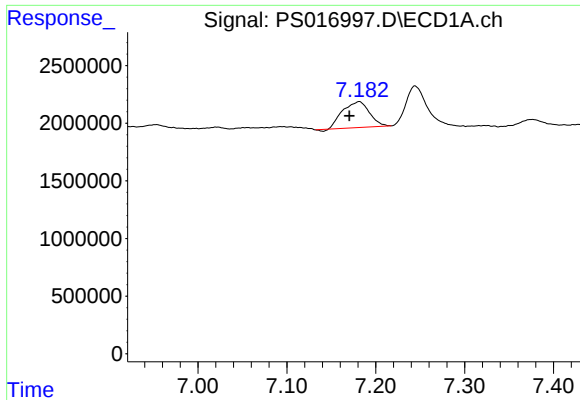

#4 2,4-DCAA


R.T.: 7.181 min
Delta R.T.: 0.011 min
Response: 4691715
Conc: 3.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

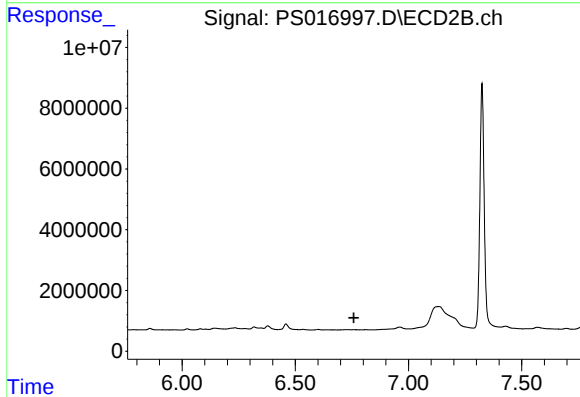


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

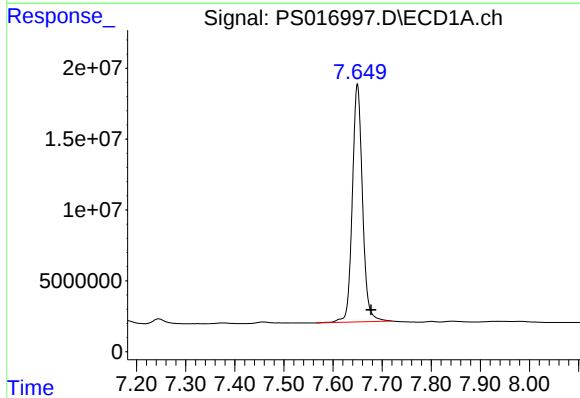


#7 MCPA

R.T.: 7.650 min
Delta R.T.: -0.028 min
Response: 241343330
Conc: 39.02 ug/ml

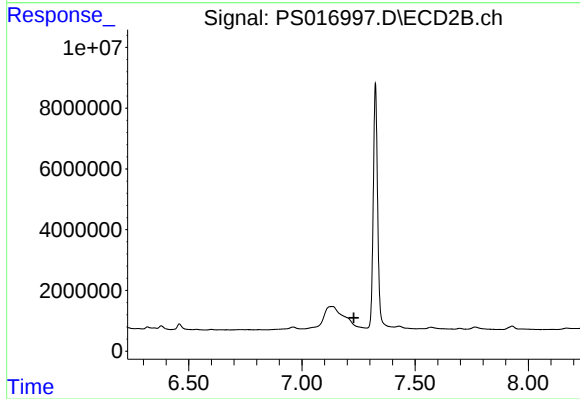

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.229 min
Response: 0
Conc: N.D.

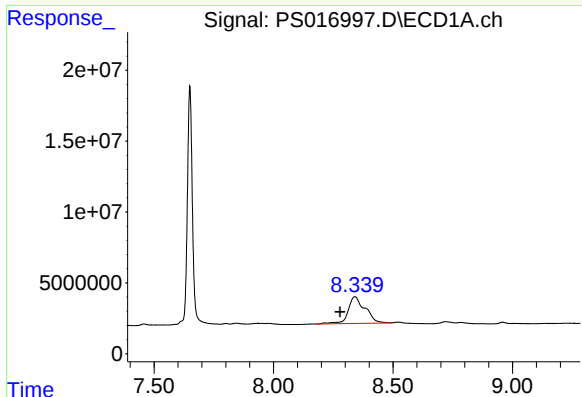

#9 2,4-D

R.T.: 8.340 min
Delta R.T.: 0.061 min
Response: 92447012
Conc: 52.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

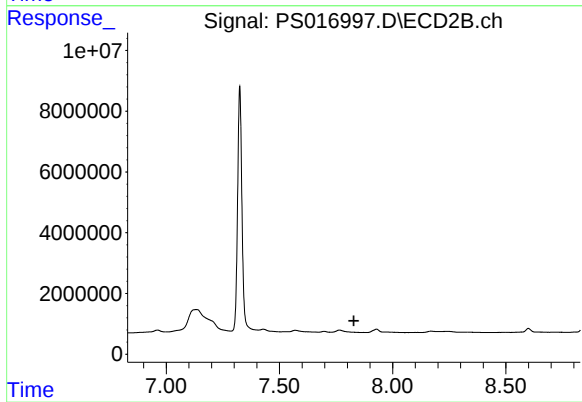

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.829 min
Response: 0
Conc: N.D.