

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100621\
 Data File : PS016999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2021 21:29
 Operator : DD\AJ
 Sample : M4047-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 02:01:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.177	0.000	33416007	0	21.933	N.D.	#
Target Compounds								
2) T	3,5-DICHL...	6.452f	0.000	6089738	0	2.862	N.D.	#
3) T	4-Nitroph...	0.000	6.375	0	8373241	N.D.	26.775	
6) T	MCP	7.588f	0.000	2849972	0	<MDL	N.D.	#
7) T	MCPA	7.650	0.000	265.3E6	0	42.892	N.D.	#
9) T	2,4-D	8.341f	7.851	82377651	14102542	46.852	18.536	#
11) T	2,4,5-TP ...	0.000	8.597	0	13932877	N.D.	3.980	
15) T	Picloram	10.958	0.000	4497090	0	<MDL	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100621\
Data File : PS016999.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2021 21:29
Operator : DD\AJ
Sample : M4047-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 02:01:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

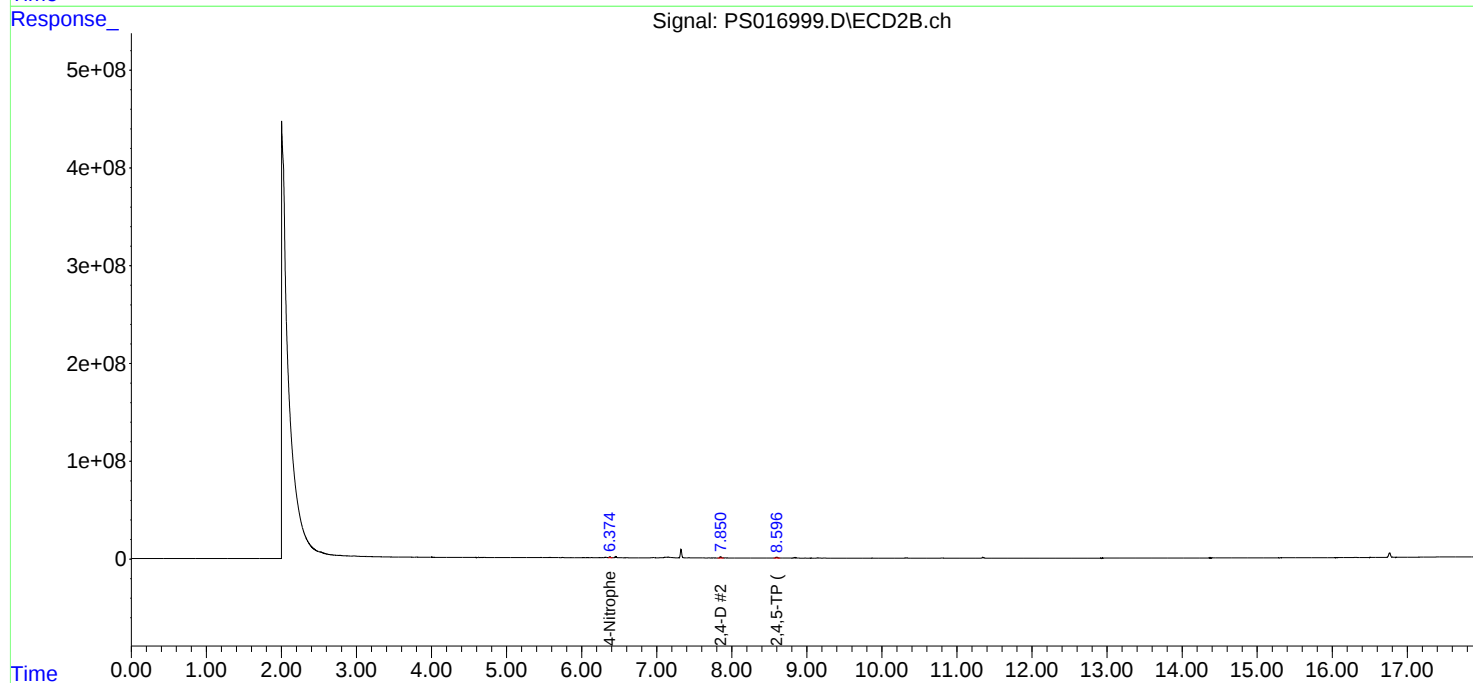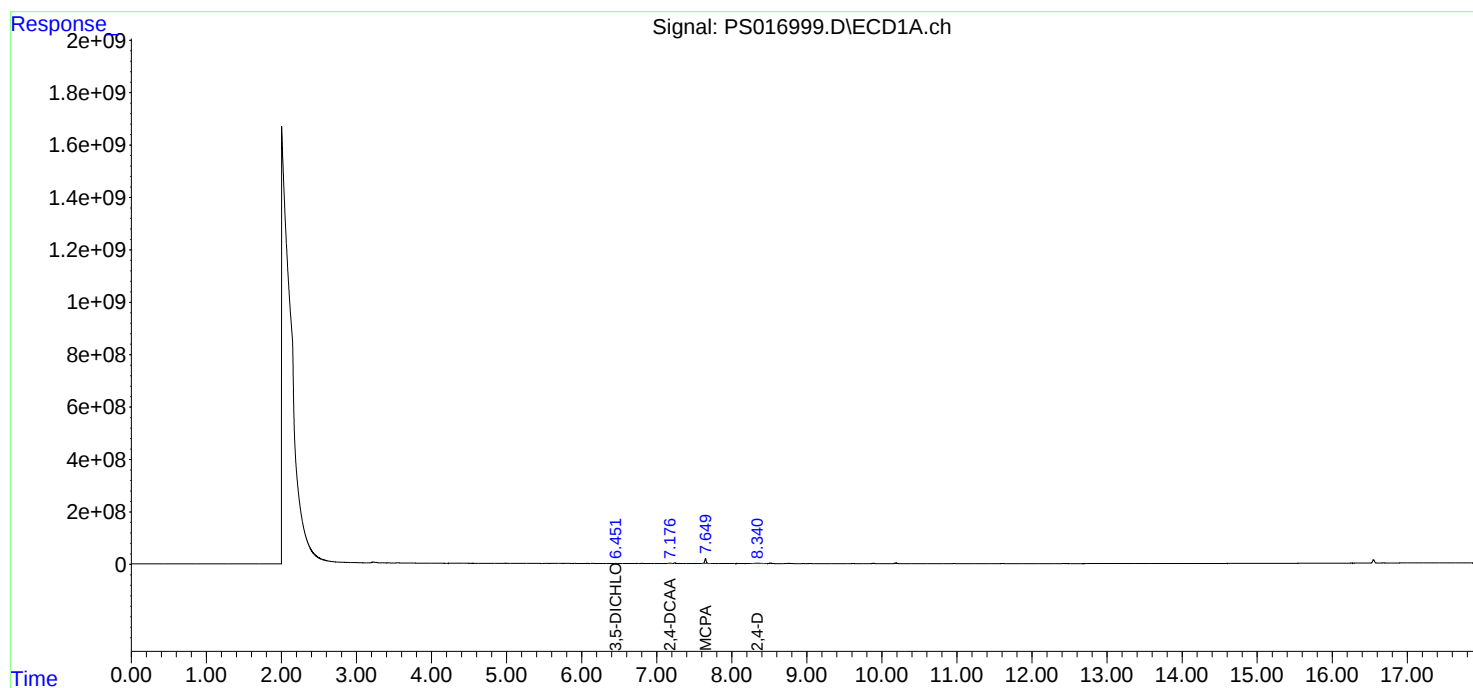


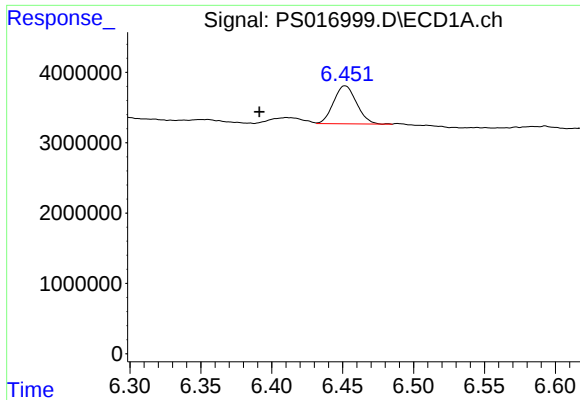

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.452 min
Delta R.T.: 0.061 min
Response: 6089738
Conc: 2.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

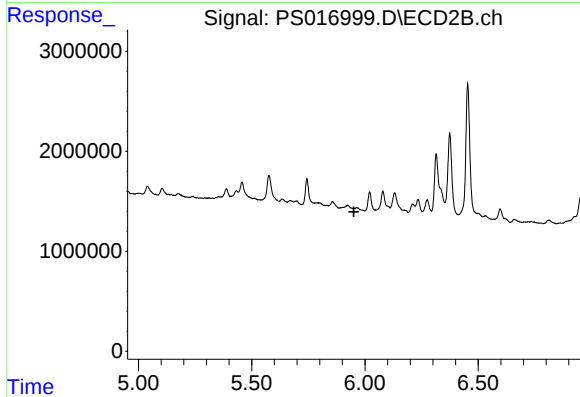


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.951 min
Response: 0
Conc: N.D.

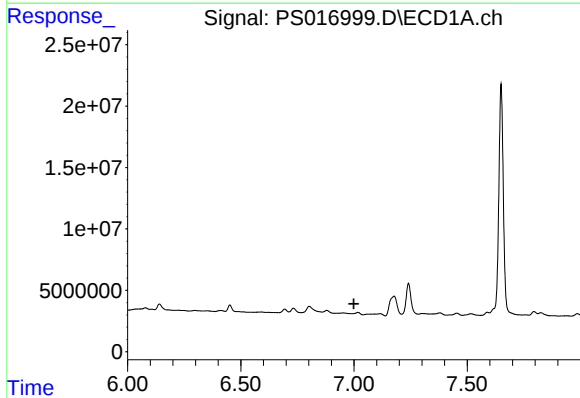


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.

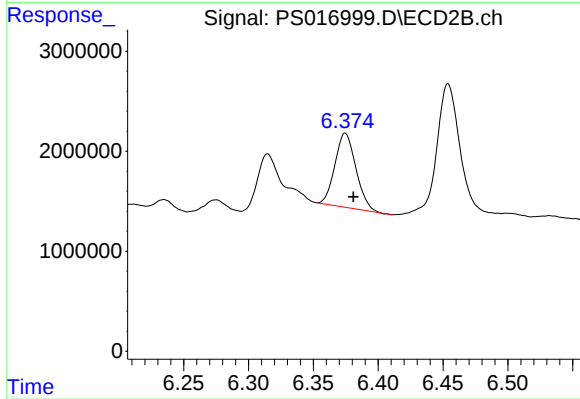

#3 4-Nitrophenol


R.T.: 6.375 min
Delta R.T.: -0.006 min
Response: 8373241
Conc: 26.78 ng/ml

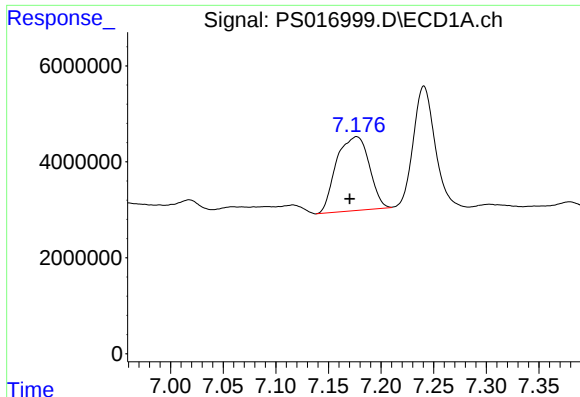

#4 2,4-DCAA


R.T.: 7.177 min
Delta R.T.: 0.006 min
Response: 33416007
Conc: 21.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

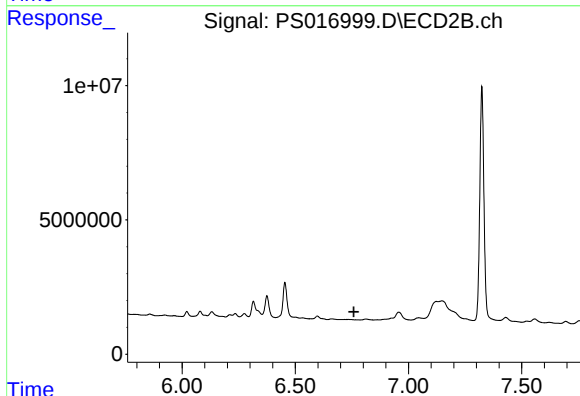


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

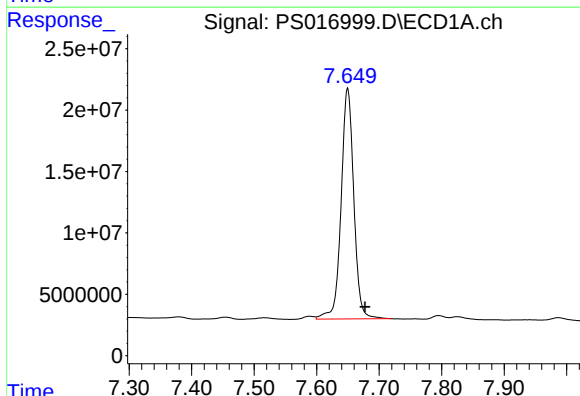


#7 MCPA

R.T.: 7.650 min
Delta R.T.: -0.028 min
Response: 265271459
Conc: 42.89 ug/ml

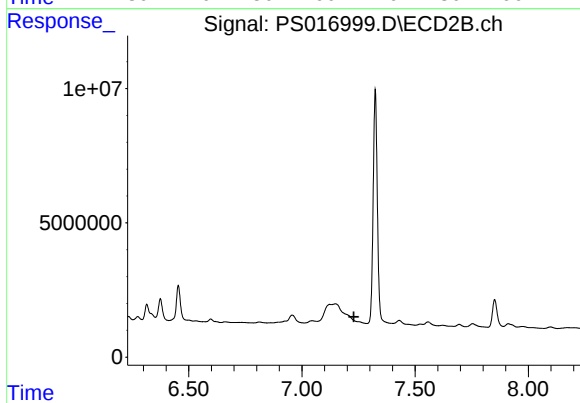

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.229 min
Response: 0
Conc: N.D.

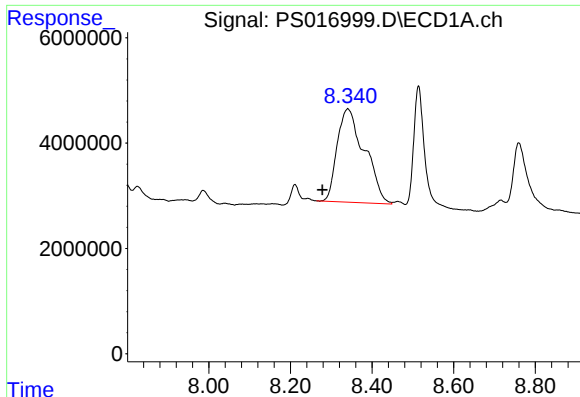

#9 2,4-D


R.T.: 8.341 min
Delta R.T.: 0.062 min
Response: 82377651
Conc: 46.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

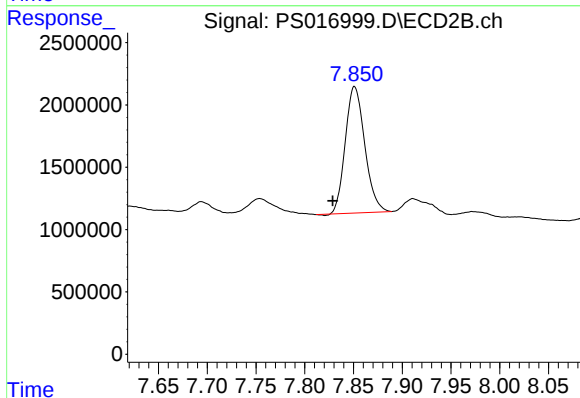


#9 2,4-D

R.T.: 7.851 min
Delta R.T.: 0.023 min
Response: 14102542
Conc: 18.54 ng/ml

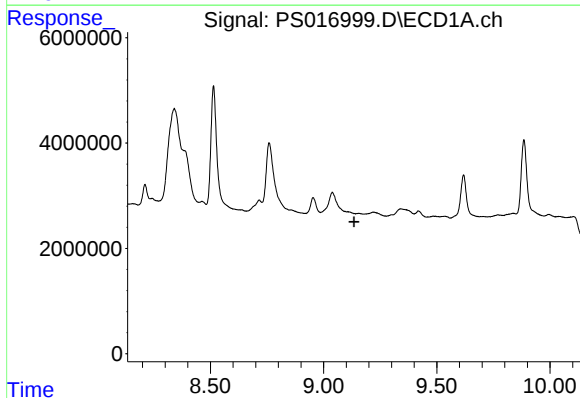

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.134 min
Response: 0
Conc: N.D.

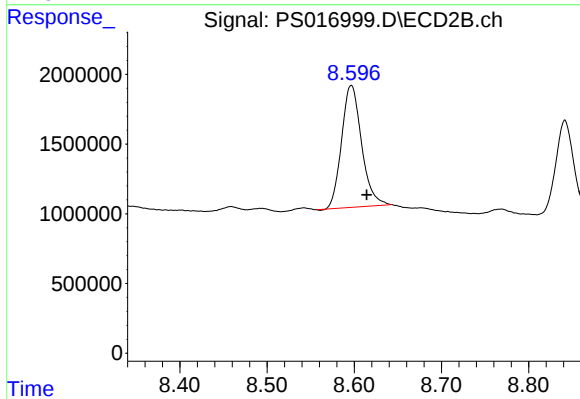

#11 2,4,5-TP (SILVEX)

R.T.: 8.597 min
Delta R.T.: -0.018 min
Response: 13932877
Conc: 3.98 ng/ml