

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100621\
 Data File : PS017003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2021 23:05
 Operator : DD\AJ
 Sample : M4057-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 02:02:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.162	0.000	10043627	0	6.592	N.D. #
Target Compounds							
7) T	MCPA	7.650	0.000	155.3E6	0	25.111	N.D. #
9) T	2,4-D	8.339f	7.853	54631864	23892451	31.072	31.403



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100621\
Data File : PS017003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2021 23:05
Operator : DD\AJ
Sample : M4057-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 02:02:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

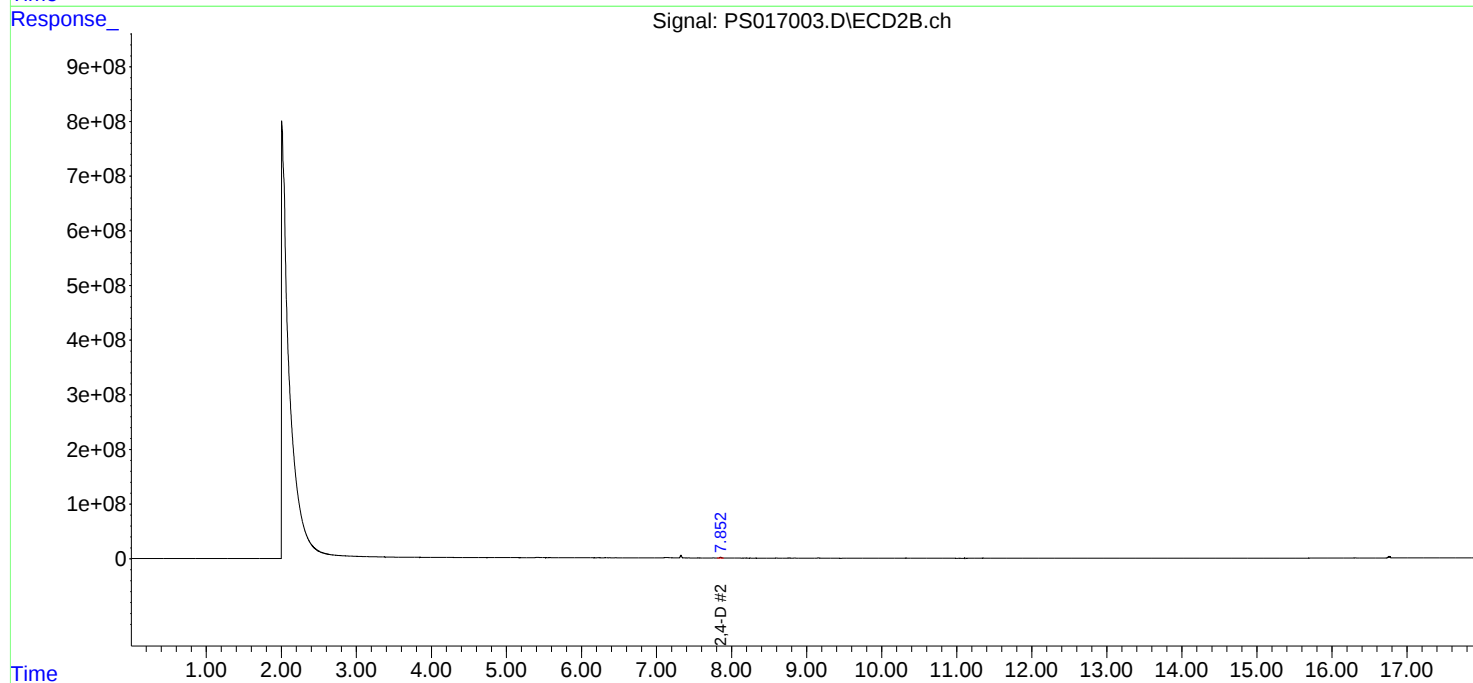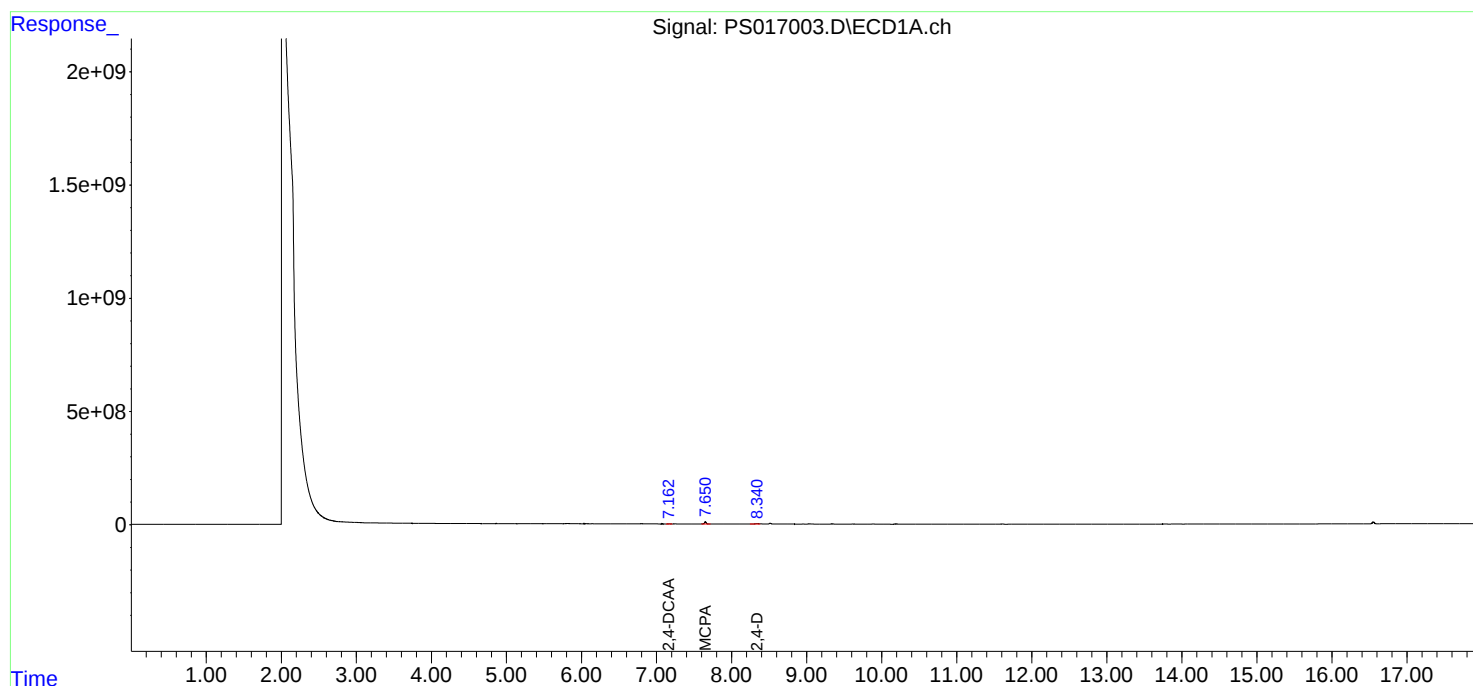


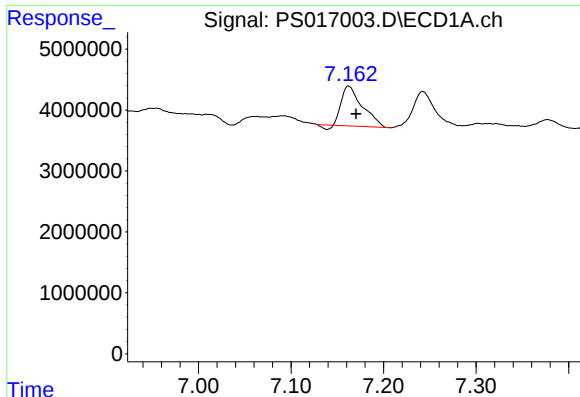

#4 2,4-DCAA


R.T.: 7.162 min
Delta R.T.: -0.008 min
Response: 10043627
Conc: 6.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

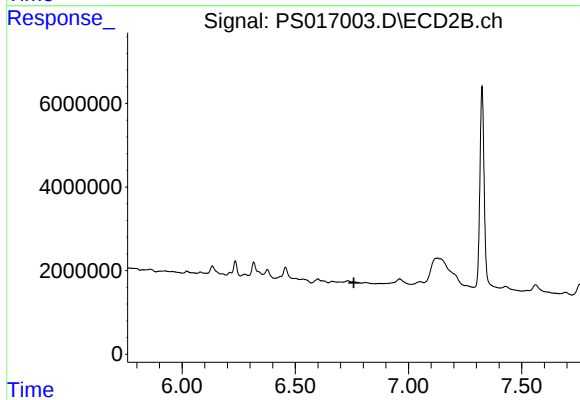


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

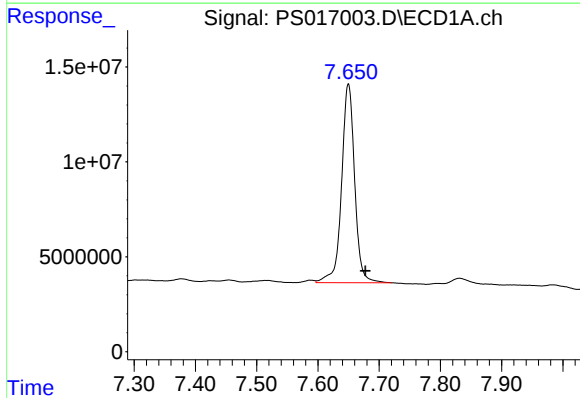


#7 MCPA

R.T.: 7.650 min
Delta R.T.: -0.028 min
Response: 155301761
Conc: 25.11 ug/ml

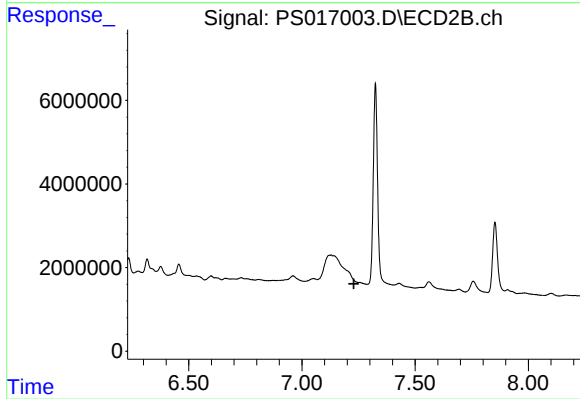

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.229 min
Response: 0
Conc: N.D.

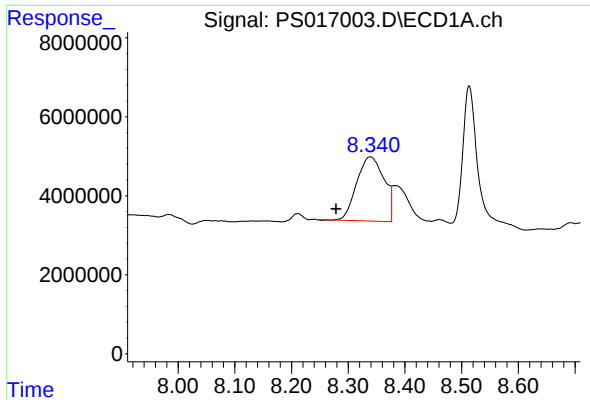

#9 2,4-D

R.T.: 8.339 min
Delta R.T.: 0.061 min
Response: 54631864
Conc: 31.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

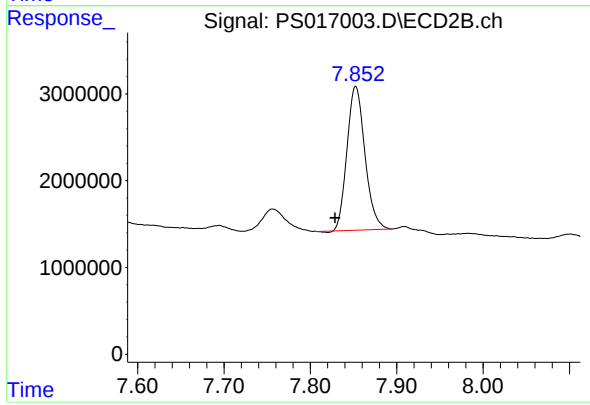

#9 2,4-D

R.T.: 7.853 min
Delta R.T.: 0.024 min
Response: 23892451
Conc: 31.40 ng/ml