

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS100621\  
 Data File : PS017005.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 06 Oct 2021 23:53  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 07 02:02:50 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS092021.M  
 Quant Title : 8080.M  
 QLast Update : Tue Sep 21 01:52:13 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1   | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|----------|--------|-------|----------|---------|---------|---------|
| -----                       |          |        |       |          |         |         |         |
| System Monitoring Compounds |          |        |       |          |         |         |         |
| 4) S                        | 2,4-DCAA | 7.161  | 6.748 | 640.3E6  | 278.3E6 | 420.300 | 474.663 |
| Target Compounds            |          |        |       |          |         |         |         |
| 7) T                        | MCPA     | 7.630f | 0.000 | 7826919  | 0       | 1.266   | N.D. #  |
| 9) T                        | 2,4-D    | 8.341f | 0.000 | 76507747 | 0       | 43.513  | N.D. #  |
| 15) T                       | Picloram | 10.907 | 0.000 | 3920831  | 0       | <MDL    | N.D. #  |
| -----                       |          |        |       |          |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS100621\  
Data File : PS017005.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 06 Oct 2021 23:53  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 07 02:02:50 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS092021.M  
Quant Title : 8080.M  
QLast Update : Tue Sep 21 01:52:13 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

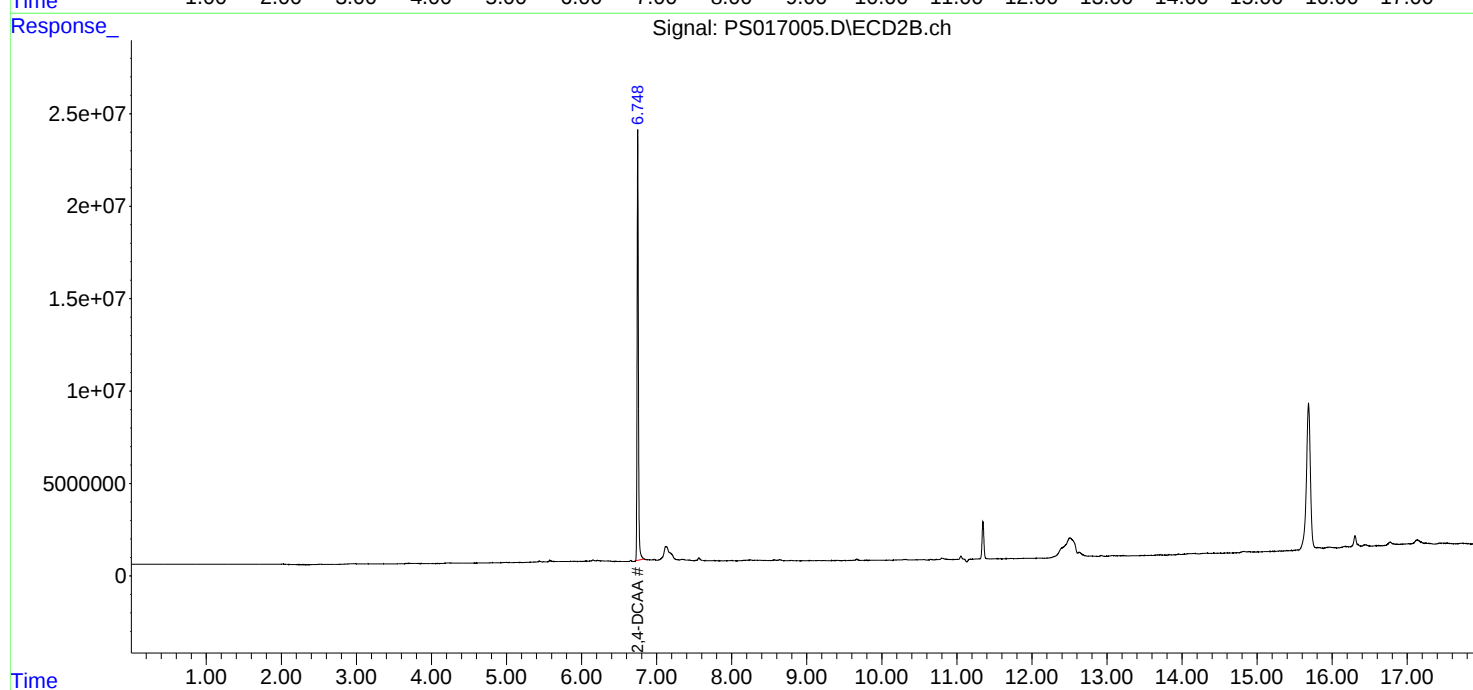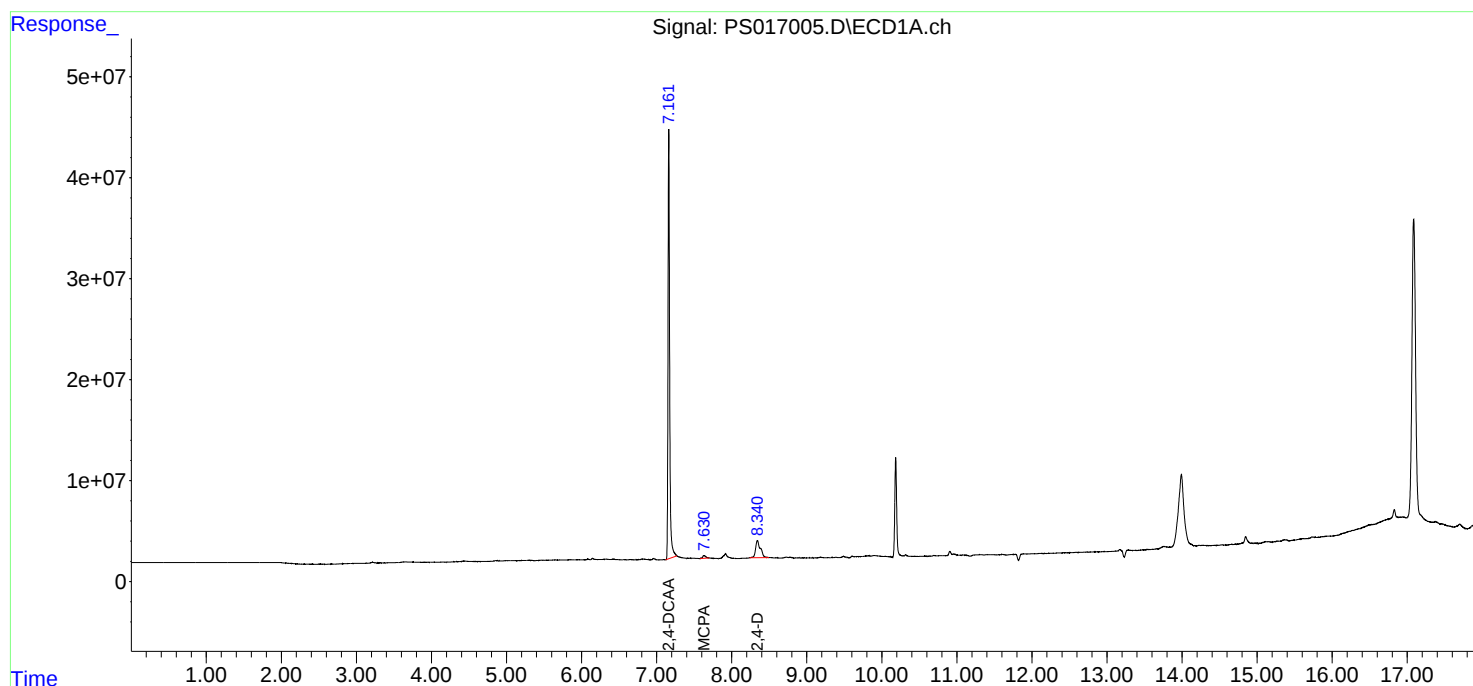


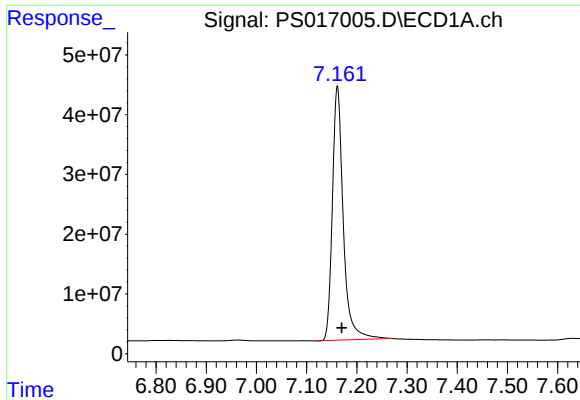

#4 2,4-DCAA


R.T.: 7.161 min  
Delta R.T.: -0.009 min  
Response: 640348313  
Conc: 420.30 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

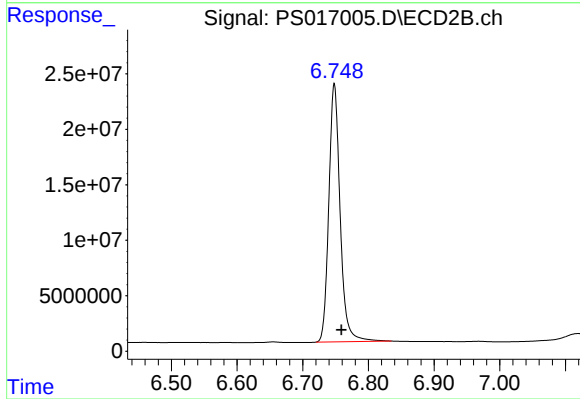


#4 2,4-DCAA

R.T.: 6.748 min  
Delta R.T.: -0.011 min  
Response: 278324829  
Conc: 474.66 ng/ml

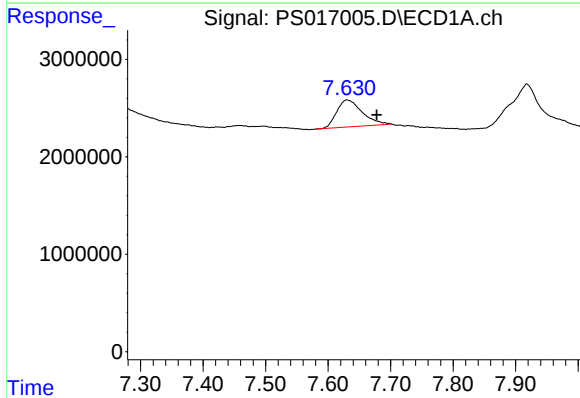


#7 MCPA

R.T.: 7.630 min  
Delta R.T.: -0.047 min  
Response: 7826919  
Conc: 1.27 ug/ml

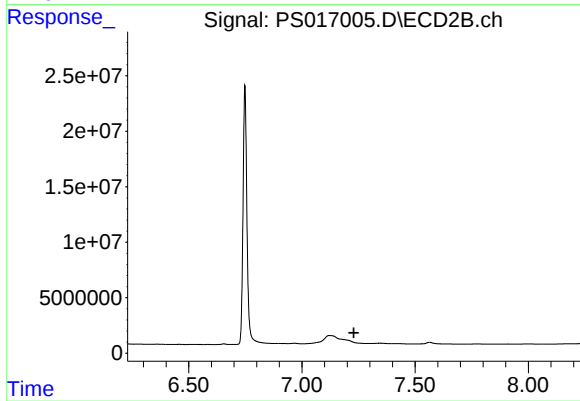

#7 MCPA


R.T.: 0.000 min  
Exp R.T.: 7.229 min  
Response: 0  
Conc: N.D.

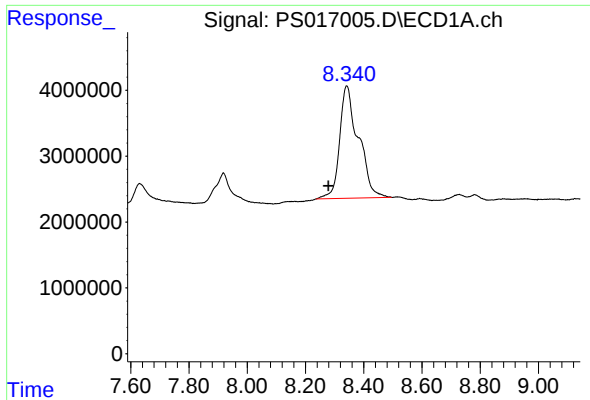

#9 2,4-D

R.T.: 8.341 min  
Delta R.T.: 0.063 min  
Response: 76507747  
Conc: 43.51 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

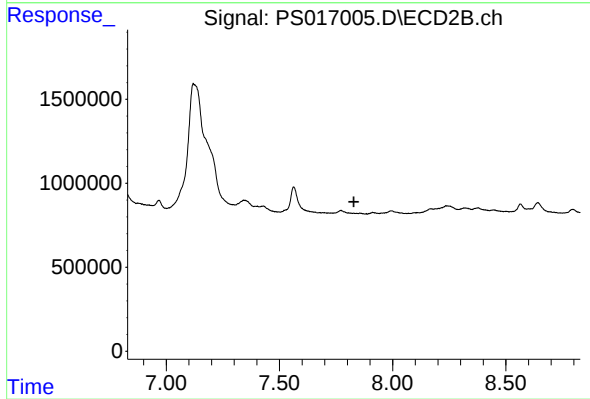

#9 2,4-D

R.T.: 0.000 min  
Exp R.T. : 7.829 min  
Response: 0  
Conc: N.D.