

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100622\
 Data File : PS020742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2022 21:18
 Operator : AR\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 06:00:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 05:57:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.422	6.868	1381.8E6	987.7E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.510	2.585	1884.5E6	1166.0E6	682.500	682.500
2) T	3,5-DICHL...	5.788	6.035	2042.5E6	1380.8E6	697.500	697.500
3) T	4-Nitroph...	6.256	6.473	903.3E6	555.1E6	682.500	682.500
5) T	DICAMBA	6.569	7.037	5535.2E6	4137.7E6	705.000	705.000
6) T	MCPD	6.730	7.137	414.0E6	308.3E6	70.500	70.500
7) T	MCPA	6.857	7.351	588.3E6	424.7E6	69.750	69.750
8) T	DICHLORPROP	7.171	7.665	1383.2E6	1008.6E6	705.000	705.000
9) T	2,4-D	7.370	7.956	1687.2E6	1237.6E6	705.000	705.000
10) T	Pentachlo...	7.607	8.393	19259.4E6	14199.6E6	712.500	712.500
11) T	2,4,5-TP ...	8.135	8.755	7910.7E6	5989.3E6	712.500	712.500
12) T	2,4,5-T	8.392	9.131	7807.5E6	5764.7E6	712.500	712.500
13) T	2,4-DB	8.903	9.641	1602.6E6	795.0E6	712.500	712.500
14) T	DINOSEB	9.968	9.973	5694.1E6	4255.4E6	705.000	705.000
15) T	Picloram	9.789	10.943	11760.6E6	8419.0E6	712.500	712.500
16) T	DCPA	10.234	10.907	9848.4E6	7320.1E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100622\
Data File : PS020742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2022 21:18
Operator : AR\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 06:00:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 05:57:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

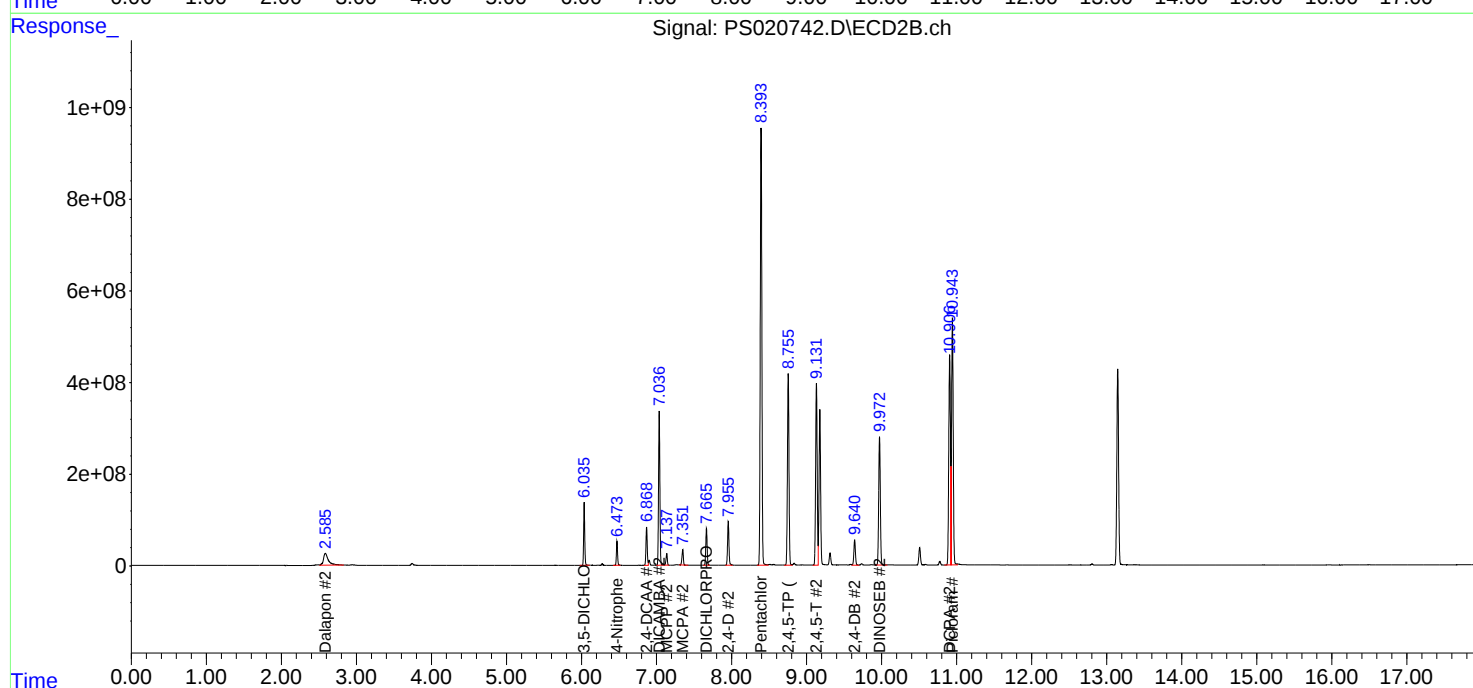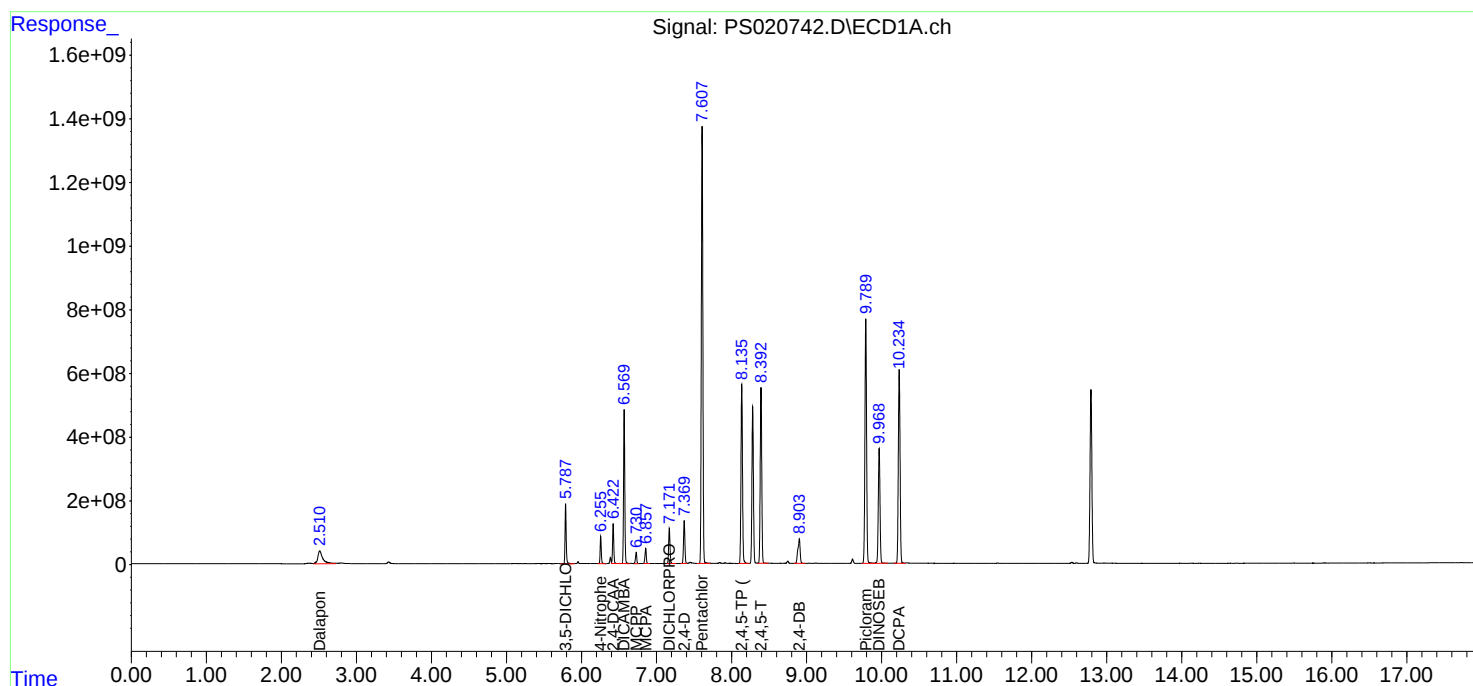


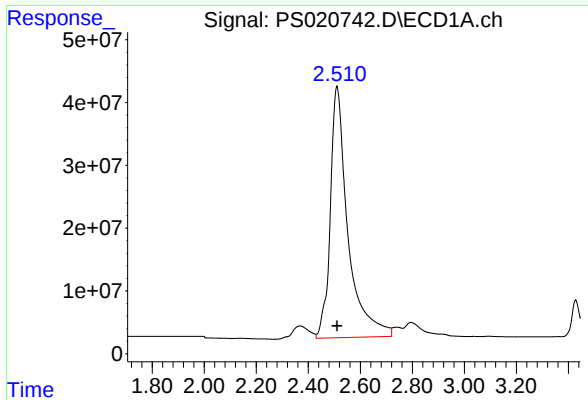

#1 Dalapon


R.T.: 2.510 min
Delta R.T.: 0.000 min
Response: 1884498673
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

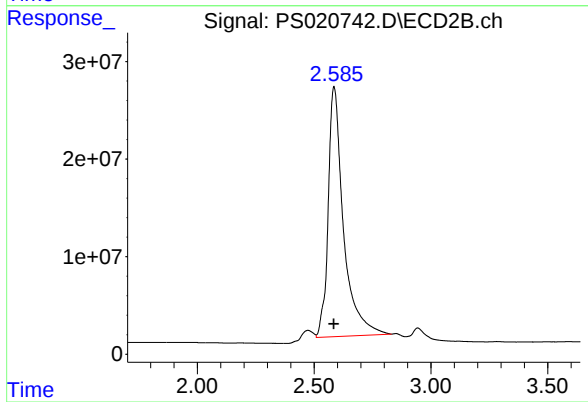


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: 0.000 min
Response: 1166023563
Conc: 682.50 ng/ml

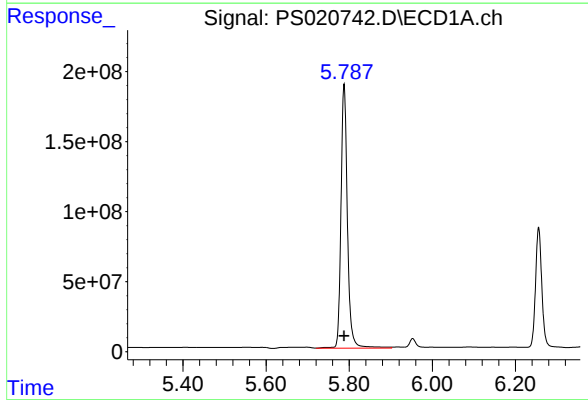


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.788 min
Delta R.T.: 0.000 min
Response: 2042495386
Conc: 697.50 ng/ml

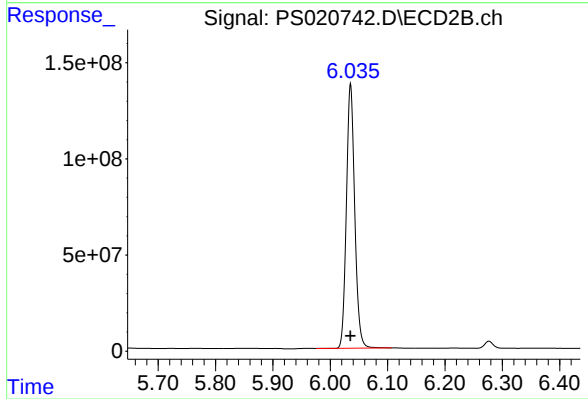

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 1380813858
Conc: 697.50 ng/ml

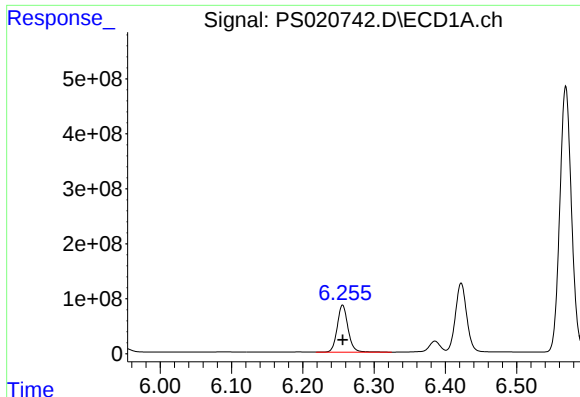

#3 4-Nitrophenol


R.T.: 6.256 min
Delta R.T.: 0.000 min
Response: 903291552
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

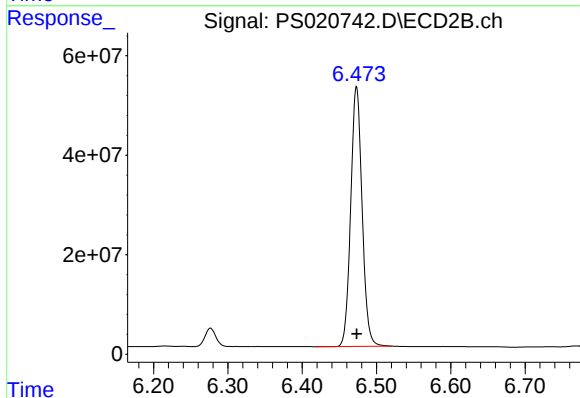


#3 4-Nitrophenol

R.T.: 6.473 min
Delta R.T.: 0.000 min
Response: 555056288
Conc: 682.50 ng/ml

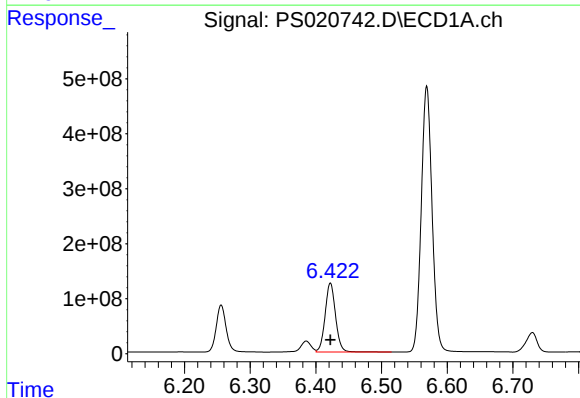


#4 2,4-DCAA

R.T.: 6.422 min
Delta R.T.: 0.000 min
Response: 1381759830
Conc: 750.00 ng/ml

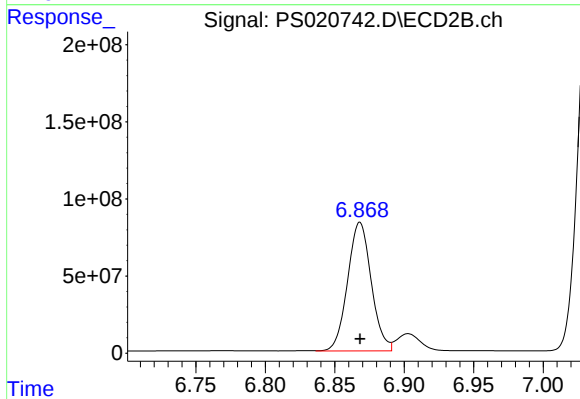

#4 2,4-DCAA


R.T.: 6.868 min
Delta R.T.: 0.000 min
Response: 987679580
Conc: 750.00 ng/ml

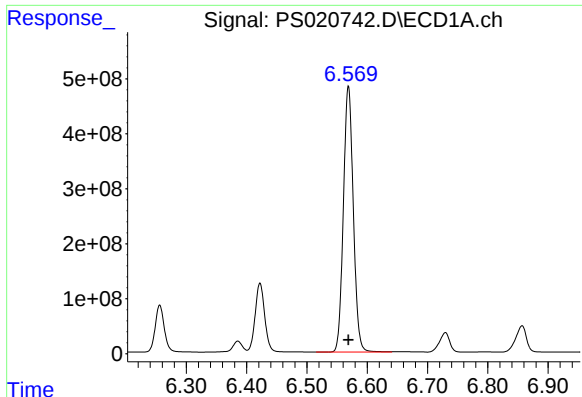

#5 DICAMBA


R.T.: 6.569 min
Delta R.T.: 0.000 min
Response: 5535207055
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

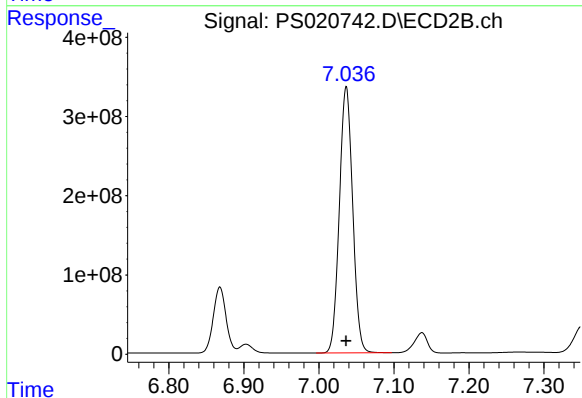


#5 DICAMBA

R.T.: 7.037 min
Delta R.T.: 0.000 min
Response: 4137707334
Conc: 705.00 ng/ml

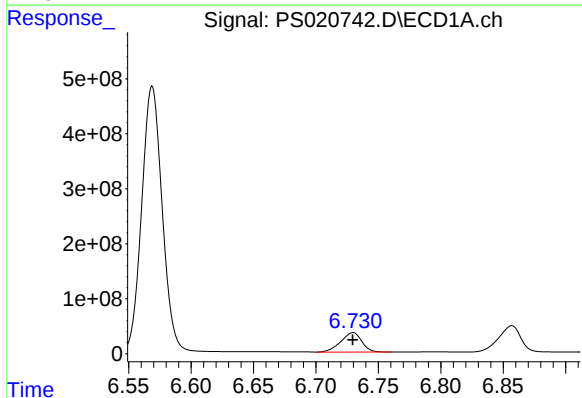


#6 MCP

R.T.: 6.730 min
Delta R.T.: 0.000 min
Response: 414015887
Conc: 70.50 ug/ml

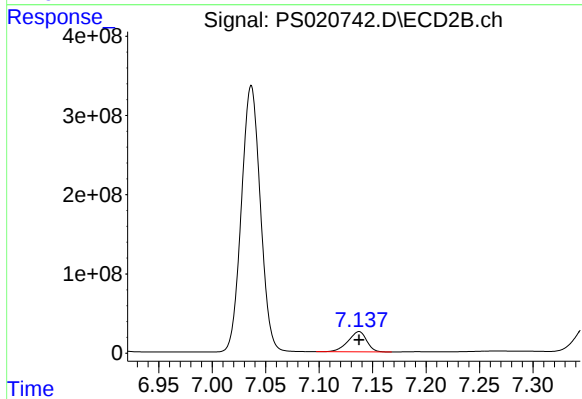

#6 MCP


R.T.: 7.137 min
Delta R.T.: 0.000 min
Response: 308337297
Conc: 70.50 ug/ml

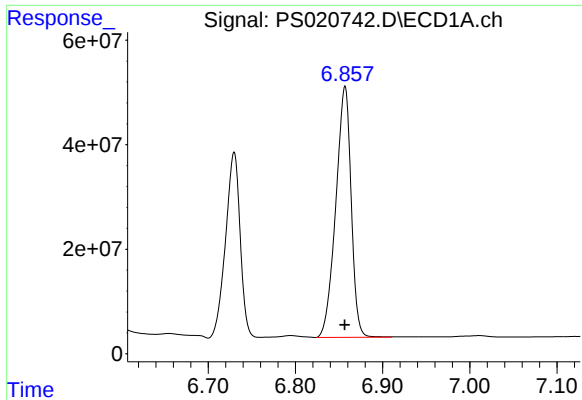

#7 MCPA


R.T.: 6.857 min
Delta R.T.: 0.000 min
Response: 588346920
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

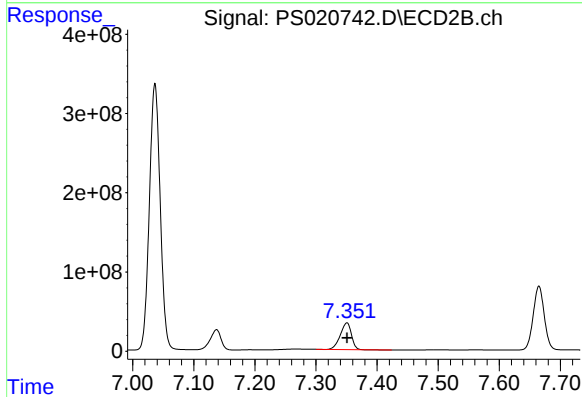


#7 MCPA

R.T.: 7.351 min
Delta R.T.: 0.000 min
Response: 424711491
Conc: 69.75 ug/ml

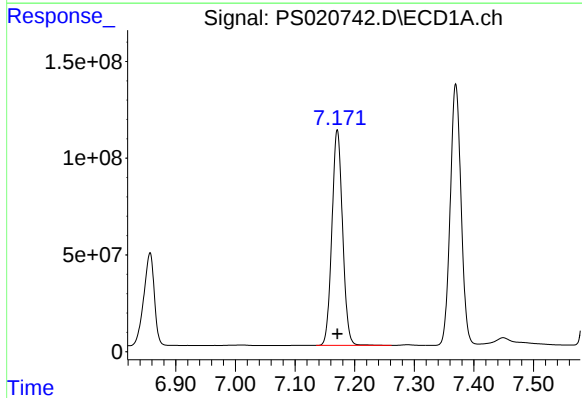


#8 DICHLORPROP

R.T.: 7.171 min
Delta R.T.: 0.000 min
Response: 1383174810
Conc: 705.00 ng/ml

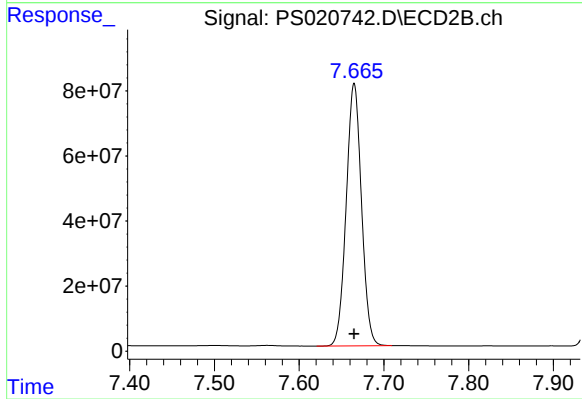

#8 DICHLORPROP


R.T.: 7.665 min
Delta R.T.: 0.000 min
Response: 1008634376
Conc: 705.00 ng/ml

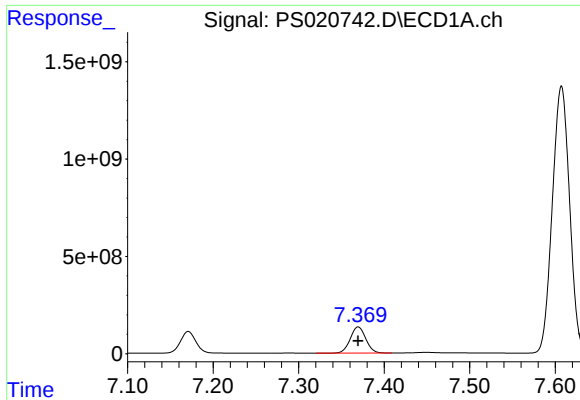

#9 2,4-D


R.T.: 7.370 min
Delta R.T.: 0.000 min
Response: 1687179388
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

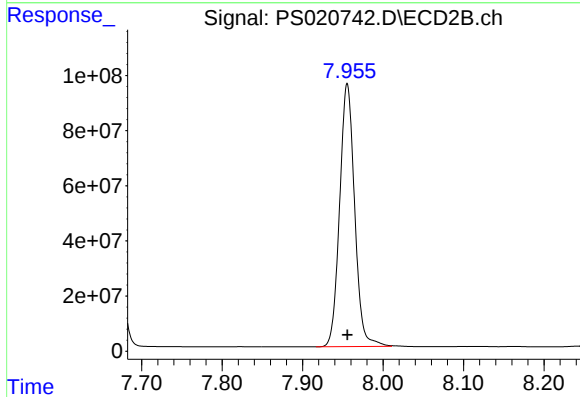


#9 2,4-D

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 1237559688
Conc: 705.00 ng/ml

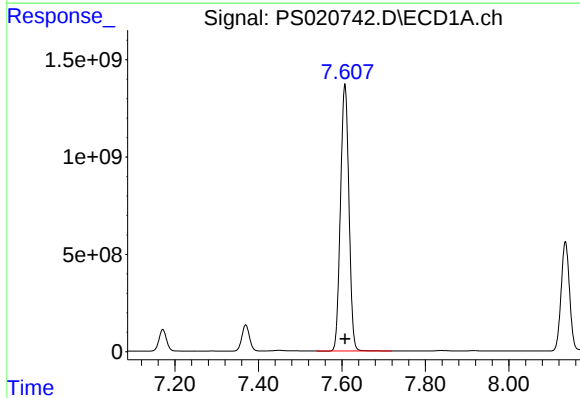


#10 Pentachlorophenol

R.T.: 7.607 min
Delta R.T.: 0.000 min
Response: 19259399050
Conc: 712.50 ng/ml

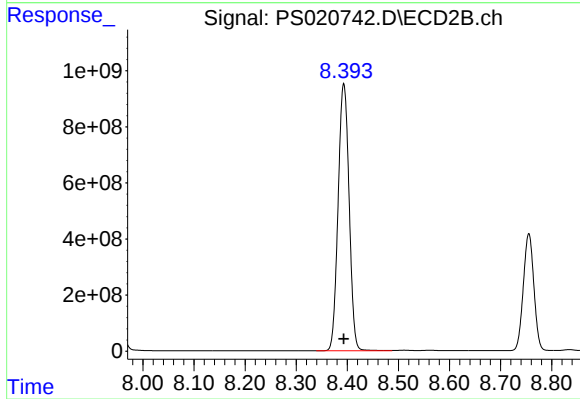

#10 Pentachlorophenol


R.T.: 8.393 min
Delta R.T.: 0.000 min
Response: 14199632673
Conc: 712.50 ng/ml

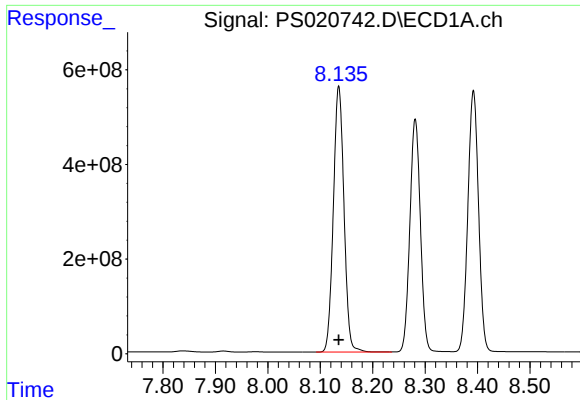

#11 2,4,5-TP (SILVEX)


R.T.: 8.135 min
Delta R.T.: 0.000 min
Response: 7910713582
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

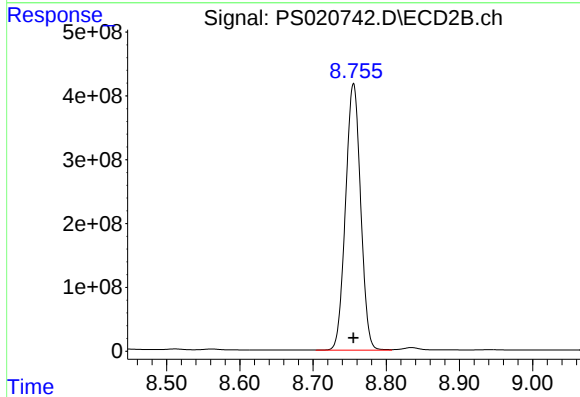


#11 2,4,5-TP (SILVEX)

R.T.: 8.755 min
Delta R.T.: 0.000 min
Response: 5989288979
Conc: 712.50 ng/ml

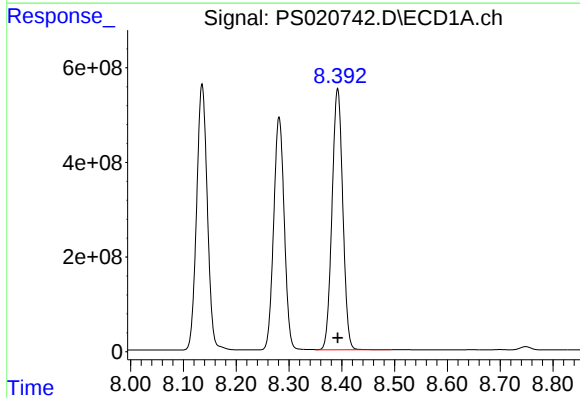


#12 2,4,5-T

R.T.: 8.392 min
Delta R.T.: 0.000 min
Response: 7807452829
Conc: 712.50 ng/ml

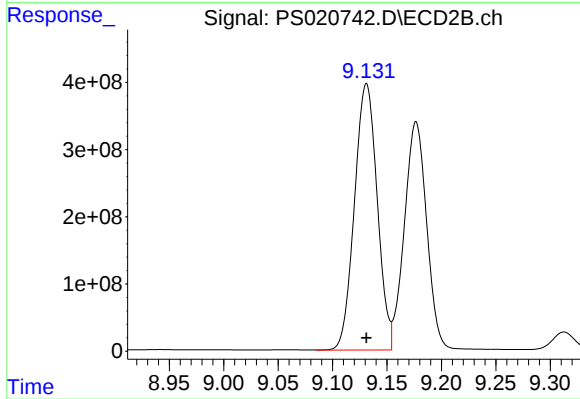

#12 2,4,5-T


R.T.: 9.131 min
Delta R.T.: 0.000 min
Response: 5764679873
Conc: 712.50 ng/ml

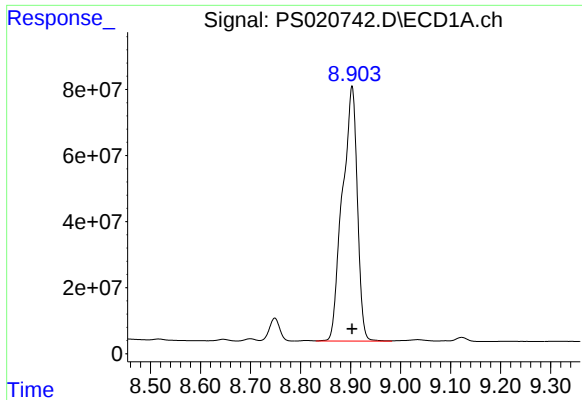

#13 2,4-DB


R.T.: 8.903 min
Delta R.T.: 0.000 min
Response: 1602584171
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

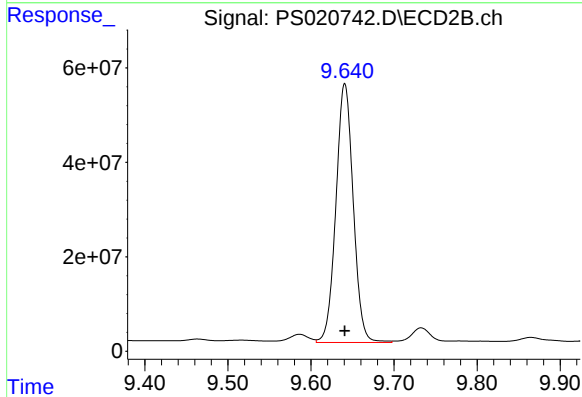


#13 2,4-DB

R.T.: 9.641 min
Delta R.T.: 0.000 min
Response: 794974279
Conc: 712.50 ng/ml

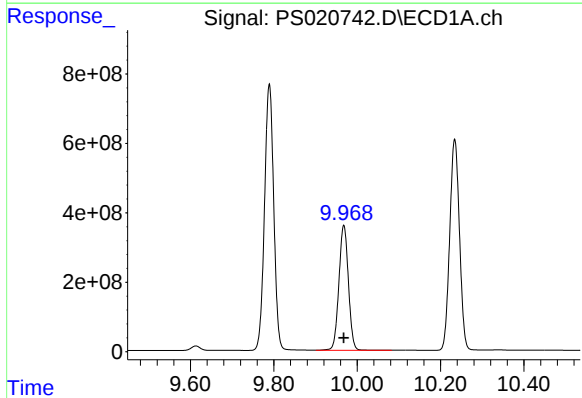


#14 DINOSEB

R.T.: 9.968 min
Delta R.T.: 0.000 min
Response: 5694101085
Conc: 705.00 ng/ml

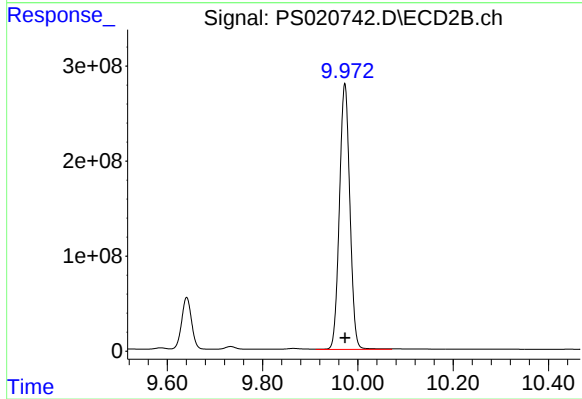

#14 DINOSEB


R.T.: 9.973 min
Delta R.T.: 0.000 min
Response: 4255362531
Conc: 705.00 ng/ml

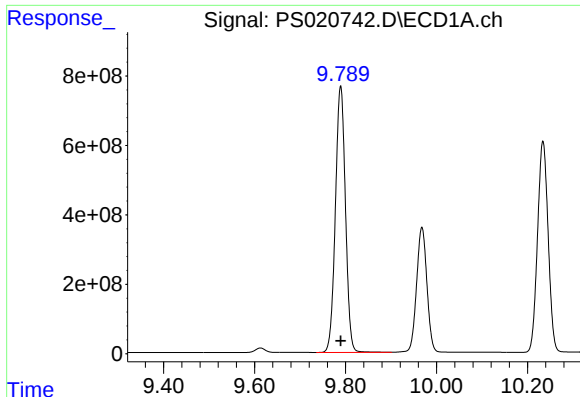

#15 Picloram


R.T.: 9.789 min
Delta R.T.: 0.000 min
Response: 11760573057
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

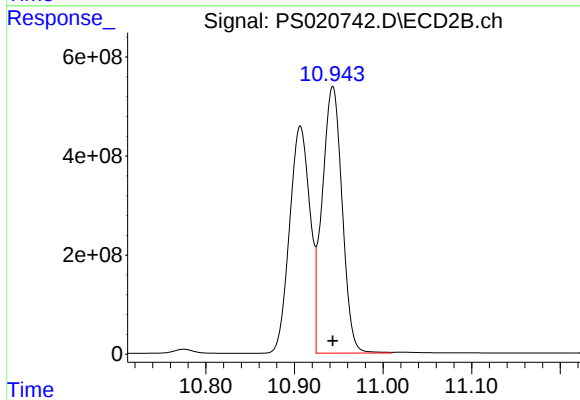


#15 Picloram

R.T.: 10.943 min
Delta R.T.: 0.000 min
Response: 8419026048
Conc: 712.50 ng/ml

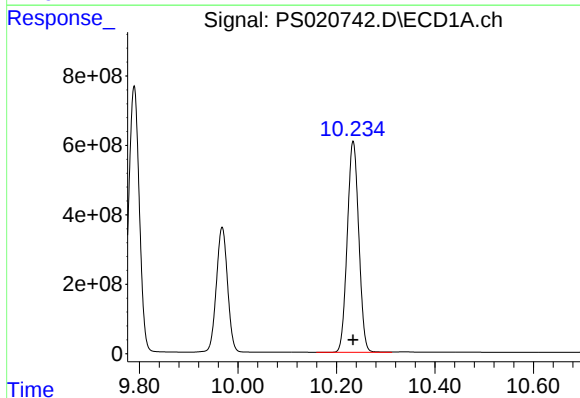

#16 DCPA

R.T.: 10.234 min
Delta R.T.: 0.000 min
Response: 9848387183
Conc: 720.00 ng/ml

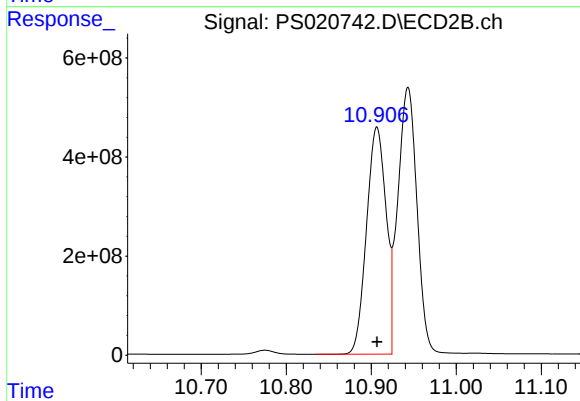

#16 DCPA

R.T.: 10.907 min
Delta R.T.: 0.000 min
Response: 7320104703
Conc: 720.00 ng/ml