

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100625\
 Data File : PS031956.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2025 16:36
 Operator : AR\AJ
 Sample : PB169991BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB169991BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 03:00:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.284	7.739	1598.7E6	441.4E6	443.896	485.655
Target Compounds							
1) T	Dalapon	0.000	2.649f	0	1512.8E6	N.D.	536.904
2) T	3,5-DICHL...	6.450	0.000	6485115	0	1.216	N.D. #
6) T	MCP	7.637	0.000	7158624	0	<MDL	N.D. #
8) T	DICHLORPROP	8.186	8.668	12394547	4293852	3.480	2.951
10) T	Pentachlo...	8.707	9.498	10878839	38997296	<MDL	<MDL #
11) T	2,4,5-TP ...	9.258f	9.880	349138	275.9E6	<MDL	18.327 #
12) T	2,4,5-T	9.609f	10.345f	188.5E6	117.6E6	10.299	8.739
13) T	2,4-DB	10.189f	10.922f	310.0E6	11657627	132.909	10.895 #
14) T	DINOSEB	11.330	11.288	103.7E6	49029554	7.188	5.044 #
15) T	Picloram	11.175	0.000	18736836	0	1.040	N.D. #
16) T	DCPA	11.626f	12.324	40355567	24454252	1.497	1.015 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100625\
Data File : PS031956.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2025 16:36
Operator : AR\AJ
Sample : PB169991BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB169991BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 03:00:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

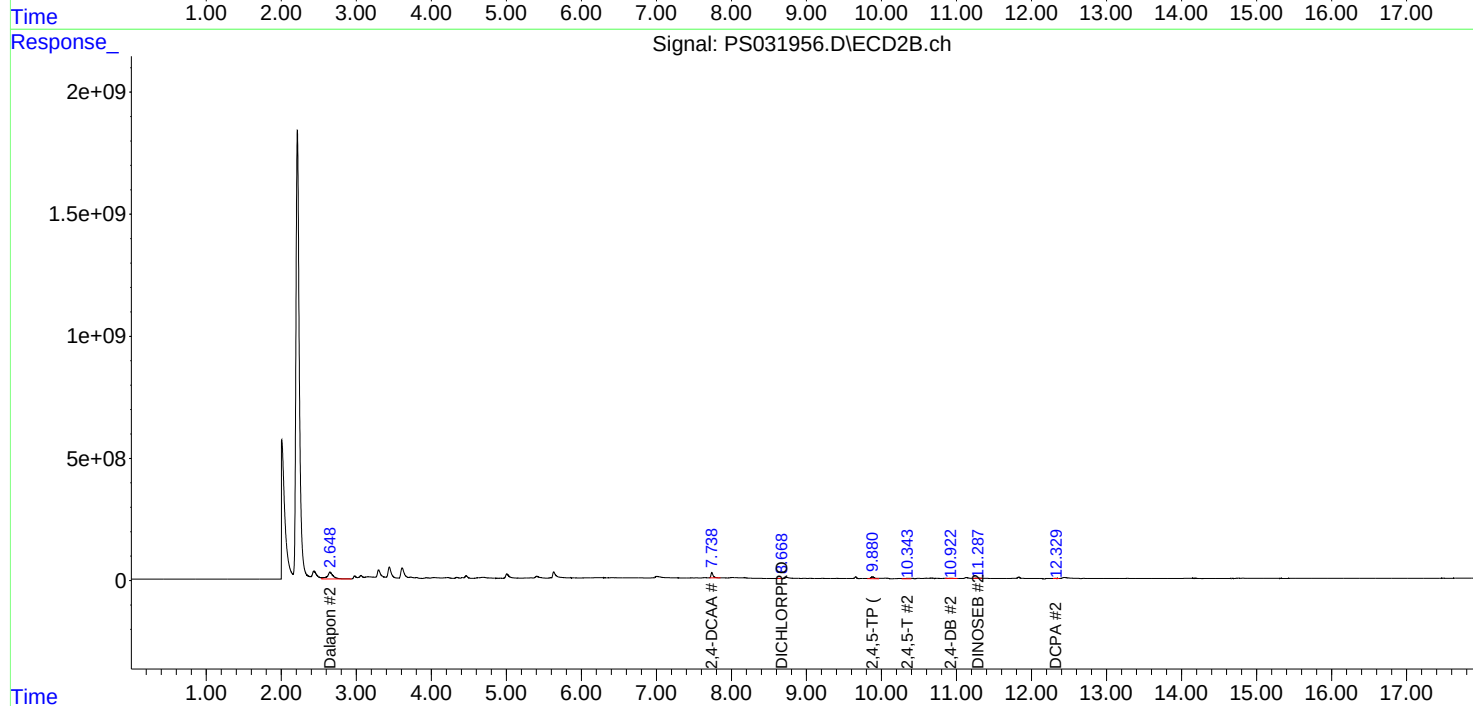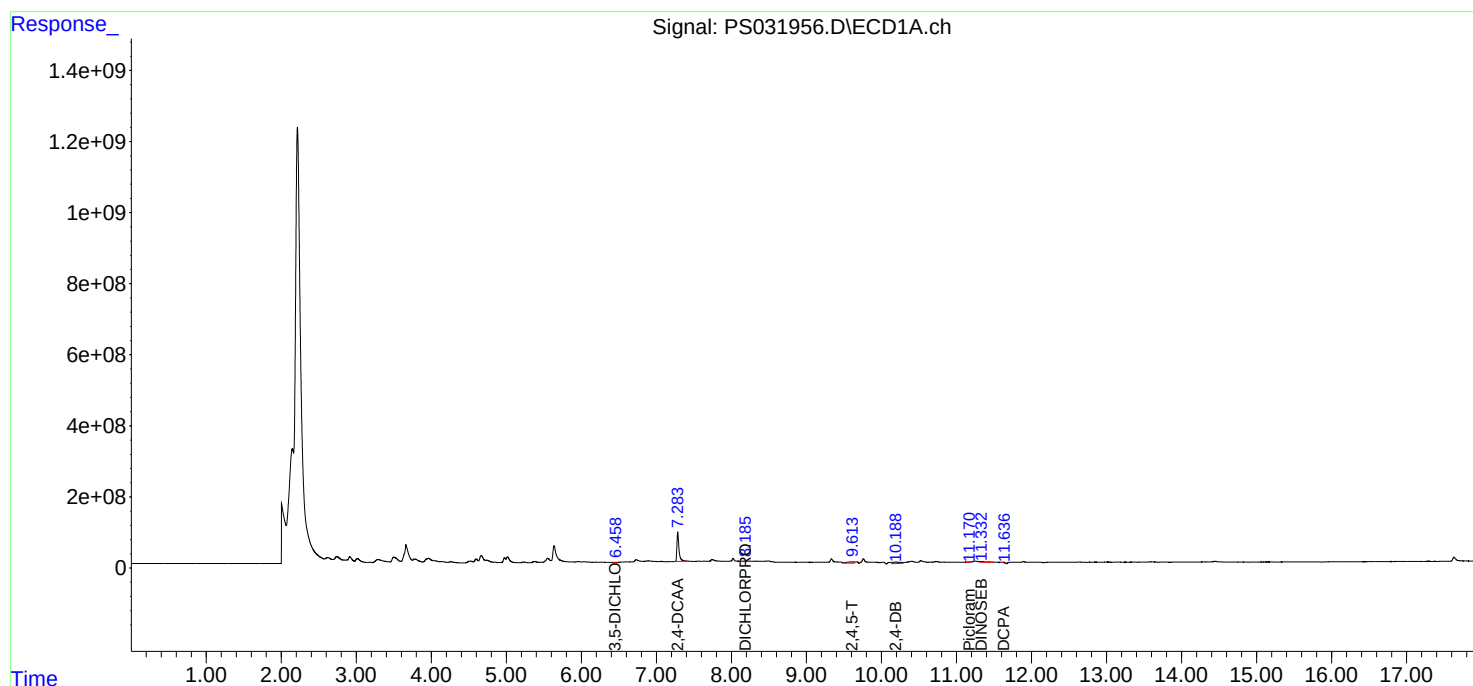


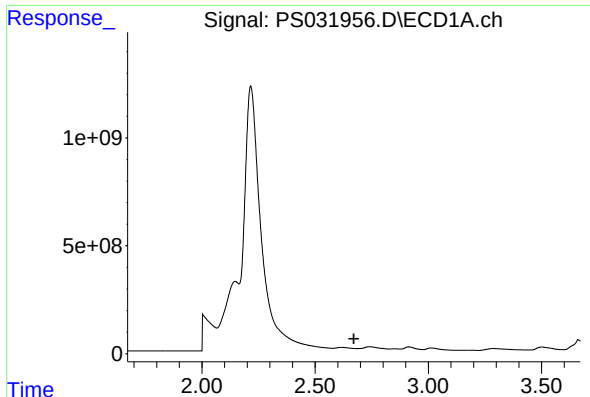

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB169991BL

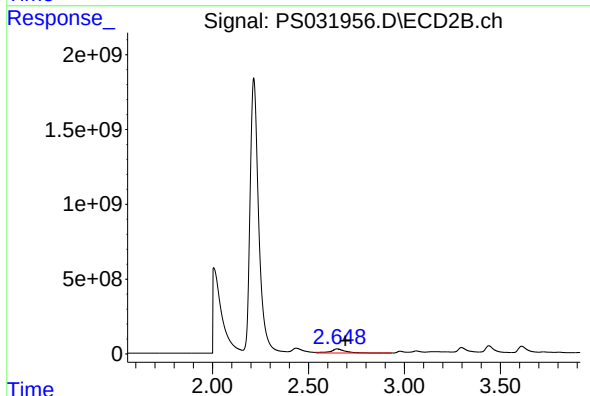


#1 Dalapon

R.T.: 2.649 min
Delta R.T.: -0.043 min
Response: 1512795531
Conc: 536.90 ng/ml

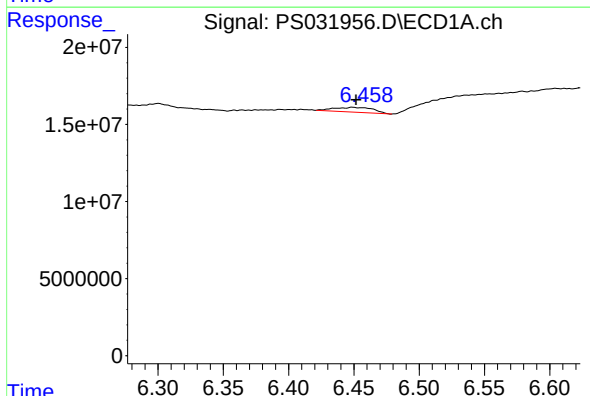


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.450 min
Delta R.T.: -0.002 min
Response: 6485115
Conc: 1.22 ng/ml

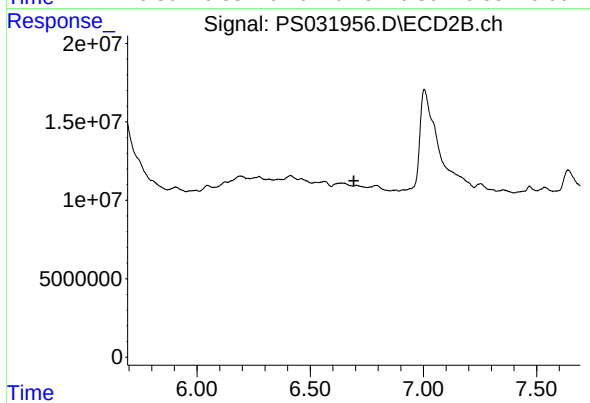

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

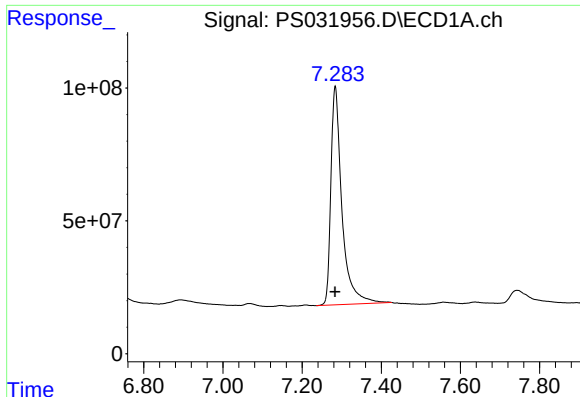

#4 2,4-DCAA


R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 1598703580
Conc: 443.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB169991BL

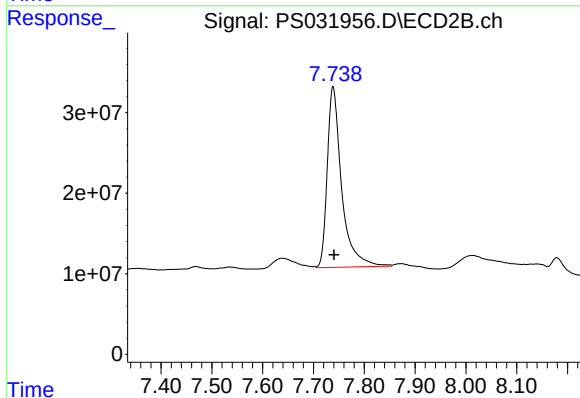


#4 2,4-DCAA

R.T.: 7.739 min
Delta R.T.: -0.002 min
Response: 441411396
Conc: 485.65 ng/ml

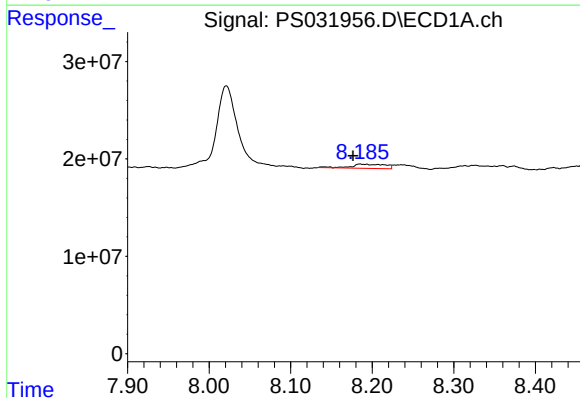


#8 DICHLORPROP

R.T.: 8.186 min
Delta R.T.: 0.010 min
Response: 12394547
Conc: 3.48 ng/ml

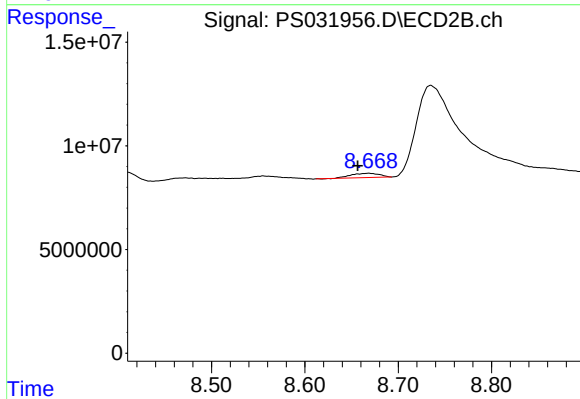

#8 DICHLORPROP


R.T.: 8.668 min
Delta R.T.: 0.012 min
Response: 4293852
Conc: 2.95 ng/ml

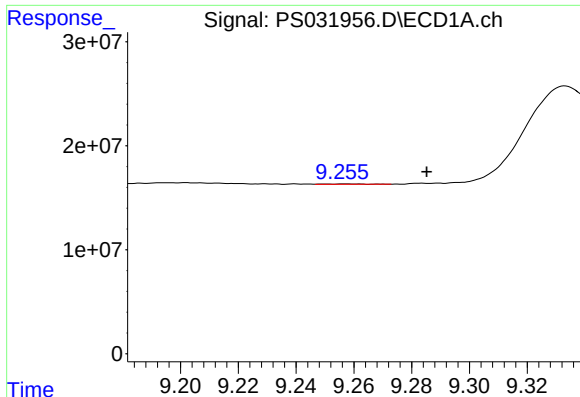

#11 2,4,5-TP (SILVEX)


R.T.: 9.258 min
Delta R.T.: -0.028 min
Response: 349138
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB169991BL

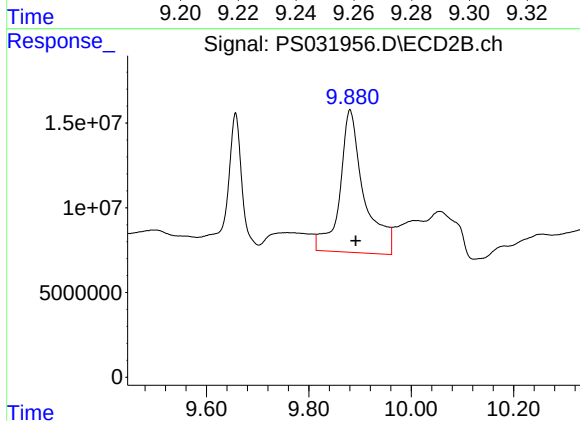


#11 2,4,5-TP (SILVEX)

R.T.: 9.880 min
Delta R.T.: -0.011 min
Response: 275901940
Conc: 18.33 ng/ml

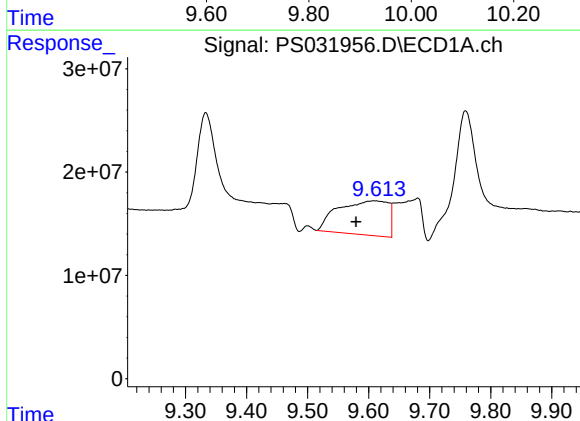


#12 2,4,5-T

R.T.: 9.609 min
Delta R.T.: 0.030 min
Response: 188451641
Conc: 10.30 ng/ml

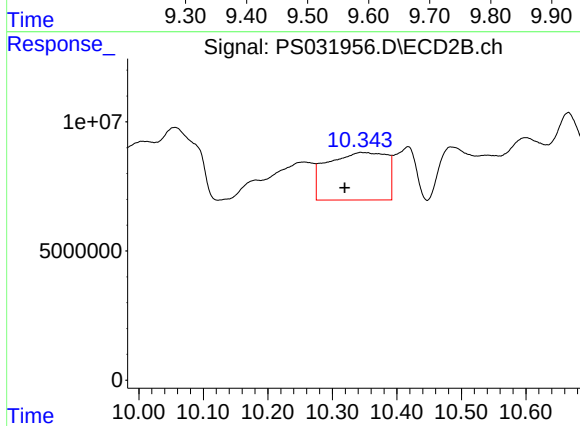

#12 2,4,5-T


R.T.: 10.345 min
Delta R.T.: 0.026 min
Response: 117597638
Conc: 8.74 ng/ml

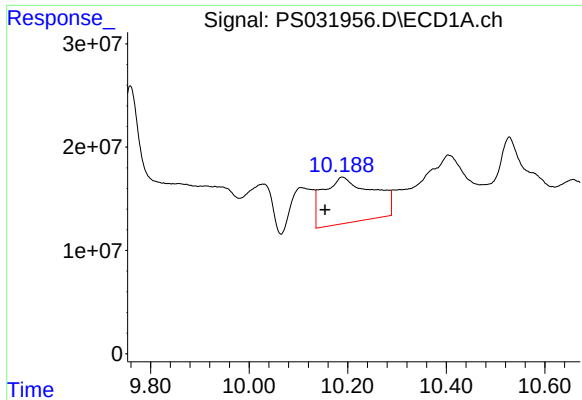

#13 2,4-DB


R.T.: 10.189 min
Delta R.T.: 0.035 min
Response: 310046521
Conc: 132.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB169991BL

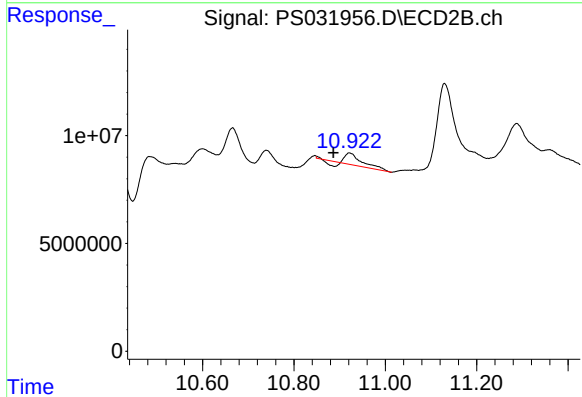


#13 2,4-DB

R.T.: 10.922 min
Delta R.T.: 0.035 min
Response: 11657627
Conc: 10.89 ng/ml

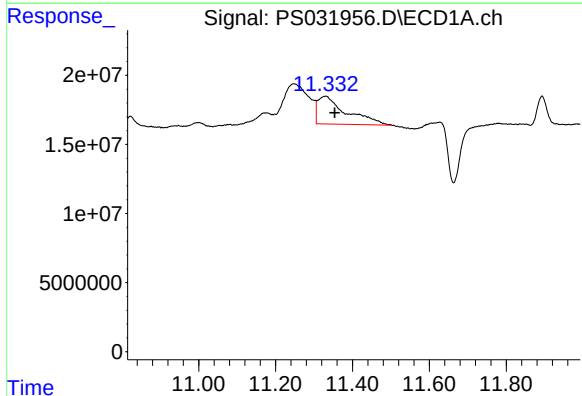


#14 DINOSEB

R.T.: 11.330 min
Delta R.T.: -0.024 min
Response: 103667051
Conc: 7.19 ng/ml

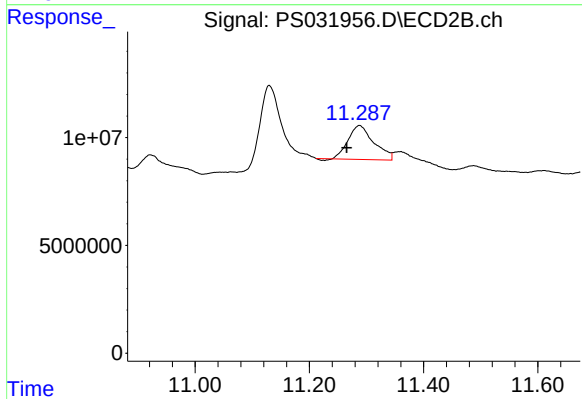

#14 DINOSEB


R.T.: 11.288 min
Delta R.T.: 0.022 min
Response: 49029554
Conc: 5.04 ng/ml

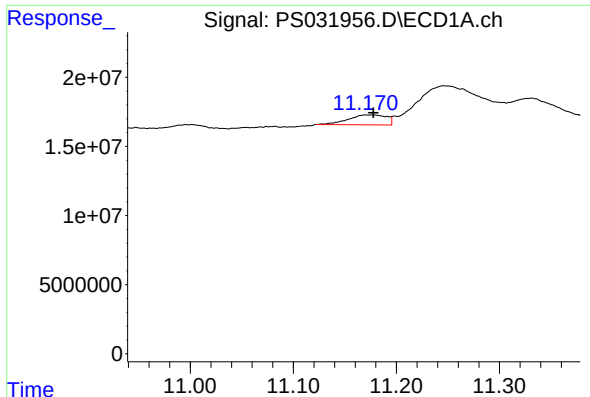

#15 Picloram


R.T.: 11.175 min
Delta R.T.: -0.003 min
Response: 18736836
Conc: 1.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB169991BL

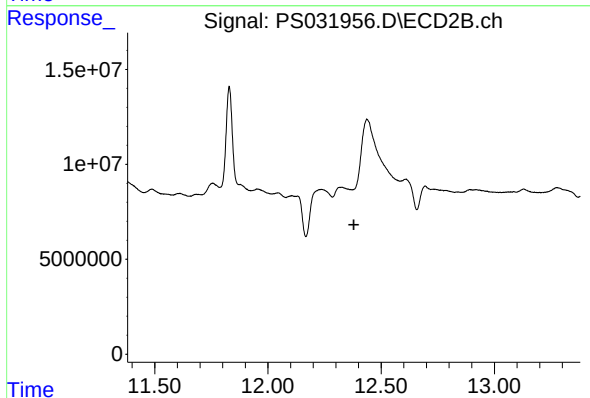


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 12.380 min
Response: 0
Conc: N.D.

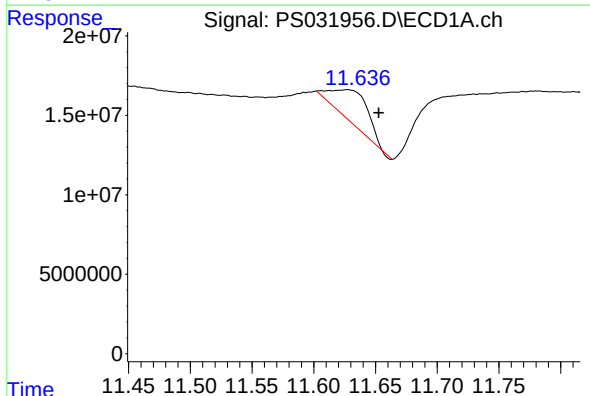

#16 DCPA

R.T.: 11.626 min
Delta R.T.: -0.026 min
Response: 40355567
Conc: 1.50 ng/ml

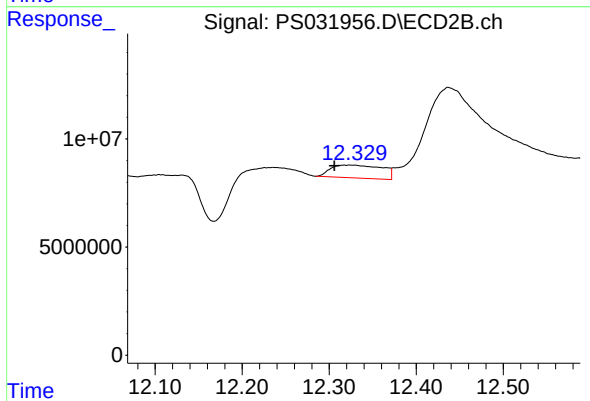

#16 DCPA

R.T.: 12.324 min
Delta R.T.: 0.018 min
Response: 24454252
Conc: 1.01 ng/ml