

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100719\
 Data File : PS007071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2019 10:23
 Operator : SM\AJ
 Sample : PB123645BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB123645BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 15:27:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.482	5.208	542.0E6	341.8E6	593.064	743.310 #
Target Compounds							
1) T	Dalapon	2.112	1.829	97052079	-5475982	90.838	N.D. #
2) T	3,5-DICHL...	0.000	4.536	0	36175181	N.D.	62.929
3) T	4-Nitroph...	5.334	0.000	13937533	0	36.553	N.D. #
5) T	DICAMBA	0.000	5.338	0	10740727	N.D.	6.381
7) T	MCPA	5.958	0.000	8922681	0	2.868	N.D. #
8) T	DICHLORPROP	6.337	0.000	113.5E6	0	147.865	N.D. #
9) T	2,4-D	6.456	6.129	10829226	6909717	13.214	13.546
10) T	Pentachlo...	6.742	6.518	12980791	11647555	1.089	1.851 #
12) T	2,4,5-T	0.000	7.293	0	43359882	N.D.	20.061
15) T	Picloram	9.038	8.985	235.7E6	67997744	35.154	18.682 #
16) T	DCPA	9.438	8.985	89483087	67997744	15.334	21.400 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100719\
Data File : PS007071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2019 10:23
Operator : SM\AJ
Sample : PB123645BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB123645BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 15:27:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

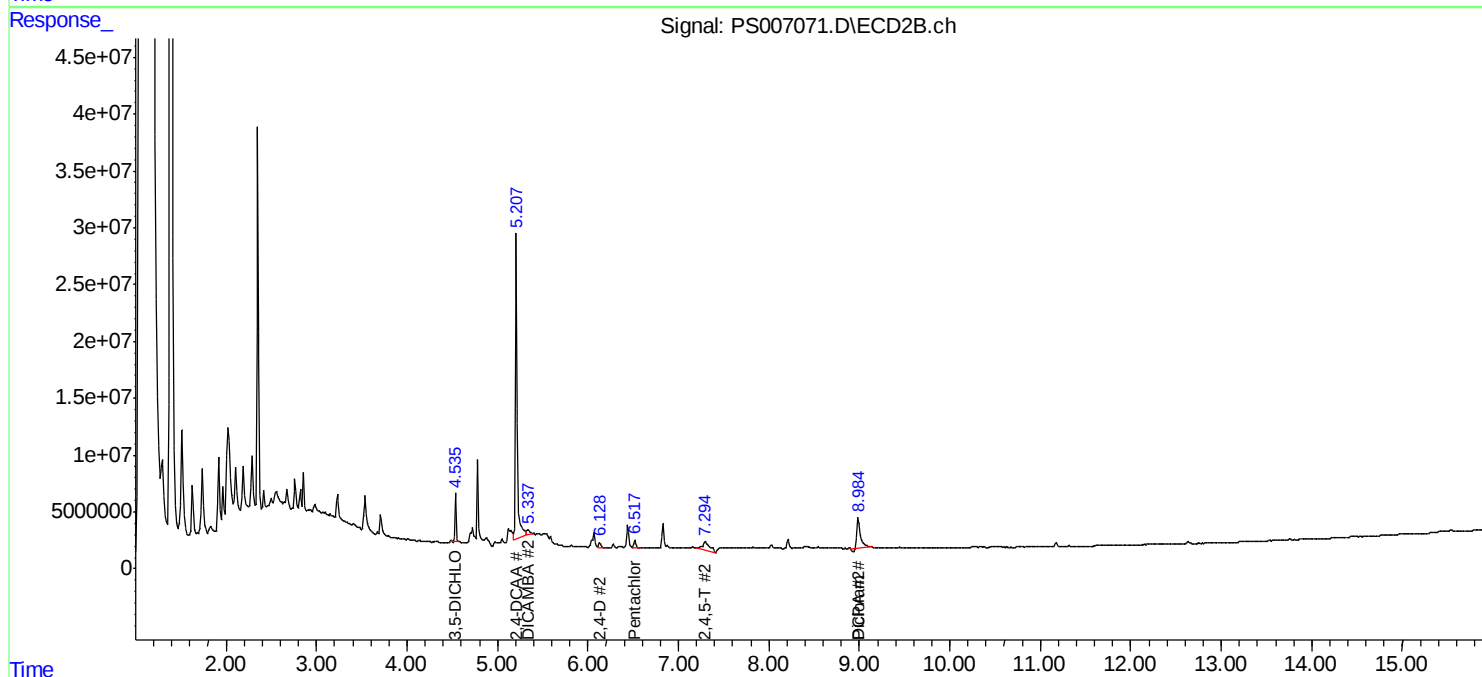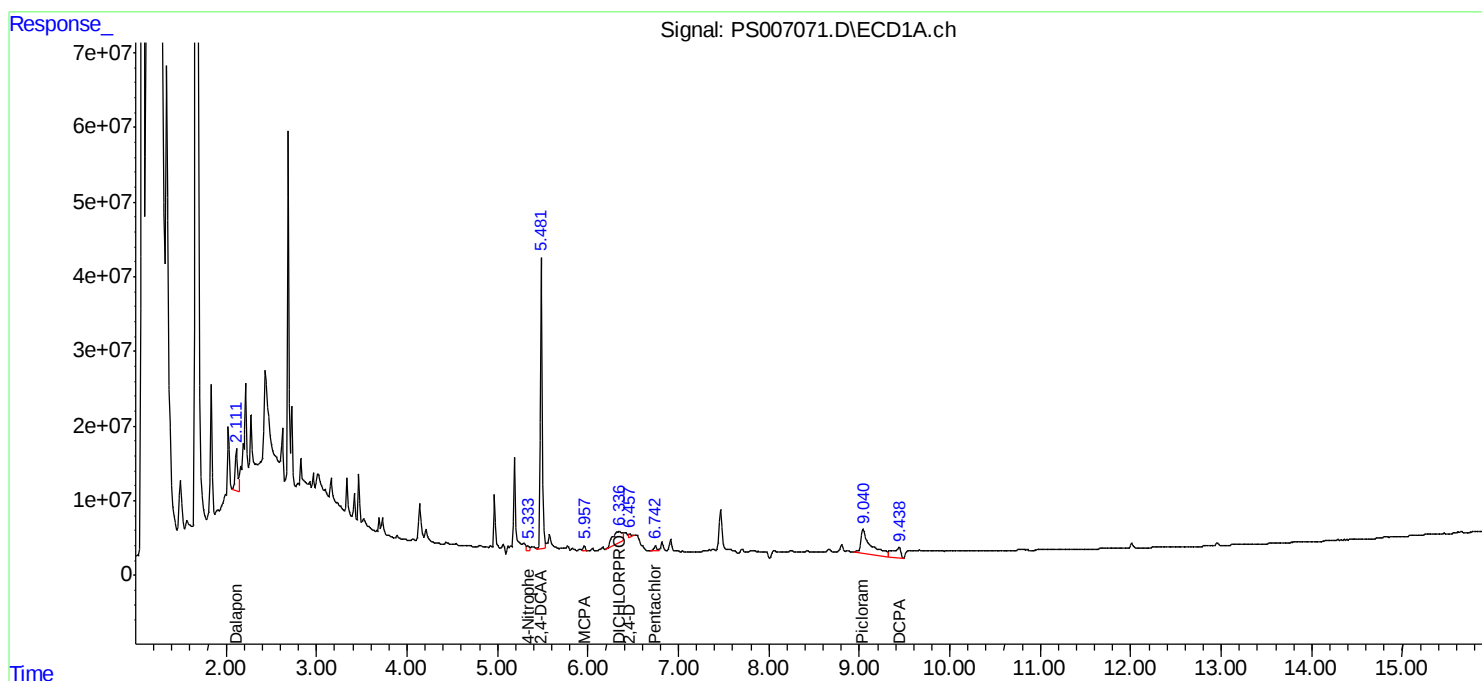


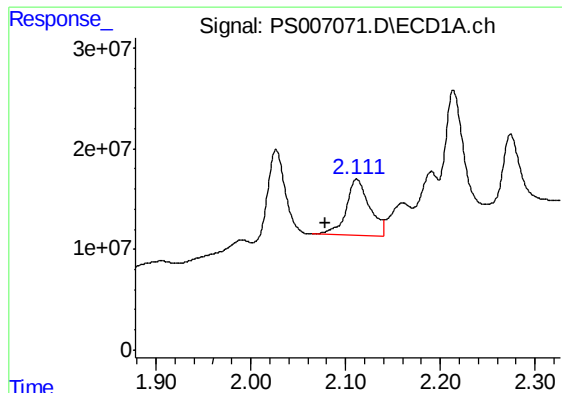

#1 Dalapon


R.T.: 2.112 min
Delta R.T.: 0.033 min
Response: 97052079
Conc: 90.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123645BL

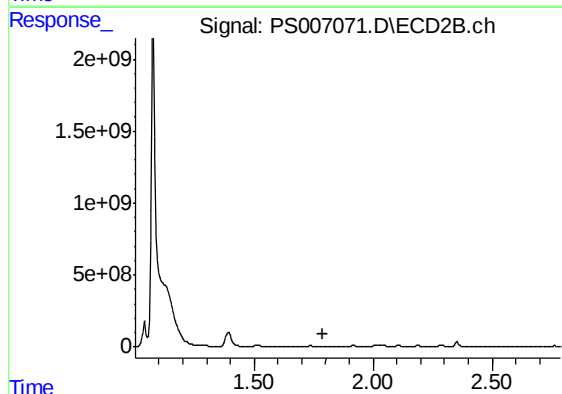


#1 Dalapon

R.T.: 1.829 min
Delta R.T.: 0.040 min
Response: -5475982
Conc: N.D.

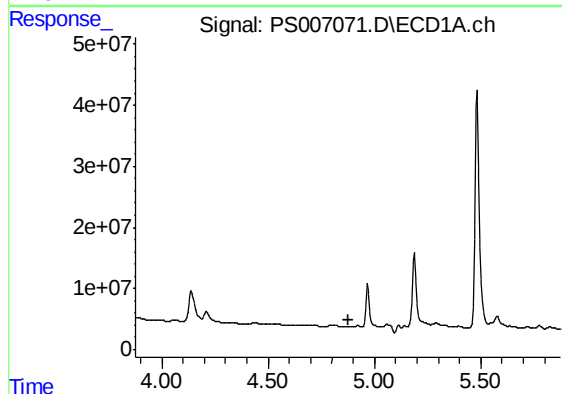


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.876 min
Response: 0
Conc: N.D.

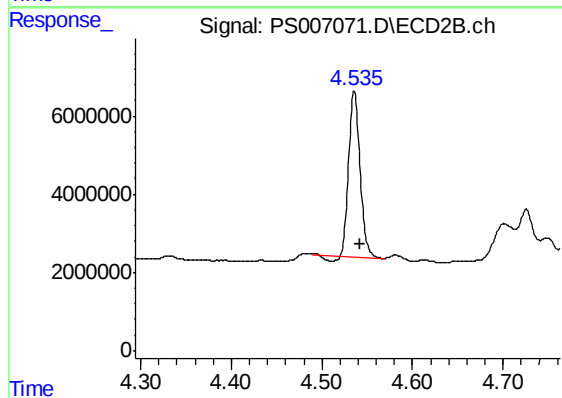

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.536 min
Delta R.T.: -0.006 min
Response: 36175181
Conc: 62.93 ng/ml

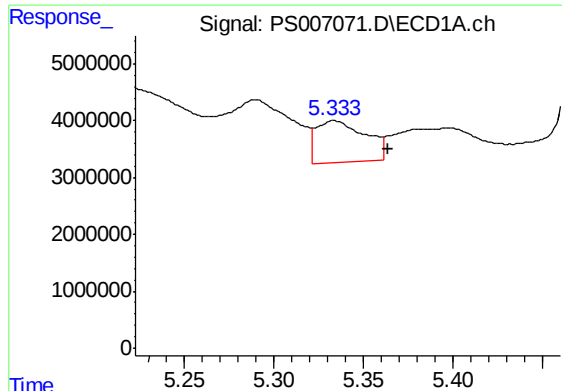

#3 4-Nitrophenol


R.T.: 5.334 min
Delta R.T.: -0.030 min
Response: 13937533
Conc: 36.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123645BL

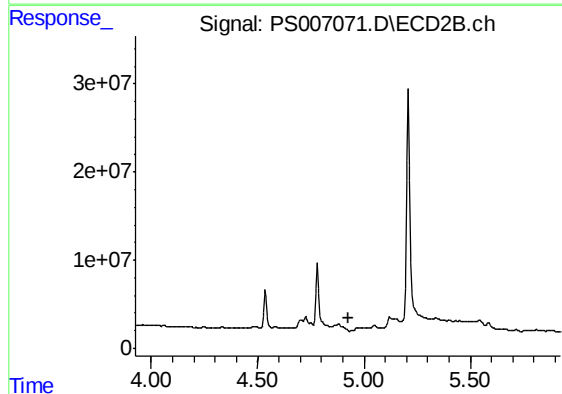


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

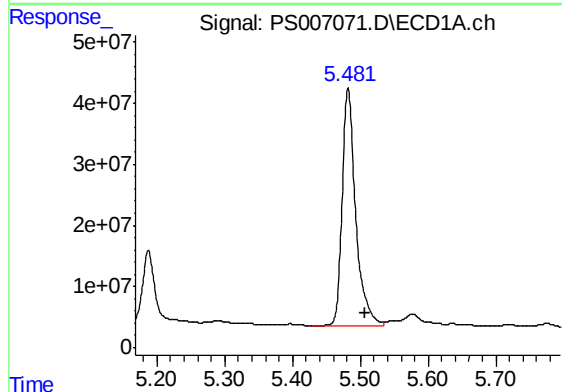


#4 2,4-DCAA

R.T.: 5.482 min
Delta R.T.: -0.026 min
Response: 541950435
Conc: 593.06 ng/ml

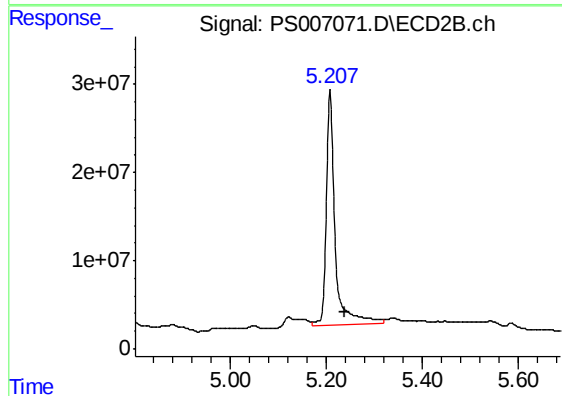

#4 2,4-DCAA


R.T.: 5.208 min
Delta R.T.: -0.030 min
Response: 341804585
Conc: 743.31 ng/ml

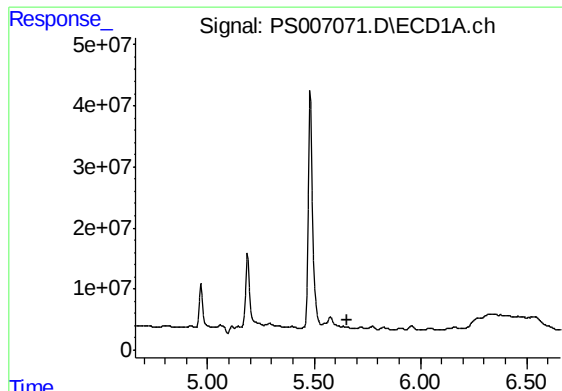

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB123645BL

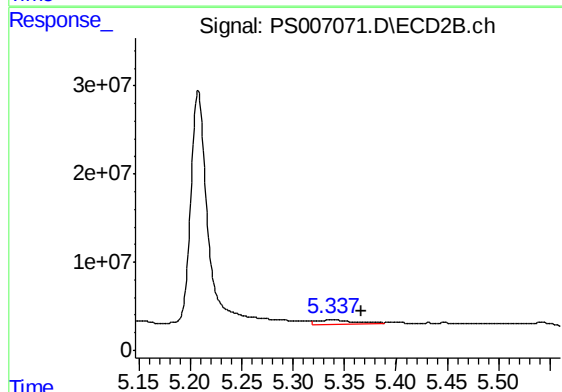


#5 DICAMBA

R.T.: 5.338 min
Delta R.T.: -0.028 min
Response: 10740727
Conc: 6.38 ng/ml

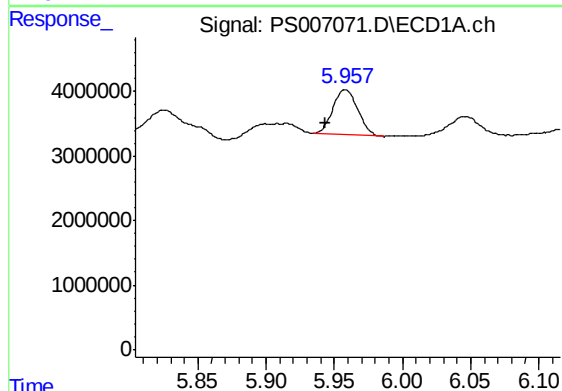


#7 MCPA

R.T.: 5.958 min
Delta R.T.: 0.015 min
Response: 8922681
Conc: 2.87 ug/ml

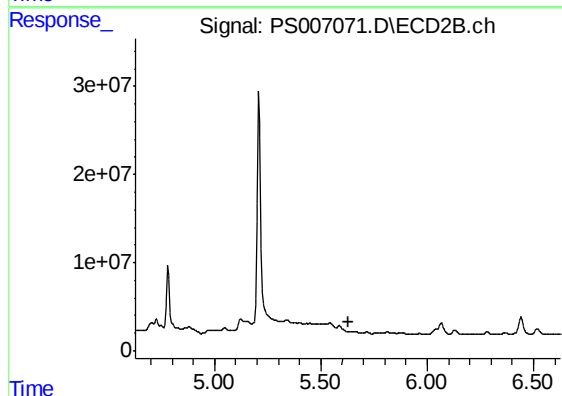

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 5.627 min
Response: 0
Conc: N.D.

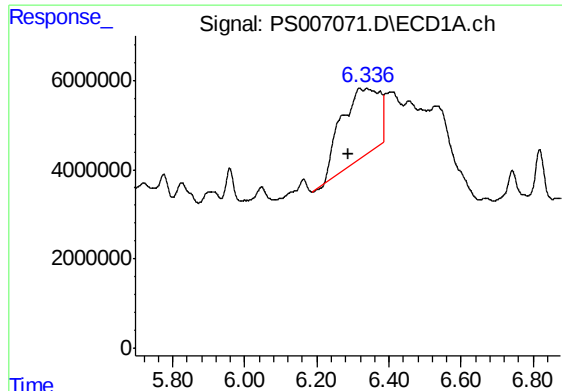

#8 DICHLORPROP


R.T.: 6.337 min
Delta R.T.: 0.049 min
Response: 113532381
Conc: 147.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123645BL

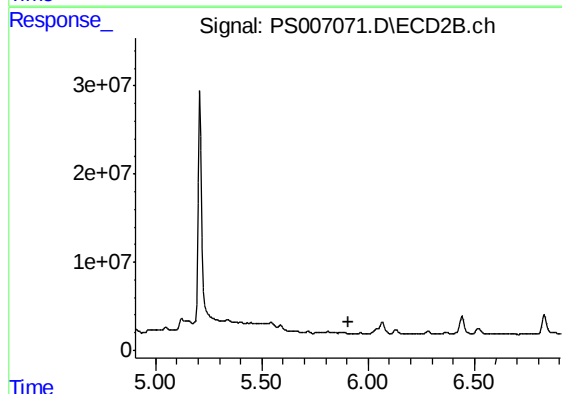


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 5.905 min
Response: 0
Conc: N.D.

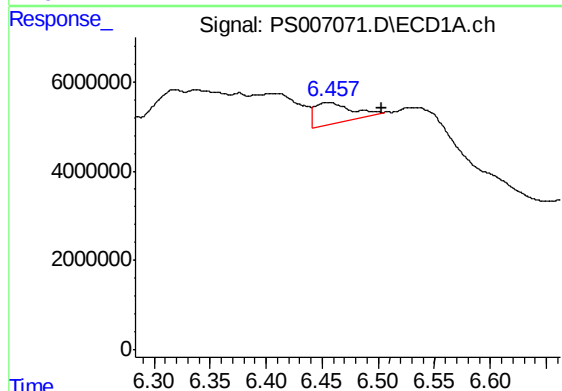


#9 2,4-D

R.T.: 6.456 min
Delta R.T.: -0.048 min
Response: 10829226
Conc: 13.21 ng/ml

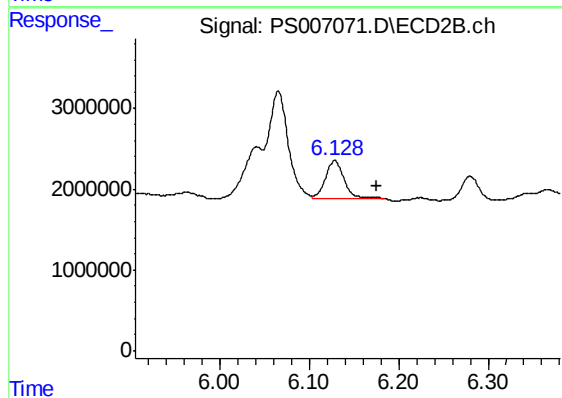

#9 2,4-D


R.T.: 6.129 min
Delta R.T.: -0.048 min
Response: 6909717
Conc: 13.55 ng/ml

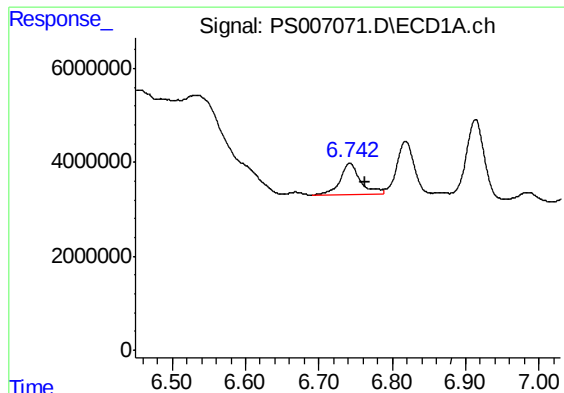

#10 Pentachlorophenol


R.T.: 6.742 min
Delta R.T.: -0.021 min
Response: 12980791
Conc: 1.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123645BL

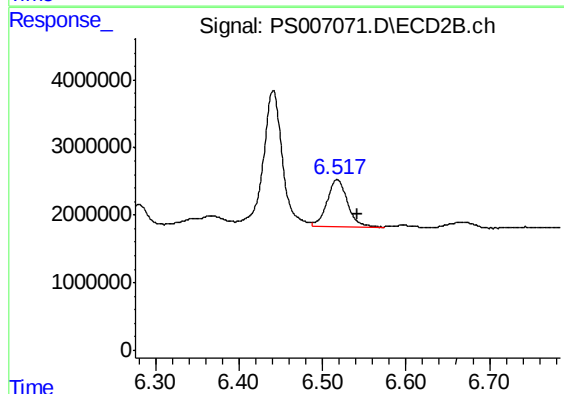


#10 Pentachlorophenol

R.T.: 6.518 min
Delta R.T.: -0.024 min
Response: 11647555
Conc: 1.85 ng/ml

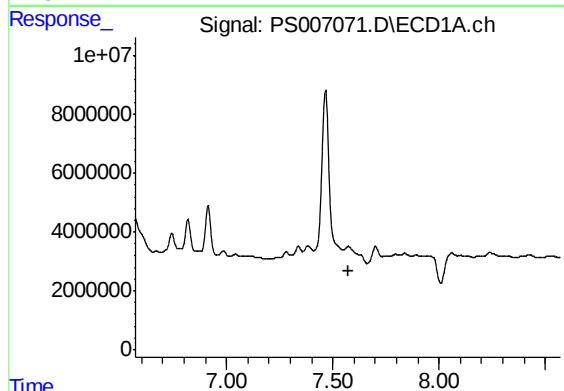


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.572 min
Response: 0
Conc: N.D.

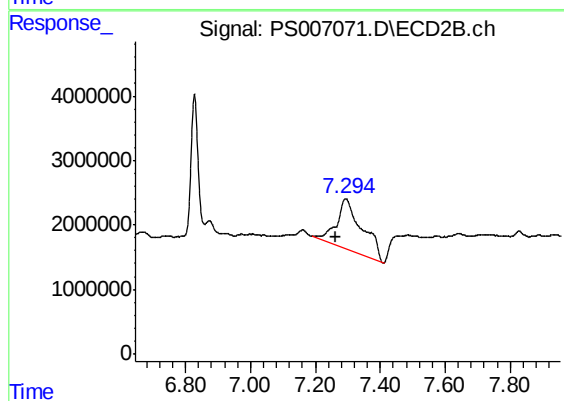

#12 2,4,5-T


R.T.: 7.293 min
Delta R.T.: 0.029 min
Response: 43359882
Conc: 20.06 ng/ml

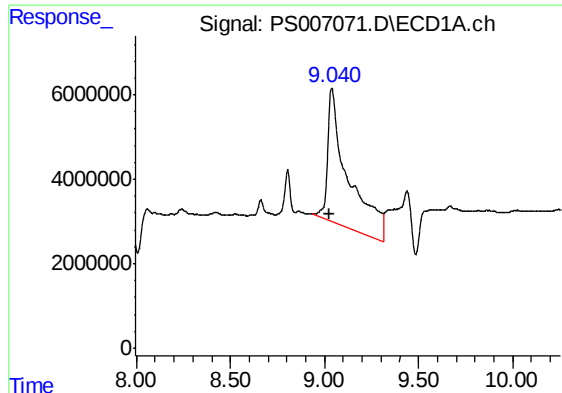

#15 Picloram


R.T.: 9.038 min
Delta R.T.: 0.013 min
Response: 235732444
Conc: 35.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123645BL

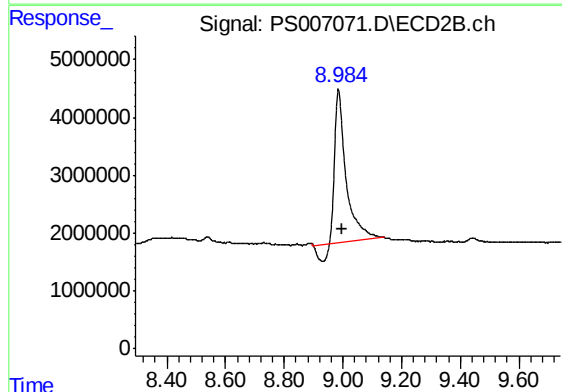


#15 Picloram

R.T.: 8.985 min
Delta R.T.: -0.014 min
Response: 67997744
Conc: 18.68 ng/ml

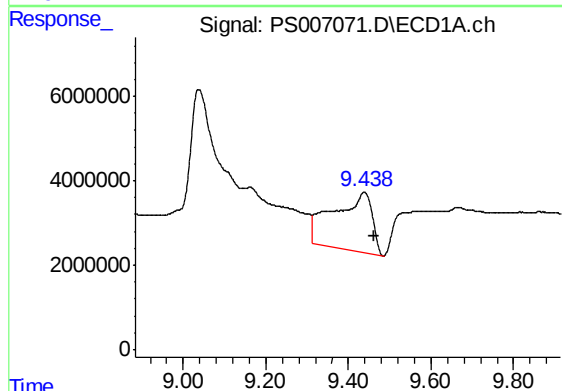

#16 DCPA

R.T.: 9.438 min
Delta R.T.: -0.024 min
Response: 89483087
Conc: 15.33 ng/ml

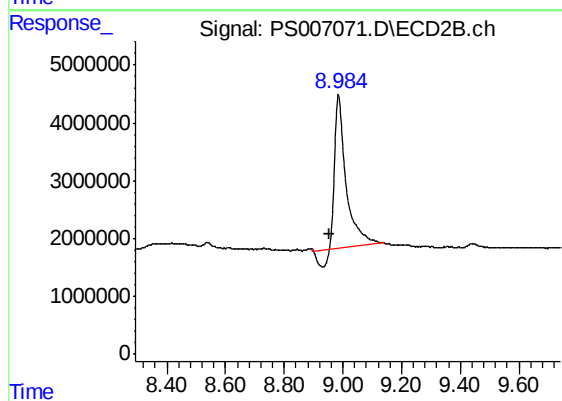

#16 DCPA

R.T.: 8.985 min
Delta R.T.: 0.029 min
Response: 67997744
Conc: 21.40 ng/ml