

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100719\
 Data File : PS007079.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2019 13:57
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 15:29:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.489	5.213	352.3E6	165.6E6	385.526	360.016
Target Compounds							
5) T	DICAMBA	5.637	0.000	31810099	0	9.845	N.D. #
9) T	2,4-D	6.547	0.000	206.5E6	0	251.967	N.D. #
12) T	2,4,5-T	7.535	7.316	31156068	15124889	6.123	6.998
15) T	Picloram	9.075	9.001	128.9E6	62009730	19.227	17.037
16) T	DCPA	0.000	9.001	0	62009730	N.D.	19.515



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100719\
Data File : PS007079.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2019 13:57
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 15:29:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

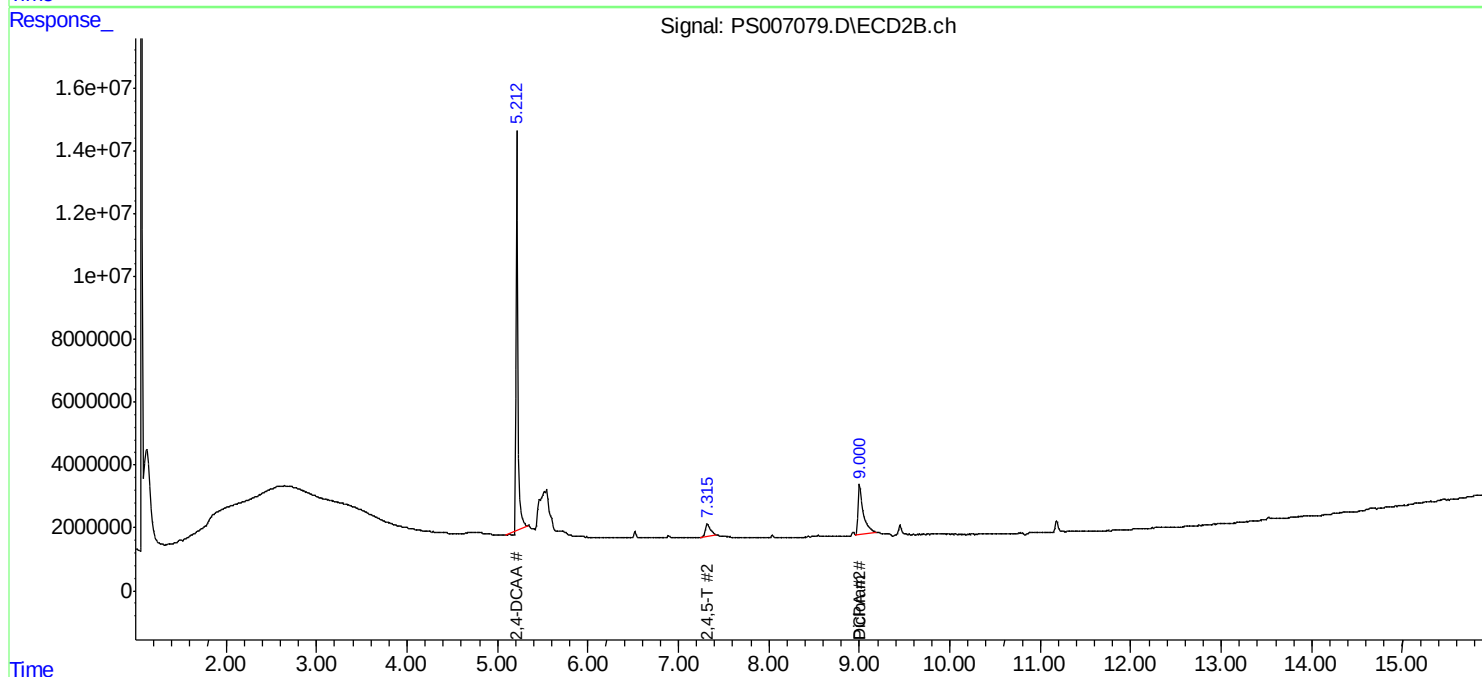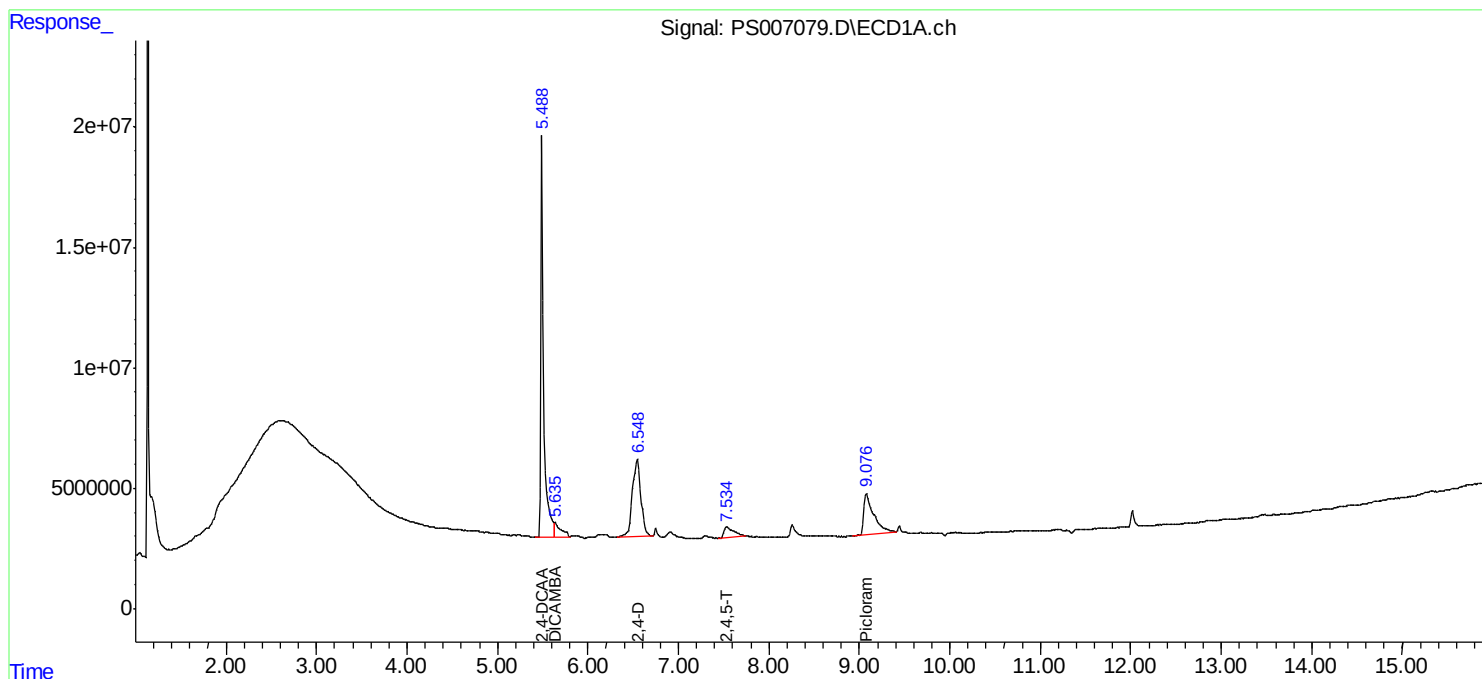


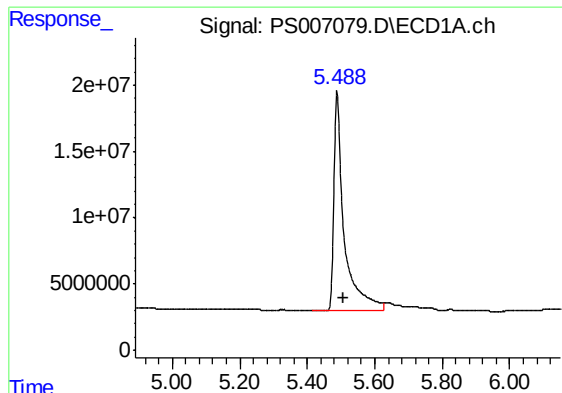

#4 2,4-DCAA


R.T.: 5.489 min
Delta R.T.: -0.019 min
Response: 352299250
Conc: 385.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

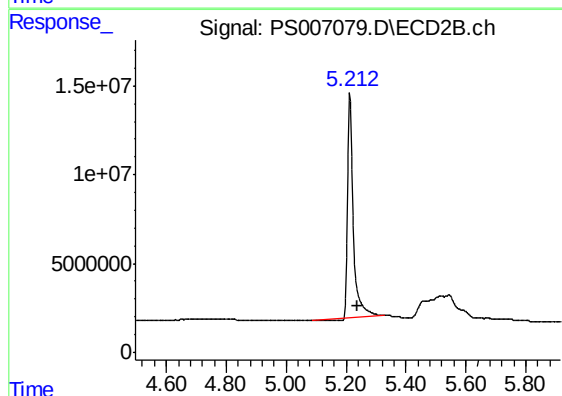


#4 2,4-DCAA

R.T.: 5.213 min
Delta R.T.: -0.025 min
Response: 165550081
Conc: 360.02 ng/ml

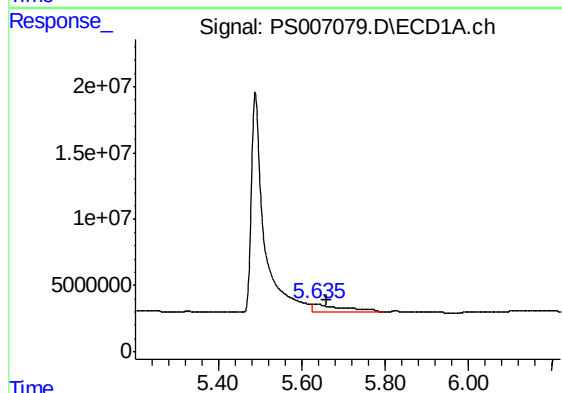


#5 DICAMBA

R.T.: 5.637 min
Delta R.T.: -0.023 min
Response: 31810099
Conc: 9.85 ng/ml

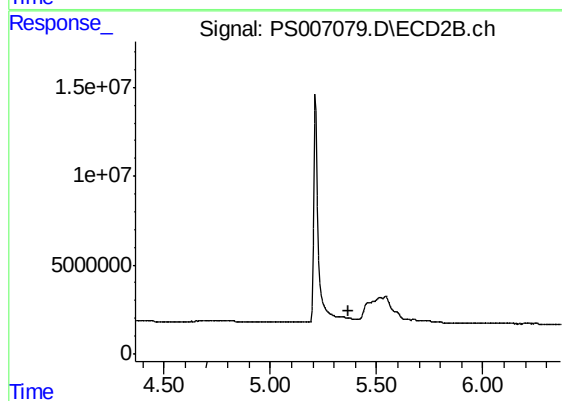

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.366 min
Response: 0
Conc: N.D.

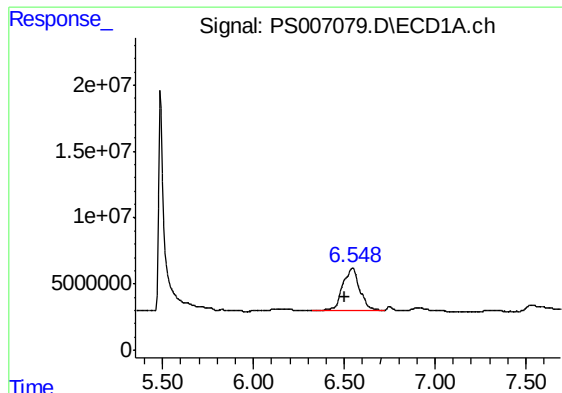

#9 2,4-D


R.T.: 6.547 min
Delta R.T.: 0.043 min
Response: 206490269
Conc: 251.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

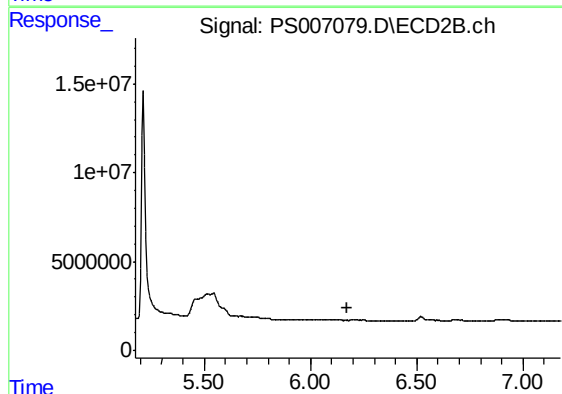


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

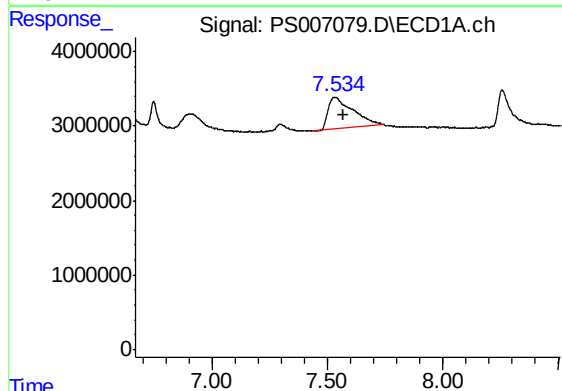


#12 2,4,5-T

R.T.: 7.535 min
Delta R.T.: -0.036 min
Response: 31156068
Conc: 6.12 ng/ml

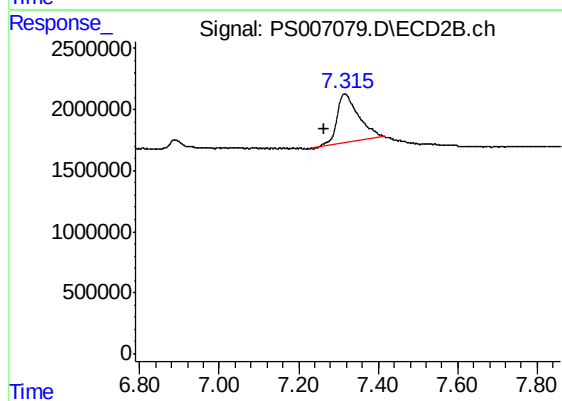

#12 2,4,5-T


R.T.: 7.316 min
Delta R.T.: 0.051 min
Response: 15124889
Conc: 7.00 ng/ml

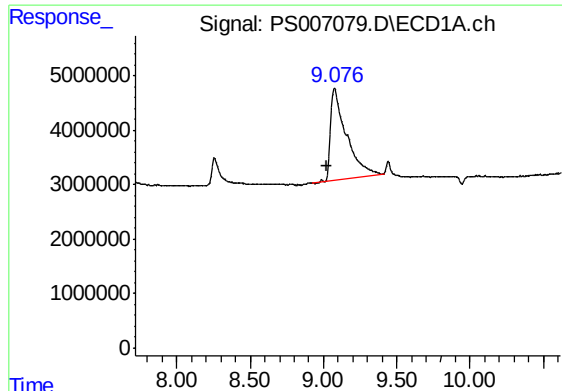

#15 Picloram


R.T.: 9.075 min
Delta R.T.: 0.050 min
Response: 128933112
Conc: 19.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

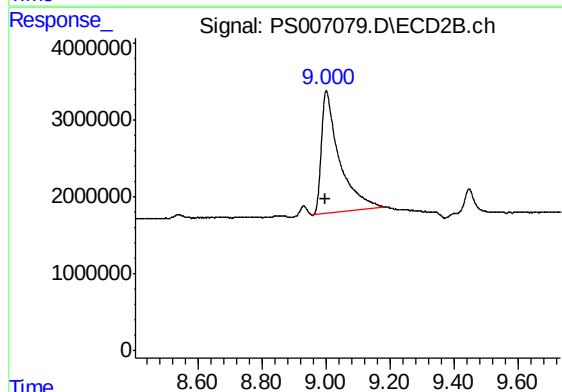


#15 Picloram

R.T.: 9.001 min
Delta R.T.: 0.003 min
Response: 62009730
Conc: 17.04 ng/ml

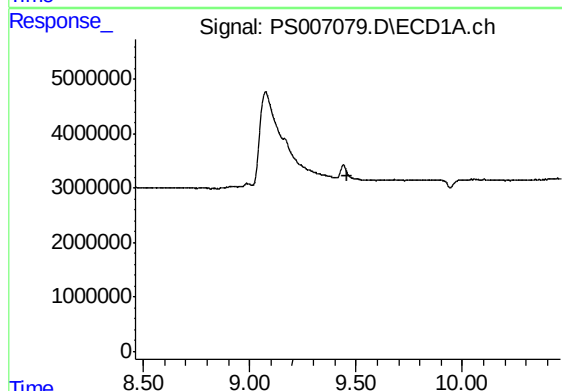

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.462 min
Response: 0
Conc: N.D.

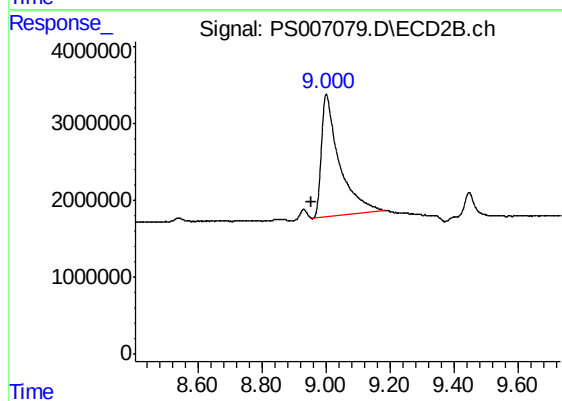

#16 DCPA

R.T.: 9.001 min
Delta R.T.: 0.046 min
Response: 62009730
Conc: 19.52 ng/ml