

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100722\
 Data File : PS020747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2022 08:54
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 23:32:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.421	6.867	951.9E6	667.1E6	504.587	498.196
Target Compounds							
1) T	Dalapon	2.470	0.000	139286	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.808	6.024	2426288	343948	<MDL	<MDL #
3) T	4-Nitroph...	6.258	6.457	7231540	771146	1.052	<MDL #
5) T	DICAMBA	6.620f	0.000	3523161	0	<MDL	N.D. #
6) T	MCPD	6.750	0.000	8317711	0	1.415	N.D. #
7) T	MCPA	6.789f	0.000	5441147	0	<MDL	N.D. #
8) T	DICHLORPROP	7.187	7.681	160101	2084525	<MDL	1.437 #
9) T	2,4-D	7.338	8.005f	262997	88859	<MDL	<MDL #
10) T	Pentachlo...	7.652f	8.389	2016326	4520575	<MDL	<MDL #
11) T	2,4,5-TP ...	8.113	0.000	1136852	0	<MDL	N.D. #
12) T	2,4,5-T	8.389	9.174f	1025597	2345531	<MDL	<MDL #
13) T	2,4-DB	8.848f	9.581f	5907023	1937396	2.586	1.729 #
14) T	DINOSEB	9.971	0.000	884185	0	<MDL	N.D. #
15) T	Picloram	9.788	10.941	14755717	12652330	<MDL	1.073 #
16) T	DCPA	10.232	10.897	3004281	4359207	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100722\
Data File : PS020747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2022 08:54
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 23:32:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

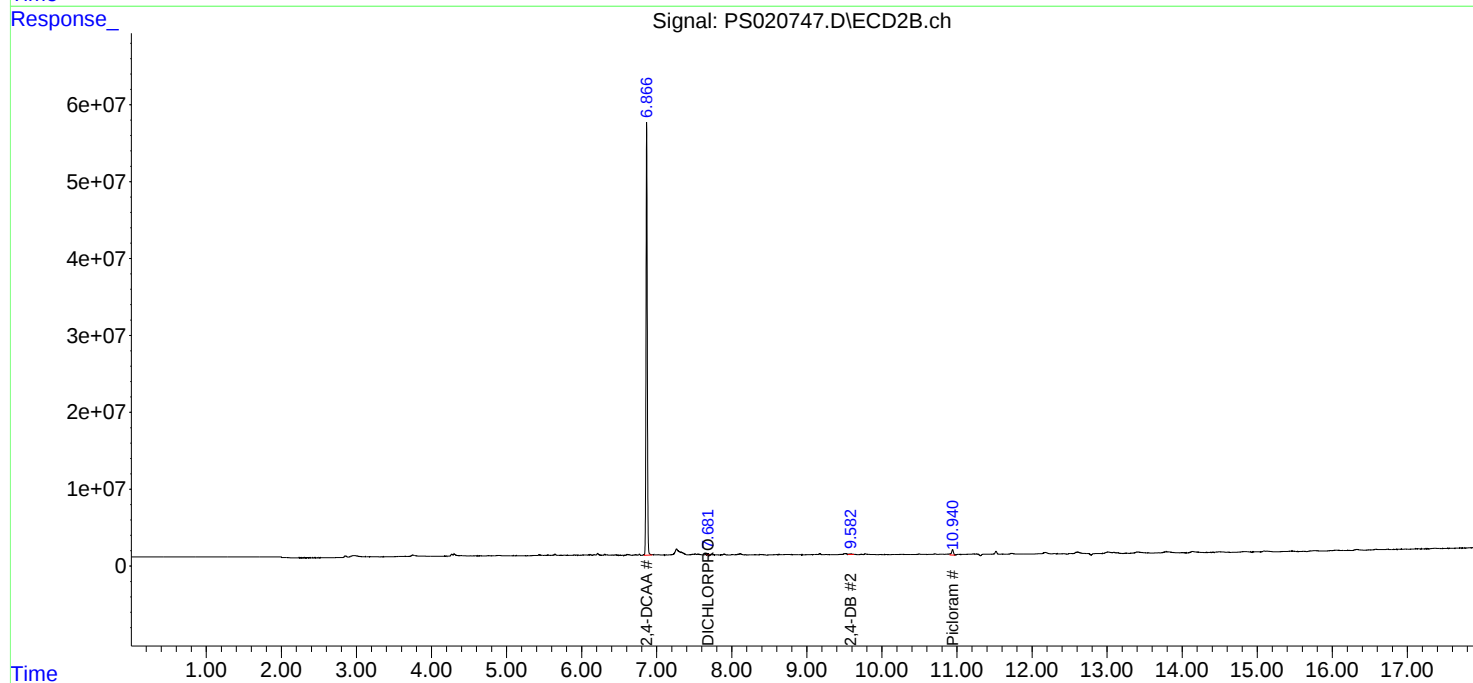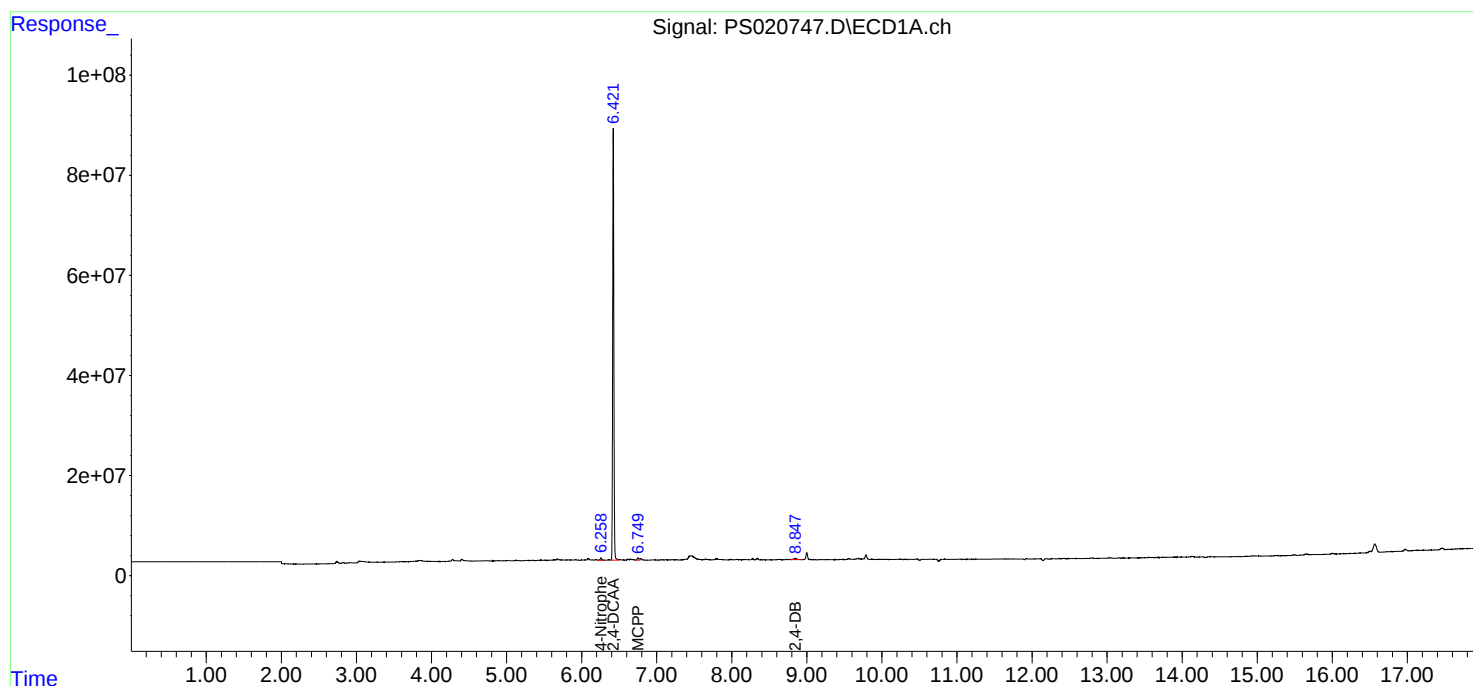


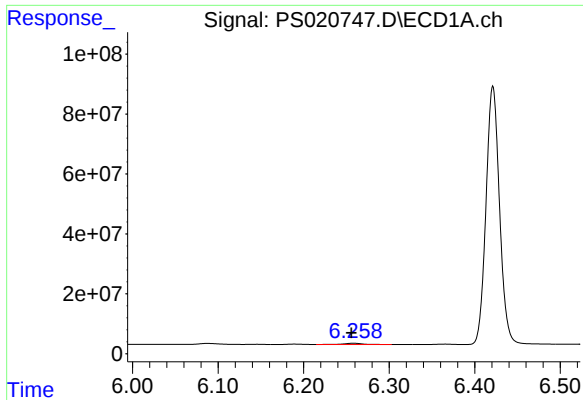

#3 4-Nitrophenol


R.T.: 6.258 min
Delta R.T.: 0.002 min
Response: 7231540
Conc: 1.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

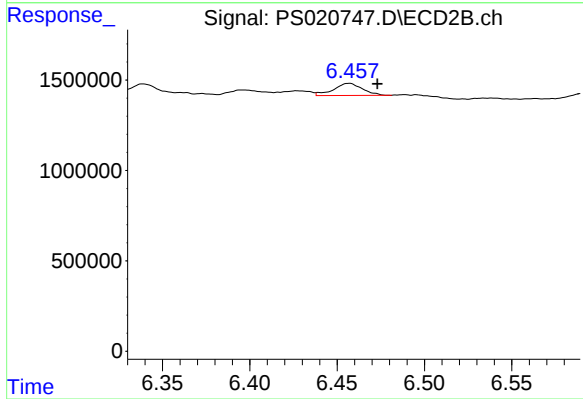


#3 4-Nitrophenol

R.T.: 6.457 min
Delta R.T.: -0.016 min
Response: 771146
Conc: N.D.

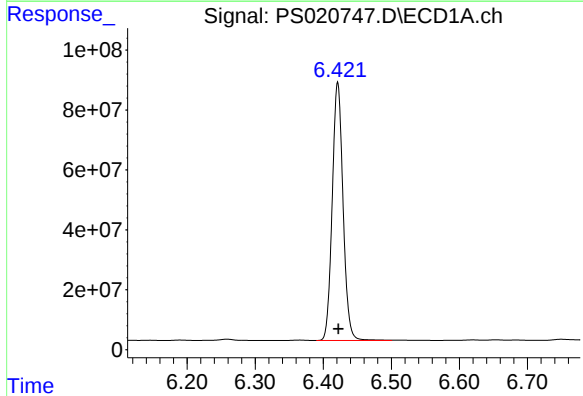


#4 2,4-DCAA

R.T.: 6.421 min
Delta R.T.: 0.000 min
Response: 951877353
Conc: 504.59 ng/ml

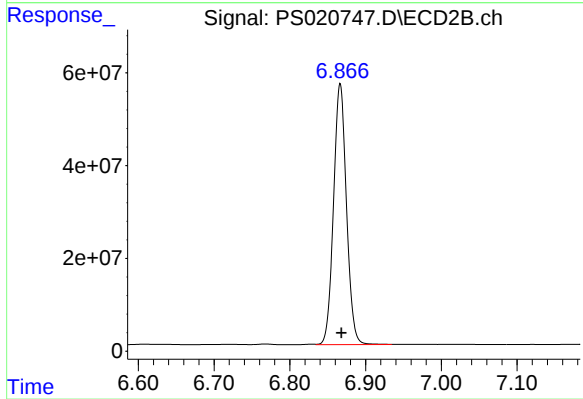

#4 2,4-DCAA


R.T.: 6.867 min
Delta R.T.: -0.002 min
Response: 667075168
Conc: 498.20 ng/ml

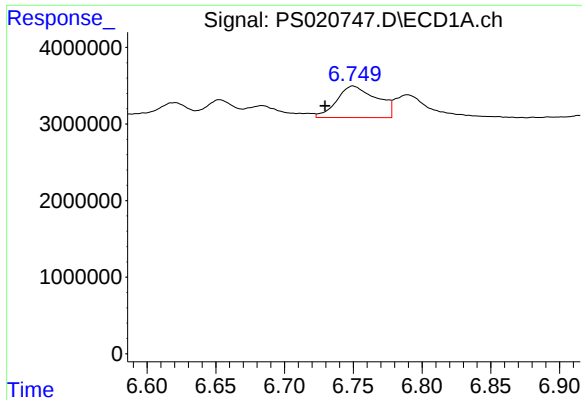

#6 MCP


R.T.: 6.750 min
Delta R.T.: 0.020 min
Response: 8317711
Conc: 1.42 ug/ml

Instrument :
ECD_S
ClientSampleId :

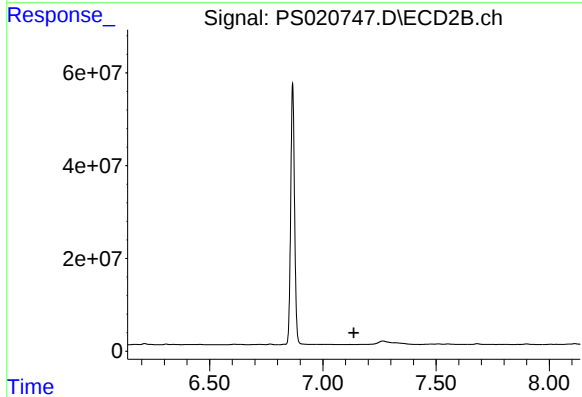


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.137 min
Response: 0
Conc: N.D.

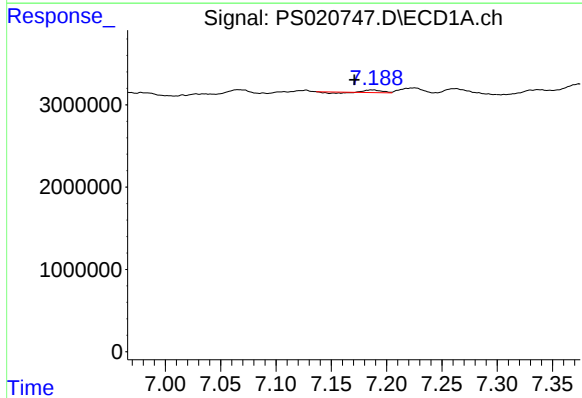


#8 DICHLORPROP

R.T.: 7.187 min
Delta R.T.: 0.016 min
Response: 160101
Conc: N.D.

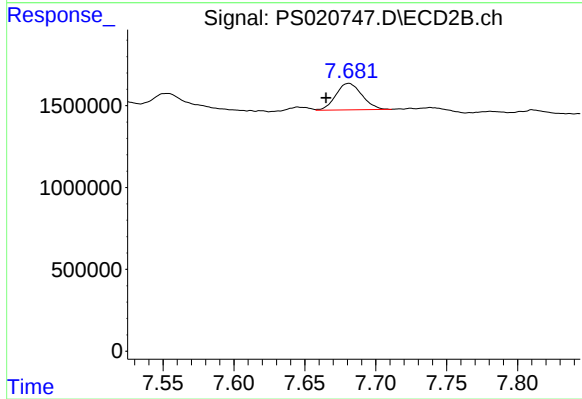

#8 DICHLORPROP


R.T.: 7.681 min
Delta R.T.: 0.016 min
Response: 2084525
Conc: 1.44 ng/ml

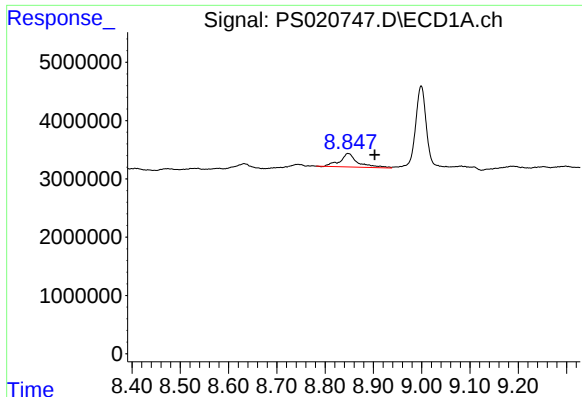

#13 2,4-DB


R.T.: 8.848 min
Delta R.T.: -0.055 min
Response: 5907023
Conc: 2.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

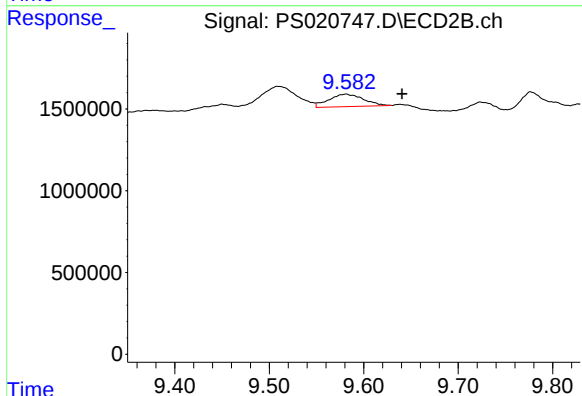


#13 2,4-DB

R.T.: 9.581 min
Delta R.T.: -0.059 min
Response: 1937396
Conc: 1.73 ng/ml

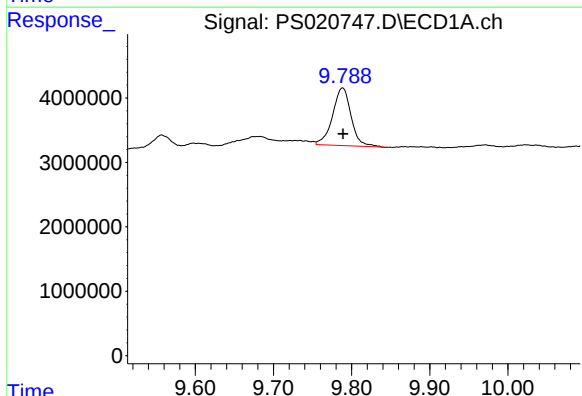

#15 Picloram

R.T.: 9.788 min
Delta R.T.: 0.000 min
Response: 14755717
Conc: N.D.

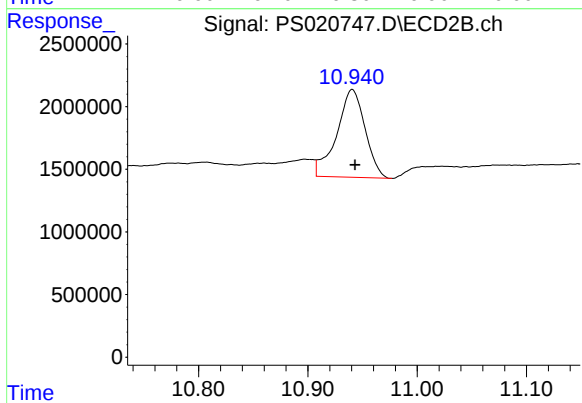

#15 Picloram

R.T.: 10.941 min
Delta R.T.: -0.003 min
Response: 12652330
Conc: 1.07 ng/ml