

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100722\
 Data File : PS020751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2022 12:44
 Operator : AR\AJ
 Sample : PB148124BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB148124BL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/10/2022
 Supervised By :Ankita Jodhani 10/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 23:33:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.421	6.866	1086.0E6	748.6E6	575.700m	559.109

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100722\
Data File : PS020751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2022 12:44
Operator : AR\AJ
Sample : PB148124BL
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
PB148124BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/10/2022
Supervised By : Ankita Jodhani 10/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 23:33:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

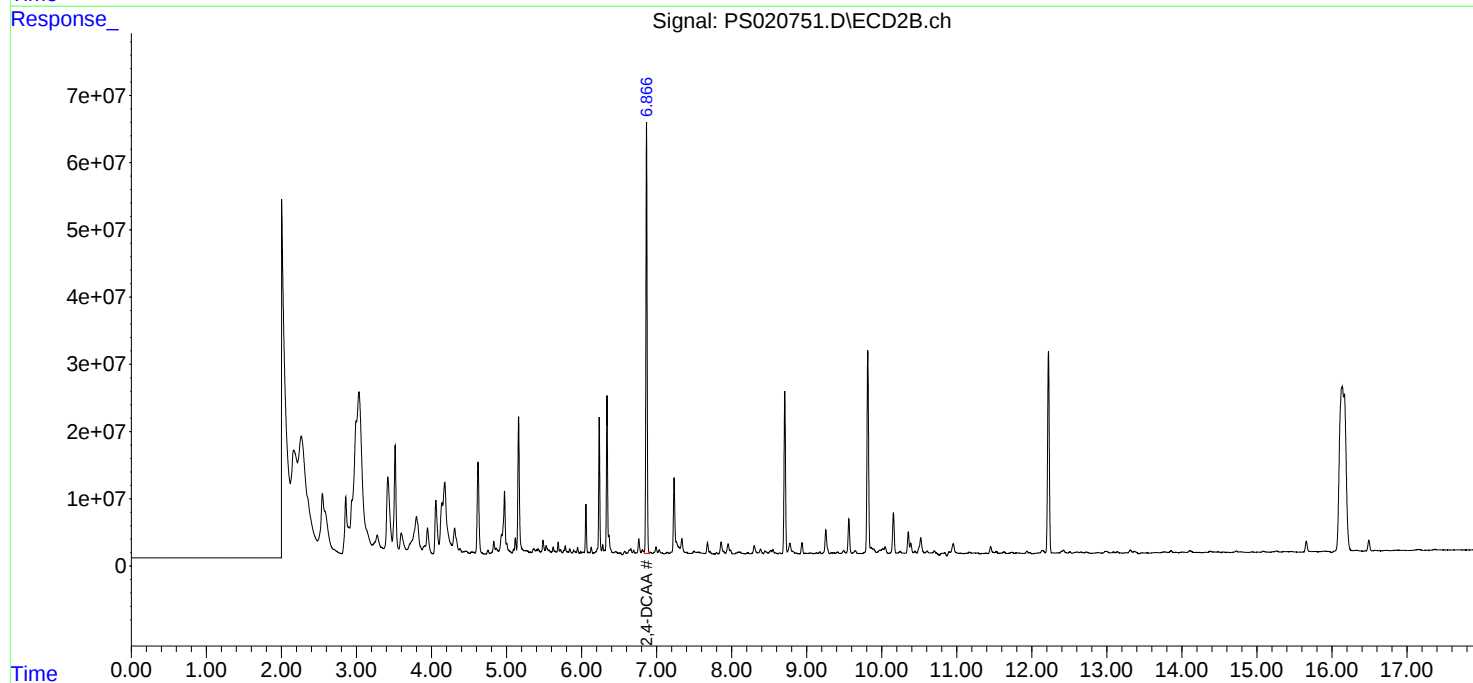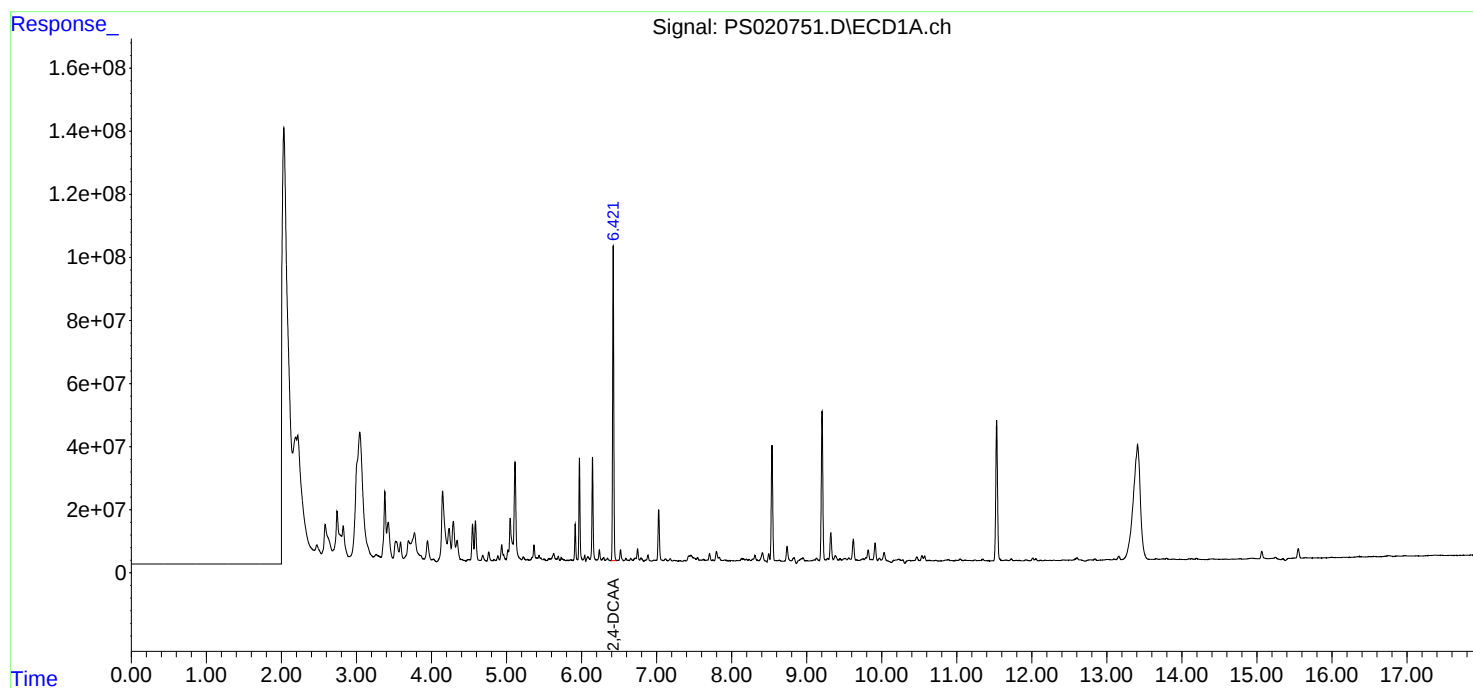

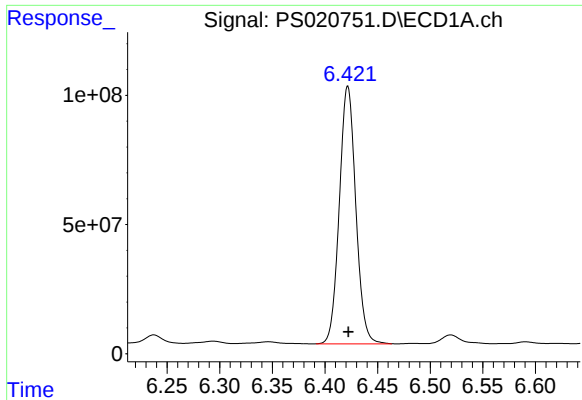


#4 2,4-DCAA

R.T.: 6.421 min
Delta R.T.: 0.000 min
Response: 1086030122
Conc: 575.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB148124BL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/10/2022
Supervised By :Ankita Jodhani 10/11/2022

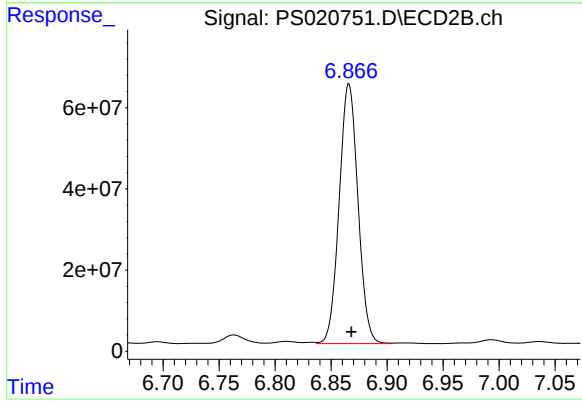

#4 2,4-DCAA

R.T.: 6.866 min
Delta R.T.: -0.002 min
Response: 748636829
Conc: 559.11 ng/ml