

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100724\
 Data File : PS027861.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2024 13:38
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 14:15:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 07 13:46:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.099	7.628	1351.9E6	469.8E6	501.760	472.802
Target Compounds							
1) T	Dalapon	2.589f	2.657f	103.3E6	161792	23.014	<MDL #
2) T	3,5-DICHL...	6.298	0.000	541100	0	<MDL	N.D. #
3) T	4-Nitroph...	6.898	0.000	5951399	0	3.259	N.D. #
5) T	DICAMBA	0.000	7.827	0	5296373	N.D.	1.523
6) T	MCPD	7.415f	0.000	3134696	0	<MDL	N.D. #
7) T	MCPA	7.638f	0.000	863144	0	<MDL	N.D. #
8) T	DICHLORPROP	7.951	8.571f	958874	1108805	<MDL	1.123 #
11) T	2,4,5-TP ...	9.009f	9.708f	7586781	7777149	<MDL	1.570 #
12) T	2,4,5-T	9.337	10.152	4761657	8505100	<MDL	1.976 #
13) T	2,4-DB	9.887	0.000	523292	0	<MDL	N.D. #
14) T	DINOSEB	11.063	11.077	3000789	1145539	<MDL	<MDL #
15) T	Picloram	10.889	12.180	70376599	6088355	3.269	1.457 #
16) T	DCPA	11.361	12.111	2239382	3072581	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100724\
Data File : PS027861.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2024 13:38
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 14:15:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
Quant Title : 8080.M
QLast Update : Mon Oct 07 13:46:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

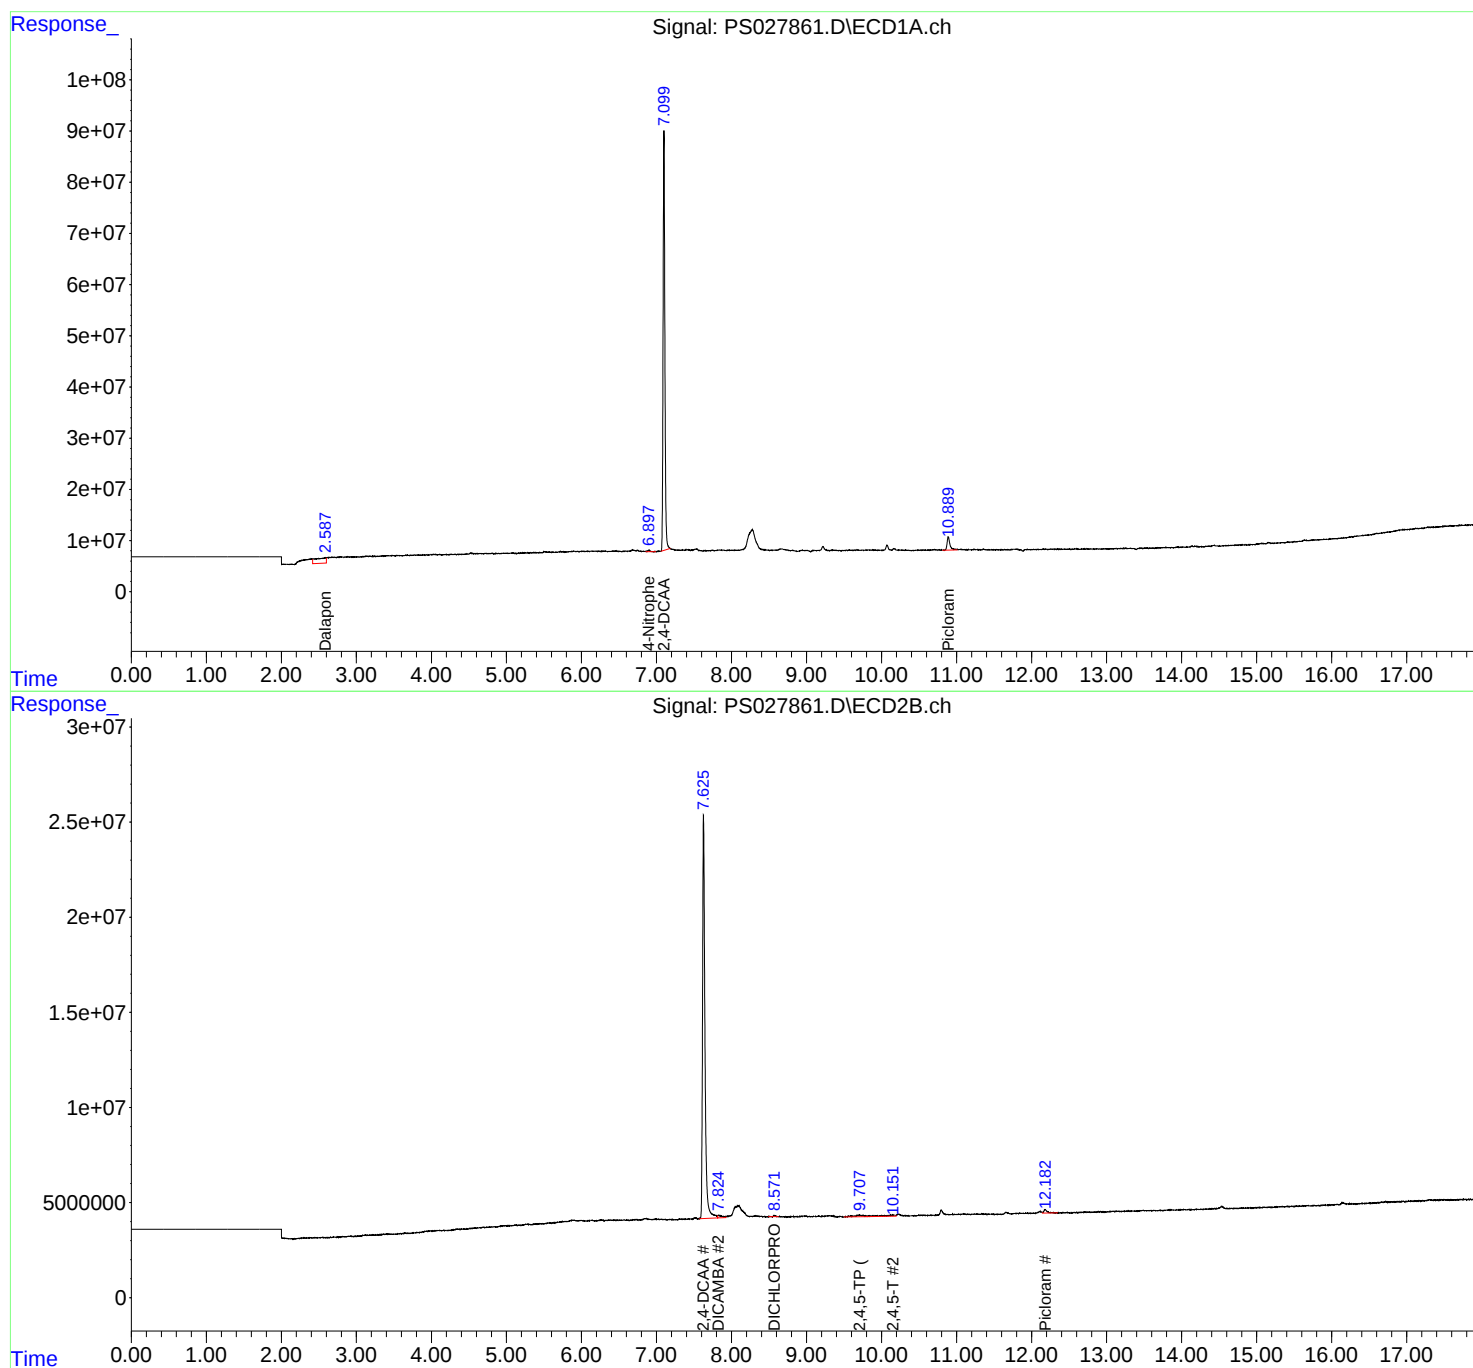


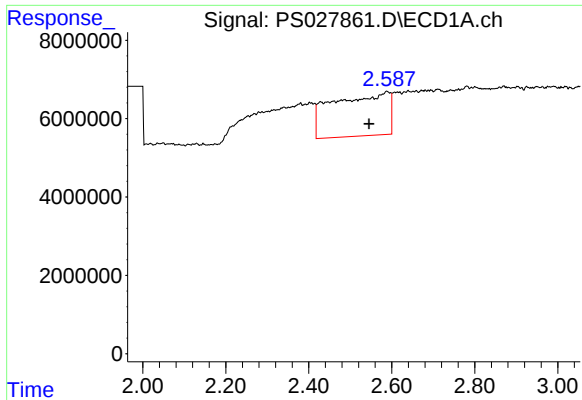

#1 Dalapon


R.T.: 2.589 min
Delta R.T.: 0.044 min
Response: 103283630
Conc: 23.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

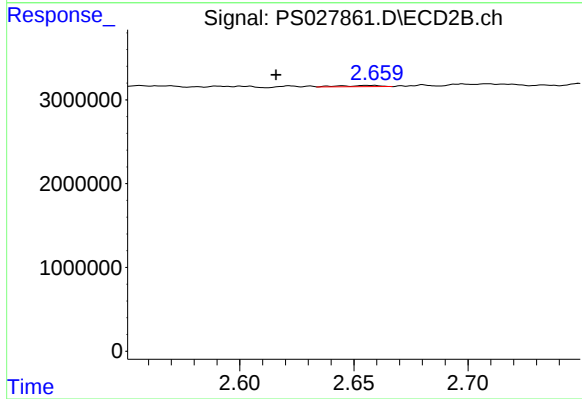


#1 Dalapon

R.T.: 2.657 min
Delta R.T.: 0.041 min
Response: 161792
Conc: N.D.

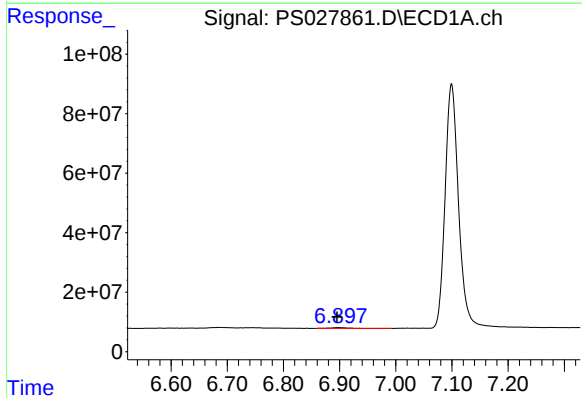


#3 4-Nitrophenol

R.T.: 6.898 min
Delta R.T.: 0.003 min
Response: 5951399
Conc: 3.26 ng/ml

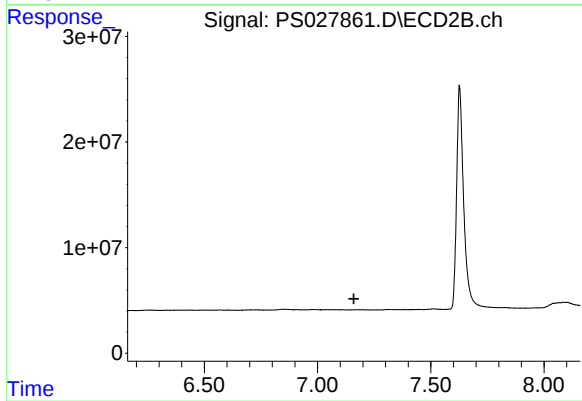

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.160 min
Response: 0
Conc: N.D.

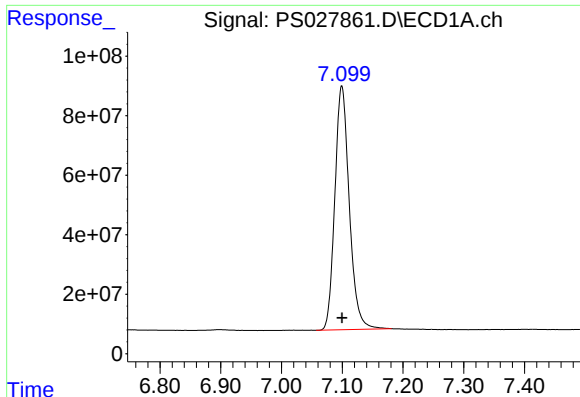

#4 2,4-DCAA


R.T.: 7.099 min
Delta R.T.: 0.000 min
Response: 1351887242
Conc: 501.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

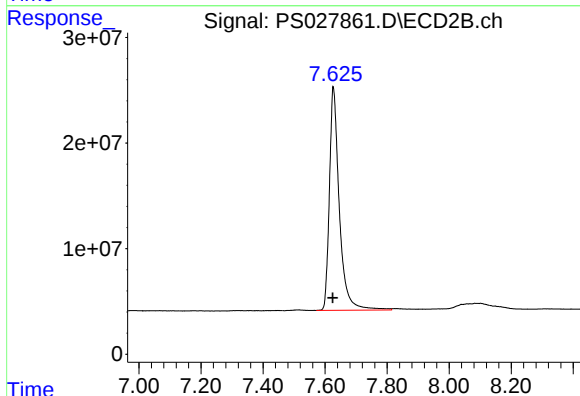


#4 2,4-DCAA

R.T.: 7.628 min
Delta R.T.: 0.003 min
Response: 469816845
Conc: 472.80 ng/ml

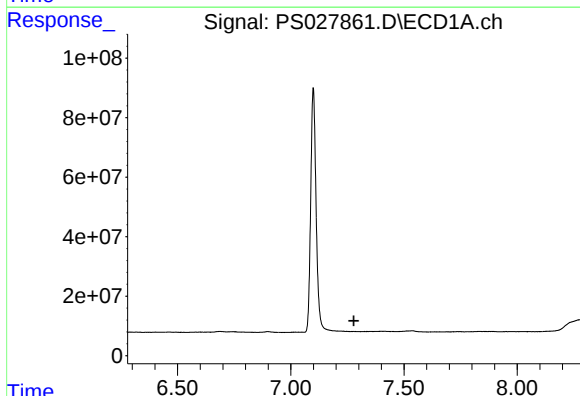


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.279 min
Response: 0
Conc: N.D.

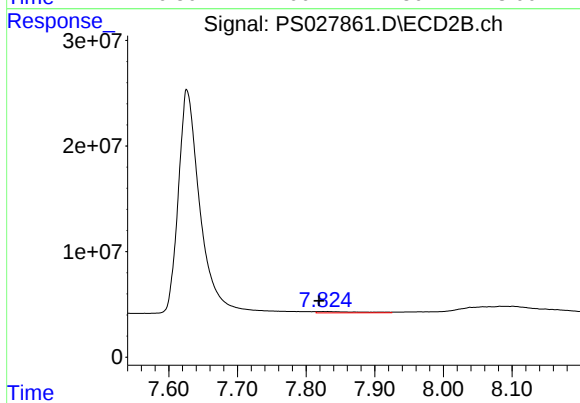

#5 DICAMBA


R.T.: 7.827 min
Delta R.T.: 0.008 min
Response: 5296373
Conc: 1.52 ng/ml

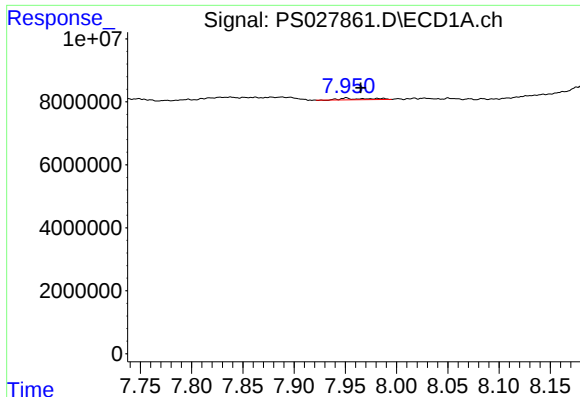

#8 DICHLORPROP


R.T.: 7.951 min
Delta R.T.: -0.014 min
Response: 958874
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

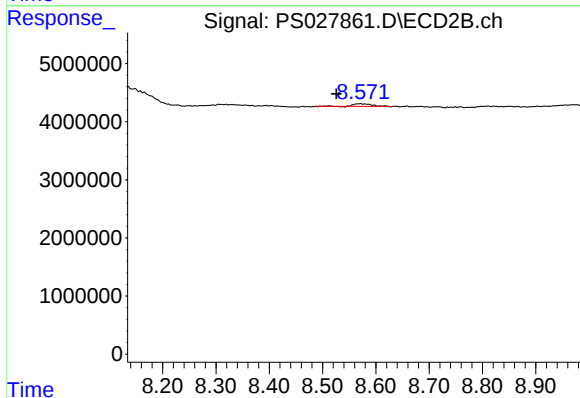


#8 DICHLORPROP

R.T.: 8.571 min
Delta R.T.: 0.045 min
Response: 1108805
Conc: 1.12 ng/ml

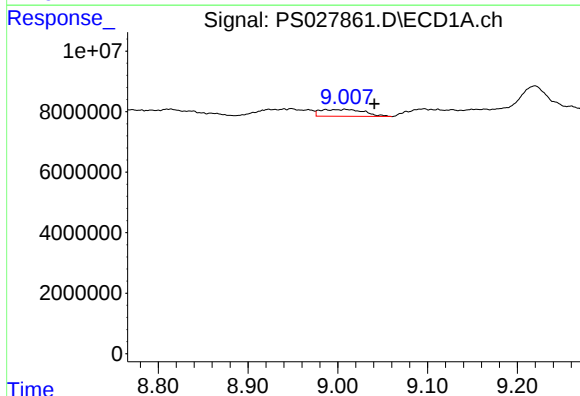


#11 2,4,5-TP (SILVEX)

R.T.: 9.009 min
Delta R.T.: -0.032 min
Response: 7586781
Conc: N.D.

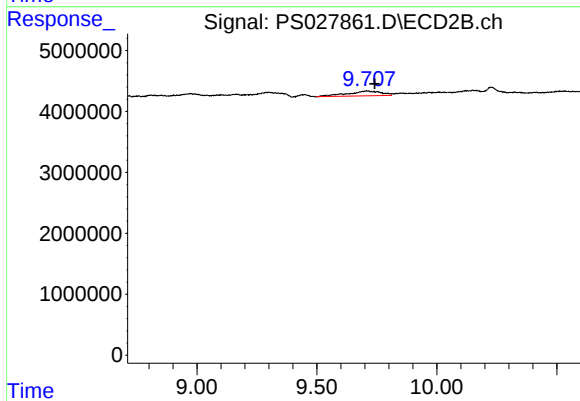

#11 2,4,5-TP (SILVEX)


R.T.: 9.708 min
Delta R.T.: -0.034 min
Response: 7777149
Conc: 1.57 ng/ml

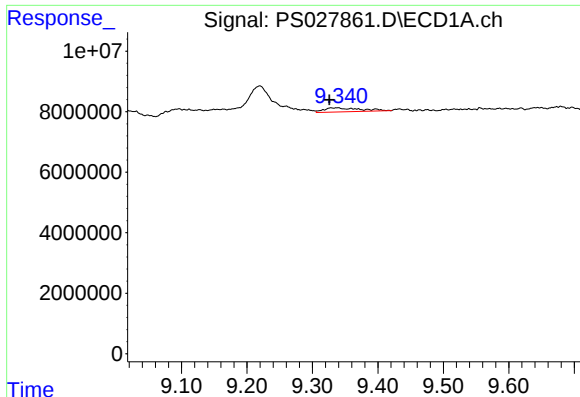

#12 2,4,5-T


R.T.: 9.337 min
Delta R.T.: 0.011 min
Response: 4761657
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

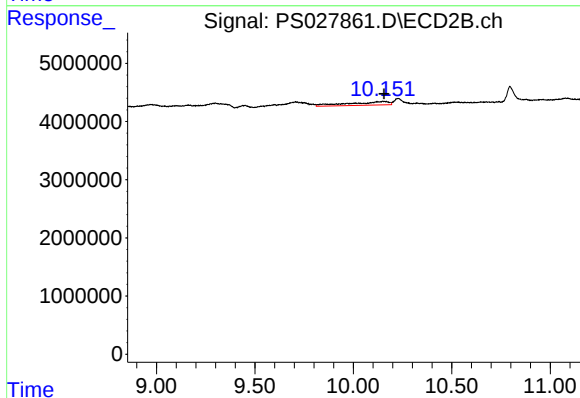


#12 2,4,5-T

R.T.: 10.152 min
Delta R.T.: -0.004 min
Response: 8505100
Conc: 1.98 ng/ml

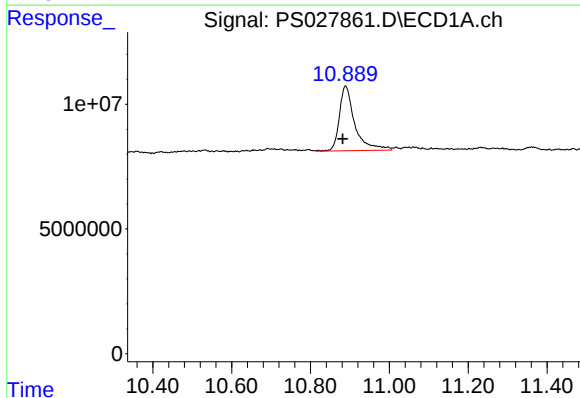

#15 Picloram

R.T.: 10.889 min
Delta R.T.: 0.007 min
Response: 70376599
Conc: 3.27 ng/ml

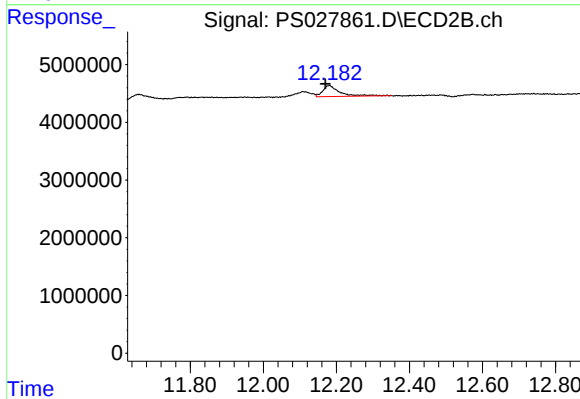

#15 Picloram

R.T.: 12.180 min
Delta R.T.: 0.010 min
Response: 6088355
Conc: 1.46 ng/ml